

# A portable test-bench for real-time radiation damage measurements in scintillating and wavelength-shifting fibres

Peter R. Hobson<sup>a, b</sup>, David R. Smith<sup>a</sup>



<sup>a</sup> Brunel University London, College of Engineering, Design and Physical Sciences, Kingston Lane, Uxbridge, Middlesex, UB8 3PH, UK

<sup>b</sup> School of Physics and Astronomy, Queen Mary University of London, Mile End Road, London, E1 4NS, UK

## Motivation


A portable test-bench has been designed and constructed as part of the AIDA-2020 project [1] to enable the real-time measurement of radiation-induced absorption in scintillating and wavelength-shifting fibres typically used in the readout of fibre calorimeters or scintillating tiles such as those used in some hadron calorimeters. The test-bench has been designed to be used in a range of facilities, such as <sup>60</sup>Co irradiators or high-intensity test beam facilities, and can accommodate fibres with length up to 300 mm and diameter greater than 1.0 mm.

## Test-bench Operation

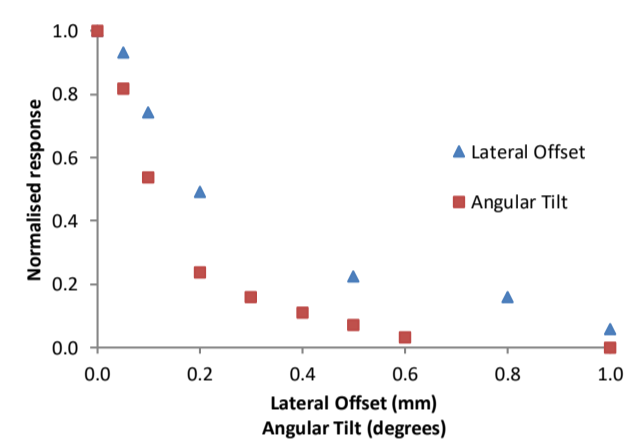
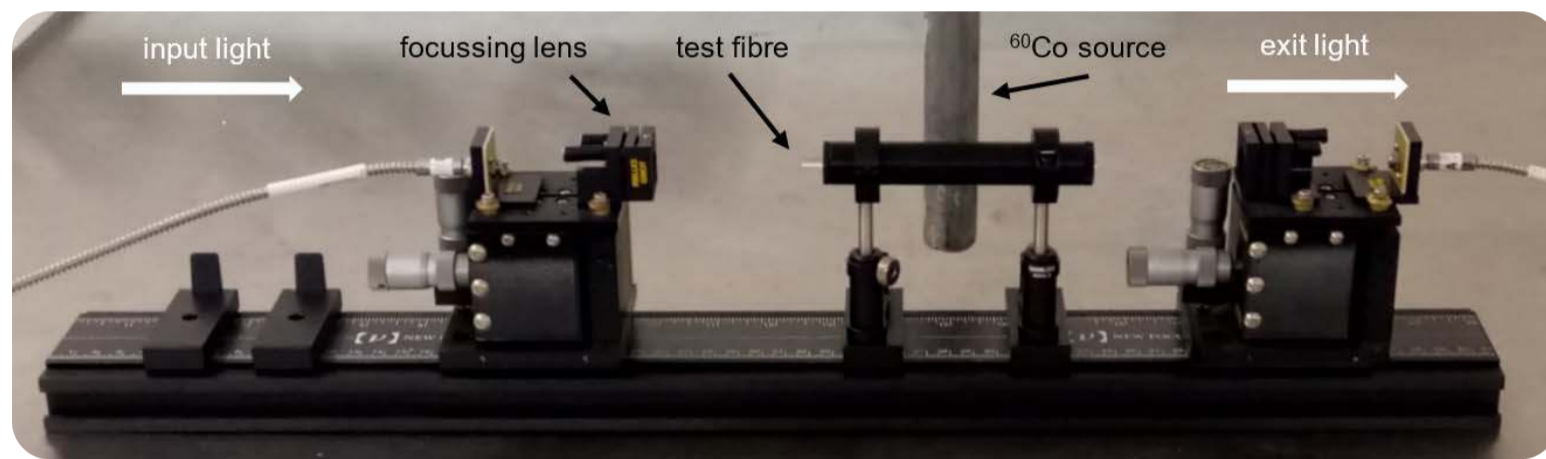


Fibres are illuminated by a combined deuterium and halogen light source focussed onto the end of the fibre with a 0.25 NA radiation-tolerant quartz lens. Light transmitted by the fibre is collected by an identical lens and measured as a function of wavelength with a linear CCD spectrometer covering a wavelength range of 190 to 850 nm. We simulated the sensitivity to misalignment using ZEMAX [2]

## Experimental Results

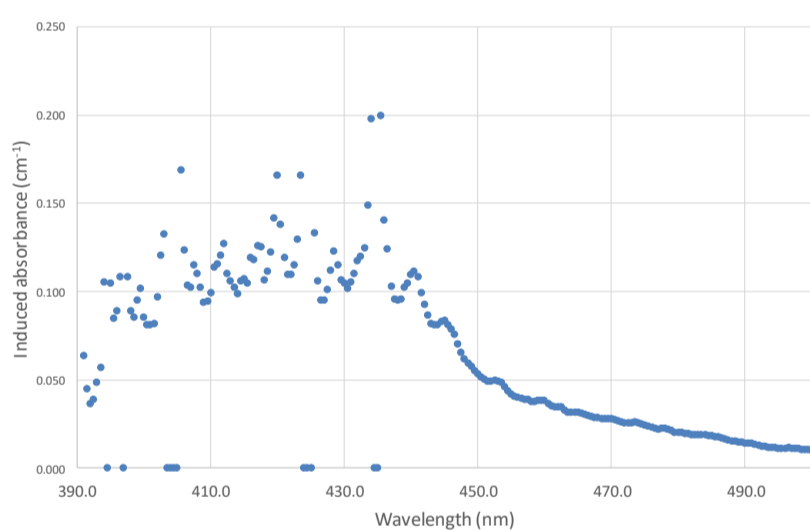


The result of a four-day continuous gamma irradiation, to a total dose of approximately 10 kGy, of a 3 mm diameter commercial polymethyl methacrylate (PMMA) rod that was highly absorbing prior to irradiation at wavelengths shorter than 390 nm due to a UV absorbing additive.

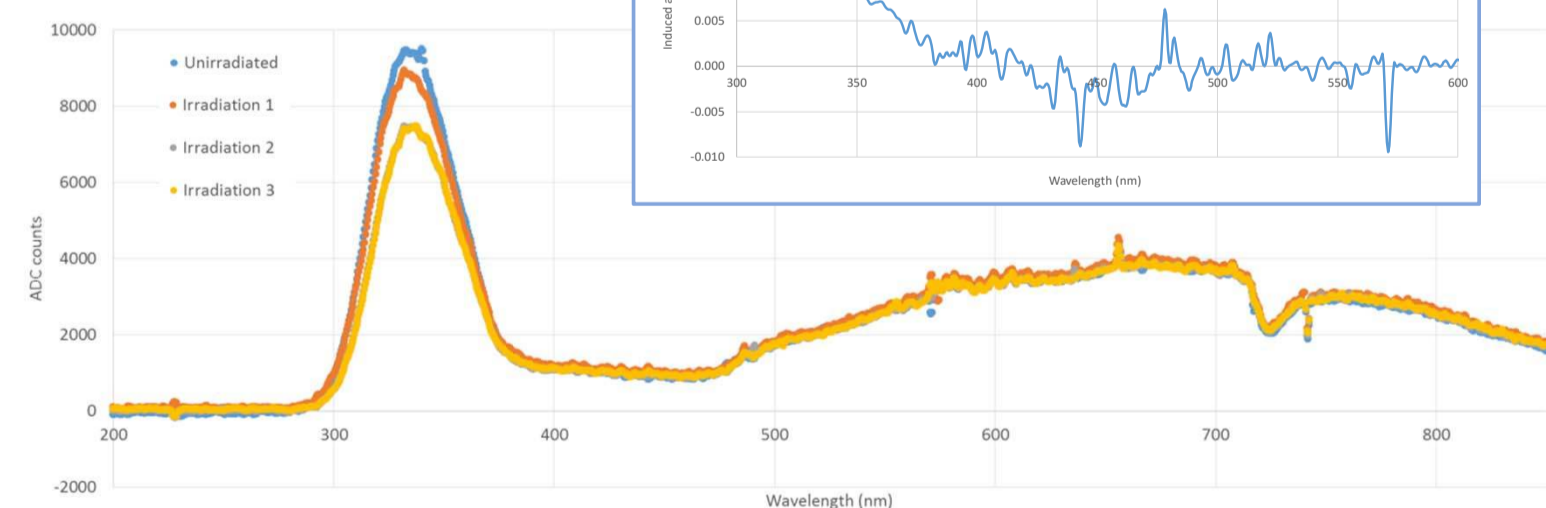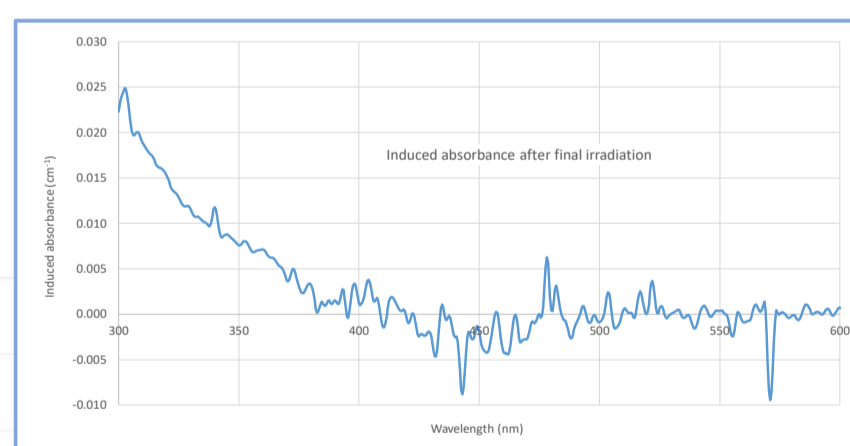

The result of a three-day continuous gamma irradiation, to a total dose of approximately 0.44 kGy, of a 3 mm diameter silica rod. Data are dark count corrected [3]. The transmission dip near 725 nm is due to the 40 m of high-OH silica fibre in the total light path.

The major systematic error is the stability of the light sources which show peak variations of up to 1% between successive measurements taken at 120 s intervals or between repeated measurements taken 360 s after switching on the light sources from cold.

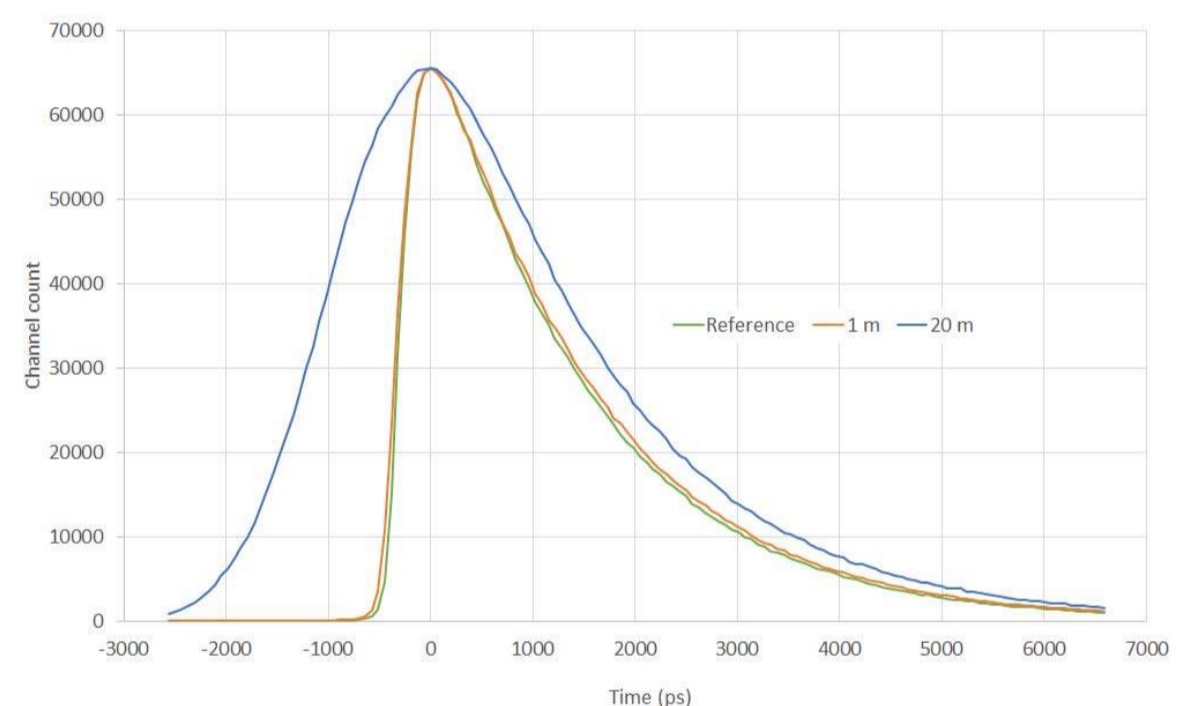

We considered the possibility to measure in real-time the effect of radiation on fluorescent properties of scintillating and WLS fibres.

Using an 80 ps 377 nm diode laser, a fast SiPM based photon detector and a PicoHarp 300 time correlator the effect of time dispersion via the large core diameter multi-mode fibre was investigated.

We used 10 cm (reference), 1 m and 20 m long optical fibres and measured the decay time constant of a fast plastic scintillator (polystyrene with PPO and PPOP fluors) at 20 °C.

Fibre Length (m)	Decay Time (ns)	Error (ns)	Chi-square / DOF
0.1	1.53	± 0.01	6.0
1.0	1.57	± 0.01	8.8
20.0	1.64	± 0.01	6.3

Effect of fibre length on fitted decay constant (single exponential tail fit starting 1 ns after peak).

## Acknowledgement

We acknowledge financial support for the development of the fibre test-bench via the AIDA-2020 collaboration which is funded by the EU Horizon 2020 Research and Innovation programme under Grant Agreement no. 654168.

### Contact Information:

Prof. Peter Hobson  
p.hobson@qmul.ac.uk  
Tel: +44 (0)2078 826957

### References:

[1] Advanced European Infrastructures for Detectors at Accelerators (AIDA-2020). [Online]. Available: <http://aida2020.web.cern.ch/activities/wp14-infrastructure-advanced-calorimeters>

[2] Zemax OpticStudio. [Online]. Available: <https://www.zemax.com/products/opticstudio>

[3] D. R. Smith, P. R. Hobson, "Spectrometer Testing: Dark frame evaluation of StellarNet Black Comet spectrometer", Brunel University London, Uxbridge, UK. Brunel\_Spectrometer\_Testing\_TN\_001.01, Feb. 2016. [Online]. Available: <http://bura.brunel.ac.uk/handle/2438/14089>