



Heriot-Watt University  
Research Gateway

## Aberration analysis based on pinhole-z-scan method near the focal point of refractive systems

### Citation for published version:

Castro-Marín, P, Garduño-Mejía, J, Rosete-Aguilar, M, Bruce, NC, Reid, DT, Farrell, C & Sandoval-Romero, GE 2016, Aberration analysis based on pinhole-z-scan method near the focal point of refractive systems. in MA Kahan & MB Levine-West (eds), *Optical Modeling and Performance Predictions VIII.*, 99530Q, Proceedings of SPIE, vol. 9953, SPIE, Optical Modeling and Performance Predictions VIII, San Diego, United States, 31/08/16. <https://doi.org/10.1117/12.2238239>

### Digital Object Identifier (DOI):

[10.1117/12.2238239](https://doi.org/10.1117/12.2238239)

### Link:

[Link to publication record in Heriot-Watt Research Portal](#)

### Document Version:

Peer reviewed version

### Published In:

Optical Modeling and Performance Predictions VIII

### Publisher Rights Statement:

Copyright 2016 Society of Photo Optical Instrumentation Engineers. One print or electronic copy may be made for personal use only. Systematic reproduction and distribution, duplication of any material in this paper for a fee or for commercial purposes, or modification of the content of the paper are prohibited.

### General rights

Copyright for the publications made accessible via Heriot-Watt Research Portal is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

### Take down policy

Heriot-Watt University has made every reasonable effort to ensure that the content in Heriot-Watt Research Portal complies with UK legislation. If you believe that the public display of this file breaches copyright please contact [open.access@hw.ac.uk](mailto:open.access@hw.ac.uk) providing details, and we will remove access to the work immediately and investigate your claim.

# Aberration analysis based on pinhole-z-scan method near the focal point of refractive systems

Pablo Castro-Marín<sup>1</sup>, Jesús Garduño-Mejía\*<sup>1</sup>, Martha Rosete-Aguilar<sup>1</sup>, Neil Ch. Bruce<sup>1</sup>,

Derryck T. Reid<sup>2</sup>, C. Farrell<sup>2</sup>, Gabriel E. Sandoval-Romero<sup>1</sup>

<sup>1</sup>Centro de Ciencias Aplicadas y Desarrollo Tecnológico, Universidad

Nacional Autónoma de México, México, Circuito Exterior S/N, Apdo. Postal 70-186, México D.F., 04510, México.

<sup>2</sup>Ultrafast Optics Group, School of Engineering and Physical Sciences, Heriot-Watt University, Riccarton, Edinburgh EH14 4AS, UK

\*e-mail: [jesus.garduno@ccadet.unam.mx](mailto:jesus.garduno@ccadet.unam.mx)

## ABSTRACT

In this work we present a method used to study the spherical and chromatic aberrations contribution near the focal point of a refractive optical system. The actual focal position is measured by scanning a pinhole attached on the front of a power detector, which are scanned along the optical axis using a motorized stage with 1  $\mu\text{m}$  resolution.

Spherical aberration contribution was analyzed by changing the pupil aperture, by modifying the size of the input iris diaphragm and for each case, measuring the actual laser power vs the detector position. Chromatic aberration was analyzed by performing the same procedure but in this case we used an ultra-broad-band femtosecond laser. The results between ML and CW operation were compare. Experimental results are presented.

**Keywords:** Femtosecond pulses, spherical and chromatic aberrations, group and phase focusing

## 1. INTRODUCTION

Temporal and spatial aberration compensation and compression of femtosecond pulses near the Diffraction Limit and Bandwidth Limited (BL) at the focal plane is fundamental for applications where maximum peak intensity or resolution is necessary. For instance in nonlinear fluorescence microscopy <sup>[1]</sup>, nanophotonic applications <sup>[2-3]</sup>, photolithography <sup>[4]</sup> and super-resolution imaging <sup>[5]</sup>.

A fundamental part for usage of high intensity light is the focusing system. In general, main aberrations are mostly associate with spherical aberration, and chromatic effects such has the Group Velocity Dispersion (GVD), and Propagation Time Delay (PTD) <sup>[6][7]</sup>.

The state of the art on ultrashort laser pulses focusing demands a better understanding of phase and group focusing effects, considering the difference of the group refractive index instead of the phase refractive index and its effects on optical distortion of the pulse front and temporal aberrations <sup>[8-14]</sup>.

In this work, we present experimental results of focusing broadband Mode-Locked (ML) femtosecond pulses and continuous wave (CW) using an achromatic doublet, typically used for femtosecond pulses focusing, to study the differences between the phase and group focusing. Experimental results of focusing performance has been achieved by

applying a method based on a pinhole masked linear z-scan along the optical axis using a home-made Erbium Doped Fiber Laser (EDFL) @1550 nm.

## 2. EXPERIMENTAL SETUP

To measure the difference between phase and group focusing we have used a broadband femtosecond @ 1550 nm, delivered from an EDFL, operating during CW and ML operation regime. The transversal beam was expanded through free spatial propagation of couple of meters. At the entrance of the experimental setup, just at the entrance of the optical focusing system, an iris aperture was located to control the input beam diameter. Iris aperture was adjusted from 0.53mm up to 7.67 mm to full fill completely all the focusing systems apertures. A 20 $\mu$ m pinhole was attached to a power meter (Coherent, LM-2IR sensor) and both together mounted in a motorized translation stage with 1 $\mu$ m resolution (Newport, M-UTM50CC1DD). The experiment was performed under different input beam diameters, CW and ML operation for the optical system under test. Experimental setup is demonstrated in figure 1.

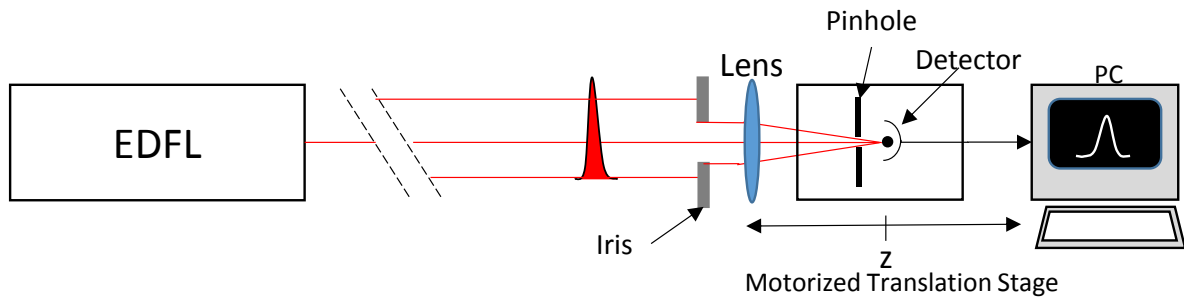


Figure 1. Experimental set-up of the pinhole masked linear z-scan method

A typical measurement of intensity vs. position, along the z axis is presented in figure 2.



Figure 2. Typical experimental measurement of z vs Intensity (left). Experimental unsymmetrical trace of  $z_r$  vs Intensity example due a misalignment condition (right).

A trace of z vs Intensity is obtained by varying the pinhole position (attached on the detector) with the translation stage and recording the power meter reading as a function of the z position. We have called this method as Pinhole Masked Linear z-scan (PML z-scan).

In the trace, we can associate three parameters: distribution width @ FWHM ( $w_R$ ), maximum intensity value ( $I_{max}$ ) and focal position shift ( $z_r$ ), relative to the paraxial focal position ( $z_r=0$ ). The location of the paraxial focal point was measured by locating  $z_r$  with the iris aperture open at 2 mm (at CW operation), below this aperture diameter the diffraction effect produced a shift of the focal position further away. The selection of the pinhole diameter is important in order to keep a

compromise between a good signal contrast and good resolution for the peak position location ( $z_r$ ). If the pinhole diameter is too large,  $w_R$  becomes too wide and  $z_r$  difficult to locate, and the opposite, if the pinhole diameter is too small,  $z_r$  is easy to locate and  $w_R$  too narrow to be measured. Additionally with a pinhole diameter too small the system becomes more difficult to align and diffraction effects comes into a play. Also, in this case, the active area of the power sensor must be very close to the pinhole in order to collect all the energy emerging from the pinhole. A good guidance, during alignment procedure, consist on checking a symmetric trace retrieval. This will guaranty that the z-scan has been performed along the optical axis with the pinhole centered, all the way long, respect the center of the transverse beam. In figure 2 also is presented an example of a case of unsymmetrical trace of  $z_r$  vs Intensity due a misalignment condition.

The motion of the translation stage and the acquisition of the signal was automatized, synchronized and registered with a computer trough LabView program.

With this method is possible to measure relative focal position shifts, respect the paraxial focal position, the  $w_R$ , which is can be related with the Rayleigh range and peak intensity  $I_{max}$ . With these parameters we have compared the phase and group focusing process in a refractive optical system.

The EDFL can be easily controlled to operate in CW or ML regime. The experiment was performed by keeping some laser parameters constant as average power and spectral intensity.

The laser parameters are: CW and ML,  $P_{avg}=100$  mW (average power),  $\lambda_{CW}=1530$  nm (CW central wavelength)  $\lambda_{ML}=1584$  nm (ML center of mass of the spectral intensity),  $\Delta\lambda=100$  nm (spectral bandwidth) .

The CW and ML spectral intensity characterization is presented in figure 3.

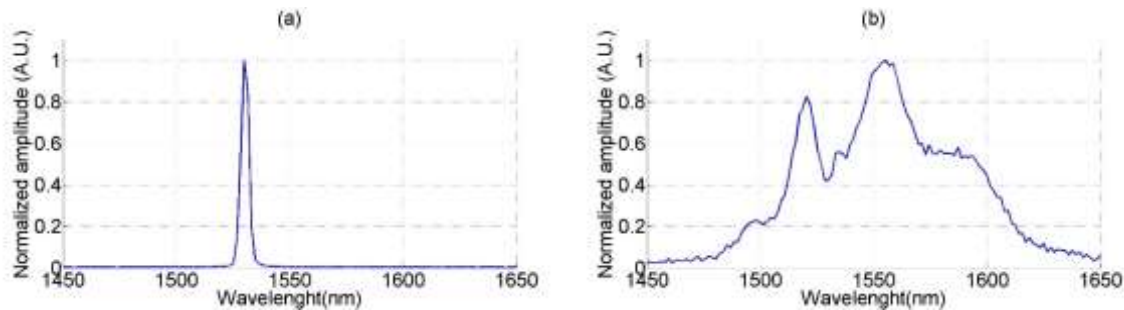


Figure 3. (a) CW Spectral Intensity and (b) ML Spectral intensity of the EDFL

The optical system under study was an Achromatic Doublet (Edmund, 12mm diameter x 30mm focal length, N-LAK22/N-SF6) designed for the NIR.

### 3. RESULTS

In figure 4, the rows (a), (b) and (c) correspond to Iris aperture vs  $z_r$ , Iris aperture vs  $I_{max}$  and Iris aperture vs  $w_R$ . Inset figures represents the results with Iris apertures from 0.53mm to 2 mm, considered the region where diffraction comes into play. The red solid lines are for ML operation regime and blue dashed for CW.

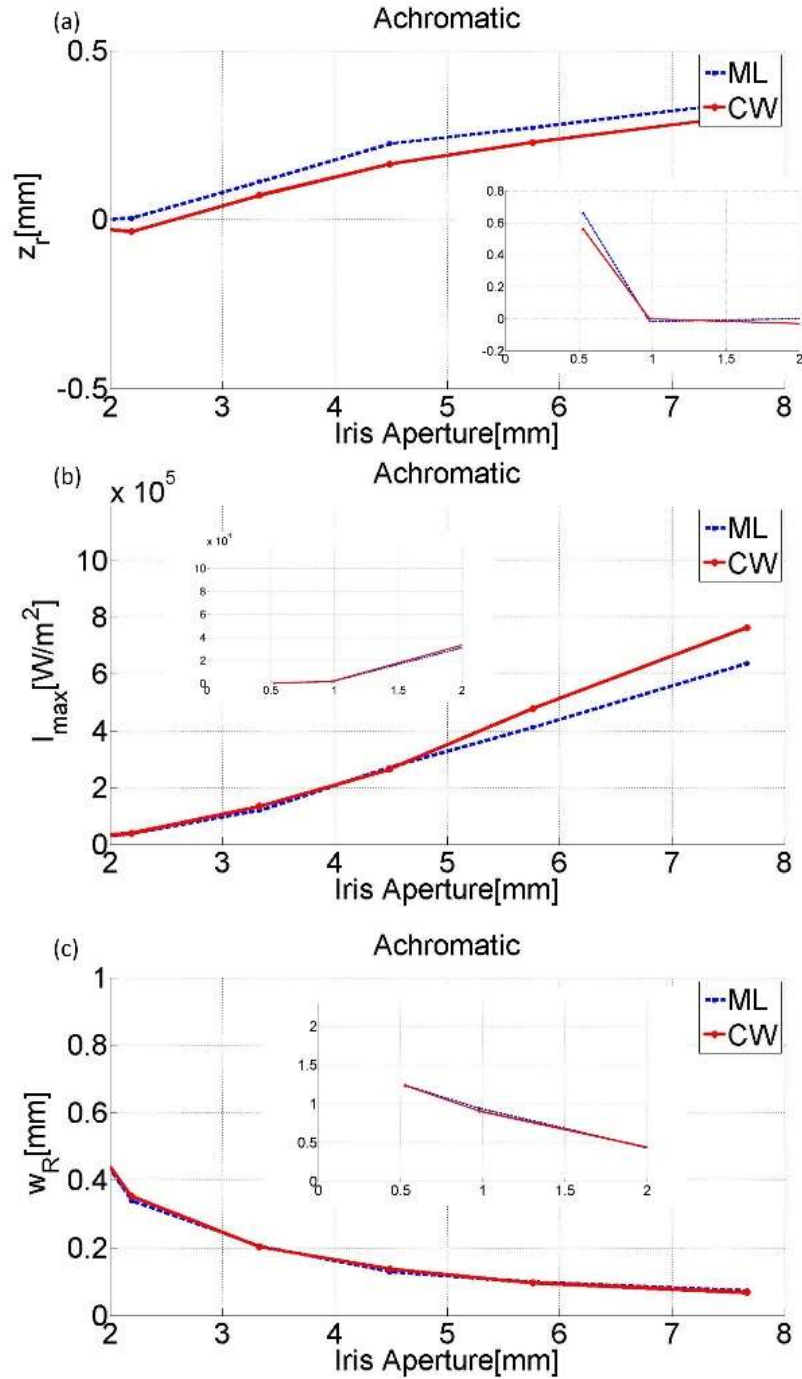


Figure 4. Achromatic doublet results (a) Iris aperture vs  $z_r$  (b)  $I_{max}$  vs  $z_r$  and (c)  $w_R$  vs  $z_r$ . The red solid lines are for ML operation regime and blue dashed for CW.

From the results presented in figure 4 (a), it can be seen that  $z_r$  shifts, respect the paraxial focus estimated at 1 mm, up to 1.3%, away from the lens. CW and ML focusing remains parallel for each aperture with a constant offset of about 0.05mm of  $z_r$ , which represents a 0.1% difference respect paraxial focal length. Also a maximum intensity value ( $I_{max}$ ) is achieved

for CW in compare with ML operation. The  $I_{\max}$  is measured with the ratio of the actual power over the pinhole area. The last results,  $w_R$  (distribution width), provide information related with the Rayleigh range which is reduced as aperture is opened.

#### 4. CONCLUSIONS

In this work, we present experimental results of focusing continuous wave (CW) and broadband Mode-Locked (ML) femtosecond pulses, delivered from a home-made Erbium Doped Fiber Laser (EDFL) @ 1550 nm. For the experiment, we have analyzed spatial effects of an achromatic lens designed for the NIR. For the system evaluation, we have applied a method that we have called as Pinhole Masked Linear z-scan (PML z-scan). With the PML z-scan is possible to measure accurately the relative focal shift, relative intensity variation along the optical axis and the variation of Rayleigh range. With these parameters, we have evaluated the optical systems and found differences between phase and group focusing based on spherical and chromatic aberration behavior. We can also conclude that with the PML z-scan method is possible to evaluate, depending the application, if a given optical system will be useful or not and if it can replace a complex system, for instance an Achromatic microscope objective, to focus broadband femtosecond pulses.

#### 5. ACKNOWLEDGEMENTS

The authors gratefully acknowledge the sponsorship for this work to DGAPA-UNAM PAPIIT IG100615. Pablo Castro-Marín gratefully acknowledges the grant from Consejo Nacional de Ciencia y Tecnología (CONACyT) México, and to the Programa de Maestría y Doctorado en Ingeniería, UNAM.

#### REFERENCES

- [1] W. Denk, J.H. Strickler and W.W. Webb, "2-photon laser scanning fluorescence microscopy", *Science* 248, 73-76, (1990).
- [2] S. B. Ippolito, B. B. Goldberg, and M. S. Unlu, "High spatial resolution subsurface microscopy," *Appl. Phys. Lett.* 78, 4071-4073 (2001) [doi:10.1063/1.1381574].
- [3] E. Ramsay, K. A. Serrels, M. J. Thomson, A. J. Waddie, M. R. Taghizadeh, R. J. Warburton, and D. T. Reid, "Three-dimensional nanoscale subsurface optical imaging of silicon circuits," *Appl. Phys. Lett.* 90, 131101 (2007) [doi:10.1063/1.2716344].
- [4] L. P. Ghislain, V. B. Elings, K. B. Crozier, S. R. Manalis, S. C. Minne, K. Wilder, G. S. Kino, and C. F. Quate, "Near-field photolithography with a solid immersion lens," *Appl. Phys. Lett.* 74, 501-503 (1999) [doi:10.1063/1.123168].
- [5] Keith A. Serrels, Euan Ramsay, Paul A. Dalgarno, Brian D. Gerardot, John A. O'Connor, Robert H. Hadfield, Richard J. Warburton, and Derryck T. Reid, *JNP*, Vol. 2, 021854 (19 December 2008), 1-29
- [6] M. K. y. W. Rudolph, "Impact of chromatic and spherical aberration on the focusing of ultrashort light pulses by lenses", "*Opt. Lett.*, vol. 18, pp. 137-139, 1993.
- [7] Z. H. Zs. Bor, "Distortion of femtosecond pulses in lenses. Wave optical," *Opt. Comm.*, vol. 94, pp. 249-258, 1992.

- [8] A. Vaughan, "Lens design using group indices of refraction," *J. Mod. Opt.*, vol. 43, no. 8, pp. 1683-1700, 1996.
- [9] Z. B. Z. L. Horváth, "How to select a lens for focusing of femtosecond pulses," *Brazilian Journal of Physics*, vol. 26, pp. 516-519, 1996.
- [10] L. G. Martínez, *Caracterización de pulsos ultracortos en la región focal de sistemas refractivos*, Ciudad de Mexico: UNAM-Posgrado de ciencias físicas, 2012.
- [11] M. K. y. W. Rudolph, "Femtosecond pulses in the focal region of lenses," *Phys.Rev. A*, vol. 48, pp. 4721-4729,, 1993.
- [12] M. Rosete-Aguilar, F.C. Estrada-Silva, C.J. Román-Moreno and R. Ortega-Marínez, "Achromatic doublets using group indices of refraction", *Laser Physics*, (2008).
- [13] Flor C. Estrada-Silva, J. Garduño-Mejía, M. Rosete-Aguilar, C. J. Román-Moreno, R. Ortega-Martínez, "Aberration effects on femtosecond pulses generated by nonideal achromatic doublets," *Applied Optics*, vol. 48, no. 24, pp. 4723-4734, 20 August 2009.
- [14] M.A. González-Galicia, M. Rosete Aguilar, J. Garduño-Mejía, N.C. Bruce and R. Ortega Martínez, "Effects of primary spherical aberration,coma, astigmatism and field curvature on the focusing of ultrashort pulses: Gaussian illumination and experiment", (2011), *J. Opt. Soc. Am. A.*, 28, 1990-1994.