

Torsten Meier  
Henning Luepschen  
Jan Karsten  
Thorsten Leibecke  
Martin Großherr  
Hartmut Gehring  
Steffen Leonhardt

## Assessment of regional lung recruitment and derecruitment during a PEEP trial based on electrical impedance tomography

Received: 10 November 2006  
Accepted: 28 June 2007  
Published online: 25 July 2007  
© Springer-Verlag 2007

T. Meier (✉) · J. Karsten · M. Großherr ·  
H. Gehring  
University Medical Center  
Schleswig-Holstein, Campus Lübeck,  
Department of Anesthesiology,  
Ratzeburger Allee 160, 23538 Lübeck,  
Germany  
e-mail: meiert@uni-luebeck.de  
Tel.: +49-451-5002766  
Fax: +49-451-5003405

T. Leibecke  
University Medical Center  
Schleswig-Holstein, Department of  
Radiology,  
Lübeck, Germany

H. Luepschen · S. Leonhardt  
RWTH Aachen University, Helmholtz  
Institute for Biomedical Engineering,  
Aachen, Germany

**Abstract** *Objective:* To investigate whether electrical impedance tomography (EIT) is capable of monitoring regional lung recruitment and lung collapse during a positive end-expiratory pressure (PEEP) trial. *Design:* Experimental animal study of acute lung injury. *Subject:* Six pigs with saline-lavage-induced acute lung injury. *Interventions:* An incremental and decremental PEEP trial at ten pressure levels was performed. Ventilatory, gas exchange, and hemodynamic parameters were automatically recorded. EIT and computed tomography (CT) scans of the same slice were simultaneously taken at each PEEP level. *Measurements and results:* A significant correlation between EIT and CT analyses of end-expiratory gas volumes ( $r = 0.98$  up to  $0.99$ ) and tidal volumes ( $r = 0.55$  up to  $r = 0.88$ ) could be demonstrated. Changes in global and regional tidal volumes and arterial oxygenation ( $\text{PaO}_2/\text{FiO}_2$ ) demonstrated recruitment/derecruitment during the trial,

but at different onsets. During the decremental trial, derecruitment first occurred in dependent lung areas. This was indicated by lowered regional tidal volumes measured in this area and by a decrease of  $\text{PaO}_2/\text{FiO}_2$ . At the same time, the global tidal volume still continued to increase, because the increase of ventilation of the non-dependent areas was higher than the loss in the dependent areas. This indicates that opposing regional changes might cancel each other out when combined in a global parameter. *Conclusions:* EIT is suitable for monitoring the dynamic effects of PEEP variations on the regional change of tidal volume. It is superior to global ventilation parameters in assessing the beginning of alveolar recruitment and lung collapse.

**Keywords** Electrical impedance tomography · Computed tomography · Acute lung injury · Lung recruitment · Positive end-expiratory pressure

### Introduction

In acute lung injury (ALI) and acute respiratory distress syndrome (ARDS), ventilation in general is inhomogeneous [1]; this leads to an increased ventilation–perfusion mismatch [2], an increased dead-space fraction [3], and possible ventilator-induced lung injury (VILI) [4, 5]. Global indices such as gas exchange parameters, pressure–volume curves, or pulmonary compliance are important parameters for assessing lung function during

ventilation. However, they provide only limited information regarding regional dynamic lung mechanisms [6, 7].

Clinical management of ARDS can be successfully examined by computed tomography (CT) analysis, which allows an assessment of the pattern of opacities of the injured lungs [8–10]. However, CT scans expose the patient to radiation. In addition, CT diagnosis is a static method and not a bedside technique. By contrast, dynamic information regarding ventilation can be obtained non-invasively by using electrical impedance tomography (EIT) [11, 12].

Although it is currently not a routine clinical technique, EIT is capable of measuring global [11] and regional [13–15] ventilation. To date, only a few studies on the potential of EIT in ALI or ARDS are available, even though evidence is accumulating that EIT is useful in monitoring regional lung recruitment and derecruitment [16–18]. The value of bedside regional EIT measurements for determining the effect of positive end-expiratory pressure (PEEP) in comparison with traditional indirect methods, such as arterial oxygenation or global tidal volumes, is still unknown.

Thus, the aim of the present study was to evaluate EIT in terms of its potential to assess changes in regional and global tidal volumes in injured lungs by comparing it with simultaneously recorded CT scans taken at the end of inspiration and expiration during a PEEP trial. Additionally, we examined changes in regional EIT measurements and global ventilation parameters regarding their ability to detect the beginning of pulmonary recruitment and lung collapse. Results were presented partly during the 2006 ISICEM [19] and ESICM meeting [20].

## Material and methods

### Animal preparation

After approval by the local authority for animal research, six pigs (25–34 kg) were included in the study. Following premedication (10 mg/kg ketamine, 2 mg/kg xylazine, 15  $\mu$ g/kg atropine), anesthesia was induced with etomidate (0.4 mg/kg). After endotracheal intubation (6.5-mm tube) anesthesia was maintained with propofol (8 mg/kg/h) and ketamine (10 mg/kg/h). Muscle paralysis was maintained with pancuronium (0.2 mg/kg, repetitive 0.1 mg/kg).

All measurements were made using a medically approved Panel PC (POC-153; Advantech, Taiwan), an electrically controllable ventilator (Servo 300; Siemens-Elementa, Sweden), an online blood gas analyzer (TrendCare Satellite; Diametrics Medical, UK), a monitor for hemodynamic parameters (Sirecust 1281; Siemens, Germany) and a capnograph (CO<sub>2</sub>SMO+; Respirationics, USA). An EIT GoEMF II prototype system (EIT evaluation kit; Dräger Medical, Germany) with 16 electrodes (Ag/AgCl EEG-EMG electrodes, CDES002822; spes medica, Italy) at a juxtadiaphragmatic level and a reference electrode approximately 10 cm below the electrode plane was used. The frequency of the injected currents was 50 kHz at an amplitude of 5 mA<sub>rms</sub>. A complete EIT measurement was made every 80 ms (12.5 frames/s) [21–23]. All parameters were continually recorded using the graphical development environment LabVIEW® (National Instruments, USA).

The animals were initially ventilated in a volume-controlled mode [tidal volume ( $V_T$ ) 8 ml/kg, PEEP 5 cmH<sub>2</sub>O, I:E 1:1, respiration rate 16–20 breaths/min

and inspiratory fraction of oxygen (FiO<sub>2</sub>) 0.5] in supine position. Volume deficits were compensated by using 8 ml/kg isotonic or 6% hydroxyethyl starch solution. Infusion of isotonic solution was continued at a rate of 5 ml/kg/h, and the intravascular volume was adapted to adjust the central venous pressure to  $\geq$  12 mmHg.


### Experimental protocol

After baseline measurements at a PEEP of 10 cmH<sub>2</sub>O [pressure-controlled ventilation (PCV), driving pressure 8 cmH<sub>2</sub>O, respiratory rate 25 breaths/min, I:E 1:1, FiO<sub>2</sub> = 0.5] had been performed, ALI was induced by repetitive lung lavage with warmed saline (8–12 l). During the procedure, the animals were ventilated with a PEEP of 5 cmH<sub>2</sub>O and a FiO<sub>2</sub> of 1.0. The lavage was repeated until the PaO<sub>2</sub> decreased to 100 mmHg for at least 1 h [24].

Thereafter, an automatic stepwise incremental and decremental PEEP trial of respective 2 min duration at ten pressure levels (i. e. 20 min overall) was performed (PEEP = 10, 15, 20, 25, 30, 25, 20, 15, 10, 5 cmH<sub>2</sub>O) (Fig. 1). During the maneuver, the animals were ventilated with a FiO<sub>2</sub> of 1.0 using the same ventilation mode and parameters as during the baseline measurements. The body temperature of the animals was held constant by body surface warming.


### EIT off-line data analysis

We used a prototype software (Dräger Medical, Germany) with a modified back-projection algorithm [23]. Additionally, all data were low-pass filtered with a cut-off frequency

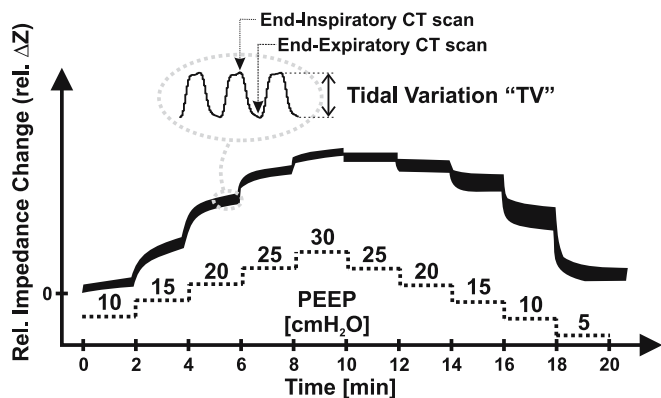

**Fig. 1** Example of an original EIT curve during the PEEP trial: the curve represents the level of measured sum of relative impedance change (rel.  $\Delta Z$ ) and its tidal change (Tidal Variation, TV). At the end of each PEEP level, two triggered dynamic CT scans were performed simultaneously with the EIT measurement at end-inspiration and end-expiration

**Fig. 2** Regions of interest (ROIs) in computed tomography (CT) and functional EIT (fEIT): Each pixel of the fEIT image is gray-tone-encoded. *Black* pixels describe areas with no ventilation, and *white* pixels indicate areas with high ventilation. In CT scans, the ventral-dorsal height of each lung was divided into four equal intervals, indicating the four ROIs

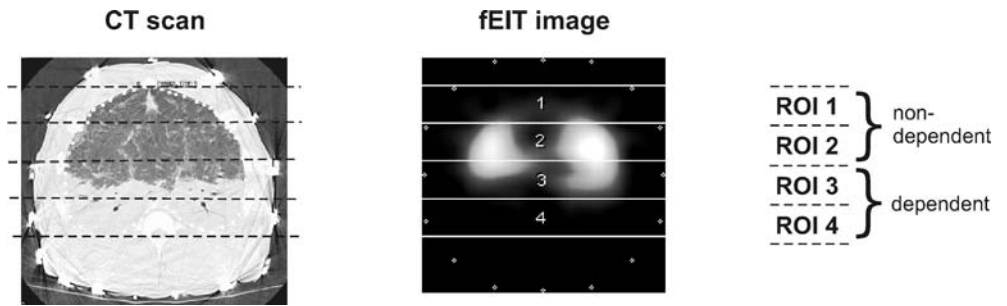

of 55 beats/min in order to reduce cardiac-related oscillations caused by the heartbeats.

The calculated images ( $32 \times 32$  color-scaled matrix) are relative EIT scans referenced to the steady-state end-expiratory values after lavage as a baseline vector. Therefore, only the relative impedance change (rel.  $\Delta Z$ ) was measured. The difference between rel.  $\Delta Z$  at the end of inspiration and at the end of expiration is defined as tidal variation (TV) (Fig. 1).

To compare TV with the CT-based tidal change of gas volume ( $\Delta GV$ ) of all pigs, TV was normalized with  $V_T$  given by the ventilator. Due to high correlation coefficients per animal of the corresponding values a linear regression model was fitted ( $[TV, V_T]$ ), and parameters were estimated using an ordinary least-squares procedure. Then, the estimated linear relationship was used to predict future response values ( $V_T$ ) based on the independent variable (TV).

Regional rel.  $\Delta Z$  ( $\Delta Z_{reg}$ ) and TV ( $TV_{reg}$ ) were calculated by offline analysis in four regions of interest (ROIs; size  $32 \times 5$  pixels), which were adjusted to the asymmetric localization of the lung within the chest of the pig (Fig. 2).

For the evaluation of the regional and global ventilation distribution, functional EIT (fEIT) images were used [25]. After normalization with  $V_T$ , the normalized fEIT images at the end of each PEEP step were subtracted from those at the end of the previous PEEP step (resulting in nine differential fEIT images, dfEIT). Consequently, these dfEIT images qualitatively depicted regional changes of  $V_T$  as  $\Delta V_T$  (i. e. an increase, a decrease, or no change) when the PEEP level was elevated or reduced. In order to quantify these changes for each dfEIT image, all pixels with positive values and all pixels with negative values were summed separately and displayed by a color scale. Thus were described the tidal volume gain (TVG) and loss (TVL) for the pulmonary cross-section and their dependent/non-dependent lung areas. The advantage of splitting  $\Delta V_T$  into TVG and TVL lies in the possibility of detecting inhomogeneous changes of regional tidal volumes.

### CT scanning and analysis

Simultaneously to the EIT measurements, a CT scanner (Toshiba Aquilion 4; Toshiba, Japan) was automatically

turned on at the end of each PEEP step to obtain reference images in the electrode plane (Fig. 1). End-inspiratory and end-expiratory CT scans were taken, triggered using the standard ECG input port of the scanner. The trigger impulses were generated by analyzing the flow signal of the respirator. Exposures were taken at 120 kV and 100 mA (collimation 2 mm,  $512 \times 512$  matrix) and were reconstructed with a high-resolution reconstruction algorithm. The ventral-dorsal height of each lung was manually divided into four equal intervals (Fig. 2), and the mean lung densities in Hounsfield units (HU) at the end of expiration and inspiration were obtained for the whole slice and for all four ROIs. The global and regional CT gas volumes ( $GV$ ;  $GV_{reg}$ ) and tidal volumes ( $\Delta GV$ ;  $\Delta GV_{reg}$ ) were calculated [26]; delta-CT scans were obtained by means of subtraction.

### Statistics

Data were analyzed by means  $\pm$  SD, median, and range with SPSS<sup>®</sup> 14.0 (SPSS, USA). For changes during the PEEP trial, means were analyzed, and if a normal distribution was unlikely and errors from multiple testing had to be avoided, we used the Friedman analysis and, in the case of significance ( $p < 0.05$ ), the Wilcoxon–Wilcoxon test ( $p < 0.05$ , two sided). The data obtained by linear regression analysis and the calculation of the correlation coefficient presented the relationship between EIT and CT measurements. To analyze the nonlinear relationship between gas/tidal volumes and time, orthogonal polynomial trend analysis was performed. Then, parameters up to degree two were compared by a Wilcoxon test for two dependent samples. Differences between the parameters were defined as statistically significant with  $p < 0.05$ .

## Results

### Global parameters


Ventilatory, gas exchange, and hemodynamic parameters are shown in Table 1. With regard to the PEEP trial, a significant depression of the mean arterial pressure

**Table 1** Ventilatory, gas exchange, and hemodynamic parameters

Parameter	Baseline Prelavage	PEEP trial Start	End
Paw, peak (cmH <sub>2</sub> O)	17.9 ± 0.15	17.8 ± 0.1	13.5 ± 1.1*†
Paw, mean (cmH <sub>2</sub> O)	17.5 ± 0.5	17.5 ± 0	11.7 ± 1.4*†
PEEP (cmH <sub>2</sub> O)	10 ± 0	10 ± 0	5 ± 0†
Respiratory rate (breaths/min)	25 ± 0	25 ± 0	25 ± 0
V <sub>T</sub> (ml)	217 ± 28.6	99.3 ± 45.7*	189.4 ± 48.8†
C <sub>rs</sub> (ml/cmH <sub>2</sub> O)	27.7 ± 3.9	11.1 ± 7.5*	20.6 ± 11.9*†
PaO <sub>2</sub> /FiO <sub>2</sub> (mmHg)	358 ± 55	79.2 ± 44.7*	101.4 ± 21.5*
PaO <sub>2</sub> (mmHg)	184.9 ± 26	78 ± 43.6*	99.9 ± 22*
pH	7.32 ± 0.04	7.13 ± 0.11*	7.12 ± 0.48*
MAP (mmHg)	96.2 ± 17.6	113.3 ± 17.2	101.6 ± 23.4
CVP (mmHg)	13.1 ± 2.5	14.3 ± 1.5	10.3 ± 2.1*†

Values are means ± standard deviation; *Paw*, Airway pressure; *V<sub>T</sub>*, tidal volume; *C<sub>rs</sub>*, respiratory compliance; *MAP*, mean arterial pressure; *CVP*, central venous pressure; \* *p* < 0.05 significant differences between baseline and PEEP trial data; † *p* < 0.05 significant differences between start and end of PEEP trial

**Fig. 3** Course of tidal change of gas volume ( $\Delta$ GV), normalized tidal variation (TV\*), tidal volume V<sub>T</sub> (ventilator), and oxygenation (PaO<sub>2</sub>/FiO<sub>2</sub>) at baseline and during the PEEP trial: the dynamic behavior of V<sub>T</sub> and PaO<sub>2</sub>/FiO<sub>2</sub> is displayed by using continuous lines (median). The box plots show the median, upper, and lower quartiles of the PaO<sub>2</sub>/FiO<sub>2</sub> and V<sub>T</sub> values at the end of each PEEP step. The whiskers indicate the range of minimum and maximum (*n* = 6). \* (PaO<sub>2</sub>/FiO<sub>2</sub>, V<sub>T</sub>), † (TV\*), § ( $\Delta$ GV); *p* < 0.05 is considered a statistically significant increase between initial and subsequent PEEP levels

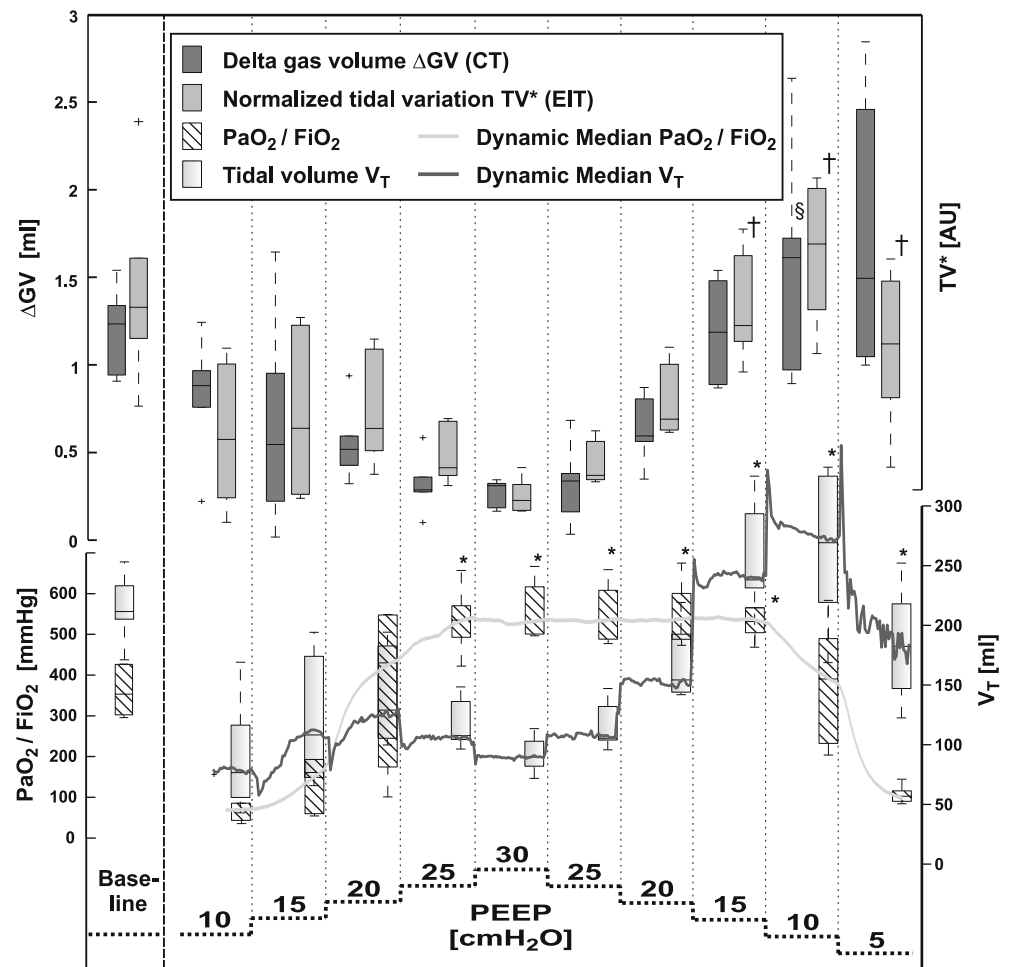

occurred (from 113.3 ± 17.2 to 88.4 ± 18.1 mmHg). During the incremental part, PaO<sub>2</sub> increased from 78 ± 43.6 to 551.7 ± 70.8 mmHg. At the same time, V<sub>T</sub> increased strikingly (from 59.3 ± 78.7 to 265.6 ± 57.9 ml).


During the decremental part, PaO<sub>2</sub> started to drop again as soon as the PEEP level was reduced to 10 cmH<sub>2</sub>O (375 ± 146.6 mmHg). V<sub>T</sub>, however, did not decrease until the PEEP level was reduced to 5 cmH<sub>2</sub>O (Fig. 3). Com-

pared to the beginning of the trial,  $V_T$  (from  $99.3 \pm 45.7$  to  $189.4 \pm 48.8$  ml) as well as static respiratory compliance ( $C_{rs}$ ) (from  $11.1 \pm 7.5$  to  $20.6 \pm 11.9$  ml/cmH<sub>2</sub>O) were still significantly higher at the end of the trial.

#### Comparison of EIT and CT scans

A significant correlation was found between rel.  $\Delta Z$  and GV at the end of inspiration ( $r=0.75$ ,  $p < 0.01$ ) and

expiration ( $r=0.78$ ,  $p < 0.01$ ) when combining the data of all animals. Comparing end-expiratory rel.  $\Delta Z$  and GV of each animal individually showed much higher linear correlations (from  $r=0.98$  to  $r=0.99$ ,  $p < 0.01$ ). Furthermore, TV and CT-based tidal volumes ( $\Delta GV$ ) showed a linear correlation (from  $r=0.55$  to  $r=0.88$ ,  $p < 0.01$ ). Trend analysis of both methods regarding increase and decrease of global tidal volumes showed no significant differences. The linear trend varied in ROI 1 and 2 ( $p=0.028$ ) and the quadratic trend varied

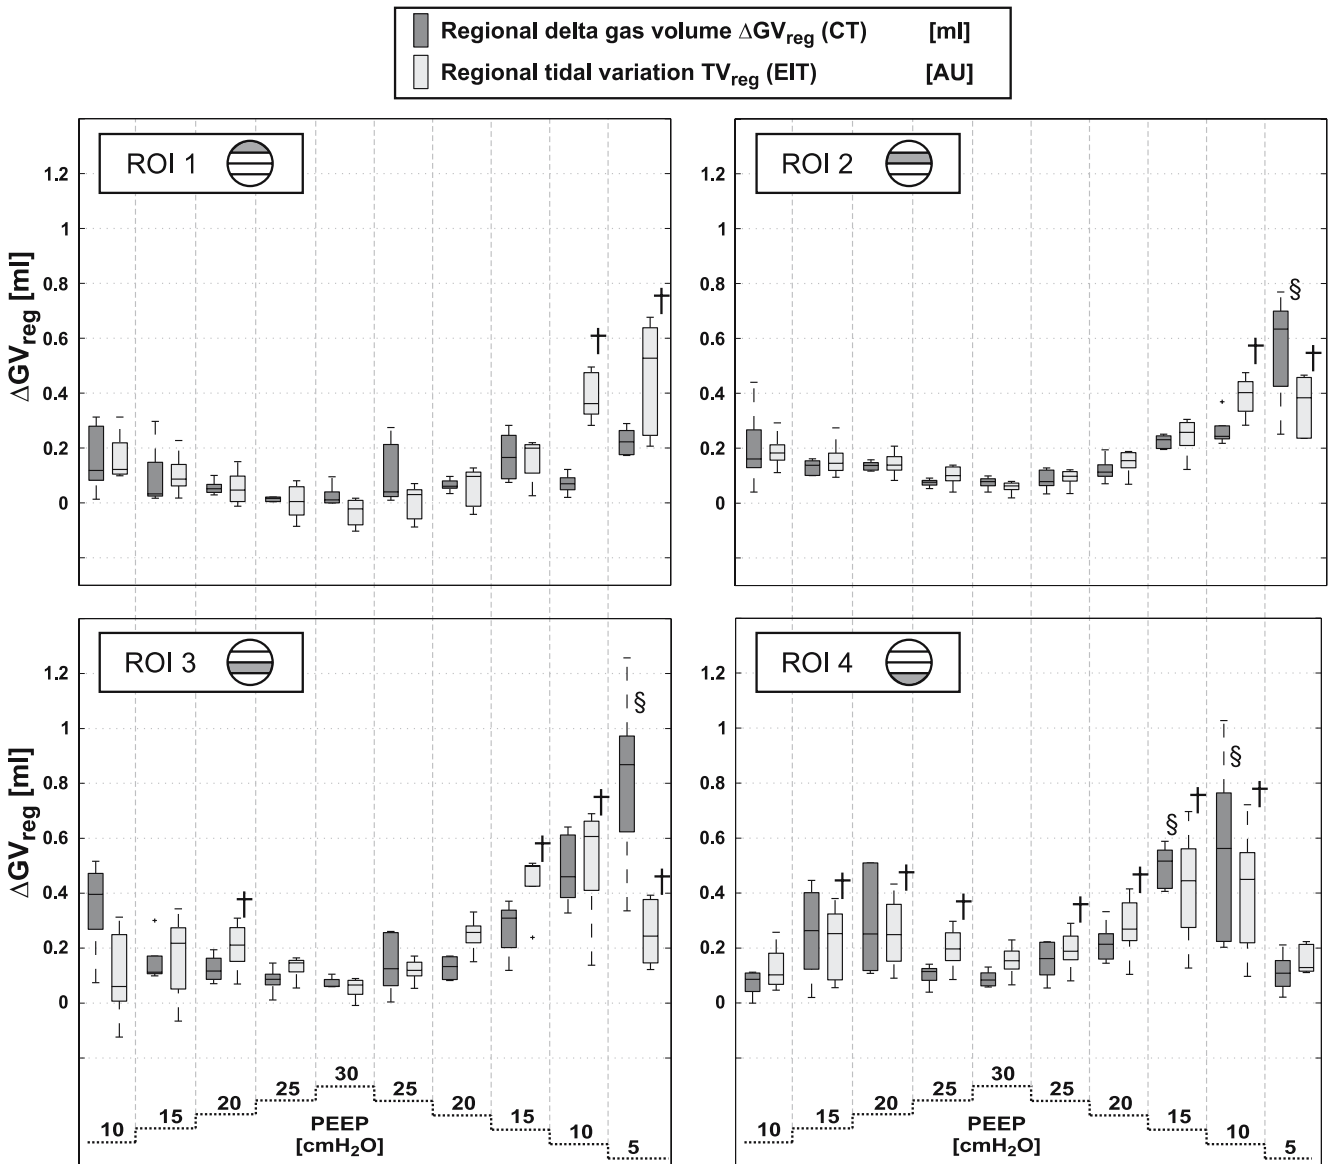

**Fig. 4** Regional tidal volume change during the PEEP trial (ROI 1–4): *box plots* representing the regional tidal change of gas volumes  $\Delta GV_{reg}$  and regional tidal variation  $TV_{reg}$  during the PEEP trial. Impedance data were not normalized. The *box plots* show the

median, upper, and lower quartiles, whereas the whiskers indicate the minimum and maximum ( $n=6$ ). § ( $\Delta GV_{reg}$ ), † ( $TV_{reg}$ );  $p < 0.05$  is considered a statistically significant increase between initial and subsequent PEEP levels



in ROI 3 ( $p = 0.046$ ), but they were indiscriminative in ROI 4.

### Global and regional changes of ventilation in EIT and CT scans


During the PEEP trial, EIT and CT were able to monitor global and regional changes in tidal volumes. Like  $V_T$ , the values for  $TV^*$  and  $\Delta GV$  improved significantly at the

decremental part of the PEEP trial when compared with the initial PEEP level (Fig. 3).

The impact of PEEP changes on the regional tidal volumes was greater in the dependent lung areas than in the non-dependent lung areas. Compared with the initial measurements,  $\Delta GV$  followed the significant changes of the EIT values but without significance in most of the pressure levels (Fig. 4).

### Distribution of regional lung recruitment and derecruitment

Figure 5 exemplarily shows the change of regional lung recruitment and derecruitment in one pig during the PEEP trial. The increase of tidal volume (EIT) in the incremental part of the PEEP trial started at between 10 and 15 cmH<sub>2</sub>O in all animals and was mainly found in the dependent part of the lung ( $TVG_{\text{dependent}} 17.8 \pm 13.3$ ,  $TVG_{\text{non-dependent}} 5.6 \pm 3.6$ ;  $p < 0.05$ ). Derecruitment of the lung started when reducing PEEP from 15 to 10 cmH<sub>2</sub>O also in the dependent parts ( $TVL_{\text{dependent}} 15.9 \pm 8.7$ ,  $TVL_{\text{non-dependent}} 0.9 \pm 0.5$ ;  $p < 0.05$ ), although the global tidal volume ( $TVG 35.6 \pm 15.3$ ) was still increasing. This coincided with the drop in oxygenation at this PEEP level (Fig. 3).

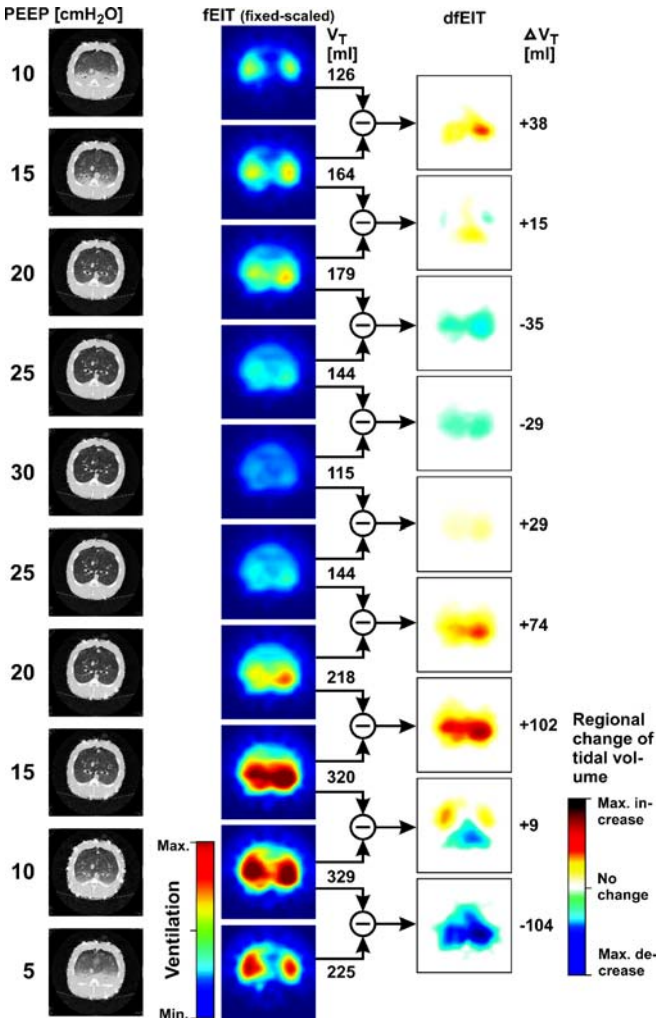

**Fig. 5** Visualization of regional changes of tidal volume: exemplary CT scans (left) and fixed-scaled functional EIT images (fEIT) (middle) from one of the six pigs. In the fEIT images, blue areas symbolize no ventilation, and red areas high ventilation. Normalization of the fEIT images with the corresponding  $V_T$  allows the calculation of differential EIT images (dfEIT) (right) by means of subtraction. dfEIT images enable a qualitative and quantitative assessment of regional change of  $V_T$  when altering the PEEP level. Of particular interest were the dfEIT images that contained areas of both increase and decrease of  $V_T$  (PEEP level 15 to 20 cmH<sub>2</sub>O and 15 to 10 cmH<sub>2</sub>O). During these steps the hidden individual starting points of regional recruitment and lung collapse can be seen

## Discussion

The aim of our study was to assess global and regional lung recruitment and lung collapse with EIT as well as CT images during an incremental and decremental PEEP trial in experimental ALI.

### Evaluation of EIT vs CT data

The present study demonstrates that EIT is able to describe global and regional changes in gas volumes and tidal volumes of an intrathoracic slice during a PEEP trial in surfactant-deficient lungs. In agreement with other studies [11, 14], the gas and tidal volumes derived from CT scans show a high linear correlation with corresponding values in the EIT (rel.  $\Delta Z$ ,  $TV$ ). Because EIT measurements do not represent absolute values and depend on different baseline references, amplification factors, and individual anatomies [27], the linear regression lines between, for example, rel.  $\Delta Z$  and  $GV$  have different slopes and axis intercepts for each animal, even though exactly the same variation of PEEP was used. Therefore, the correlation coefficient is lower when combining the data of all animals ( $r = 0.78$ ) than the intra-individual correlation of each animal (from  $r = 0.98$  to  $r = 0.99$ ).

This individual correlation of EIT and CT monitoring with regard to the end-expiratory air content during the PEEP trial carried out here is nearly identical with the cor-

relation calculated by Victorino et al. [14] ( $r = 0.96$ ) for ARDS patients without concurrently recorded CT and EIT. Their measurements were nevertheless performed during a slow inflation maneuver over 80 s and not during continuous ventilation over a longer period. In our study, all the measurements were performed simultaneously during the variation of PEEP in PCV, a setting close to clinical reality with regard to PEEP titration.

A major new approach in the present study is the comparison of global and regional tidal volumes in EIT and simultaneous CT scans. This was achieved by electronically synchronizing the CT measurement with the end of inspiration and expiration. The correlations that we obtained are not as high as those for the intrathoracic air content of the transverse thoracic plane, probably because the tidal volume changes are small compared with the gas volume content itself, which reduces the signal-to-noise ratio mainly in the delta-CT scans. Noise is introduced, for instance, by the non-transparent electrodes used and by not removing all the pulmonary vessels and bronchi from the manually defined ROIs. This problem occurred especially in ROI 3. One other reason for the lower correlation between both imaging systems is that the transverse thoracic volume measured by EIT is larger than the detected volume with the CT scan [28]. Furthermore, a precise definition of the ROI examined is difficult, because tomograms derived by EIT show no anatomical landmarks. Nevertheless, our data showed only minor differences in trend analysis between tidal volume alteration derived from EIT and CT during the PEEP trial.

#### Detection of recruitment and lung collapse

The present study shows that analysis of EIT measurements, which generally have a low spatial resolution, permits assessment of the regional changes of  $V_T$  during the PEEP maneuver, not only qualitatively, but to a certain degree also quantitatively. During the maneuver, an effect of gravity occurs regarding the onset and the degree of increase or decrease of the regional tidal volumes in the four ROIs. Because of the distribution of atelectasis in the lavage lung model, the calculation of the regional  $V_T$  derived from EIT and CT show the highest increase in the dependent ROIs. This result is in accordance with the common understanding of inhomogeneous gravity-dependent tidal volume distributions in ALI and ARDS [26, 29]. Kunst et al. [30] and Hinz et al. [31] studied this phenomenon by using EIT and demonstrated that the regional lower inflection point increases in the ventral–dorsal direction. To quantitatively investigate these changes in the regional distribution of tidal volumes after a recruitment maneuver, Kunst et al. [16] calculated the “impedance ratio”, i. e. the ratio between TV of the

dependent and non-dependent lung area. Although these authors only obtained relative values for the regional changes of tidal volumes, and not the absolute values we have, the results show the same tendency.

With conventional techniques, assessment of the beginning of the opening and collapsing of lung units is difficult during a PEEP trial at the bedside. In our study, we focused on the measurement of oxygenation,  $V_T$ , and regional EIT analysis. The data concerning oxygenation and global  $V_T$  obtained in the present study show opposing tendencies with respect to the ability to assess the beginning of recruitment and lung collapse during the PEEP trial. For instance, after reducing PEEP from 15 to 10 cmH<sub>2</sub>O, PaO<sub>2</sub> decreases, whereas  $V_T$  increases (Fig. 3). By contrast, during a rise in PEEP from 20 to 25 cmH<sub>2</sub>O, PaO<sub>2</sub> continues to increase, whereas global  $V_T$  decreases. This opposing tendency of PaO<sub>2</sub> and  $V_T$  is a consequence of a changing pulmonary shunt fraction, mainly in the dependent well-perfused lung areas, and of the overinflation of normally ventilated areas attributable to the PEEP variation [1].

The EIT technique offers the advantage of dynamically studying regional changes of lung mechanics [17]. dFEIT scans show that dependent and non-dependent lung areas differ in their responses during the PEEP trial (Fig. 5). For the assessment of lung recruitment and collapse, it seems to be reasonable to evaluate the PEEP-induced changes of the dependent lung areas in the fEIT images. These areas experience the most distinct dynamic changes, so that results are easily obtainable. Thus, in dependent lung units, recruitment can be identified at the first PEEP elevation (between 10 and 15 cmH<sub>2</sub>O). The beginning of regional lung collapse is detected during the decremental phase, when PEEP changes from 15 to 10 cmH<sub>2</sub>O, which corresponds well to the decreasing PaO<sub>2</sub>. These observations show that the EIT technique has a higher degree of sensitivity than the global ventilation parameters (i. e.,  $C_{rs}$  or  $V_T$ ) in detecting the onset of regional alveolar recruitment or lung collapse. However, these issues might differ in other lung models and have to be confirmed in clinical studies before transferring them into routine practice.

#### Conclusion

The change in global and regional tidal volume attributable to an incremental and decremental PEEP trial has been demonstrated by analysis of EIT. The initiation of regional recruitment and the start of lung collapse can be displayed more advantageously in regional EIT measurements than by extraction from global ventilation parameters. EIT can thus be used as a tool to adapt the PEEP level to the individual degree of lung injury in order to maintain recruitment.

**Acknowledgements.** The support of Eckhard Teschner, Dräger Medical AG, is gratefully acknowledged.

## References

- Gattinoni L, Pesenti A, Bombino M, Baglioni S, Rivolta M, Rossi F, Rossi G, Fumagalli R, Marcolin R, Mascheroni D, Torressin A (1988) Relationships between lung computed tomographic density, gas exchange, and PEEP in acute respiratory failure. *Anesthesiology* 69:824–832
- Sinclair SE, Albert RK (1997) Altering ventilation–perfusion relationships in ventilated patients with acute lung injury. *Intensive Care Med* 23:942–950
- Nuckton TJ, Alonso JA, Kallet RH, Daniel BM, Pittet JF, Eisner MD, Matthay MA (2002) Pulmonary dead-space fraction as a risk factor for death in the acute respiratory distress syndrome. *N Engl J Med* 346:1281–1286
- Tremblay LN, Slutsky AS (2006) Ventilator-induced lung injury: from the bench to the bedside. *Intensive Care Med* 32:24–33
- Dreyfuss D, Saumon G (1998) Ventilator-induced lung injury: lessons from experimental studies. *Am J Respir Crit Care Med* 157:294–323
- Hickling KG (1998) The pressure–volume curve is greatly modified by recruitment. A mathematical model of ARDS lungs. *Am J Respir Crit Care Med* 158:194–202
- Stenqvist O (2003) Practical assessment of respiratory mechanics. *Br J Anaesth* 91:92–105
- Gattinoni L, Caironi P, Pelosi P, Goodman LR (2001) What has computed tomography taught us about the acute respiratory distress syndrome? *Am J Respir Crit Care Med* 164:1701–1711
- Puybasset L, Cluzel P, Gusman P, Grenier P, Preteux F, Rouby JJ (2000) Regional distribution of gas and tissue in acute respiratory distress syndrome. I. Consequences for lung morphology. *CT Scan ARDS Study Group. Intensive Care Med* 26:857–869
- Malbouisson LM, Muller JC, Constantin JM, Lu Q, Puybasset L, Rouby JJ (2001) Computed tomography assessment of positive end-expiratory pressure-induced alveolar recruitment in patients with acute respiratory distress syndrome. *Am J Respir Crit Care Med* 163:1444–1450
- Frerichs I, Hinz J, Herrmann P, Weisser G, Hahn G, Dudykevych T, Quintel M, Hellige G (2002) Detection of local lung air content by electrical impedance tomography compared with electron beam CT. *J Appl Physiol* 93:660–666
- Frerichs I, Dargaville PA, Dudykevych T, Rimensberger PC (2003) Electrical impedance tomography: a method for monitoring regional lung aeration and tidal volume distribution? *Intensive Care Med* 29:2312–2316
- Frerichs I, Schiffmann H, Hahn G, Hellige G (2001) Non-invasive radiation-free monitoring of regional lung ventilation in critically ill infants. *Intensive Care Med* 27:1385–1394
- Victorino JA, Borges JB, Okamoto VN, Matos GF, Tucci MR, Carames MP, Tanaka H, Sipmann FS, Santos DC, Barbas CS, Carvalho CR, Amato MB (2004) Imbalances in regional lung ventilation: a validation study on electrical impedance tomography. *Am J Respir Crit Care Med* 169:791–800
- Frerichs I, Braun P, Dudykevych T, Hahn G, Genee D, Hellige G (2004) Distribution of ventilation in young and elderly adults determined by electrical impedance tomography. *Respir Physiol Neurobiol* 143:63–75
- Kunst PW, Vazquez de Anda G, Bohm SH, Faes TJ, Lachmann B, Postmus PE, de Vries PM (2000) Monitoring of recruitment and derecruitment by electrical impedance tomography in a model of acute lung injury. *Crit Care Med* 28:3891–3895
- Odenstedt H, Lindgren S, Olegard C, Erlandsson K, Lethvall S, Aneman A, Stenqvist O, Lundin S (2005) Slow moderate pressure recruitment maneuver minimizes negative circulatory and lung mechanic side effects: evaluation of recruitment maneuvers using electric impedance tomography. *Intensive Care Med* 31:1706–1714
- Frerichs I, Dargaville PA, van Genderingen HR, Morel DR, Rimensberger PC (2006) Lung volume recruitment after surfactant administration modifies spatial distribution of ventilation. *Am J Respir Crit Care Med* 174:772–779
- Meier T, Luepschen H, Karsten J, Leibecke T, Großherr M, Leonhardt S (2006) Comparison of regional lung recruitment in electrical impedance tomograms and CT scans in experimental acute lung injury. *Critical Care [Suppl]* 10(1):P7
- Meier T, Luepschen H, Karsten J, Großherr M, Leibecke T, Gehring H, Leonhardt S (2006) Impact of different PEEP levels on regional compliance measured by electrical impedance tomography. *Intensive Care Med [Suppl]* 32(13):S221
- Brown BH (2003) Electrical impedance tomography (EIT) a review. *J Med Eng Technol* 27:97–108
- Brown BH, Barber DC (1987) Electrical impedance tomography; the construction and application to physiological measurement of electrical impedance images. *Med Prog Technol* 13:69–75
- Barber DC (1989) A review of image reconstruction techniques for electrical impedance tomography. *Med Phys* 16:162–169
- Lachmann B, Robertson B, Vogel J (1980) In vivo lung lavage as an experimental model of the respiratory distress syndrome. *Acta Anaesthesiol Scand* 24:231–236
- Hahn G, Sipinkova I, Baisch F, Hellige G (1995) Changes in the thoracic impedance distribution under different ventilatory conditions. *Physiol Meas [Suppl]* 16:A161–A173
- Gattinoni L, Pelosi P, Crotti S, Valenza F (1995) Effects of positive end-expiratory pressure on regional distribution of tidal volume and recruitment in adult respiratory distress syndrome. *Am J Respir Crit Care Med* 151:1807–1814
- Wolf GK, Arnold JH (2005) Noninvasive assessment of lung volume: respiratory inductance plethysmography and electrical impedance tomography. *Crit Care Med [Suppl]* 33:S163–S169
- Adler A, Amyot R, Guardo R, Bates JH, Berthiaume Y (1997) Monitoring changes in lung air and liquid volumes with electrical impedance tomography. *J Appl Physiol* 83:1762–1767
- Luecke T, Meinhardt JP, Herrmann P, Weiss A, Quintel M, Pelosi P (2006) Oleic acid vs saline solution lung lavage-induced acute lung injury: effects on lung morphology, pressure–volume relationships, and response to positive end-expiratory pressure. *Chest* 130:392–401
- Kunst PW, Bohm SH, Vazquez de Anda G, Amato MB, Lachmann B, Postmus PE, de Vries PM (2000) Regional pressure volume curves by electrical impedance tomography in a model of acute lung injury. *Crit Care Med* 28:178–183
- Hinz J, Moerer O, Neumann P, Dudykevych T, Frerichs I, Hellige G, Quintel M (2006) Regional pulmonary pressure volume curves in mechanically ventilated patients with acute respiratory failure measured by electrical impedance tomography. *Acta Anaesthesiol Scand* 50:331–339