

Canadian Public Health Laboratory Network laboratory guidelines for the use of point-of-care tests for the diagnosis of syphilis in Canada

Ameeta E Singh BMBS MSc FRCPC^{1*}, Max A Chernesky PhD FIDSA FAAM FCCM^{2*},
Muhammad Morshed PhD SCCM^{3,4}, Tom Wong MD MPH CCFP FRCPC⁵

AE Singh, MA Chernesky, M Morshed, T Wong. Canadian Public Health Laboratory Network laboratory guidelines for the use of point-of-care tests for the diagnosis of syphilis in Canada. *Can J Infect Dis Med Microbiol* 2015;26(Suppl A):29A-32A.

Syphilis point-of-care tests (POCT) are widely available in developing countries enabling early diagnosis, treatment and support. The majority of commercially available tests use treponemal antigens and the presence of antibodies does not distinguish between current and past infection, which may lead to unnecessary antibiotic use and stigmatization of having a current STI. In hard-to-reach populations, the benefits may outweigh the risks. Available studies show reasonable performance of POCT with median sensitivity of 86%, specificity of 99% and positive predictive values >80% when prevalence was >0.3%. Although no syphilis POCT are approved in Canada at this time, a single study in an outreach setting in Alberta showed limited benefit due to a high prevalence of previous infection but more studies are needed. Newer dual tests employing treponemal and non-treponemal antigens look promising.

Key Words: *Canada; Dual tests; Point-of-care tests; Syphilis; Treponemal*

Les directives du Réseau des laboratoires de santé publique du Canada sur l'utilisation des tests au point de service pour diagnostiquer la syphilis au Canada

Les tests au point de service (TPdS) de la syphilis sont largement répandus dans les pays en voie de développement, ce qui favorise un diagnostic, un traitement et un soutien rapides. La majorité des tests offerts sur le marché font appel aux antigènes tréponémiques. Toutefois, la présence d'anticorps ne permet pas de distinguer une infection en cours d'une infection antérieure, ce qui peut entraîner l'utilisation inutile d'antibiotiques et une stigmatisation liée à l'ITS. Dans des populations difficiles à joindre, les avantages dépassent peut-être les risques. Selon les études existantes, les TPdS donnent des résultats raisonnables, à la sensibilité médiane de 86 %, à la spécificité de 99 % et aux valeurs prédictives positives de plus de 80 % lorsque la prévalence est supérieure à 0,3 %. Même si aucun TDdS de la syphilis n'est approuvé au Canada, une seule étude, réalisée dans un milieu communautaire en Alberta, en a démontré les avantages limités en raison de la forte prévalence d'infection antérieure, mais d'autres études s'imposent. De nouveaux doubles tests, faisant appel à des antigènes tréponémiques et non tréponémiques, semblent prometteurs.

DEFINITION OF A POINT OF CARE TEST

A point-of-care test (POCT) is a test that can be performed outside of a laboratory setting for which the result is available without reference to a laboratory and rapid enough to affect immediate patient management (1). Most POCT for syphilis are available with a short turn-around time with test results available in ≤20 min (2). For developing countries, the tests should be affordable, sensitive, specific, user friendly or simple to perform with minimal training, rapid, robust (ie, stable and not requiring cold-chain storage conditions), equipment-free and delivered to those who need it (www.who.int/std_diagnostics/about_SDI/priorities.htm).

RATIONALE FOR USING POCT FOR SYPHILIS IN CANADA

There is often a delay between testing and treatment even in compliant patients with positive (non POCT) results, during which infection can spread (3-5). Patients' not returning for results of testing for a sexually transmitted infection (STI) is a common problem (3,6-8).

Syphilis POCT are widely available for use in developing countries where they allow people to access a STI test at an earlier time point in their disease; they empower patients by allowing them to take greater responsibility for their own sexual health and expand the settings in which STI testing can be undertaken, enabling earlier diagnosis and access to rapid treatment and support (2,9).

Over the past several years, Canada has experienced syphilis outbreaks in street-involved persons, bathhouses and drop-in centres which are traditionally hard to reach through standard services. POCT would provide the ability to offer immediate testing and treatment in a single encounter to mitigate further spread, and an attractive alternative to standard testing (9,10).

Currently, there are no POCT approved for the diagnosis of syphilis in Canada. The majority of commercially available POCT are based on treponemal antigens. These tests cannot distinguish previously treated infections from untreated syphilis (11). Management based on treponemal antigen based POCT may result in unnecessary administration of antibiotics to patients and may also be psychologically detrimental to patients due to the stigma of a STI diagnosis (10). However, in hard-to-reach populations, the benefit of POCT could potentially outweigh the risks. Recognizing this trade-off, the U.S. Centers for Disease Control and Prevention recommends rapid screening and treatment for patients having positive tests at the first prenatal visit in populations in which use of "prenatal care is not optimal" (12). The United States FDA announced approval of a rapid syphilis test in September, 2011 (13). Syphilis POCT may provide 'while you wait' test results which can be confirmed by a non-treponemal test to identify high-risk patients for improved follow-up.

¹Division of Infectious Diseases, University of Alberta, Edmonton, Alberta; ²McMaster University, Hamilton, Ontario; ³BC Public Health Microbiology and Reference Laboratory; ⁴Department of Pathology and Laboratory Medicine, University of British Columbia, Vancouver, British Columbia; ⁵Public Health Agency of Canada, Ottawa, Ontario

*Denotes section lead

Correspondence: Dr Ameeta E Singh, Division of Infectious Diseases, University of Alberta, 3B20-11111 Jasper Avenue Northwest, Edmonton, Alberta T5K 0L4. Telephone 780-342-2300, fax 780-425-2194, e-mail ameeta@ualberta.ca



This open-access article is distributed under the terms of the Creative Commons Attribution Non-Commercial License (CC BY-NC) (<http://creativecommons.org/licenses/by-nc/4.0/>), which permits reuse, distribution and reproduction of the article, provided that the original work is properly cited and the reuse is restricted to noncommercial purposes. For commercial reuse, contact support@pulsus.com

TABLE 1
Treponemal tests for detection of syphilis antibodies

Test	Test name	Manufacturer	
Point of care	Determine TP	Abbott Laboratories, USA	
	Dual Syphilis POC Test	ChemBio Diagnostic Systems, USA	
	Espline TP	Fujirebio, Japan	
	Guardian One Step	Test Medica Diagnostics, USA	
	Rapid Syphilis Test	Quorum Diagnostic, Canada	
	SD Bioline 3.0	Standard Diagnostics, Korea and Pacific Biotech, Thailand	
	Syphilis Fast	Diesse Diagnostic, Italy	
	Syphilis OnSite Rapid Screening	CTK Biotech, USA	
	Syphilis Ultra Rapid	Acon, China	
	Syphicheck WB	QualPro Diagnostics, India	
	Trep-Strip IV	Phoenix Biotech, Canada	
	Visitect Syphilis	Omega Diagnostics, UK	
	Laboratory	Bioplex Syphilis	Bio-Rad, USA
		Bioplex 2200 Syphilis IgG	Bio-Rad, USA
FTA		Zeus Scientific, USA	
TPPA		Fujirebio, Japan	
TPHA		Omega Diagnostics, United Kingdom	
TrepID		Phoenix Biotech, Canada	
Trep-Check EIA		Phoenix Biotech, Canada	
Trep-Sure EIA		Phoenix Biotech, Canada	
Treponema ViraBlot		Viramed Biotech AG, Germany	

TYPES OF POCTS

a) Treponemal tests

Currently (Table 1) there are several commercial tests available internationally (10). They are of two varieties: 1) immunochromatographic strip (ICS) tests which work by having a test strip with a line that is impregnated with treponemal antigens that react with antibodies to syphilis in whole blood or serum to produce a readable change on the test strip; 2) particle agglutination tests (PATs), which use gelatin particles

coated with treponemal antigens that clump together on a test tray when combined with whole blood or serum containing antibodies to syphilis.

The Sexually Transmitted Diseases Diagnostics Initiative (SDI) conducted laboratory based evaluations on seven POCT (11). Tables 2 and 3 summarize the use of POCT in antenatal and other clinical settings. Although some of the studies reported low sensitivity values, the median sensitivity was 86% (interquartile range [IQR] 75% to 94%) and was comparable between antenatal and non-antenatal clinic sites. Two studies showed better sensitivity when serum specimens were used (11,14). Specificities ranged from 91% to 100% for studies with similar medians of 99% (IQR 97% to 100%) in all settings. The POCT also showed good positive predictive values of >80% when syphilis prevalence was >0.3%. Limited data are available to confirm if the sensitivity is maintained in HIV-infected individuals (15) and in those with high RPR titres (15,16). An Australian laboratory based study of four syphilis POCT reported that the Determine test had the highest overall sensitivity with significantly higher test sensitivities among high-RPR titre (RPR \geq 1:8) tests (17).

Only one test, the Syphilis Health Check (Trinity Biotech, USA), is United States FDA approved for use in the United States (18). This 10 min test can be used with whole blood, serum or plasma specimens, requires 25 μ L to 50 μ L of blood. According to the manufacturer, this treponemal POC test for syphilis has a reported 95.6% positive agreement and a 90.5% negative agreement with gold-standard testing, with a percent overall agreement of 90.6% (19). No published clinical data on test performance are available.

In the only published study of syphilis POCT in Canada, Bergman et al (20) reported a sensitivity of 85.3% (CI 68.9% to 95.0%), specificity of 100.0% (CI 99.6% to 100.0%), positive predictive value (PPV) of 100.0% (CI 88.1% to 100.0%), and negative predictive value (NPV) of 99.5% (CI 98.9% to 99.8%) of the SD Bioline 3.0 Syphilis Test (Standard Diagnostics, Korea) in hard-to-reach outreach settings in Edmonton, Alberta (20).

Available data on the antenatal cost-effectiveness of RPOCT show that the ICS TT tests are cost-effective for the detection of maternal syphilis in low resource settings when compared to either standard two-test testing algorithms (ie, NTT followed by TT) or a NTT alone (21-23). Owusu-Edusei et al (24) recently reported that a screening strategy employing an ICS TT was more cost saving than a dual-RPOCT (TT

TABLE 2
Selected studies of syphilis point-of-care tests in antenatal clinics (adapted from Tucker, 2010)

First author (reference), year (sample)	Location, study population	Test name	Reference standard test	Samples, n	Sensitivity, %		Syphilis antibody prevalence
					(95% CI)	(95% CI)	
Bronzan (27), 2007 (finger prick)	South Africa, 8 rural clinics	Determine	RPR, TPHA	341	86 (57-98)	91 (87-94)	6.5
Hernandez-Trejo (28), 2006 (serum)	Mexico, 2 urban clinics	Determine	VDRL, FTA-Abs	1322	100	100	0.3
Lien (29), 2000 (multiple)	Vietnam, one large urban clinic	Determine	RPR, TPPA	291	100	99	24.7
Mabey (30), 2006 (multiple)	Tanzania, one large government clinic	Determine	2 rapid tests compared with	528	60 (47-72)	99 (99-100)	10.8
		Visitectoline	treponemal tests (TPPA, etc)	528	75 (64-86)	99 (99-100)	10.8
		Syphicheck-WB		582	79 (68-89)	99 (98-100)	9.45
		SD Bioline 3.0		582	86 (77-94)	98 (97-99)	11.34
Montoya (15), 2006 (finger prick)	Mozambique, 6 rural clinics	SD Bioline 3.0	RPR, TPHA	326	86 (82-89)	97 (96-97)	8.35
Tinajeros (31), 2006 (finger prick)	Bolivia, 4 large urban clinics	Determine	RPR, TPPA	8892	92 (88-94)	98 (98-99)	3.85
Villazon-Vargas (32), 2009 (whole blood; not finger prick)	Bolivia, 1 urban clinic	Determine	RPR, FTA-Abs	489	98	100	4.5
West (33), 2002 (serum)	Gambia, 1 rural clinic	Rapid Syphilis Test	RPR, TPHA	1325	75	95	3.0

RPR Rapid plasma reagin; TPPA Treponema pallidum particle agglutination; TPHA Treponema pallidum haemagglutination test; FTA-Abs Fluorescent antibody absorbed; VDRL Venereal disease research laboratory; FSW Female sex workers

TABLE 3

Selected studies of point-of-care tests in non-antenatal settings (adapted from Tucker, 2010)

First author (reference), year (sample)	Location; study population	Test name	Reference standard test	Samples, n	Sensitivity, % (95% CI)	Specificity, % (95% CI)	Syphilis antibody prevalence
Benzaken (16), 2008 (finger prick)	Brazil, urban area and red-light clinic	Visitect	FTA-Abs VDRL	506	57 (46–67)	99 (97–100)	17.9
Campos (26), 2006 (whole blood)	Peru, Field based (STW)	Determine	RPR, TPHA	3862	55 (40–70)	99	5.1
Castro (25), 2010 (serum)	Georgia Public Health and clinic samples	Dual POC Test	RPR, TPHA	1601	96	95	62.9
Gianino (34), 2007 (whole blood; not finger prick)	Italy, one urban clinic	Determine	TPPA or other trep test	316	95 (89–98)	98 (95–99)	31.3
Herring (11), 2006 (archived serum)	Worldwide	Determine Syphilis-Fast Espline Syphicheck-WB SD Bioline 3.0 Visitect Syphilis OnSite Rapid	TPPA, TPHA	800	99 (95–98) 86 (82–89) 98 (96–99) 84 (80–88) 95 (92–99) 95 (92–99) 92 (90–95) 85 (81–88) 96 (93–99)	94 (92–96) 93 (90–95) 93 (90–96) 97 (96–99) 93 (91–94) 95 (92–97) 97 (95–99) 98 (96–99) 95 (92–99)	50
Mabey (30), 2006 (multiple)	Brazil, one urban clinic	Determine Visitect Syphicheck-WB SD Bioline 3.0	2 rapid tests compared with treponemal test (TPPA, TPHA, etc)	247 244 542 542	89 (80–97) 96 (90–100) 84 (74–94) 88 (79–97)	98 (96–100) 99 (97–100) 100 (99–100) 99 (99–100)	21.1 20.9 9.2 9.2
Mabey (30), 2006 (multiple)	Haiti, one urban clinic	Determine Visitect Syphicheck-WB SD Bioline 3.0	2 rapid tests compared with treponemal test (TPPA, TPHA, etc)	761 516 543 515	73 (59–86) 73 (61–85) 81 (68–93) 100 (n=30)	99 (98–99) 99 (98–100) 98 (97–99) 98 (97–100)	5.3 10.7 7.6 5.8
Nessa (35), 2008 (whole blood; not finger prick)	Dhaka, Bangladesh, urban clinics	Syphilis UltraRapid	RPR, TPHA	648	94	93	20.8
Siedner (14), 2004 (multiple)	San Francisco, CA, USA, one urban clinic	Determine Guardian Trep-Strip IV	TPPA	127 116 71	88 (81–96) 72 (60–84) 70 (54–85)	100 100 100	52.5
Bergman (20), 2013	Edmonton, Alberta, outreach settings	SD Bioline 3.0 Syphilis Test	Syphilis EIA, RPR and Syphilis InnoLia	1265	85.3 (68.9– 95.0)	100 (99.6– 100)	

CA California; FSW Female sex workers; FTA-Abs Fluorescent antibody absorbed; RPR Rapid plasma reagin; TPPA *Treponema pallidum* particle agglutination; TPHA *Treponema pallidum* haemagglutination test; VDRL Venereal disease research laboratory

and NTT) strategy in a high-prevalence setting but that the dual-RPOCT strategy may significantly reduce overtreatment. No cost effectiveness data are available for developed countries.

b) Non-treponemal tests

Because positive treponemal POCT may indicate new or old infections, a quantitative non-treponemal test is often helpful. However, there are no commercially available non-treponemal POC tests available as a single test at this point.

c) Dual tests

Two commercially available dual tests are currently available. Castro et al (25) evaluated a novel POCT (Chembio Diagnostics System Inc, USA) for the simultaneous detection of non-treponemal and treponemal antibodies in sera of 1601 patients. Results from the dual test were compared with rapid plasma reagin (RPR) and *Treponema pallidum* particle agglutination (TPPA) tests. When compared with the RPR, the reactive concordance of the non-treponemal result was 98.4% when the RPR was $\geq 1:2$. However, when the RPR was ≤ 1 , the sensitivity declined to 88%. When compared to the TPPA, the reactive and non-reactive concordance of the treponemal line was 96.5% and 95.5%. This dual POCT is designed for use with serum, plasma and whole blood. Span Diagnostics (India) also makes a dual test (www.span.co.in/#) but no published data on its performance in the field are available.

DIFFICULTIES ENCOUNTERED WITH POCT

Choice of test kit and specimen type are important when deciding which kit will perform optimally in any given field setting. For example, Campos et al (26) reported lower sensitivities with whole blood (finger-prick) specimens which might have been due to inadequate lighting, lack of use of heparinized capillary tubes for collection of whole blood, false negatives due to previously treated syphilis and a low proportion of samples reactive at low titres. Herring et al (11) showed variability between test lots, day to day testing and differences between testers.

Because POCT are often performed by inexperienced non-laboratorians outside of a laboratory, results can be variable. Judgment is used on subjective interpretation of a band being positive or negative in an ICS or agglutination strength in a PAT. Sufficient lighting should be provided to read results.

Programs may wish to develop procedural manuals in conjunction with a local reference laboratory to include a control and proficiency testing program. This is to ensure the competence of the testing staff as well as the integrity of the testing materials.

Some components of the QA program could include photographs of positive and negative reactions, the running of positive and negative controls, eg, with each new box of kits that is opened; the results should be recorded and logged. Storage conditions for the kits should be specified with logs kept for temperature control and logs kept as

well as procedures developed to respond to incidents, eg, actions for invalid tests, parallel testing discrepancy and control failure.

USE OF POCT FOR THE DIAGNOSIS OF SYPHILIS

It should be noted that similar to other screening tests for syphilis, a single POCT for syphilis may not be adequate for the diagnosis of syphilis and should follow recommended testing algorithms as described in the Chapter on Serologic Testing for Syphilis.

SUMMARY




Although not yet licensed or routinely available in Canada, syphilis POCT have the potential to provide immediate and rapid access to

testing and therefore treatment in 'hard-to-reach populations' or in non-traditional venues to mitigate the spread of syphilis. POCT which employ treponemal tests are also most likely to be of benefit in areas with high prevalence of new syphilis infections together with low rates of previous infection with syphilis. Further studies are needed to evaluate the utility, acceptance, effectiveness, quality control/quality assurance, potential adverse events and cost-effectiveness of syphilis POCT in clinics and field-based settings. Laboratories and clinicians should ensure the development of effective algorithms to confirm cases as well as maintain acceptable quality of POCT.

DISCLOSURES: The authors have no conflicts of interest to declare.

REFERENCES

- Dean GL. Near-patient testing will not improve the control of sexually transmitted infections. *Sex Transm Dis* 2006;82:509-12.
- Tucker JD, Brown LB, Yin Y-P, Chen X-S, Cohen MS. Accelerating worldwide syphilis screening through rapid testing: A systematic review. *Lancet Infect Dis* 2010;10:381-6.
- Swain GR, McDonald RA, Pfister JR, et al. Decision analysis: Point-of-care chlamydia testing versus laboratory based methods. *Clin Med Res* 2004;2:29-35.
- Mahilum-Tapay L, Laitila V, Wawrzyniak JJ, et al. New point of care chlamydia rapid test bridging the gap between diagnosis and treatment: Performance evaluation study. *BMJ* 2007;335:1190-4.
- Vickerman P, Watts C, Alary M, et al. Sensitivity requirements for the point of care diagnosis of *Chlamydia trachomatis* and *Neisseria gonorrhoeae* in women. *Sex Transm Infect* 2003;79:356-7.
- Singh A, Hill S, Shafran S. Non-return rates for HIV testing: Results of a 3-month retrospective review at an STD clinic in 1999. *Can Commun Disease Rep* 2000;26-18:152-5.
- Greenwald JL, Burstein GR, Pincus J, et al. A rapid review of rapid HIV antibody tests. *Current Inf Dis Reports* 2006;8:125-31.
- Kendrick SR, Kroc KA, Withum D, et al. Outcomes of offering rapid point-of-care HIV testing in a sexually transmitted disease clinic. *J Acquired Immune Deficiency Syndromes* 2005;38:142-6.
- Ward P. Near-patient testing will improve the control of sexually transmitted infections: Control of sexually transmitted infections: The arguments in favour. *Sex Transm Infect* 2006;82:506-8.
- Greer L, Wendel GD. Rapid diagnostic methods in sexually transmitted infections. *Infect Dis Clin N Am* 2008;601-17.
- Herring A, Ballard R, Pope V, et al. A multi-centre evaluation of nine rapid, point-of-care syphilis tests using archived sera. *Sex Transm Infect* 2006;82 (Suppl V):v7-v12.
- Department of Health and Human Services, Centers for Disease Control and Prevention. Sexually transmitted diseases treatment guidelines, 2006. *MMWR Recommendations and Reports*, 2006;55:No.RR-11,1-94.
- Mazzotta M. "Game changing" syphilis rapid test available in U.S.; Global implications unclear (news article). <http://sciencespeaksblog.org/2011/09/09/game-changing-syphilis-rapid-test-available-in-u-s-global-implications-unclear/?utm_source=feedburner&utm_medium=feed&utm_campaign=Feed%3A+ScienceSpeaksHivTbNews+%28Science+Speaks%3A+HIV+%26+TB+News%29> (Accessed October 4, 2011).
- Siedner M, Zapitz V, Ishida M, et al. Performance of rapid syphilis tests in venous and fingerstick whole blood specimens. *Sex Transm Dis* 2004;31:557-60.
- Montoya PJ, Lukehart SA, Brentlinger PE, et al. Comparison of the diagnostic accuracy of a rapid immunochromatographic tests and the rapid plasma reagin test for antenatal syphilis screening in Mozambique. *Bull World Health Organ* 2006;84:97-104.
- Benzaken AS, Sabido M, Galban EG, et al. Field evaluation of the performance and testing costs of a rapid point-of-care tests for syphilis in a red-light district of Manaus, Brazil. *Sex Transm Infect* 2008;84:297-302.
- Causser LM, Kaldor JM, Fairley CK, et al. A laboratory-based evaluation of four rapid point-of-care tests for syphilis. *PLoS One* 2014;9:e91504.
- Gaydos C, Hardick J. Point of care diagnostics for sexually transmitted infections: Perspectives and advances. *Expert Rev Anti Infect Ther* 2014;12:657-72.
- Syphilis health check. <www.diagnosticsdirect2u.com/images/PDF/SyphilisHC.pdf> (Accessed September 10, 2014).
- Bergman J, Gratrix J, Plitt S, Fenton J, Archibald C, Wong T, Singh AE. Feasibility and field performance of a simultaneous Syphilis and HIV point-of-care test based screening strategy in at risk populations in Edmonton, Canada. *AIDS Res Treat* 2013;819593.
- Terris-Prestholt F, Watson-Jones D, Mugeye K, et al. Is antenatal syphilis screening still cost effective in sub-Saharan Africa. *Sex Transm Infect* 2003;79:375-81.
- Levin CE, Steele M, Atherly D, et al. Analysis of operational costs of using rapid syphilis tests for the detection of maternal syphilis in Bolivia and Mozambique. *Sex Transm Dis* 2007;34:S47-54.
- Rydzak CE, Goldie SJ. Cost-effectiveness of rapid point-of-care prenatal syphilis screening in sub-Saharan Africa. *Sex Transm Dis* 2008;35:775-84.
- Owusu-Edusei K, Gift T, Ballard R. Cost effectiveness of a dual non-treponemal/treponemal syphilis point-of-care test to prevent adverse pregnancy outcomes in Sub-Saharan Africa. *Sex Transm Dis* 2011;38:997-1003.
- Castro AR, Esfaniari J, Kumar S, et al. A novel point-of-care test for the simultaneous detection of non-treponemal and treponemal antibodies in patients with syphilis. *J Clin Microbiol* 2010;48:4615-9.
- Campos PE, Buffardi AI, Chiappe M, et al. Utility of Determine Syphilis TP rapid test in commercial sex venues in Peru. *Sex Transm Infect* 2006;82(Suppl V):v22-25.
- Bronzan RN, Mwesigwa-Kayongo DC, Narkunas D, et al. Onsite rapid antenatal syphilis screening with an immunochromatographic strip improves case detection and treatment in rural South African clinics. *Sex Transm Dis* 2007;34:S55-60.
- Hernandez-Trejo M, Hernandez-Prado B, Uribe-Salas F, et al. Maternal and congenital syphilis in two Mexican hospitals: Evaluation of a rapid diagnostic test. *Rev Invest Clin* 2006;58:119-25 (Spanish).
- Lien TX, Tien NT, Chanpong GF, et al. Evaluation of rapid diagnostic tests for the detection of human immunodeficiency virus types 1 and 2, hepatitis B surface antigen and syphilis in Ho Chi Minh City, Vietnam. *Am J Trop Med Hyg* 2000;62:301-9.
- Mabey D, Peeling RW, Ballard R, Benzaken AS, et al. Prospective, multi-centre clinic based evaluation of for rapid diagnostic tests for syphilis. *Sex Transm Infect* 2006;82(Suppl V):v13-16.
- Tinajeros F, Grossman D, Richmond K, et al. Diagnostic accuracy of a point of care syphilis test when used among pregnant women in Bolivia. *Sex Transm Infect* 2006;82:v17-21.
- Villazon-Vargas N, Conde-Glez CJ, Juarez-Figueroa L, Uribe-Salas F. Evaluation of a rapid diagnostic test to assess the prevalence of maternal syphilis in Bolivia. *Rev Med Chil* 2009;137:515-21 (Spanish).
- West B, Walraven G, Morison L, et al. Performance of the rapid plasma reagin and rapid syphilis screening tests in the diagnosis of syphilis in field conditions in rural Africa. *Sex Transm Infect* 2002;78:282-5.
- Gianino MM, Dal Conte I, Sciole K, et al. Performance and costs of a rapid syphilis test in an urban population at high risk for sexually transmitted infections. *J Prev Med Hyg* 2007;48:118-22.
- Nessa K, Alam A, Chawghury FA, et al. Field evaluation of simple rapid tests in the diagnosis of syphilis. *Int J STD AIDS* 2008;19:316-20.

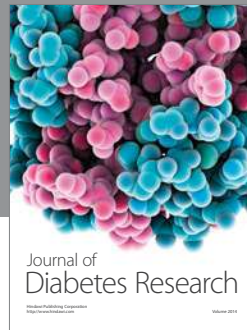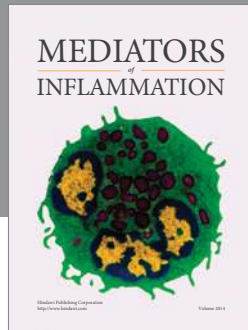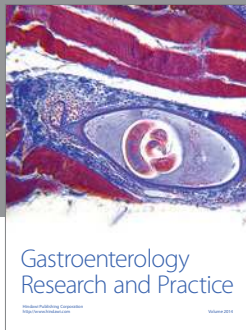

Hindawi
Submit your manuscripts at
<http://www.hindawi.com>

