

REVIEW

Correlative Fluorescence and Electron Microscopy on Ultrathin Cryosections: Bridging the Resolution Gap

John M. Robinson, Toshihiro Takizawa, Ana Pombo,¹ and Peter R. Cook

Department of Physiology and Cell Biology, Ohio State University, Columbus, Ohio (JMR); Department of Anatomy, Jichi Medical School, Tochigi, Japan (TT); and Sir William Dunn School of Pathology, University of Oxford, Oxford, United Kingdom (AP,PRC)

SUMMARY Microscopy has become increasingly important for analysis of cells and cell function in recent years. This is due in large part to advances in light microscopy that facilitate quantitative studies and improve imaging of living cells. Analysis of fluorescence signals has often been a key feature in these advances. Such studies involve a number of techniques, including imaging of fluorescently labeled proteins in living cells, single-cell physiological experiments using fluorescent indicator probes, and immunofluorescence localization. The importance of fluorescence microscopy notwithstanding, there are instances in which electron microscopy provides unique information about cell structure and function. Correlative microscopy in which a fluorescence signal is reconciled with a signal from the electron microscope is an additional tool that can provide powerful information for cellular analysis. Here we review two different methodologies for correlative fluorescence and electron microscopy using ultrathin cryosections and the advantages attendant on this approach. (*J Histochem Cytochem* 49:803–808, 2001)

KEY WORDS

correlative microscopy
ultrathin cryosections
immunocytochemistry
fluorescence microscopy
transcription factories
electron microscopy
immunogold

THE PAST FEW YEARS have witnessed a renaissance in biological optical microscopy. This has resulted largely from the availability of relatively inexpensive computers, sophisticated electronic cameras, computer software dedicated to imaging and microscopy, and many reagents for labeling cells and tissues. Many advances in the elucidation of structure–function relationships have relied upon fluorescence labeling. These advances notwithstanding, investigators are often confronted by the question: What is the true size and shape of a structure seen in the light microscope? Often this question can be answered only using an electron microscope. When this has been done, the fluorescence signal has often been collected from one cell or section and the electron microscopy signal collected from another. In some instances adjacent sections have been used. However, in these cases we face

an additional question: How do the structures seen with one method relate to those seen with the other method? Obviously, it would be best to image the exact same structures in both microscopes. Such a combination of light and electron microscopy can be referred to as correlative microscopy. Here, we review some applications of correlative microscopy and go on to describe a simple methodology that makes use of ultrathin cryosections and antibody probes labeled with both fluorochromes (for detection by light microscopy) and gold cluster compounds or colloidal gold particles (for electron microscopy).

Some Examples of Correlative Microscopy

Correlative microscopy can provide unique information that is difficult to obtain with a single imaging regimen. A recent example is provided by a study of the cytoskeletal proteins myosin II and tubulin (Svitkina and Borisy 1998). These proteins were fluorescently labeled and microinjected into living cells so that their dynamic behavior could be determined in real time in the fluorescence microscope. Then, the cells were prepared for electron microscopy by which the character-

Correspondence to: John M. Robinson, Dept. of Physiology and Cell Biology, Ohio State University, 302 Hamilton Hall, 1645 Neil Ave., Columbus, OH 43210. E-mail: robinson.21@osu.edu

Received for publication March 12, 2001; accepted March 26, 2001 (1R5499).

¹Present address: MRC Clinical Sciences Centre, Imperial College School of Medicine, London, UK.

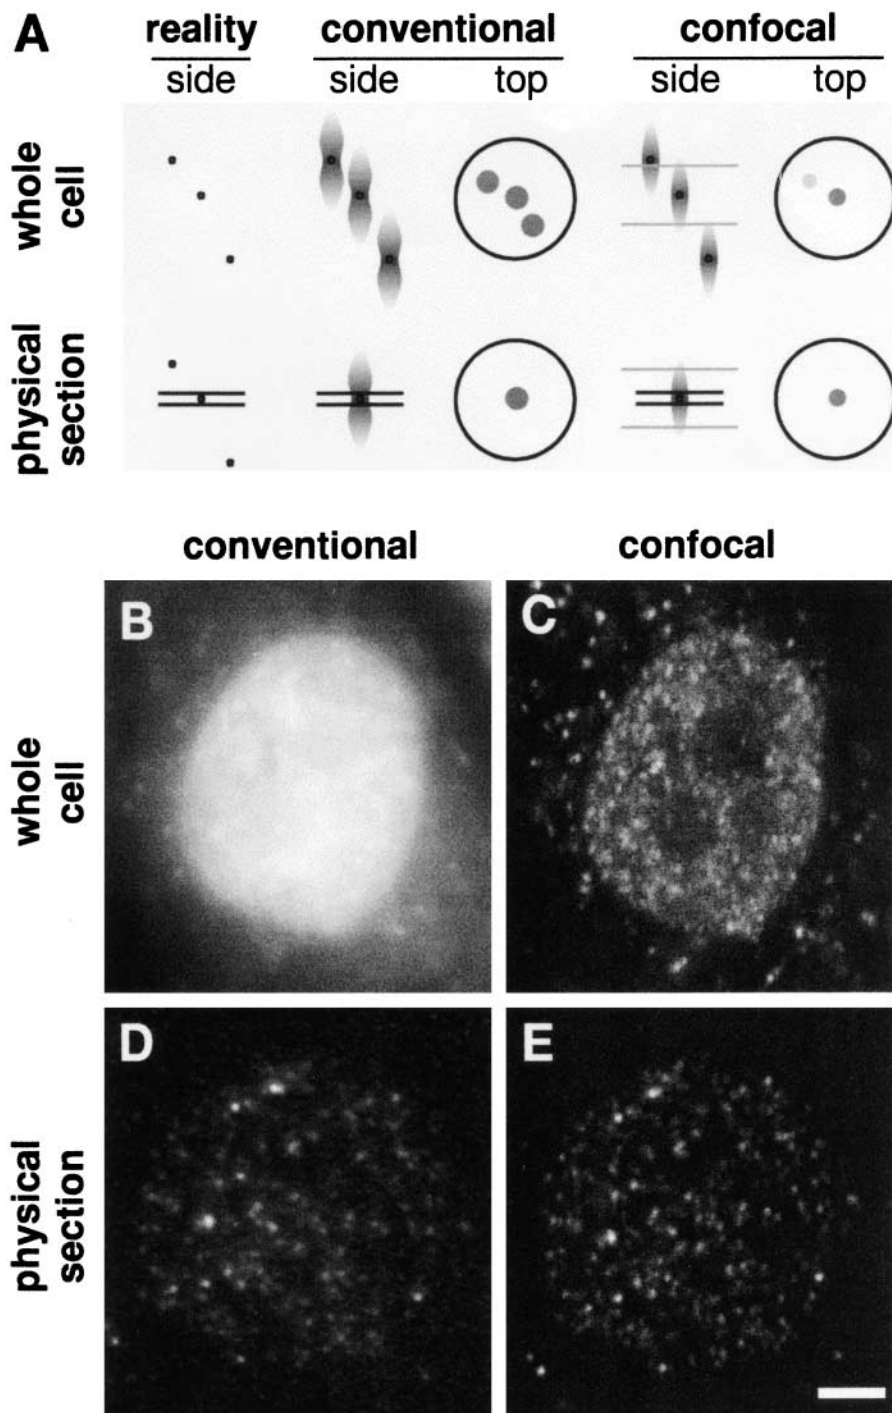


Figure 1 The theoretical basis of the improved resolution obtained when viewing small objects (diameter ~ 50 nm) within cells and improved resolution in practice using ultrathin cryosections, as illustrated by imaging transcription sites in HeLa cells. **(A)** The three spheres illustrated appear more elongated (side views of z-axis) and wider (top views of x-y-axes) than they really are when imaged using a conventional (i.e., widefield) or a confocal microscope. Their precise appearance depends on the point-spread function (typical ones are illustrated) associated with the optics of a particular microscope. When the whole cell is imaged using a conventional microscope, all three objects are seen as large circles; two are seen in the confocal, as the optical section (along the thin horizontal lines) contains no light from the third. After physically sectioning the sample (along the thick horizontal lines), only one sphere remains. **(B–E)** To visualize transcription sites, HeLa cells were permeabilized in a “physiological” buffer, allowed to extend nascent transcripts in Br-UTP for 15 min, fixed, and sites containing Br-RNA (real diameters ~ 40 nm) indirectly immunolabeled for fluorescence detection. “Raw” images of sites in whole cells or cryosections (~ 150 nm) were collected using a conventional or confocal microscope. In the conventional microscope, **(B)** foci appear blurred. In a confocal, **(C)** some individual foci can be resolved in the thinner optical section, although many apparently merge one into another. Cryosectioning yields simpler images; even in the conventional microscope **(D)**, foci are well resolved, and in the confocal **(E)** they appear even sharper. Bar = $2.5 \mu\text{m}$. From Pombo et al. (1999), with permission.

istic morphology of structures containing these proteins could be analyzed. However, most proteins lack distinctive features visible by conventional electron microscopy and therefore must be detected indirectly, usually with antibodies. In some cases, two secondary probes are used, one with a fluorochrome and the other with a gold particle (Tokuyasu et al. 1978; van Dam et al. 1991; Sun et al. 1995). In other cases, the

antibody, usually the secondary, bears both tags (Powell et al. 1997; Takizawa et al. 1998; Pombo et al. 1999). Care must be taken to ensure that the fluorescence signal in such probes is not reduced (Goodman et al. 1991) by fluorescence resonance energy transfer to the gold particle (Powell et al. 1998). Metal (e.g., gold) cluster compounds (0.8–1.4-nm diameter) can be used as alternatives to colloidal gold as particulate im-

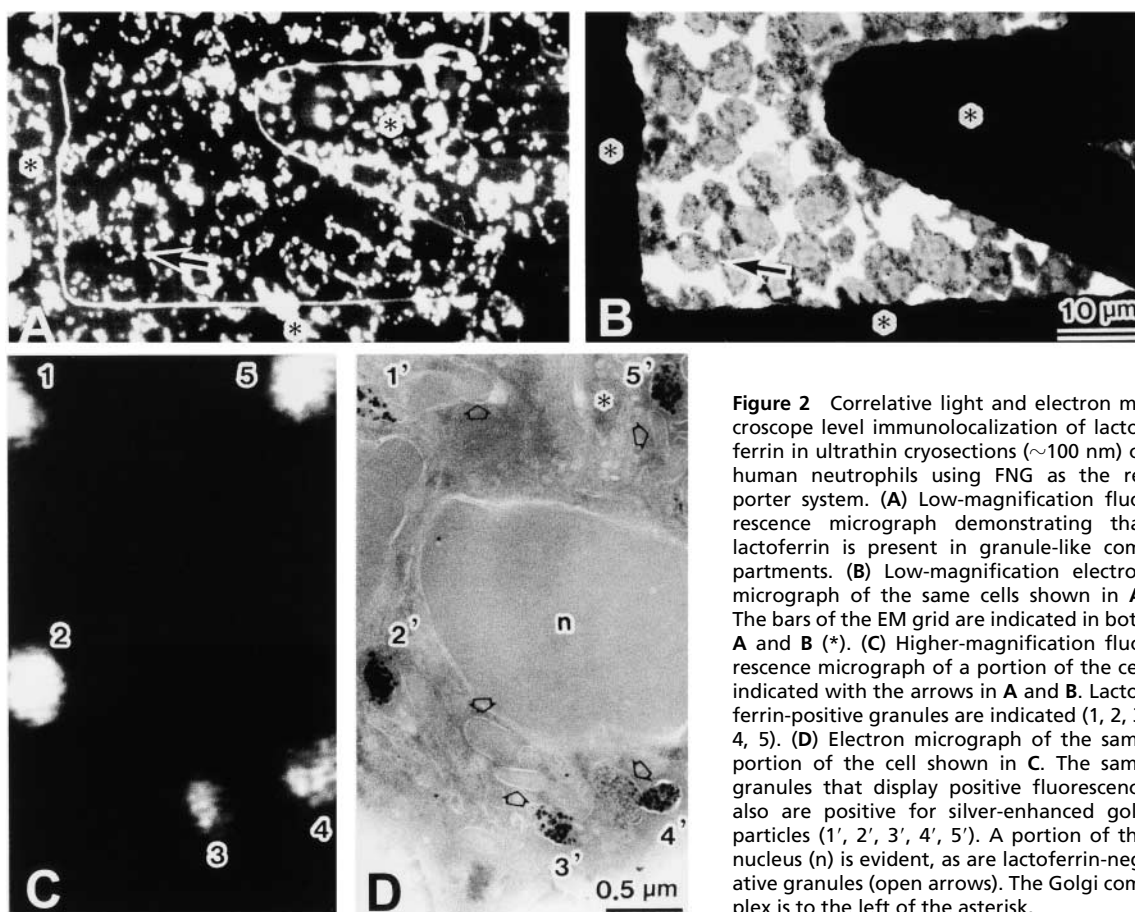


Figure 2 Correlative light and electron microscope level immunolocalization of lactoferrin in ultrathin cryosections (~ 100 nm) of human neutrophils using FNG as the reporter system. (A) Low-magnification fluorescence micrograph demonstrating that lactoferrin is present in granule-like compartments. (B) Low-magnification electron micrograph of the same cells shown in A. The bars of the EM grid are indicated in both A and B (*). (C) Higher-magnification fluorescence micrograph of a portion of the cell indicated with the arrows in A and B. Lactoferrin-positive granules are indicated (1, 2, 3, 4, 5). (D) Electron micrograph of the same portion of the cell shown in C. The same granules that display positive fluorescence also are positive for silver-enhanced gold particles (1', 2', 3', 4', 5'). A portion of the nucleus (n) is evident, as are lactoferrin-negative granules (open arrows). The Golgi complex is to the left of the asterisk.

munoprobe (Hainfeld and Furuya 1992). They contain a defined number of atoms and can be covalently attached to antibodies. (Proteins bind to colloidal gold electrostatically.) Fluorochromes can be coupled subsequently to generate unique immunoprobes known as FluoroNanogold (FNG). Conjugation of a fluorochrome and a gold cluster compound to generate FNG does not appear to affect the fluorescence intensity (Powell et al. 1998). Advantages and disadvantages of FNG have been reviewed (Robinson et al. 1998,2000). Photo-oxidation of diaminobenzidine (DAB) has also been used to couple fluorescence and electron microscopy (Maranto 1982; Pagano et al. 1989; Deernick et al. 1994). The use of green fluorescent protein (GFP)-tagged proteins for correlative light and electron microscopy offers exciting opportunities to probe further into the relationship between cell structure and function. Combined live cell fluorescence microscopy of GFP-vesicular stomatitis virus G protein (VSVG) and immunoelectron microscopy for localization of VSVG have been applied to the analysis of transport intermediates from the Golgi to plasma membrane (Polishchuk et al. 2000).

Bridging the Resolution Gap with Ultrathin Cryosections

It is often important to section cells and tissues before microscopic examination. However, biological materials are usually fragile and optimal sections cannot be obtained without embedding the sample in a supporting medium. Waxes and resins are often used for this purpose. Alternatively, samples can be frozen before sectioning. Methodology for preparing ultrathin cryosections in which the sample is fixed, frozen, and the vitrified sample is sectioned has been developed (e.g., Bernhard and Leduc 1967; Christensen 1971). This technique proved especially valuable for immunocytochemistry (Tokuyasu and Singer 1976; Tokuyasu 1980).

The resolution of the confocal microscope is typically ~ 200 nm in the x- and y-axes and ~ 500 nm in the z-axis (Inoué 1995). The resolving power of the transmission electron microscope is at least two orders of magnitude greater. There are many situations in which improvement in resolution is important in the analysis of supramolecular complexes. The relatively poorer resolution of conventional optical microscopy, particularly in the z-axis, can be improved with the

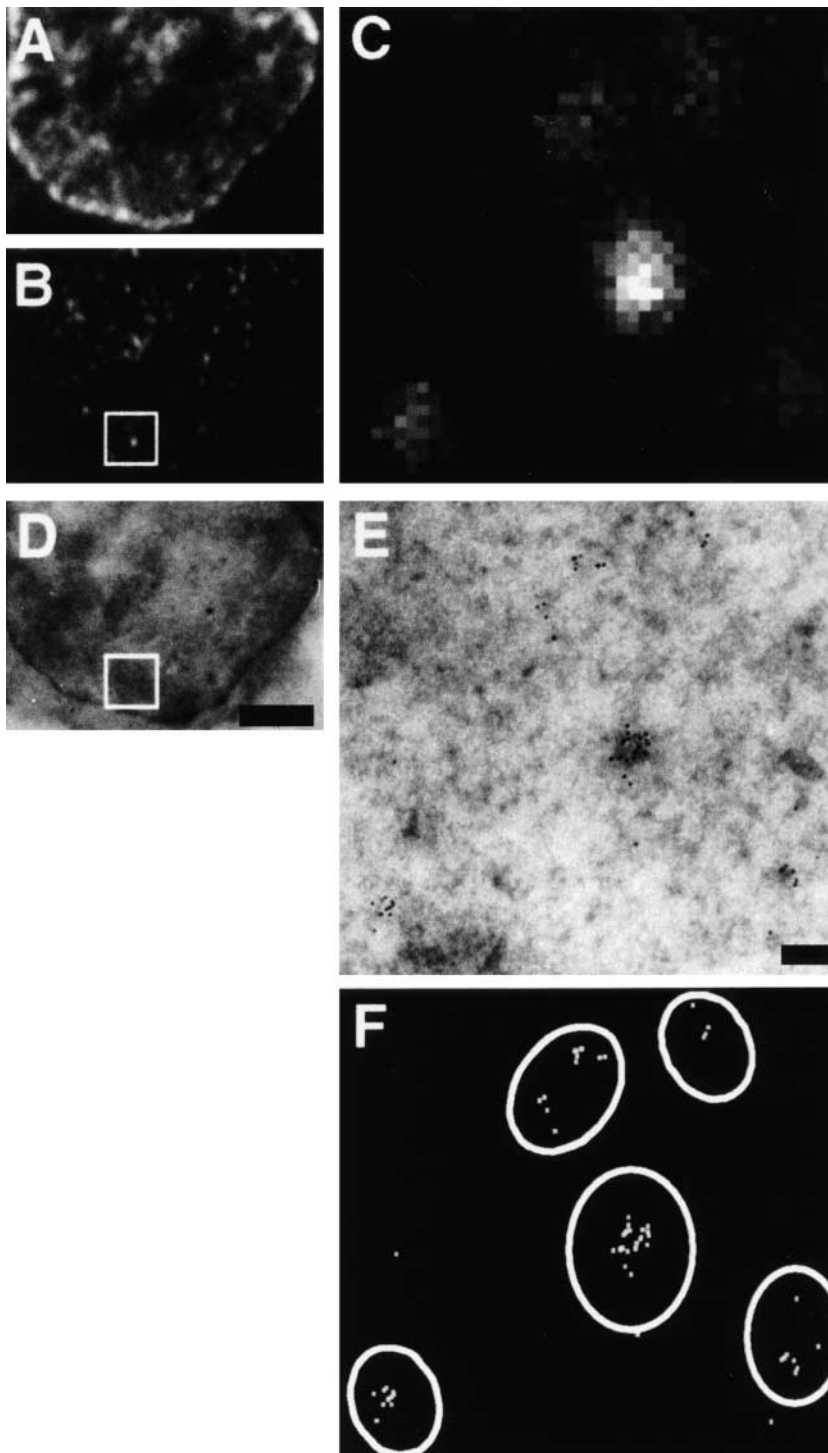


Figure 3 Imaging the same transcription sites by confocal and electron microscopy. HeLa cells were permeabilized, allowed to extend nascent transcripts in Br-UTP for 15 min, fixed, and cryosections (~ 150 nm) prepared. One cryosection was transferred onto a glass coverslip, Br-RNA indirectly immunolabeled with FITC-protein A adsorbed to 6-nm gold particles, and nucleic acids counterstained with TOTO-3. Green (FITC; Br-RNA) and far-red (TOTO; nucleic acids) images were collected on the confocal microscope. Then the section was flat-embedded in Epon, and the resulting block resectioned. Finally, the end section (~ 150 nm) was imaged in the electron microscope. (A–C). Confocal microscopy. The low-power views illustrate the distribution of nucleic acids (A) and Br-RNA (B) in one nucleus; (C) an enlargement of the area in the box in B. (D,E). Electron microscopy. The low-power view (D) confirms that the same cell is imaged. (E) An enlargement of the boxed area in D; Br-RNA is marked by clusters of gold particles. (F). Co-localization. The boundaries of the foci seen in C are overlaid over the gold particles (shown in white) seen in D, thus illustrating their co-localization. All sites are seen in both microscopes. Bars: A,B,D = 2 μ m; C,E,F = 100 nm. From Pombo et al. (1999), with permission.

use of sophisticated deconvolution software (Agard and Sedat 1983; Carrington et al. 1995; Scalettar et al. 1996) or confocal microscopy (White et al. 1987). Both approaches have been applied extensively to fluorescence microscopy. The thickness of an optical section (e.g., in the confocal microscope) is governed by optical parameters that are reviewed by Majlof and Forsgren (1993). They describe the thickness of a con-

focal section (Rd) for the special case of an infinitely small confocal aperture as:

$$Rd = 1.4n_o\lambda/NA^2$$

where n_o is the refractive index of the immersion medium, λ is the wavelength, and NA is the numerical aperture. In normal microscopy preparations with a

wavelength of 500 nm and an NA of 1.4, R_d is ~ 500 nm.

In addition to confocal and deconvolution microscopy, one can minimize problems associated with z-axis resolution (i.e., ~ 500 nm) by imaging thin sections (100–150 nm in thickness) (Ishiko et al. 1998; Takizawa et al. 1998; Pombo et al. 1999). In this case, all fluorescence signals must come from within the thickness of the cryosection (Figure 1). This has the practical effect of improving z-axis resolution. This apparent, or practical, improvement is especially noted when small and numerous objects are imaged.

The use of thin cryosections can also reduce the chromatic aberration inevitably associated with the simultaneous collection of multicolor images. Consider, for example, imaging two different antigens in one multiprotein complex with red and green fluorochromes to determine if they co-localize. Because light of different wavelengths is diffracted to different degrees, the red and green images cannot both be exactly in focus. This chromatic aberration becomes acute when objects lying at different depths in cells (or confocal sections) are imaged. However, it can be minimized simply by using cryosections. An in-focus image of one fluorochrome is collected, filters are switched, the microscope refocused, and an image of the second fluorochrome collected (Pombo et al. 1999). Then both images are in focus, easing comparison.

Correlative Microscopy with Ultrathin Cryosections: Two Applications

Neutrophils display a characteristic range of physiological and biochemical responses on exposure to appropriate stimuli (e.g., phagocytosable particles, chemotactic peptides). Most biochemical studies of stimulus-dependent events (e.g., exocytosis) are carried out on neutrophils in suspension. Lactoferrin has been localized to granules in these rounded cells using rabbit primary antibodies and FNG secondary antibodies (Takizawa et al. 1998). Not surprisingly, it is impossible to resolve individual granules in fluorescence images of whole cells; the cell “glows” as granules in the focal plane are obscured by out-of-focus flare from those lying above and below. Confocal microscopy of whole-cell preparations increases resolution of individual granules (not shown), but those preparations are not directly amenable to subsequent electron microscopy. We therefore employed ultrathin cryosections and FNG as the detection system for immunolocalization. Then, discrete fluorescent granules were observed, while the gold clusters could be seen in the electron microscope after silver enhancement. (Size enhancement of the ultrasmall immunogold is required for routine visualization.) Imaging the same cryosections by light and electron microscopy allows comparison of the two signals

(Figure 2). These results illustrate the power and convenience of this methodology.

The visualization of transcription sites provides a second example (Pombo et al. 1999). Permeabilized HeLa cells were allowed to incorporate Br-UTP into RNA. Then nascent transcripts at the site of transcription were indirectly immunolabeled with a primary antibody that reacts with Br-RNA, a secondary antibody, and a protein A–FITC–gold (6-nm) complex (Figure 3). Finally, samples were prepared and imaged in the light and electron microscopes. All sites seen in the light microscope could be detected in the electron microscope and, surprisingly, 83% of the sites were resolved by the light microscope (Pombo et al. 1999).

Benefits of Ultrathin Cryosections for Correlative Microscopy

Immunofluorescence microscopy can allow high throughputs and detection of several different antigens with great sensitivity. The use of ultrathin cryosections brings additional advantages. First, immunolabeling is improved, antigenicity is preserved, and anti-

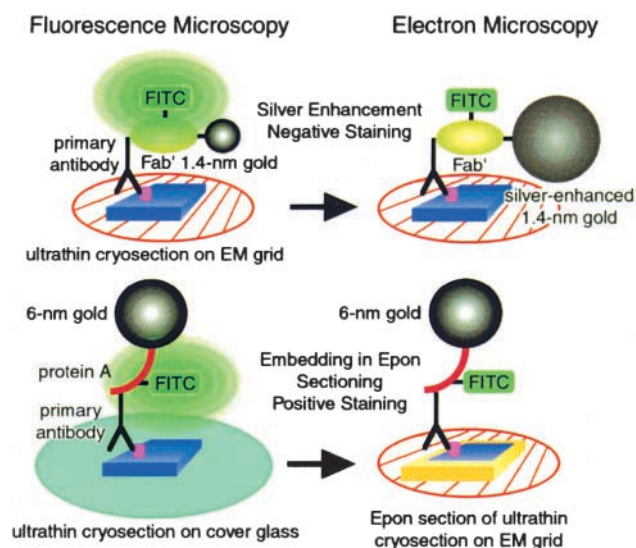


Figure 4 Summary of the preparative procedures used in Figures 2 and 3. The upper portion illustrates the use of FNG as the reporter system for imaging ultrathin cryosections by fluorescent and electron microscopy. In this case, the ultrathin section was collected on an EM grid before immunolabeling. It was subsequently mounted between a microscope slide and a coverslip for light microscopy. The slide preparation was then disassembled and the size of the FNG increased by silver enhancement before electron microscopy. The lower portion of the figure illustrates the second approach. Here the ultrathin section was collected on a glass coverslip before immunolabeling; the reporter system was colloidal gold (6 nm) to which protein A and FITC were conjugated. After observation with the fluorescence microscope, the ultrathin cryosection was embedded in Epon resin. Sections from the Epon block were cut and collected on EM grids, stained, and observed with the electron microscope. In both instances, the same subcellular structures were observed by both fluorescence and electron microscopy.

bodies penetrate more easily deeply into thin sections. Second, images are sharper; z-axis resolution is higher, backgrounds are lower (because out-of-focus flare is eliminated), and one kind of chromatic aberration can be reduced (see above). Third, correlative microscopy is facilitated. This brings additional resolution and, importantly, the ability to confirm that a structure seen by light microscopy is the same as another seen by electron microscopy. The two different preparative procedures we have employed are summarized in Figure 4. Of course, correlative microscopy depends on probes that can be imaged in both light and electron microscopes, and fortunately such probes are now available or can be prepared easily. Although the methods described here are useful for work with single cells, their most important applications may be in the study of tissues, in which correlative microscopy has been more difficult to accomplish.

Acknowledgments

Supported in part by the following grants: NIH HD38764, HD35121, and the American Heart Association (JMR); The Wellcome Trust (PRC), Royal Society (AP), and grants-in-aid for scientific research and project grants of the Center for Molecular Medicine of Jichi Medical School from the Ministry of Education, Science, Sports, and Culture of Japan (TT).

Literature Cited

- Agard DA, Sedat JW (1983) Three-dimensional architecture of a polytene nucleus. *Nature* 302:676–681
- Bernhard W, Leduc EH (1967) Ultrathin frozen sections. I. Methods and ultrastructural preservation. *J Cell Biol* 34:757–771
- Carrington WA, Lynch RM, Moore ED, Isenberg G, Fogarty KE, Fay FS (1995) Superresolution three-dimensional images of fluorescence in cells with minimal light exposure. *Science* 268:1483–1487
- Christensen AK (1971) Frozen thin sections of fresh tissue for electron microscopy, with a description of pancreas and liver. *J Cell Biol* 51:772–804
- Deernick TJ, Martone ME, Lev-Ram V, Green DPL, Tsien RY, Spector DL, Huang S, Ellisman MH (1994) Fluorescence photooxidation with eosin: a method for high resolution immunolocalization and in situ hybridization detection for light and electron microscopy. *J Cell Biol* 126:901–910
- Goodman SL, Park K, Albrecht RM (1991) A correlative approach to colloidal gold labeling with video-enhanced light microscopy, low-voltage scanning electron microscopy, and high-voltage electron microscopy. In Hayat MA, ed. *Colloidal Gold: Principles, Methods, and Applications*. Vol 3. San Diego, Academic Press, 369–409
- Hainfeld JF, Furuya FR (1992) A 1.4-nm gold cluster covalently attached to antibodies improves immunolabeling. *J Histochem Cytochem* 40:177–184
- Inoué S (1995) Foundations of confocal scanned imaging in light microscopy. In Pawley JB, ed. *Handbook of Biological Confocal Microscopy*. 2nd ed. New York, Plenum Press, 1–17
- Ishiko A, Shimizu H, Masunaga T, Kurihara Y, Nishikawa T (1998) Detection of antigens by immunofluorescence on ultrathin cryosections of skin. *J Histochem Cytochem* 46:1455–1460
- Majlof L, Forsgren PO (1993) Confocal microscopy: important considerations for accurate imaging. *Methods Cell Biol* 38:79–95
- Maranto AR (1982) Neuronal mapping: a photooxidation reaction makes Lucifer yellow useful for electron microscopy. *Science* 217:953–955
- Pagano RE, Sepanski MA, Martin OC (1989) Molecular trapping of fluorescent ceramide analogue at the Golgi apparatus of fixed cells: interaction with endogenous lipids provides a trans-Golgi marker for both light and electron microscopy. *J Cell Biol* 109:2067–2079
- Polishchuk RS, Polishchuk EV, Marra P, Alberti S, Buccione R, Luini A, Mironov AA (2000) Correlative light-electron microscopy reveals the tubular-saccular ultrastructure of carriers operating between Golgi apparatus and plasma membrane. *J Cell Biol* 148:45–58
- Pombo A, Hollinshead M, Cook PR (1999) Bridging the resolution gap: imaging the same transcription factories in cryosections by light and electron microscopy. *J Histochem Cytochem* 47:471–480
- Powell RD, Halsey CM, Hainfeld JF (1998) Combined fluorescent and gold immunoprobes: reagents and methods for correlative light and electron microscopy. *Microsc Res Tech* 42:2–12
- Powell RD, Halsey CM, Spector DL, Kaurin SL, McCann J, Hainfeld JF (1997) A covalent fluorescent-gold immunoprobe: simultaneous detection of pre-mRNA splicing factor by light and electron microscopy. *J Histochem Cytochem* 45:947–956
- Robinson JM, Takizawa T, Vandré DD (2000) Applications of gold cluster compounds in immunocytochemistry and correlative microscopy: comparison with colloidal gold. *J Microsc* 199:163–179
- Robinson JM, Takizawa T, Vandré DD, Burry RW (1998) Ultra-small immunogold particles: important probes for immunocytochemistry. *Microsc Res Tech* 42:13–23
- Scalettar BA, Swedlow JR, Sedat JW, Agard DA (1996) Dispersion, aberration and deconvolution in multi-wavelength fluorescence images. *J Microsc* 182:50–60
- Sun XJ, Tolbert LP, Hildebrand JG (1995) Using laser scanning confocal microscopy as a guide for electron microscopic study: a simple method for correlation of light and electron microscopy. *J Histochem Cytochem* 43:329–335
- Svitkina TM, Borisy GG (1998) Correlative light and electron microscopy of the cytoskeleton of cultured cells. *Methods Enzymol* 298:570–592
- Takizawa T, Suzuki K, Robinson JM (1998) Correlative microscopy using FluoroNanogold on ultrathin cryosections. Proof of principle. *J Histochem Cytochem* 46:1097–1102.
- Tokuyasu KT (1980) Immunocytochemistry on ultrathin frozen sections. *Histochem J* 12:381–403
- Tokuyasu KT, Singer SJ (1976) Improved procedures for immunoferritin labeling of ultrathin frozen sections. *J Cell Biol* 71:894–906
- Tokuyasu KT, Slot JW, Singer SJ (1978) Simultaneous observations of immunolabeled frozen sections in LM and EM. *Proc 9th Int Cong Electron Microsc* 2:164–165
- van Dam GJ, Bogitsh BJ, Franssen JA, Kornelis D, Van Zeyl RJ, Deelder AM (1991) Application of the FITC–anti-FITC–gold system to ultrastructural localization of antigens. *J Histochem Cytochem* 39:1725–1728
- White JG, Amos WB, Fordham M (1987) An evaluation of confocal versus conventional imaging of biological structures by fluorescence light microscopy. *J Cell Biol* 105:41–48