

Deep Learning for Ultrasound Image Formation: CUBDL Evaluation Framework & Open Datasets

Dongwoon Hyun*, Alycen Wiacek**, Sobhan Goudarzi, Sven Rothlübbers, Amir Asif, Klaus Eickel, Yonina C. Eldar*, Jiaqi Huang*, Massimo Mischi*, Hassan Rivaz, David Sinden, Ruud J.G. van Sloun*, Hannah Strohm, Muyinatu A. Lediju Bell*

Abstract—Deep learning for ultrasound image formation is rapidly garnering research support and attention, quickly rising as the latest frontier in ultrasound image formation, with much promise to balance both image quality and display speed. Despite this promise, one challenge with identifying optimal solutions is the absence of unified evaluation methods and datasets that are not specific to a single research group. This paper introduces the largest known international database of ultrasound channel data and describes associated evaluation methods that were initially developed for the Challenge on Ultrasound Beamforming with Deep Learning (CUBDL), which was offered as a component of the 2020 IEEE International Ultrasonics Symposium. We summarize the challenge results and present qualitative and quantitative assessments using both the initially closed CUBDL evaluation test dataset (which was crowd-sourced from multiple groups around the world) and additional *in vivo* breast ultrasound data contributed after the challenge was completed. As an example quantitative assessment, single plane wave images from the CUBDL Task 1 dataset produced a mean generalized contrast-to-noise ratio (gCNR) of 0.67 and a mean lateral resolution of 0.42 mm when formed with delay-and-sum beamforming, compared to a mean gCNR as high as 0.81 and a mean lateral resolution as low as 0.32 mm

when formed with networks submitted by the challenge winners. We also describe contributed CUBDL data that may be used for training of future networks. The compiled database includes a total of 576 image acquisition sequences. We additionally introduce a neural network-based global sound speed estimator implementation that was necessary to fairly evaluate results obtained with this international database. The integration of CUBDL evaluation methods, evaluation code, network weights from the challenge winners, and all datasets described herein are publicly available (visit <https://cubdl.jhu.edu> for details).

Index Terms—beamforming, channel data, deep learning benchmark, evaluation metrics, sound speed estimation, ultrasound image formation

I. INTRODUCTION

SIGNIFICANT research has been dedicated recently to developing methods for deep learning in ultrasound imaging, as summarized in several recent review articles and special issue editorials [1]–[4]. The merger of deep learning and ultrasound image formation is promising because it has the potential to shed light on features that are not considered by algorithmic approaches that underlie the mathematical, model-based component of image formation with multiple input, output, and training options [5]–[7]. These data-driven deep learning approaches have the potential to be more robust than traditional model-based beamforming methods, as they do not require parameter changes when switching to different scanners, they are able to generalize across different data sets, and they can infer from advanced beamforming methods in less time than that required to perform the otherwise computationally intensive calculations associated with advanced beamformers [8]–[11]. Despite the promising potential of deep learning approaches applied to ultrasound imaging, there has been a noticeable dearth of publicly available frameworks to evaluate new deep learning methods with the same reference data. Such open frameworks are useful for benchmarking and comparing methods against each other, as demonstrated in the fields of visual recognition [12] and computed tomography [13].

One outcome of the Challenge on Ultrasound Beamforming with Deep Learning (CUBDL), offered as a component of the 2020 IEEE International Ultrasonics Symposium, was the development of an open evaluation framework that may be used as a standard for deep learning image formation methods in ultrasound imaging. The overarching goal of this

*CUBDL Organizers

**Post-CUBDL Evaluator and Post-CUBDL Data Curator

M.A.L.B. and A.W. acknowledge the National Institutes of Health (NIH) Trailblazer Award R21 EB025621 for partial support of their time on this project. H.R. and S.G. acknowledge the support of the Natural Sciences and Engineering Research Council of Canada (NSERC) RGPIN-2020-04612.

Dongwoon Hyun is with the Department of Radiology, Stanford University, Palo Alto, CA USA

Alycen Wiacek is with the Department of Electrical and Computer Engineering, Johns Hopkins University, Baltimore, MD, 21218 USA

Sobhan Goudarzi and Hassan Rivaz are with the Department of Electrical and Computer Engineering, Concordia University, Montreal, Quebec, Canada

Sven Rothlübbers, Hannah Strohm, and David Sinden are with the Fraunhofer Institute for Digital Medicine MEVIS, Bremen, Germany

Amir Asif is with the Department of Electrical Engineering and Computer Science at York University, Toronto, ON, Canada

Klaus Eickel is with the University of Bremen, Bremen, Germany

Yonina C. Eldar is with the Department of Math and Computer Science, Weizmann Institute of Science, Rehovot, Israel

Jiaqi Huang is with the Department of Biomedical Engineering, Johns Hopkins University, Baltimore, MD, 21218 USA

Massimo Mischi and Ruud J. G. van Sloun are with the Department of Electrical Engineering, Eindhoven University of Technology, Netherlands

Ruud J. G. van Sloun is also with Philips Research, Eindhoven, Netherlands

Muyinatu A. Lediju Bell is with the Department of Electrical and Computer Engineering and also with the Department of Biomedical Engineering and the Department of Computer Science, Johns Hopkins University, Baltimore, MD, 21218 USA (e-mail: mledijubell@jhu.edu)

challenge was to explore the potential of deep learning to improve ultrasound image quality and to balance these improvements with implementation practicality (i.e., reasonable display frame rates) [14]. Comparisons were completed on the same datasets and with the same evaluation methods and framework.

This paper summarizes and compares submissions to CUBDL using the evaluation framework developed for this challenge. We present results on both the initially closed CUBDL evaluation test dataset as well as additional *in vivo* breast ultrasound data contributed after the completion of the challenge. Components of this evaluation framework were publicly available while CUBDL was in progress, and the framework is now merged with the CUBDL test data and the additional datasets described herein. This framework merger and associated datasets are publicly available at [15] and [16], respectively (visit <https://cubdl.jhu.edu> for more details). The summary within this paper and the accessibility of our data and code are provided in efforts to enable future benchmarking and evaluation of new methods.

The remainder of this paper is organized as follows. Section II provides an overview of the CUBDL challenge, including dates associated with major milestones. Section III describes details of the open datasets, the top challenge submissions, the CUBDL evaluation process, scoring and ranking methods, and the post-CUBDL analyses implemented to ensure robustness and reproducibility of our shared code and challenge winner declaration. This section is organized to align with the sequential timeline of events and is effectively a combination of materials utilized and methods implemented by three categories of contributors to this manuscript: (1) the CUBDL organizers who implemented data set curation, evaluation, scoring, assessment, and rankings, (2) the top challenge participants who provided network details, and (3) A.W. who completed the independent post-CUBDL evaluations and curation of the post-CUBDL datasets. Section IV presents the results from the perspective of the CUBDL organizers, detailing our evaluation and analysis findings, with post-CUBDL contributions from A.W. Section V discusses results within the broader context of the current state of the field from the perspective of the CUBDL organizers. Finally, Section VI concludes the manuscript.

II. CHALLENGE SUMMARY & TIMELINE

Organization of this challenge initiated on October 13, 2019. The complete challenge setup, submission process, and discussion of the challenge organization are described in detail in the associated conference proceedings co-authored by the challenge organizers [20]. To briefly summarize details in [20] that are relevant to this manuscript, the challenge was designed with no specific training data provided by the CUBDL organizers, because a review of current literature on the topic of deep learning for ultrasound beamforming reveals that there are multiple possibilities for both training approaches and training datasets. Therefore, the CUBDL organizers decided to keep the training open ended, with the goals of encouraging a wide variety of submission approaches, enabling participants to

innovate on the training methods, and challenging participants to produce a network that achieved specific tasks and met specified requirements. Publicly available PICMUS data [21] was additionally advertised and considered to serve as possible training data for participants who desired more structure. From November 22, 2019 to January 23, 2020, test data were crowd-sourced from multiple groups around the world, representing the largest known international database of ultrasound channel data.

The challenge opened to participants on January 30, 2020 and closed to participants on the submission deadline of June 23, 2020. Although three optional tasks were conceived by the CUBDL organizers [20] and advertised on the CUBDL website [14], all participants submitted networks to be evaluated for Task 1, which was beamforming with deep learning after a single plane wave transmission, with two optional subtasks. Task 1a was explicitly focused on creating a high-quality image from a single plane wave to match a higher quality image created from multiple plane waves. Three participants submitted to this subtask. Task 1b allowed more flexibility to create images with the highest possible image quality metrics, including metrics that exceeded those obtained with multiple plane wave transmissions. One participant submitted to this subtask. Note that the dates that CUBDL was open to participants overlapped with the onset and peaks of the global COVID-19 pandemic [22], which likely affected participation rates.

Participants were instructed to train networks using their preferred machine learning frameworks (e.g., TensorFlow, PyTorch) and submit final model files to the IEEE DataPort website [16]. The CUBDL organizers then downloaded the submitted models and launched a Python script to perform evaluation [15] on the internationally crowd-sourced database of test data [16]. Evaluation metrics advertised since the launch of the CUBDL website [14] were pre-selected by the CUBDL organizers based on literature from multiple groups reporting beamforming with deep learning (e.g., [8], [9], [11], [23]) and based on common computer vision literature containing assessments of network complexity (e.g., [24]–[26]).

After evaluation, two participants (one submitting to Task 1a, the other submitting to Task 1b) produced networks that showed evidence of overfitting to the training data when tested on the closed CUBDL test dataset for Task 1 [19], [27]. These participants were declared the runners up of the challenge. Details about their networks and performance results are available in [19], [27] and in the presentation document published on the CUBDL website [14], which was initially prepared for the live CUBDL challenge session on September 11, 2020 at the 2020 IEEE International Ultrasonics Symposium. The remaining two network submissions [28], [29] are compared and evaluated in greater detail in this publication, which upholds the commitment advertised on the CUBDL website that only top submissions would be included in the journal publication associated with the challenge [14]. Also as promised on the CUBDL website, the trained model weights for these top submissions are available with the public release of the CUBDL evaluation code [15] and datasets [16].

TABLE I
SUMMARY OF CUBDL TASK 1 TEST DATA AND ADDITIONAL POST-CUBDL EVALUATION DATA

Institution	Total # of Sequences	Data Type	US Scanner	Transducer	Center Frequency (MHz)	Sampling Frequency (MHz)	Number of Plane Waves	Image Depth (mm)	Reference
TSH	1	<i>In Vivo</i>	Verasonics Vantage 256	L10-5	7.5	6.25	31	40	[17]
MYO	5	Phantom	Verasonics Vantage 256	L11-4v	6.25	28.96	75	63.8	–
UFL	4	Phantom	ULA-OP256	LA533 (Esaote)	8	78.125	75	50	–
EUT	2	Phantom	Verasonics Vantage 128	Phillips S5-1	3.1	12.5	75	100	–
INS	3	Phantom	Verasonics Vantage 256	L7-4	5.2	20.8	75	56.7	–
INS	4	Phantom	Verasonics Vantage 256	L12-5	7.8	31.25	75	56.7	–
OSL	1	Phantom	Verasonics Vantage 256	L7-4	5.2	20.8	75	50	–
OSL	1	Simulation	Field II	N/A	5.13	20.8	75	50	[18]
JHU*	9	<i>In Vivo</i>	Alpinion ECUBE-12R	L8-17	12.5	40	73-75	30	[19]
JHU*	2	<i>In Vivo</i>	Alpinion ECUBE-12R	L3-8	5.5	40	75	30	[19]

*Post-CUBDL evaluation data

III. MATERIALS & METHODS

A. Open Datasets

1) *CUBDL Task 1 Dataset*: The test data for Task 1 of the challenge consisted of 21 image acquisition sequences crowd-sourced from 6 institutions, referenced hereafter by the shorthand 3-letter code provided in parentheses: (1) Department of Biomedical Engineering, Tsinghua University, China (TSH); (2) Department of Radiology, Mayo Clinic, US (MYO); (3) Microelectronic Systems Design Laboratory, University of Florence, Italy (UFL); (4) Signal Processing Systems group, Eindhoven University of Technology, Netherlands (EUT); (5) CREATIS, Insa Lyon, France (INS); and (6) Research Group for Digital Signal Processing and Image Analysis, University of Oslo, Norway (OSL).

Test data from these institutions consisted of 21 image acquisition sequences from targets including phantoms, simulation, and an *in vivo* brachioradialis. The phantom data consisted of a total of 9 different phantoms from 3 manufacturers including: (1) CIRS models 040, 049, 054GS, 050, and ATS549; (2) GAMMEX models 404GSLE, 403, and 410 SCG; and (3) NPL Thermal Test Phantom. Two MYO phantom acquisitions included a layer of *ex vivo* porcine abdominal tissue to introduce acoustic clutter. The *in vivo* data were acquired after informed consent and ethics approval. This wide range of channel data was acquired with 3 ultrasound scanners (i.e., Verasonics Vantage 128, Verasonics Vantage 256, and ULA-OP) and 5 ultrasound transducers. The acquisition center frequencies ranged from 3.1 MHz to 8 MHz. The sampling frequencies ranged from 6.25 MHz to 78.125 MHz. The ultrasound transducers consisted of linear and phased arrays.

Each contributed dataset for Task 1 consisted of acquisitions from 31 or 75 steered plane waves, with transmission angles ranging -15° to 15° or -16° to 16° . Additional summary details

and acquisition parameters are reported in Table I, along with references to reports in which the data first appeared. The full list of sequence numbers and more specific details are available in the Appendix, which contains information that was provided in the CUBDL Data Guide while the challenge was open.

2) *JHU In Vivo Breast Dataset for Post-CUBDL Evaluation*: To improve the variety of *in vivo* datasets, the Photoacoustic and Ultrasonic Systems Engineering Lab, Johns Hopkins University, USA (3-letter code: JHU) contributed additional test data for network evaluation after the challenge was closed. These *in vivo* breast ultrasound data (initially reported by Li *et al.* [19]) consisted of 11 acquisition sequences, acquired from 6 patients, including two orthogonal scans (i.e., radial and anti-radial) of 5 patients and a radial scan of 1 patient. These data were acquired after informed consent and with approval from the Johns Hopkins Medicine Institutional Review Board (IRB). Specifically, raw plane wave radiofrequency channel data were acquired with an Alpinion ECUBE-12R research ultrasound scanner connected to either an L8-17 or L3-8 linear array ultrasound transducer, with 75 plane wave transmissions including angles ranging -16° to 16° , or with 73 plane wave transmissions including angles ranging -8° to 8° . The sampling frequency was 40 MHz. Additional details and acquisition parameters are reported in Table I and in the Appendix.

3) *Additional Dataset Contributions*: A subset of contributed data not selected by the CUBDL organizers for evaluation of Task 1 are included in the open dataset [16] published with this paper for potential future training of new networks. There were various reasons these data were not selected for Task 1, including a desire to maintain sufficient variability, to avoid dominance of data from one group, phantom, subject, or system setting, and to exclude data acquired with focused transmissions for the unattempted Task 3. These additional data consisted of 544 image acquisition sequences (including

529 acquired with plane wave transmissions and 15 acquired with focused transmissions), contributed from MYO, UFL, TSH, EUT, INS, OSL, and JHU. Image targets included simulated structures, experimental phantoms, and *in vivo* heart, breast, brachioradialis, and carotid. The *in vivo* data from JHU and OSL were acquired after informed consent and IRB approval, as noted in [30] and [31], respectively. The *in vivo* data from TSH were acquired after informed consent and ethics approval. The phantom data consisted of 13 different phantoms from 6 manufacturers including: (1) CIRS models 040, 049, 054GS, 050, 059, and AT5549; (2) GAMMEX models 404GSLE, 403, and 410 SCG; (3) NPL Thermal Test Phantom; (4) CAE Blue Phantom Elastography Breast Model; (5) True Phantom Solutions Brain Phantom; and (6) Dansk Phantom Service Model 453. One of these phantom acquisitions (i.e., from MYO) included a layer of *ex vivo* porcine abdominal tissue to introduce acoustic clutter. These data were acquired with 5 ultrasound scanners (i.e., Verasonics Vantage 256, Verasonics Vantage 128, Alpinion ECUBE12-R, ULA-OP, and Philips) and 8 ultrasound transducers. The acquisition center frequencies ranged from 2.97 MHz to 12.5 MHz. The sampling frequencies for this dataset ranged from 6.25 MHz to 100 MHz, representing a larger range than that reported in Section III-A.1. The ultrasound transducers consisted of linear and phased arrays. Additional details and acquisition parameters are reported in the Appendix.

4) *Sound Speed Correction Applied to Phantom Data:* In ultrasound imaging, the sound speed is often assumed to be globally constant at 1540 m/s when computing focusing time delays. However, the true sound speed often differs from this assumption and depends on specific properties of the underlying tissue. For example, the sound speed of fat is lower than that of liver or muscle [32], [33], and the sound speeds of calibrated tissue-mimicking phantoms are known to vary with the ambient temperature [34]. Improper focusing can degrade image quality, lead to worsened metrics such as contrast and point target resolution, and cause incorrect positioning of image targets. As CUBDL evaluation heavily depended on these and other image quality parameters [20], the CUBDL organizers applied an initial sound speed correction to the contributed test data.

Sound speed correction is an active area of research with many proposed figures of merit, including speckle brightness [35], [36], coherence factor [37], among many others [38]–[41]. Considering this multitude of validated options, the CUBDL organizers selected speckle brightness maximization for its simplicity and its wide acceptance as a criterion of focusing quality [35]. More specifically, the correct global sound speed was selected as the one that maximized the average brightness in a homogeneous region of speckle [36].

PyTorch [42] provides a convenient differentiable framework to perform per-image optimization. Using the same PyTorch implementation of delay-and-sum (DAS) plane wave beamforming provided to CUBDL participants, the sound speed was adjusted via gradient ascent until speckle brightness was maximized using the Adam optimizer (initial step size: 10 m/s, decay rate: 0.9, 30 steps). Despite the use of PyTorch, we emphasize that this sound speed correction did not involve

any actual deep learning. Specifically, no parameters were trained, and no future predictions of sound speed were performed. PyTorch was simply used to execute a well-known and previously validated sound speed correction algorithm [36] on a per-image basis. This sound speed correction was a necessary step implemented by the CUBDL organizers to enable fair evaluations, and the corrected sound speed values were not shared with the participants while the challenge was open.

For each of the 49 phantom acquisition sequences acquired using plane wave transmissions (including 19 of the plane wave sequences described in Sec. III-A.1 and 30 of the plane wave sequences described in Sec. III-A.3), the PyTorch DAS beamformer and associated sound speed correction implementation processed the 75 plane-wave raw data in a pixel grid corresponding to a homogeneous region of speckle. Fig. 1(a) shows the sound speeds obtained throughout 30 iterations of

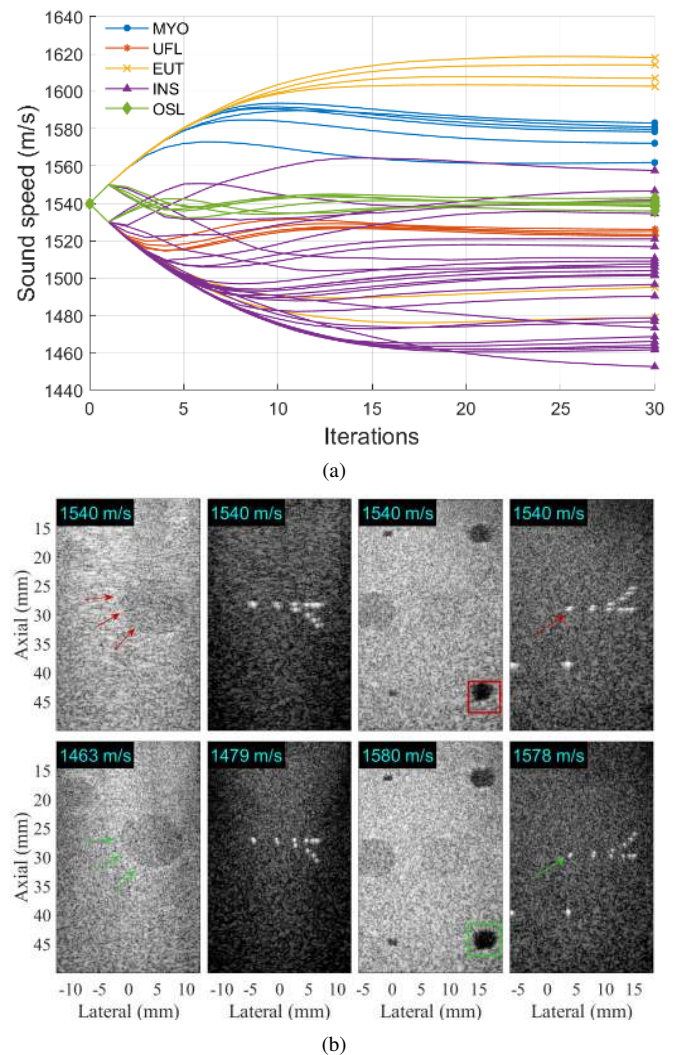


Fig. 1. (a) A wide range of optimal sound speeds were observed in contributed phantom datasets after 30 iterations of speckle brightness maximization. (b) Phantom images from sequences INS023, INS018, MYO001, and MYO003 are shown (from left to right, respectively) before (top) and after (bottom) global sound speed correction, displayed with 50 dB dynamic range. Arrows and boxes highlight locations where lesion boundaries are considerably sharper, point targets are visually more separable, and targets are repositioned to calibrated depths after sound speed correction.

speckle brightness maximization for each of the 49 phantom acquisition sequences. After 30 iterations, a wide range of optimal sound speeds were observed across these contributed datasets, ranging from 1453 m/s to 1618 m/s. The corrected value is largely grouped by institution. The two sequences from MYO acquired with the clutter layer (i.e., MYO004 and MYO005) are most deviant in comparison to the remaining sequences from the same institution. The data submitted by INS, which included 9 different phantoms, demonstrated the largest variation. The sound speed correction was sensitive to the chosen speckle region for some of these phantoms.

Fig. 1(b) shows example phantom images created from sequences INS023, INS018, MYO001, and MYO003. The sound speed included in the files submitted by data contributors for these four data sequences was 1540 m/s (although the sound speed values provided on data sheets from the associated phantom manufacturers were unlisted, 1540 m/s, 1580 m/s, and 1580 m/s, respectively). When using 1540 m/s as the sound speed to create images, lesion inclusions and point targets were visible, yet with degraded contrast and resolution, as seen in the top row of Fig. 1(b). However, when the same channel data were used to create images with the corrected sound speeds, this update yielded considerably sharper lesion boundaries, more visually separable point targets, and target repositioning to calibrated depths, as seen in the bottom row of Fig. 1(b). The specific sound speed values used to create the example images in Fig. 1(b) are reported in the top left corner of each image.

The corrected sound speeds for the 49 phantoms are now available with the CUBDL evaluation code [15] and associated datasets [16]. During the evaluation process, the corrected sound speeds were provided as inputs to the networks submitted by participants and were utilized to calculate the image quality metrics reported throughout the manuscript.

5) *Summary of Compiled Open Datasets*: In summary, the complete CUBDL + Post-CUBDL datasets released with this publication contain a total of 576 acquisition sequences with the following breakdown: (1) 49 experimental phantom data sequences acquired with plane wave transmissions; (2) 11 *in vivo* data sequences from the breast of six patients, each acquired with plane wave transmissions; (3) 500 *in vivo* data sequences from the brachioradialis of a healthy volunteer, each acquired with plane wave transmissions; (4) 6 experimental phantom data sequences acquired with focused transmissions; (5) 8 *in vivo* data sequences comprised of the carotid artery of a healthy volunteer, the heart of two healthy volunteers, and the breast of two patients, each acquired with focused transmissions; and (6) 2 Field II [43], [44] simulations.

The phantom data consisted of a total of 12 different phantoms from 6 manufacturers including: (1) CIRS models 040, 049, 054GS, 050 and 059; (2) GAMMEX models 404GSLE, 403, and 410 SCG; (3) NPL Thermal Test Phantom; (4) CAE Blue Phantom Elastography Breast Model; (5) True Phantom Solutions Brain Phantom; and (6) Dansk Phantom Service Model 453. Three of the phantom acquisitions (i.e., from MYO) included a layer of *ex vivo* porcine abdominal tissue to introduce acoustic clutter.

This wide range of channel data was acquired with 4 ultra-

sound scanners and 8 ultrasound transducers. The acquisition center frequencies ranged from 2.97 MHz to 12.5 MHz. The sampling frequencies ranged from 6.25 MHz to 100 MHz. The ultrasound transducers consisted of linear and phased arrays. These data were provided by 7 groups total: (1) MYO; (2) UFL; (3) EUT; (4) INS; (5) OSL; (6) TSH; and (7) JHU. More details about these data are available in Tables IV through X in the Appendix.

We additionally provide sound speeds for the 49 phantom acquisition sequences acquired using plane wave transmissions with the released datasets [16], including corrected sound speeds from the procedure described in Section III-A.4, sound speeds submitted by data contributors, and sound speeds reported in publicly available datasheets from phantom manufacturers for comparison.

B. Top Challenge Submissions

1) *Rothlübbers et al. [28]*: A fully convolutional network was submitted by Rothlübbers *et al.* [28], and the following summary includes details that are not available in [28]. The network had 4 layers. The network input was time-delayed, magnitude-normalized, complex-valued data from the 0° plane wave transmission angle. The network output was a real valued (scalar) weighting factor for each reconstructed pixel. The network was designed to model the united sign coherence factor (USCF) [45] by computing pixel-wise weighting. The final pixel values were obtained by multiplying the unweighted sum absolute pixel values by the network output pixel weights, followed by log compression and a correction for the maximum value.

Batch normalization and ReLU activation followed each convolution. To account for memory limitations during training and inference, a patch-based approach was utilized, dividing input and target data into patches of size 200×200 . Convolutions were applied in the channel domain only, resulting in individually processed pixels. This network used an Adam optimizer with a learning rate decay of 0.1 every 5 epochs, and it was trained for 15 epochs. The loss was computed as a linear combination of mean-squared error (MSE) and multiscale structural similarity (MS-SSIM) [46] loss on the log compressed, normalized final images. The trained network weights are available with the evaluation code provided with this publication.

Training data consisted of 107 US raw data sets of a phantom (Model 054GS, CIRS, Norfolk, VA), acquired with multiple angles using a 128-element linear array transducer (DiPhAS, Fraunhofer IBMT, Sankt Ingbert, Germany) operating at 4 MHz. High-quality target images were reconstructed using multi-angle USCF imaging [45], utilizing data from seven plane wave angles. The reconstruction grid was chosen with an equidistant isotropic pixel spacing of a third of the wavelength and positioned such that artifact prone areas such as for example near the transducer were excluded. The publicly available PICMUS dataset [47] was used to test the model prior to submitting it to the challenge.

2) *Goudarzi et al. [29]*: The details in the following summary parallel the details provided in Section III-B.1 if direct

comparison between the two networks is desired, and this summary includes additional details that are not available in [29]. The submission by Goudarzi *et al.* [29] utilized the MobileNetV2 [48] architecture, which consists of depth-wise separable convolution building blocks, linear bottlenecks between layers, and shortcut connections between the bottlenecks. The network input was a $2 \times m \times n$ matrix in which first the two channels were the real and imaginary parts of in-phase and quadrature (IQ) data, n is the number of channels and m is the length of the window considered for temporal averaging to preserve the speckle statistics. The network output was a two-dimensional vector containing real and imaginary parts of the beamformed data. The network was designed to estimate and apply an apodization window to the input IQ channel data for minimum variance beamforming [49]. The output IQ data was then envelope detected and log compressed to obtain the final B-mode ultrasound image. This network used an AdamW optimizer [50] with default parameters (i.e., $\beta_1 = 0.9$ and $\beta_2 = 0.999$). The loss was computed as the L1-norm between the network output and the IQ pixel values obtained using the minimum variance beamformer. The trained network weights are available with the evaluation code provided with this publication.

Training data for this network consisted of the publicly available plane wave and focused transmission datasets available in the Ultrasound Toolbox [47], [51], [52]. This toolbox contains replicates of data sequences OSL008-OSL009 [53], OSL011-OSL014 [31], and OSL015 [54] in a different file format. Plane wave datasets from this toolbox were acquired with a Verasonics Vantage 256 scanner and L11-4v probe (phantom and *in vivo* data), an Alpinion E-Cube12R scanner and L3-8 probe (phantom data), and Field II simulated data. Focused imaging datasets were acquired with a Verasonics Vantage 256 scanner connected to a P4-2v probe and an Alpinion E-Cube12R scanner connected to a L3-8 probe. Although up to 75 plane waves were available, images were reconstructed from data received after only a single 0° plane wave transmission as the ground truth output images during training, because the objective when implementing this network was to mimic minimum variance beamforming [49] (which is a real mapping function on the channel data).

C. Evaluation Metrics

1) *Local Image Quality Metrics*: Contrast, contrast-to-noise ratio (CNR), generalized contrast-to-noise ratio (gCNR) [53], [55], and signal-to-noise ratio (SNR) within selected regions of interest (ROIs) were measured on the envelope of beamformed images from CUBDL Task 1 data as follows:

$$\text{Contrast} = 20 \log_{10} \left(\frac{\mu_1}{\mu_2} \right) \quad (1)$$

$$\text{CNR} = \frac{\mu_1 - \mu_2}{\sqrt{\sigma_1^2 + \sigma_2^2}} \quad (2)$$

$$\text{gCNR} = 1 - \sum_x \min\{f_1(x), f_2(x)\} \quad (3)$$

$$\text{SNR} = \frac{\mu_o}{\sigma_o} \quad (4)$$

where μ_i , σ_i , and f_i represent the mean, standard deviation, and histogram, respectively, of ROI i . The gCNR metric was calculated with 256 bins. The SNR metric was used to measure speckle preservation with the ground truth derived from the 75 plane wave image. In addition to the above metrics, the axial and lateral full-width at half maximum (FWHM) of point targets was calculated to determine resolution. Details surrounding the specific ROIs chosen for each test case are available in the Appendix and in our public evaluation code [15]. This code will further include routines for evaluating speckle pattern autocorrelations for resolution measurements.

2) *Global Image Quality Metrics*: The more global ℓ_1 loss, ℓ_2 loss, peak signal-to-noise ratio (PSNR), and normalized cross correlation (ρ) metrics were computed from CUBDL Task 1 data for image-to-image comparisons between network-produced envelope images and the corresponding 75 (or 31 for sequence TSH002) plane wave envelope image:

$$\ell_1 = \frac{1}{N} \sum_{n=1}^N |x_n - y_n| \quad (5)$$

$$\ell_2 = \sqrt{\frac{1}{N} \sum_{n=1}^N |x_n - y_n|^2} \quad (6)$$

$$\text{PSNR} = 20 \log_{10} \frac{\text{Dynamic Range}}{\sqrt{\frac{1}{N} \sum_{n=1}^N |x_n - y_n|^2}} \quad (7)$$

$$\rho = \frac{\sum_n (x_n - \mu_x)(y_n - \mu_y)}{\sqrt{\left(\sum_n |x_n - \mu_x|^2\right) \left(\sum_n |y_n - \mu_y|^2\right)}} \quad (8)$$

where x and y denote the two images being compared, each containing N pixels. The image comparisons were performed using pixels within the dynamic range of -40 dB to 0 dB with respect to the maximum pixel value of the ground truth image to avoid overemphasis of small magnitude differences and to avoid penalizing networks that do not reproduce the acoustic clutter that resides at magnitudes less than -40 dB [56]. In addition, both the ℓ_1 and ℓ_2 losses were computed for images on a linear scale (i.e., before log compression, denoted as ℓ_1 and ℓ_2 , respectively) and on a log-compressed scale (i.e., after log compression, denoted as ℓ_1 -log and ℓ_2 -log, respectively). The linear scale is expected to be more sensitive to high-amplitude variations (e.g., edges), whereas the log scale is more sensitive to low-amplitude variations (e.g., speckle). These metrics were computed on images that were normalized to minimize the achievable loss, as described in the Appendix of [11]. Overall, these global image quality metrics provide quantitative information that is not subject to the region selection requirement of the local metrics.

3) *Network Complexity*: Network complexity was determined by the number of learnable parameters in each submitted model. Although the CUBDL organizers initially intended to include network speed as an additional parameter to assess network complexity, there was greater variety in the “preprocessing” prior to entering the network than anticipated, which complicated fair comparisons of network speed. For example, the submission by Goudarzi *et al.* [29] needed the

TABLE II

SUMMARY OF LOCAL IMAGE QUALITY COMPARISONS AND NETWORK COMPLEXITY, WITH [28] AND [29] EVALUATED ON SINGLE PLANE WAVE DATA.

	Contrast (dB)	CNR	gCNR	Speckle SNR	Lateral FWHM (mm)	Axial FWHM (mm)	Number of Learned Parameters
Single Plane Wave	-10.50 ± 5.40	1.05 ± 0.44	0.67 ± 0.23	1.85 ± 0.04	0.42 ± 0.07	0.36 ± 0.15	0
Rothlübbers <i>et al.</i> [28]	-9.82 ± 4.93	0.67 ± 0.26	0.53 ± 0.20	1.19 ± 0.16	0.32 ± 0.10	0.33 ± 0.13	3,059
Goudarzi <i>et al.</i> [29]	-13.77 ± 3.07	1.34 ± 0.25	0.81 ± 0.09	1.81 ± 0.06	0.34 ± 0.10	0.36 ± 0.15	2,226,146
75 Plane Waves	-24.71 ± 5.55	1.53 ± 0.32	0.95 ± 0.05	1.81 ± 0.08	0.36 ± 0.07	0.34 ± 0.14	0

data to be reshaped and reformatted into 1D kernels along the axial dimension, all of which was implemented outside of PyTorch, whereas the two submissions from the runners up [19], [27] needed a 2D image interpolation in numpy. For this reason, the CUBDL organizers only considered network size, as each participant successfully addressed the proposed task which purposefully did not specify which component of the image formation process had to be learned.

D. Scoring and Ranking

The four CUBDL participants were evaluated using the test data described in Section III-A.1 and received a rank based on each quantitative network performance described in Section III-C. These rankings were grouped into two categories: (1) image quality and (2) network complexity, considering that participants were challenged to balance both image quality and display frame rates. We averaged the ranks of the metrics obtained by each participant within these two groups. The average rank from each group was summed. This scoring system is represented mathematically as follows:

$$\text{Final Score} = \frac{\sum \text{image quality metric rankings}}{T_{\text{IQ}}} + \frac{\sum \text{Network complexity metric rankings}}{T_{\text{NC}}} \quad (9)$$

where T_{IQ} and T_{NC} are the total numbers of image quality metric rankings and network complexity rankings, respectively.

E. Post-CUBDL Analyses

To improve the robustness of our evaluation methods and to ensure the robustness of our open-source code, two additional analyses were implemented. First, a two-sample, two-tailed t -test with a 5% significance level was performed to determine the statistical significance of differences among the top two submitted networks described in Section III-B when evaluating the global image-to-image metrics described in Section III-C.2. Second, the test data was evaluated by an independent user (A.W.) after the challenge was closed to new submissions. This independent user provided feedback to increase compatibility of the evaluation framework and also used this framework to evaluate the submitted networks with the Post-CUBDL data described in Section III-A.2.

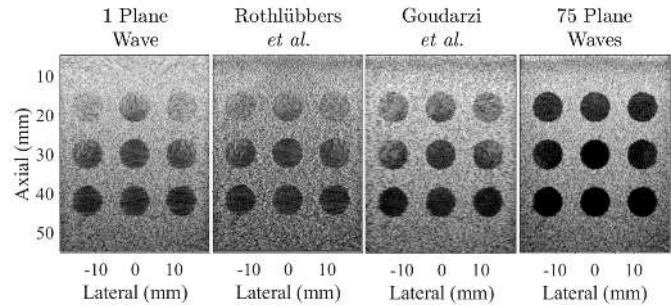


Fig. 2. Results from the baseline PICMUS dataset [21] of simulated anechoic lesions, displayed with 60 dB dynamic range.

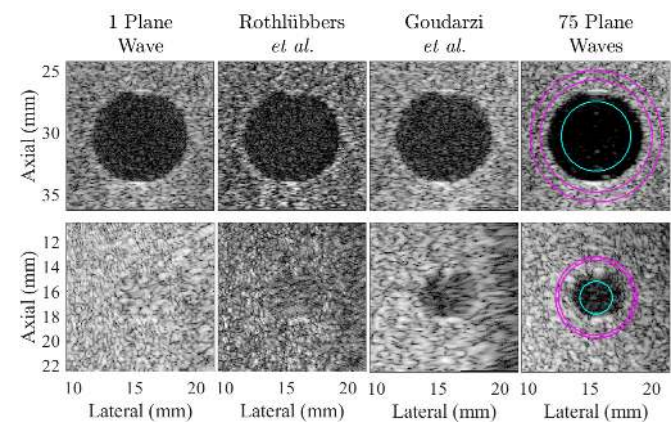


Fig. 3. Example results from the lesion test set, taken from dataset sequences UFL001 (top) and MYO001 (bottom), displayed with 40 dB dynamic range. The ROIs used for image quality metrics are overlaid on the 75 plane wave image, which served as the ground truth.

IV. RESULTS

A. Network Performance Evaluation

1) *Baseline Evaluation*: To ensure that participant submissions from different deep learning frameworks (e.g., TensorFlow and PyTorch) were properly loaded into our evaluation code, we utilized a baseline evaluation on publicly available PICMUS data [21], as shown in Fig. 2. All submissions were confirmed to produce images morphologically similar to the single and 75 plane wave images before proceeding with the evaluation [14].

2) *Lesion Targets*: Fig. 3 shows two lesion examples from dataset sequences UFL001 and MYO001. Each column contains the results produced by the top two submitted networks, with the single and 75 plane transmission results shown for comparison on the far left and far right, respectively. Both submitted networks successfully created the larger lesion shown on the top of Fig. 3 with contrast, CNR, and gCNR

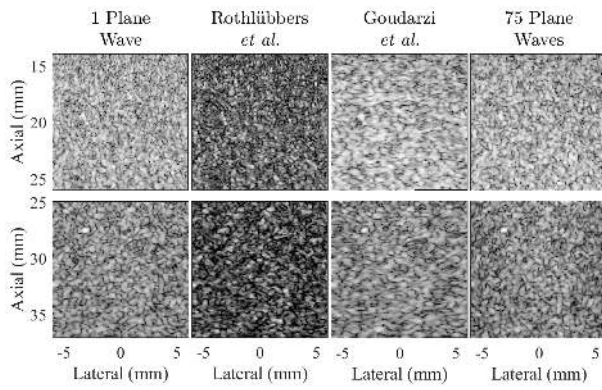


Fig. 4. Example results from the speckle test set, taken from dataset sequences MYO002 (top) and INS016 (bottom), displayed with 40 dB dynamic range.

of -15.29 dB, 1.40, and 0.86, respectively, for the network submitted by Goudarzi *et al.* [29] and -11.13 dB, 0.84, and 0.62, respectively, for the network submitted by Rothluebbers *et al.* [28]. The corresponding contrast, CNR, and gCNR of the single and 75 plane wave results for this lesion were -14.65 dB, 1.38, and 0.84, and -25.84 dB, 1.58, and 0.96, respectively.

For the smaller lesion on the bottom of Fig. 3, the network submitted by Goudarzi *et al.* [29] produced the only successful result for this lesion (contrast, CNR, and gCNR of -12.38 dB, 1.44, and 0.82, respectively), which is remarkable considering that a single plane wave transmission was not sufficient to visualize this lesion with traditional beamforming methods. The corresponding contrast, CNR, and gCNR of the single and 75 plane wave results for this lesion were -1.16 dB, 0.19, and 0.24 and -17.25, 1.35, and 0.88, respectively.

The quantitative results for lesion visibility was measured for a total of 8 ROIs from the following 7 sequences: UFL001, UFL005 (two independent ROIs from this sequence), OSL007, MYO001, MYO004, INS008, and INS021. The mean \pm standard deviation of the contrast, CNR, and gCNR for the 8 ROIs are reported in Table II. No participants achieved greater lesion visibility or detectability than that obtained with 75 plane wave transmissions. Goudarzi *et al.* [29] achieved the best lesion visibility with the least variance overall and also achieved the closest metrics to the 75 plane wave results, while in some cases exceeding the single plane wave result.

3) *Speckle Targets*: Fig. 4 shows examples from two speckle targets taken from dataset sequences MYO002 and INS016. Most participants achieved results that qualitatively resembled speckle texture. Goudarzi *et al.* [29] best achieved the goal of preserving speckle SNR from both single and 75 plane wave transmissions, when measured from 6 ROIs total from the following sequences: UFL004, OSL007, MYO002, EUT003, INS004, and INS016. The mean \pm standard deviation of speckle SNR within these 6 ROIs is reported in Table II.

4) *Point Targets*: Fig. 5 shows example results from the point target evaluation, taken from dataset sequence UFL004. There were a total of 4 ROIs from sequences MYO002, MYO003, UFL002, and UFL004, each containing 3-5 points that were evaluated. The mean \pm standard deviation of the

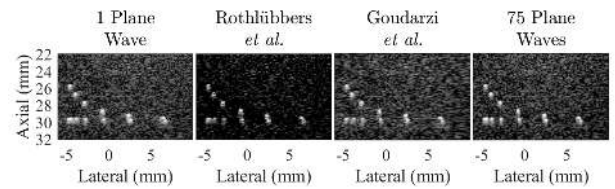


Fig. 5. Example results from the point target test set, taken from dataset sequence UFL004, displayed with 40 dB dynamic range.

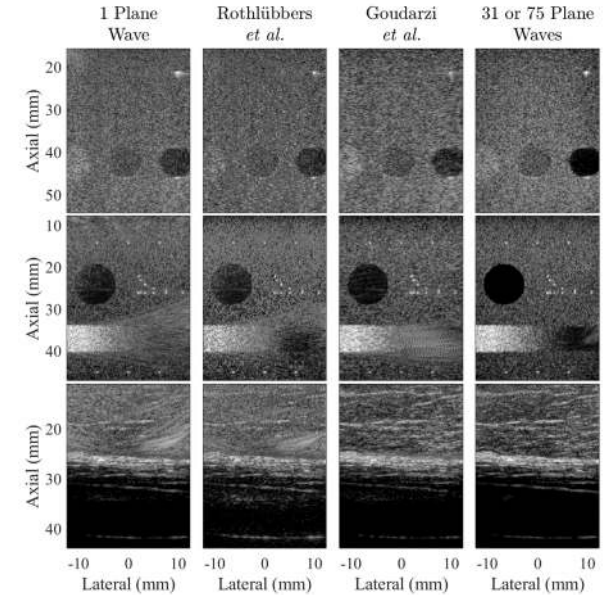


Fig. 6. Example results from the image test set, taken from dataset sequences INS008, OSL010, and TSH002, from top to bottom, respectively, displayed with 60 dB dynamic range. The right column shows images created after 31 (TSH002) or 75 (INS008, OSL010) plane wave transmissions.

lateral and axial resolution of these point targets is reported in Table II as axial and lateral FWHM, respectively. It is remarkable that the networks submitted by Rothluebbers *et al.* [28] and Goudarzi *et al.* [29] achieved better resolution results when compared to standard DAS imaging with both single and 75 plane wave transmissions, considering that the network images were created from channel data acquired after a single plane wave transmission.

5) *Image Targets*: Fig. 6 shows examples from three image targets. These example images were taken from data sequences OSL010, INS008, and TSH002. Network and single plane wave results were compared to the 75 plane wave images, using the global image-to-image metrics described in Section III-C.2 and the 12 images created with data sequences: EUT006, INS006, INS008, INS015, INS019, MYO001, MYO002, MYO004, MYO005, OSL010, UFL002, and TSH002. The corresponding image-to-image comparison results are reported in Table III.

Summarizing the results in Table III, there were no statistically significant differences ($p > 0.05$) when comparing the mean ℓ_1 , ℓ_1 -log, ℓ_2 , and PSNR of the networks submitted by Goudarzi *et al.* [29] and Rothluebbers *et al.* [28]. However, there were statistically significant differences ($p < 0.05$) when comparing the mean ℓ_2 -log and ρ of the networks submitted

TABLE III
SUMMARY OF GLOBAL IMAGE QUALITY COMPARISONS (WITH BOLD INDICATING THE BEST MEAN RESULTS FOR EACH METRIC).

		ℓ_1	ℓ_1 -log	ℓ_2	ℓ_2 -log	ρ	PSNR
CUBDL Task 1 Image Targets	RothlÜbbers <i>et al.</i>	0.05 ± 0.05	0.48 ± 0.13	0.06 ± 0.05	0.71 ± 0.19*	0.83 ± 0.04*	29.03 ± 5.96
	Goudarzi <i>et al.</i>	0.03 ± 0.03	0.42 ± 0.08	0.05 ± 0.04	0.56 ± 0.11*	0.91 ± 0.04*	29.10 ± 6.76
	Single Plane Wave	0.03 ± 0.03	0.39 ± 0.09	0.04 ± 0.04	0.53 ± 0.11	0.93 ± 0.03	30.36 ± 7.43
Post-CUBDL In Vivo Data	RothlÜbbers <i>et al.</i>	0.04 ± 0.01	0.62 ± 0.06*	0.06 ± 0.01*	0.80 ± 0.08*	0.77 ± 0.03*	25.90 ± 2.06
	Goudarzi <i>et al.</i>	0.03 ± 0.01	0.54 ± 0.04*	0.05 ± 0.01*	0.71 ± 0.05*	0.84 ± 0.02*	26.02 ± 1.65
	Single Plane Wave	0.03 ± 0.01	0.61 ± 0.10	0.05 ± 0.01	0.77 ± 0.12	0.84 ± 0.05	26.12 ± 2.40

*indicates statistically significant differences ($p < 0.05$) between RothlÜbbers *et al.* [28] and Goudarzi *et al.* [29]

by Goudarzi *et al.* [29] and RothlÜbbers *et al.* [28]. The corresponding image quality metrics obtained when the single plane wave results were compared to the 75 plane wave results from the same datasets are also reported in Table III for additional comparison. With the exception of ℓ_1 , these single plane wave results produce the best mean values across the 12 image targets included in the CUBDL evaluation dataset (as indicated by the bold text in Table III), where lower values of ℓ_1 , ℓ_1 -log, ℓ_2 , ℓ_2 -log, and higher values of ρ and PSNR indicate better matches with the ground truth 75 plane wave results. Note that for cases with identical mean ℓ_1 and ℓ_2 values in Table III, corresponding values with the lower mean ℓ_1 -log and ℓ_2 -log, respectively, were bolded.

6) Rankings: Based on the first additive term of Eq. 9, the images created with 75 plane wave transmissions achieved the highest rank in a majority of cases (i.e., 1), followed by images created with DAS beamforming after a single plane wave transmission, then the network submitted by Goudarzi *et al.* [29], then the network submitted by RothlÜbbers *et al.* [28]. Specifically, the average ranks for image quality (i.e., the first additive term of Eq. 9) were 1.25, 2.58, 2.67, and 3.58, respectively, for the rank order provided in the preceding sentence. Based on the second additive term of Eq. 9, RothlÜbbers *et al.* [28] submitted a network with significantly less network complexity (i.e., 3,059 parameters) when compared to that of Goudarzi *et al.* [29] (i.e., 2,226,146 parameters), as reported in Table II. Therefore, RothlÜbbers *et al.* [28] received a rank of 3 in the network complexity category, followed by Goudarzi *et al.* [29] receiving a rank of 4, considering that both single and 75 plane wave DAS implementations had 0 trainable parameters for this evaluation.

When combining the two additive terms in Eq. 9 to determine the winner, RothlÜbbers *et al.* [28] and Goudarzi *et al.* [29] achieved final scores of 6.58 and 6.67, respectively, resulting in both being declared by the CUBDL organizers as the challenge winners. This declaration was made because Goudarzi *et al.* [29] achieved both qualitatively and quantitatively high quality images, and at the same time, it was remarkable that RothlÜbbers *et al.* [28] produced a network with significantly low complexity (and generally acceptable image quality with the best lateral and axial resolution overall).

B. Performance with Post-CUBDL In Vivo Data

Fig. 7 shows example *in vivo* breast images from the JHU Post-CUBDL dataset described in Section III-A.2. These

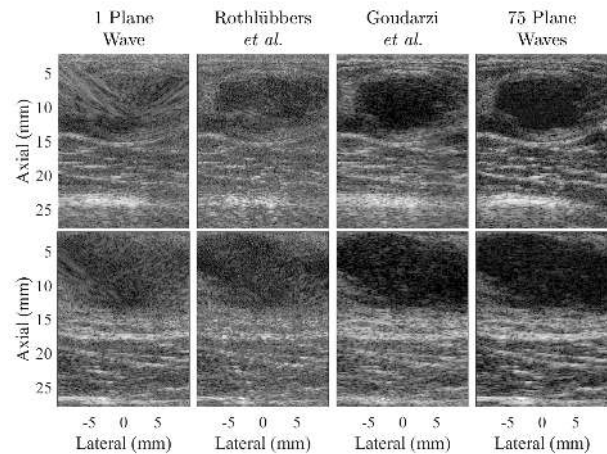


Fig. 7. Example results of *in vivo* breast masses from the Post-CUBDL test set, taken from sequences JHU028 (top) and JHU030 (bottom), displayed with 60 dB dynamic range.

example images were taken from data sequences JHU028 and JHU030. Network and single plane wave results were compared to the 75 plane wave images, using the global image-to-image metrics described in Section III-C.2 and the 11 images created with data sequences JHU024 through JHU034. The quantitative image-to-image comparison results for this dataset are reported in Table III.

The framework developed using the initial CUBDL evaluation test set was able to seamlessly incorporate the JHU Post-CUBDL *in vivo* breast data, which was not included in the initial test set. Remarkably, the submitted networks also generalized to these new data from a different imaging environment. We observed qualitative differences between the *in vivo* breast images produced by the two submitted networks, and the results in Table III demonstrate that the ℓ_2 -log and ρ metrics consistently show statistically significant differences across both datasets (i.e., CUBDL and Post-CUBDL data). Table III also shows that the network submitted by Goudarzi *et al.* [29] produced consistently better quantitative image-to-image comparisons than the network submitted by RothlÜbbers *et al.* [28] across both datasets. In addition, the results obtained when testing this network [29] on the Post-CUBDL *in vivo* dataset were consistently better than results obtained with DAS beamforming of the single plane wave data (as indicated by the bold in Table III). For this Post-CUBDL dataset, the network submitted by RothlÜbbers *et al.* [28] also produced

better qualitative results in some cases (e.g., Fig. 7, sequence JHU028) than the corresponding single plane wave result.

V. DISCUSSION

A. Overview of Challenge Outcomes

The details described in this paper serve the three-fold purpose of: (1) summarizing, comparing, and drawing insights from the top CUBDL submissions; (2) providing a detailed description of the evaluation process for future benchmarking of deep neural networks designed to create ultrasound images; and (3) describing the totality of shared evaluation code and datasets for ease of future reproducibility and replication. The first step to achieving these goals was to ensure that the image reconstruction process offered a fair comparison despite the wide range of test data from multiple groups. Hence, the development of the neural network-based PyTorch DAS beamformer and associated sound speed correction (described in Section III-A.4) were key contributions to enable fair comparisons. While these contributions are the first to implement a differential framework for sound speed correction, there are other solutions that implement DAS within a computational framework capable of automatic differentiation (e.g., PyTorch or TensorFlow) [57]–[59].

The results from these sound speed correction contributions (i.e., Fig. 1) support the importance of including a standardized international dataset for deep learning network development (e.g., training, testing, and evaluation). In particular, a dataset containing incorrect sound speeds and limited acquisition parameter variability may not generalize well to data acquired under different conditions. Sound speed differences within groups (e.g., INS) and between groups (e.g., MYO and UFL) that imaged the same phantom models can be attributed to a combination of ambient environment, the presence of an *ex vivo* tissue layer producing acoustic clutter, and phantom construction differences. Considering that many of the observed phantom variations occurred in the absence of tissue layers and the speckle brightness sound speed correction method was previously validated [36], environmental factors (e.g., ambient temperatures, phantom degradation) are considered to be the primary contributor to these observed differences.

B. Quality of Image Formation with Deep Learning

One of the underlining questions surrounding CUBDL Task 1 was an inquiry regarding the capability of deep learning to create high quality images after a single plane wave transmission. The image quality summary in Table II indicates three insights and capabilities of deep neural networks implemented for beamforming. First, they are capable of preserving speckle SNR. Second, they may be capable of improving resolution. Third, the submitted networks (which created images after only a single 0° plane wave transmission) were capable of producing better qualitative, quantitative, and lesion detectability results than the single plane wave DAS result in some cases (e.g., Fig. 3 sequence MYO001, Figs. 5–7, Tables II and III). It remains to be determined whether the latter two capabilities can be attributed to the choice of target beamformer (i.e., USCF, minimum variance) during training,

as opposed to the function-approximating nature of the deep learning approach itself. In addition, the submitted networks had difficulty obtaining better lesion detectability than the 75 plane wave DAS images. These observations are based on the presented image quality metrics and are supported by the image quality rankings, with associated limitations discussed in more detail in Section V-E. For example, although speckle SNR was quantitatively preserved in some cases (see Table II), it was not always qualitatively preserved (e.g., MYO002 in Fig. 4), when comparing both single plane wave results and network results to the 75 plane wave results.

We also observed that learning a single, intermediate step of the image formation pipeline (as pursued by Goudarzi *et al.* [29] and Rothlübbers *et al.* [28]) represents a more clearly defined transformation for the presented task, as opposed to attempts to learn the entire beamforming process (i.e., the approach taken by [19], [27], which suffered from overfitting to the training data, as shown in the presentation of all challenge results [14]). To briefly summarize for the context of this manuscript, overfitting manifested as an inability of the submitted networks to detect point targets in the unseen test data, recreate lesions from the unseen test data, or replicate the gradation from light to dark shown in Fig. 6 (sequence OSL010). Instead, the images looked more like the learned tissue texture or lesions in the training images in most cases. The training datasets curated by the respective authors of these two runner-up submissions contained similar data to each corresponding testing dataset, and the ability of the resulting networks to produce acceptable results on these similar data are evident in the papers describing the associated submissions [19], [27]. These two networks were also able to successfully reproduce the results shown in Fig. 2, as presented in [14], likely because the PICMUS data were included in the training sets of both networks. These observations highlight successes that can be achieved when training and testing sets are similar, with a discussion of the overfitting implications available in Section V-D in the context of future recommendations.

C. Speed of Image Formation

It is promising that the improvements to image quality were obtained with network complexity levels that indicate a possibility for improved speed compared to traditional implementations of advanced beamforming approaches. Although the CUBDL organizers did not specify which parts of the image formation task had to be learned, participants were aware that they would be evaluated based on the number of trainable parameters within submitted networks. Participants therefore had the freedom to decide whether they used a network to replace the delay step, the sum step, both steps, a post-processing filter step, etc. This freedom somewhat complicated the network complexity evaluation, considering that a neural network has the potential to outperform deterministic DAS at the cost of adding parameters that need to be trained. If a network replaces both “delay” and “sum”, it might be more complex than a network that replaces just the “sum”, but it may also rely on fewer assumptions and thus would have greater potential to give better results. This tradeoff was considered to

be captured sufficiently by counting the number of trainable parameters.

It is possible that an additional dimension of complexity could have been included by adding a metric for “number of processing components replaced”. However, this addition is not trivial to implement, considering the wide range of possible steps outside of basic DAS beamforming. While different network architectures with the same number of parameters may have different inference speeds, oftentimes this difference in speed is due to nuanced hardware- and software-specific optimizations. It is also possible that we could have estimated the number of floating point operations (FLOPs), but there are multiple methods and implementations for estimation with no clear standard. These considerations point to the additional importance of learning from these CUBDL challenge results to produce updated guidelines if a similar undertaking is attempted in the future.

D. Future Recommendations

The observations summarized in Section V-B highlight the importance of a truly blind test set to detect and prevent possible overfitting, which is a secondary outcome of the CUBDL challenge (i.e., the newly available database [16] and evaluation code [15] being released with the publication of this manuscript). Regarding the choice not to provide training data for CUBDL participants, the intent was to create a challenge that represented the current state of ultrasound imaging research. In particular, prior to the dataset contribution described in this manuscript, there was no previously curated standard training set specifically catered to deep learning tasks for ultrasound image formation. Instead, the CUBDL organizers encouraged participants to make intellectual contributions on both the choice of architecture and training data, rather than to find a single optimal architecture for a given training dataset.

Now that the challenge is completed, we propose the use of the datasets described in Sections III-A.1 and III-A.2 as testing data (with caution to avoid overfitting if the dataset described in Section III-A.3 is also used for training). Similarly, we propose the use of the top CUBDL challenge submissions as benchmarks for future work in this research domain. For example, related work on the topic of CUBDL Task 1 published after the close of the challenge [60]–[64] can potentially be reevaluated and compared using the CUBDL data [16] and code [15] released with this publication, with no alterations to network training weights and with attention to the overfitting challenges experienced by the runners-up, particularly when considering that some these methods were similarly trained and tested with PICMUS data. We are essentially challenging the community to achieve better results than the CUBDL submissions and to make more headway toward explaining why results are better based on the open research questions articulated in this discussion of challenge results. We also welcome new contributions to the field of ultrasound beamforming with deep learning (and possibly beamforming without deep learning) based on new ideas conceived while reading this manuscript and while working with our open source data and code. The shared datasets and code provide a

major step toward making meaningful comparisons in future work.

E. Limitations and Additional Considerations

Three possible factors that may be viewed as limitations of administering CUBDL include the novelty of the sound speed correction approach, the subjectivity of decisions surrounding the ranking method (which is arguably a limitation of any challenge [65]), and the diversity of the datasets.

First, sound speed optimization is not widely utilized, and its implementation in a deep learning framework (PyTorch) may be considered novel and thus inappropriate to introduce in a challenge. The decision to include sound speed correction was three-fold: (1) correction was critically needed to enable fair contrast and resolution evaluations in the challenge (see Fig. 1b); (2) the sound speed correction algorithm itself was based on a well-established criterion [35] (see Section III-A.4); and (3) the specific implementation of the algorithm (e.g., traditional brute-force search vs. PyTorch optimization) does not affect the final result. Thus, the PyTorch-optimized sound speeds were included in the challenge. A potential limitation of this work is that further validation of the sound speed correction was considered out of scope and thus not performed. However, we note that this correction was intended solely as a coarse improvement over assuming 1540 m/s rather than as a perfect sound speed correction, which cannot be achieved by any assumed global sound speed due to the heterogeneity of real targets.

Second, CUBDL placed an equal weighting on the objectives of image quality and network complexity, which may be considered arbitrary and subjective. Indeed, establishing absolute rankings in any multi-objective task is non-trivial because it is possible to be optimal in one metric but suboptimal in another, i.e., to be “Pareto-optimal”. In such a system (known as a *partial order*), the only way for one method to be definitively superior is to dominate all others in all categories. Although a worthy goal, such an optimum often does not exist and thus cannot be relied upon for challenge administration. Furthermore, it is important to recognize that each image quality metric alone measures a narrow aspect of image quality, such that optimality in that individual metric may not correspond to perceived image quality. For example, speckle SNR measures only first-order statistics and does not capture second-order statistics of speckle structures, making it a poor indicator of image quality alone; however, the ℓ_1 and ℓ_2 losses provide complementary spatial information. To reliably obtain a final rank (a *total order*) from multiple independent categories, one must necessarily apply subjective opinions as to the importance and weighting of each category.

Our chosen approach (detailed in Section III-D) effectively placed less weight on any individual image quality metric and greater weight on overall network complexity. The CUBDL organizers made a conscious decision to emphasize network complexity as a distinguishing factor in anticipation of numerous submissions with similar imaging performance, considering that ultrasound beamforming needs to be real-time for practical application and implementation. It is possible that a

low-complexity network producing poor image quality would have achieved a good score with the chosen approach. In particular, according to the image quality rankings reported in Section IV-A.6, the current approach favored single plane wave DAS over the submitted networks due to a combination of the better rank performance of the global metrics (summarized in Table III for Task 1 data) and the absence of trainable parameters with traditional DAS beamforming (despite the better performance of the networks over single plane wave DAS images with regard to local metrics, as summarized in Table II). Other weightings are equally subjective, thus equally valid, and may result in different final rankings. The CUBDL organizers are making all data and evaluation scripts available with the publication of this manuscript, leaving room for others to implement alternative analyses if desired.

Finally, while the diversity of the test datasets is viewed as a strength with regard to assessing network generalizability (as discussed in Section V-A) and with regard to detecting possible overfitting to training data (as discussed in Section V-D), this diversity may have also been viewed as a barrier for entry into the challenge. In particular, variations in multiple parameters that are routinely modified to achieve a desired ultrasound image were advertised (e.g., variations in transducers, ultrasound systems, system operators, plane wave angles, center frequencies, sampling frequencies, bandwidths, transducer properties, image depths, and imaging targets), with example images provided in the CUBDL Data Guide [14] and replicated in [20]. Although the PICMUS data were advertised and available, the PICMUS data did not contain this wide range of varying parameters. Concerns regarding limited knowledge of either beamforming or deep learning may have also been a barrier to entry. However, the CUBDL participants reported experience levels with beamforming and deep learning that ranged from novice to expert [14], [20].

VI. CONCLUSION

This manuscript summarizes the results of the CUBDL challenge, as well as the detailed evaluation process implemented by the CUBDL organizers and associated insights gained from the evaluation process and challenge results. Evaluation was further analyzed independently, and the associated evaluation code and datasets are newly released with this publication. The open datasets include the CUBDL test data, additional *in vivo* breast data included after the close of the challenge, and a subset of internationally crowd-sourced data that were not used for evaluation, but may potentially be used for future network training and comparison to the results presented within this manuscript. The complete dataset includes 576 image acquisition sequences and represents the largest known open international database of ultrasound channel data. We are releasing this combination of CUBDL results, evaluation code, and open datasets to our community in efforts to help standardize and accelerate research at the intersection of ultrasound beamforming and deep learning. We additionally propose the use of the top CUBDL challenge submissions as benchmarks for future work in this research domain, and we share the totality of released resources to enable meaningful comparisons of future methods.

ACKNOWLEDGMENTS

We thank our sponsors (Verasonics, Inc., IEEE, and IUS) for their generous support of CUBDL, as well as the many individuals and groups who contributed data to make this challenge possible. The following 15 individuals provided contributions to the open CUBDL-Related Datasets from 7 institutions worldwide: Jiaqi Huang, Alicyn Wiacek, and Muyinatu Bell from Johns Hopkins University, USA; Ping Gong and Shigao Chen from Mayo Clinic, USA; Alessandro Ramalli and Piero Tortoli from University of Florence, Italy; Ben Luijten and Massimo Mischi from Eindhoven University of Technology, Netherlands; Ole Marius Hoel Rindal from University of Oslo, Norway; Vincent Perrot and Hervé Liebgott from Creatis, University of Lyon, INSA, France; Xi Zhang and Jiawen Luo from Tsinghua University, China; and Olivier Bernard created data sequence OSL010. The authors additionally thank breast radiologists Eniola Oluyemi, MD and Emily Ambinder, MD from Johns Hopkins Medicine for their assistance with the Post-CUBDL *in vivo* breast data acquisitions. These individuals are listed as authors of our internationally crowd-sourced database of ultrasound channel data [16], ordered by date of receipt.

APPENDIX

This Appendix presents the 18 ROIs used to calculate the local image quality metrics (Fig. 8), followed by seven tables describing contributed ultrasound channel data (Tables IV-X).

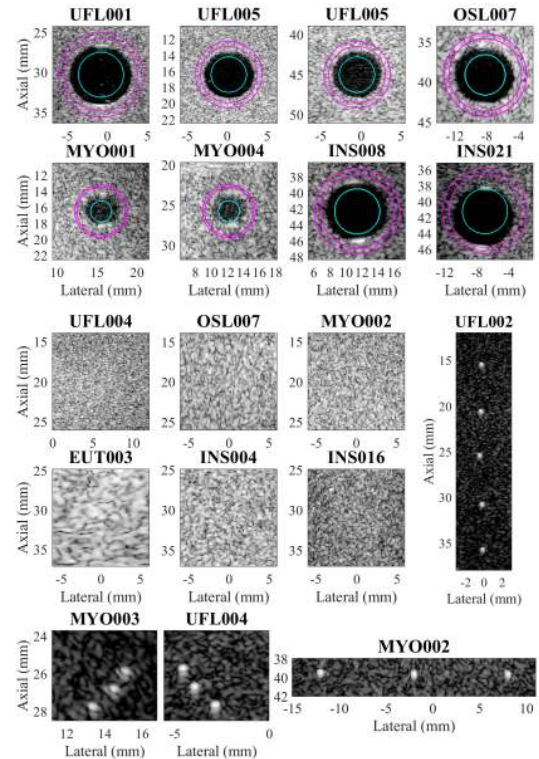


Fig. 8. Images created with 75 plane wave transmissions showing the ROIs used to measure contrast, CNR, gCNR (where ROI₁ is indicated by the inner circle and ROI₂ is indicated by the concentric outer circles), speckle SNR, and point target FWHM. These images are displayed with 40 dB dynamic range.

TABLE IV
PHANTOM AND SIMULATED TEST DATA FOR CUBDL TASK 1

Data Info			Acquisition Info						Phantom Info					
Sequence #	Trans-mission type	# of angles	Plane wave angle range	US scanner	Transducer	Center Frequency [MHz]	Sampling Frequency [MHz]	Bandwidth [MHz]	Aperture Width [mm]	Element Width [mm]	Pitch [mm]	Image Depth [mm]	Targets Included	Ref.
MYO001	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L11-4v	6.25	28.96	6.78	38.4	0.27	0.3	63.8	wire targets and inclusions	-
MYO002	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L11-4v	6.25	28.96	6.78	38.4	0.27	0.3	63.8	wire targets and inclusions	-
MYO003	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L11-4v	6.25	28.96	6.78	38.4	0.27	0.3	63.8	wire targets and inclusions	-
MYO004	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L11-4v	6.25	28.96	6.78	38.4	0.27	0.3	63.8	wire targets, inclusions, and clutter	-
MYO005	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L11-4v	6.25	28.96	6.78	38.4	0.27	0.3	63.8	wire targets, inclusions, and clutter	-
UFL001	Plane Wave	75	[-15, 15]	ULA-OP256	LA533 (Esaote)	8	78.125	4.9	31.36	0.215	0.245	50	Hypoechoic target, grey scale target and wire targets	-
UFL002	Plane Wave	75	[-15, 15]	ULA-OP256	LA533 (Esaote)	8	78.125	4.9	31.36	0.215	0.245	50	wire targets, grey scale targets	-
UFL004	Plane Wave	75	[-15, 15]	ULA-OP256	LA533 (Esaote)	8	78.125	4.9	31.36	0.215	0.245	50	Wire targets	-
UFL005	Plane Wave	75	[-15, 15]	ULA-OP256	LA533 (Esaote)	8	78.125	4.9	31.36	0.215	0.245	50	Hypoechoic targets	-
EUT003	Plane Wave	75	[-16, 16]	Verasonics Vantage 128	Phillips S5-1	3.125	12.5	4	20.3	0.25	0.254	100	Wire targets	-
EUT006	Plane Wave	75	[-16, 16]	Verasonics Vantage 128	Phillips S5-1	3.125	12.5	4	20.3	0.25	0.254	100	Wire targets	-
INS004	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Stiff inclusions	-
INS006	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Cysts	-
INS008	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Cysts and wire	-
INS015	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Vessel and wires with flow circulation	-
INS016	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Stiff inclusions	-
INS019	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Cysts	-
INS021	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Cysts + wire	-
OSL007	Plane Wave	75	[-16, 16]	Verasonics Vantage 256 Simulation	L7-4	5.208333	20.866720	3.1248	38.100005	0.25	0.298	50	Cysts	-
OSL010	Plane Wave	75	[-16, 16]	Field II	N/A	5.13	20.8	-	38.1	-	0.3	50	Dynamic range phantom	[18]

TABLE V
IN VIVO TEST DATA FOR CUBDL TASK 1

Data Info			Acquisition Info						In Vivo Info						
Sequence #	Trans-mission Type	Total # of plane waves	Angle range	US scanner	Transducer	Center Frequency [MHz]	Sampling Frequency [MHz]	Bandwidth [MHz]	Aperture Width [mm]	Element Width [mm]	Pitch [mm]	Image Depth [mm]	Data from	Organ	Ref.
TSH002	Plane Wave	31	[-15,15]	Verasonics Vantage 256	L10-5	7.5	6.25	5	38.37	0.27	0.3	40	Volunteer	Brachioradialis	[17]

TABLE VI
IN VIVO DATA ACQUIRED WITH PLANE WAVE TRANSMISSIONS FOR THE POST-CUBDL ANALYSIS (AVAILABLE AS PART OF THE ENTIRE OPEN DATASET)

Sequence #	Data Info			Acquisition Info						In Vivo Info					
	Trans-mission Type	Total # of plane waves	Angle range	US scanner	Trans-ducer	Center Frequency [MHz]	Sampling Frequency [MHz]	Bandwidth [MHz]	Aperture Width [mm]	Element Width [mm]	Pitch [mm]	Image Depth [mm]	Data from	Organ	Ref.
JHU024	Plane Wave	73	[-8,8]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU025	Plane Wave	73	[-8,8]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU026	Plane Wave	73	[-8,8]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU027	Plane Wave	73	[-8,8]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU028	Plane Wave	75	[-16,16]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU029	Plane Wave	75	[-16,16]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU030	Plane Wave	73	[-8,8]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU031	Plane Wave	75	[-16,16]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU032	Plane Wave	75	[-16,16]	Alpionion ECUBE12-R	L8-17	12.5	40	9	25.6	0.11	0.2	30	Patient	Breast	[19]
JHU033	Plane Wave	75	[-16,16]	Alpionion ECUBE12-R	L3-8	5.5	40	5	38.4	0.24	0.3	30	Patient	Breast	[19]
JHU034	Plane Wave	75	[-16,16]	Alpionion ECUBE12-R	L3-8	5.5	40	5	38.4	0.24	0.3	30	Patient	Breast	[19]

TABLE VII
REMAINING IN VIVO DATA ACQUIRED WITH PLANE WAVE TRANSMISSIONS (NOT USED FOR THE CUBDL TASK 1 EVALUATIONS, BUT AVAILABLE AS PART OF THE ENTIRE OPEN DATASET)

Sequence #	Data Info			Acquisition Info						In Vivo Info					
	Trans-mission Type	Total # of plane waves	Angle range	US scanner	Trans-ducer	Center Frequency [MHz]	Sampling Frequency [MHz]	Bandwidth [MHz]	Aperture Width [mm]	Element Width [mm]	Pitch [mm]	Image Depth [mm]	Data from	Organ	Ref.
TSH003-TSH501	Plane Wave	31	[-15,15]	Verasimics Vantage 256	L10-5	7.5	6.25	5	38.37	0.27	0.3	40	Volunteer	Brachioradialis	[17]

TABLE VIII
REMAINING PHANTOM DATA ACQUIRED WITH PLANE WAVE TRANSMISSIONS (NOT USED FOR THE CUBDL TASK 1 EVALUATIONS, BUT AVAILABLE AS PART OF THE ENTIRE OPEN DATASET)

Sequence #	Data Info			Acquisition Info							Phantom Info		
	Trans-mission type	# of angles	Plane wave angle range	US scanner	Transducer	Center Frequency [MHz]	Sampling Frequency [MHz]	Bandwidth [MHz]	Aperture Width [mm]	Element Width [mm]	Pitch [mm]	Image Depth [mm]	Targets Included
MYO006	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L11-4v	6.25	28.96	6.78	38.4	0.27	0.3	63.8	Wire targets, inclusions, and clutter
UFL003	Plane Wave	75	[-15, 15]	ULA-OP256	LA533 (Esate)	8	78.125	4.9	31.36	0.215	0.245	50	Wire targets and hyperechoic target
EUT001	Plane Wave	75	[-16, 16]	Verasonics Vantage 128	Philips SS-1	3.125	12.5	4	20.3	0.25	0.254	100	Wire targets
EUT002	Plane Wave	75	[-16, 16]	Verasonics Vantage 128	Philips SS-1	3.125	12.5	4	20.3	0.25	0.254	100	Wire targets
EUT004	Plane Wave	75	[-16, 16]	Verasonics Vantage 128	Philips SS-1	3.125	12.5	4	20.3	0.25	0.254	100	Wire targets
EUT005	Plane Wave	75	[-16, 16]	Verasonics Vantage 128	Philips SS-1	3.125	12.5	4	20.3	0.25	0.254	100	Wire targets
INS001	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Vessel and wires
INS002	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Vessel and wires with flow circulation
INS003	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Homogeneous
INS005	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Wires
INS007	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Wires
INS009	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Inclusions
INS010	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Inclusions
INS011	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Brain structure
INS012	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Brain structure
INS013	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208	20.833	3.1248	37.846	0.25	0.298	56.7	Vessel
INS014	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Vessel and wires
INS017	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Homogeneous
INS018	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Wires
INS020	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Wires
INS022	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Inclusions
INS023	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Inclusions
INS024	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Brain structure
INS025	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Brain structure
INS026	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L12-5	7.813	31.25	4.6878	24.8	0.1703	0.1953	56.7	Vessel
OSL002	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208333	20.866720	3.1248	38.100000	0.25	0.298	50	Wires
OSL003	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208333	20.866720	3.1248	38.100001	0.25	0.298	50	Wires and cysts
OSL004	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208333	20.866720	3.1248	38.100002	0.25	0.298	50	Wires and cysts
OSL005	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208333	20.866720	3.1248	38.100003	0.25	0.298	50	Cysts
OSL006	Plane Wave	75	[-16, 16]	Verasonics Vantage 256	L7-4	5.208333	20.866720	3.1248	38.100004	0.25	0.298	50	Cysts

TABLE IX
PHANTOM DATA AND SIMULATED DATA ACQUIRED WITH FOCUSED TRANSMISSIONS (CROWD-SOURCED FOR CUBDL TASK 3 AND AVAILABLE AS PART OF THE ENTIRE OPEN DATASET)

Sequence #	Data Info				Acquisition Info							Phantom Info			
	Trans- mission type	# of steering angles	Steering angle range	Focal Depth [mm]	US scanner	Trans- ducer	Center Frequency [MHz]	Sampling Frequency [MHz]	Bandwidth [MHz]	Aperture Width [mm]	Element Width [mm]	Pitch [mm]	Image Depth [mm]	Targets Included	Ref.
OSL001	Focused	-	-	22	Simulation Field II	N/A	5.13	100	-	38.1	-	0.3	50	Dynamic range phantom	[54]
OSL015	Focused	-	-	50	Verasonics Vantage 256	L11-5	5.00	20.42	3.12	38.10	0.25	0.298	50	Cyst and point targets	[54]
JHU019	Focused	128	[-45,45]	50	Verasonics Vantage 128	P4-2v	2.97	11.90	3	18.90	0.295	0.3	50	Point targets	-
JHU020	Focused	128	[-45,45]	60	Verasonics Vantage 128	P4-2v	2.97	11.90	3	18.90	0.295	0.3	60	Cyst and point targets	-
JHU021	Focused	128	[-45,45]	85	Verasonics Vantage 128	P4-2v	2.97	11.90	3	18.90	0.295	0.3	85	Cyst and point targets	-
JHU022	Focused	128	[-45,45]	73	Verasonics Vantage 128	P4-2v	2.97	11.90	3	18.90	0.295	0.3	73	Cyst	-
JHU023	Focused	128	[-45,45]	36	Verasonics Vantage 128	P4-2v	2.97	11.904762	3	18.90	0.295	0.3	36	Cyst and point targets	-

TABLE X
IN VIVO DATA ACQUIRED WITH FOCUSED TRANSMISSIONS (CROWD-SOURCED FOR CUBDL TASK 3 AND AVAILABLE AS PART OF THE ENTIRE OPEN DATASET)

Sequence #	Data Info			Acquisition Info							In Vivo Info					
	Trans- mission type	# of steering angles	Steering angle range	Focal Depth [mm]	US scanner	Trans- ducer	Center Frequency [MHz]	Sampling Frequency [MHz]	Bandwidth [MHz]	Aperture Width [mm]	Element Width [mm]	Pitch [mm]	Image Depth [mm]	Data from	Organ	Ref.
JHU001	Focused	-	-	20	Alpington ECUBE12-R	L3-8	5.5	40	5	38.1	0.24	0.3	40	Patient	Breast	[30]
JHU002	Focused	-	-	20	Alpington ECUBE12-R	L8-17	12.5	40	9	25.4	0.11	0.2	40	Patient	Breast	[30]
OSL008	Focused	-	-	22	Verasonics Vantage 256	L7-4	5.2	20.8	3.1248	37.8	0.25	0.298	40	Volunteer	Carotid	[53]
OSL009	Focused	-	-	22	Verasonics Vantage 256	L7-4	5.2	20.8	3.1248	37.8	0.25	0.298	40	Volunteer	Carotid	[53]
OSL011	Focused	101	[-37.5, 37.5]	67	Verasonics Vantage 256	P4-2	3.0	11.9	3	18.9	0.295	0.3	120	Volunteer	Heart	[31]
OSL012	Focused	101	[-37.5, 37.5]	52	Verasonics Vantage 256	P7-4	3.0	11.9	3	18.9	0.295	0.3	120	Volunteer	Heart	[31]
OSL013	Focused	101	[-37.5, 37.5]	52	Verasonics Vantage 256	P4-2	3.0	11.9	3	18.9	0.295	0.3	120	Volunteer	Heart	[31]
OSL014	Focused	101	[-37.5, 37.5]	52	Verasonics Vantage 256	P4-2	3.0	11.9	3	18.9	0.295	0.3	120	Volunteer	Heart	[31]

REFERENCES

- [1] S. Liu, Y. Wang, X. Yang, B. Lei, L. Liu, S. X. Li, D. Ni, and T. Wang, "Deep learning in medical ultrasound analysis: a review," *Engineering*, vol. 5, no. 2, pp. 261–275, 2019.
- [2] R. J. van Sloun, R. Cohen, and Y. C. Eldar, "Deep learning in ultrasound imaging," *Proceedings of the IEEE*, vol. 108, no. 1, pp. 11–29, 2019.
- [3] C. Shan, S. Wu, and J. A. Schnabel, "Guest editorial: Deep learning in ultrasound imaging," *IEEE Journal of Biomedical and Health Informatics*, vol. 24, no. 4, pp. 929–930, 2020.
- [4] M. Mischi, M. A. L. Bell, R. J. van Sloun, and Y. C. Eldar, "Deep learning in medical ultrasound—formation to image analysis," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 67, no. 12, pp. 2477–2480, 2020.
- [5] A. A. Nair, T. D. Tran, A. Reiter, and M. A. L. Bell, "A deep learning based alternative to beamforming ultrasound images," in *2018 IEEE International Conference on Acoustics, Speech and Signal Processing (ICASSP)*. IEEE, 2018, pp. 3359–3363.
- [6] M. Bhatt, A. A. Nair, K. M. Kempfski, and M. A. L. Bell, "Multi-task learning for ultrasound image formation and segmentation directly from raw in vivo data," in *2020 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2020, pp. 1–4.
- [7] J. Tierney, A. Luchies, M. Berger, and B. Byram, "Evaluating input domain and model selection for deep network ultrasound beamforming," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, 2021.
- [8] A. Wiacek, E. González, and M. A. L. Bell, "CohereNet: A Deep Learning Architecture for Ultrasound Spatial Correlation Estimation and Coherence-Based Beamforming," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 67, no. 12, pp. 2574–2583, 2020.
- [9] B. Luijten, R. Cohen, F. J. De Bruijn, H. A. Schmeitz, M. Mischi, Y. C. Eldar, and R. J. Van Sloun, "Adaptive ultrasound beamforming using deep learning," *IEEE Transactions on Medical Imaging*, vol. 39, no. 12, pp. 3967–3978, 2020.
- [10] S. Khan, J. Huh, and J. C. Ye, "Adaptive and compressive beamforming using deep learning for medical ultrasound," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 67, no. 8, pp. 1558–1572, 2020.
- [11] D. Hyun, L. L. Brickson, K. T. Looby, and J. J. Dahl, "Beamforming and speckle reduction using neural networks," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 66, no. 5, pp. 898–910, 2019.
- [12] O. Russakovsky, J. Deng, H. Su, J. Krause, S. Satheesh, S. Ma, Z. Huang, A. Karpathy, A. Khosla, M. Bernstein *et al.*, "Imagenet large scale visual recognition challenge," *International Journal of Computer Vision*, vol. 115, no. 3, pp. 211–252, 2015.
- [13] K. Murphy, B. Van Ginneken, J. M. Reinhardt, S. Kabus, K. Ding, X. Deng, K. Cao, K. Du, G. E. Christensen, V. Garcia *et al.*, "Evaluation of registration methods on thoracic CT: the EMPIRE10 challenge," *IEEE Transactions on Medical Imaging*, vol. 30, no. 11, pp. 1901–1920, 2011.
- [14] M. A. L. Bell, J. Huang, D. Hyun, Y. Eldar, R. van Sloun, and M. Mischi, "Challenge on Ultrasound Beamforming with Deep Learning (CUBDL)." [Online]. Available: <https://cubdl.jhu.edu/>
- [15] [Online]. Available: <https://gitlab.com/dongwoon.hyun/cubdl>
- [16] M. A. L. Bell, J. Huang, A. Wiacek, P. Gong, S. Chen, A. Ramalli, P. Tortoli, B. Luijten, M. Mischi, O. M. H. Rindal, V. Perrot, H. Liebgott, X. Zhang, J. Luo, O. Bernard, E. Oluyemi, and E. Ambinder, "Challenge on Ultrasound Beamforming with Deep Learning (CUBDL) Datasets." [Online]. Available: <http://dx.doi.org/10.21227/f0hn-8f92>
- [17] X. Zhang, J. Li, Q. He, H. Zhang, and J. Luo, "High-quality reconstruction of plane-wave imaging using generative adversarial network," in *2018 IEEE International Ultrasonics Symposium (IUS)*, Oct 2018, pp. 1–4.
- [18] PICMUS, "Plane-wave imaging evaluation framework for medical ultrasound," 2020. [Online]. Available: <https://www.creatis-insa-lyon.fr/EvaluationPlatform/picmus/>
- [19] Z. Li, A. Wiacek, and M. A. L. Bell, "Beamforming with deep learning from single plane wave RF data," in *2020 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2020, pp. 1–4.
- [20] M. A. L. Bell, J. Huang, D. Hyun, Y. Eldar, R. van Sloun, and M. Mischi, "Challenge on Ultrasound Beamforming with Deep Learning (CUBDL)," in *2020 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2020.
- [21] H. Liebgott, A. Rodriguez-Molares, F. Cervenansky, J. A. Jensen, and O. Bernard, "Plane-wave imaging challenge in medical ultrasound," in *2016 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2016, pp. 1–4.
- [22] E. Dong, H. Du, and L. Gardner, "An interactive web-based dashboard to track covid-19 in real time," *The Lancet infectious diseases*, vol. 20, no. 5, pp. 533–534, 2020.
- [23] A. A. Nair, K. N. Washington, T. D. Tran, A. Reiter, and M. A. L. Bell, "Deep learning to obtain simultaneous image and segmentation outputs from a single input of raw ultrasound channel data," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, 2020.
- [24] A. G. Howard, M. Zhu, B. Chen, D. Kalenichenko, W. Wang, T. Weyand, M. Andreetto, and H. Adam, "Mobilenets: Efficient convolutional neural networks for mobile vision applications," *arXiv preprint arXiv:1704.04861*, 2017.
- [25] F. N. Iandola, S. Han, M. W. Moskewicz, K. Ashraf, W. J. Dally, and K. Keutzer, "SqueezeNet: AlexNet-level accuracy with 50x fewer parameters and <0.5 MB model size," *arXiv preprint arXiv:1602.07360*, 2016.
- [26] C. Kawatsu, F. Koss, A. Gillies, A. Zhao, J. Crossman, B. Purman, D. Stone, and D. Dahn, "Gesture recognition for robotic control using deep learning," in *NDIA Ground Vehicle Systems Engineering and Technology Symposium*, 2017.
- [27] Y. Wang, K. Kempfski, J. U. Kang, and M. A. L. Bell, "A conditional adversarial network for single plane wave beamforming," in *2020 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2020, pp. 1–4.
- [28] S. Rothlübbers, H. Strohm, K. Eickel, J. Jenne, V. Kuhlen, D. Sinden, and M. Günther, "Improving image quality of single plane wave ultrasound via deep learning based channel compounding," in *2020 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2020, pp. 1–4.
- [29] S. Goudarzi, A. Asif, and H. Rivaz, "Ultrasound beamforming using mobilenetv2," in *2020 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2020, pp. 1–4.
- [30] A. Wiacek, O. M. H. Rindal, E. Falomo, K. Myers, K. Fabrega-Foster, S. Harvey, and M. A. Lediju Bell, "Robust short-lag spatial coherence imaging of breast ultrasound data: Initial clinical results," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 66, no. 3, pp. 527–540, March 2019.
- [31] O. M. H. Rindal, S. Aakhus, S. Holm, and A. Austeng, "Hypothesis of improved visualization of microstructures in the interventricular septum with ultrasound and adaptive beamforming," *Ultrasound in Medicine & Biology*, vol. 43, no. 10, pp. 2494 – 2499, 2017.
- [32] F. A. Duck, "Acoustic properties of tissue at ultrasonic frequencies," *Physical properties of tissue: A comprehensive reference book*, pp. 73–124, 1990.
- [33] B. Park, A. Whittaker, R. Miller, and D. Hale, "Predicting intramuscular fat in beef longissimus muscle from speed of sound," *Journal of Animal Science*, vol. 72, no. 1, pp. 109–116, 1994.
- [34] G. Ghoshal, A. C. Luchies, J. P. Blue, and M. L. Oelze, "Temperature dependent ultrasonic characterization of biological media," *The Journal of the Acoustical Society of America*, vol. 130, no. 4, pp. 2203–2211, 2011.
- [35] L. Nock, G. E. Trahey, and S. W. Smith, "Phase aberration correction in medical ultrasound using speckle brightness as a quality factor," *The Journal of the Acoustical Society of America*, vol. 85, no. 5, pp. 1819–1833, 1989.
- [36] M. Anderson, M. McKeag, and G. Trahey, "The impact of sound speed errors on medical ultrasound imaging," *The Journal of the Acoustical Society of America*, vol. 107, no. 6, pp. 3540–3548, 2000.
- [37] R. Mallart and M. Fink, "Adaptive focusing in scattering media through sound-speed inhomogeneities: The van cittert zernike approach and focusing criterion," *The Journal of the Acoustical Society of America*, vol. 96, no. 6, pp. 3721–3732, 1994.
- [38] S. Flax and M. O'Donnell, "Phase-aberration correction using signals from point reflectors and diffuse scatterers: Basic principles," *IEEE transactions on ultrasonics, ferroelectrics, and frequency control*, vol. 35, no. 6, pp. 758–767, 1988.
- [39] M. E. Anderson and G. E. Trahey, "The direct estimation of sound speed using pulse-echo ultrasound," *The Journal of the Acoustical Society of America*, vol. 104, no. 5, pp. 3099–3106, 1998.
- [40] M. Imbault, A. Faccinotto, B.-F. Osmanski, A. Tissier, T. Deffieux, J.-L. Gennisson, V. Vilgrain, and M. Tanter, "Robust sound speed estimation for ultrasound-based hepatic steatosis assessment," *Physics in Medicine & Biology*, vol. 62, no. 9, p. 3582, 2017.
- [41] V. Perrot, M. Polichetti, F. Varray, and D. Garcia, "So you think you can das? a viewpoint on delay-and-sum beamforming," *Ultrasonics*, vol. 111, p. 106309, 2021.
- [42] A. Paszke, S. Gross, F. Massa, A. Lerer, J. Bradbury, G. Chanan, T. Killeen, Z. Lin, N. Gimelshein, L. Antiga, A. Desmaison,

A. Kopf, E. Yang, Z. DeVito, M. Raison, A. Tejani, S. Chilamkurthy, B. Steiner, L. Fang, J. Bai, and S. Chintala, "Pytorch: An imperative style, high-performance deep learning library," in *Advances in Neural Information Processing Systems 32*, H. Wallach, R. Larochelle, A. Beygelzimer, F. d'Alché-Buc, E. Fox, and R. Garnett, Eds. Curran Associates, Inc., 2019, pp. 8024–8035. [Online]. Available: <http://papers.neurips.cc/paper/9015-pytorch-an-imperative-style-high-performance-deep-learning-library.pdf>

[43] J. Jensen, "Field: A program for simulating ultrasound systems," *Medical & Biological Engineering & Computing*, vol. 34, no. sup. 1, pp. 351–353, 1997.

[44] J. A. Jensen and N. B. Svendsen, "Calculation of pressure fields from arbitrarily shaped, apodized, and excited ultrasound transducers," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 39, no. 2, pp. 262–267, March 1992.

[45] C. Yang, Y. Jiao, T. Jiang, Y. Xu, and Y. Cui, "A united sign coherence factor beamformer for coherent plane-wave compounding with improved contrast," *Applied Sciences*, vol. 10, no. 7, p. 2250, 2020.

[46] Z. Wang, E. P. Simoncelli, and A. C. Bovik, "Multiscale structural similarity for image quality assessment," in *The Thirty-Seventh Asilomar Conference on Signals, Systems & Computers, 2003*, vol. 2. Ieee, 2003, pp. 1398–1402.

[47] H. Liebgott, A. Rodriguez-Molares, F. Cervenansky, J. A. Jensen, and O. Bernard, "Plane-wave imaging challenge in medical ultrasound," in *2016 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2016, pp. 1–4.

[48] M. Sandler, A. Howard, M. Zhu, A. Zhmoginov, and L.-C. Chen, "MobileNetV2: Inverted residuals and linear bottlenecks," in *Proceedings of the IEEE Conference on Computer Vision and Pattern Recognition, 2018*, pp. 4510–4520.

[49] J.-F. Synnevag, A. Austeng, and S. Holm, "Benefits of minimum-variance beamforming in medical ultrasound imaging," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 56, no. 9, pp. 1868–1879, 2009.

[50] I. Loshchilov and F. Hutter, "Decoupled weight decay regularization," *arXiv preprint arXiv:1711.05101*, 2017.

[51] A. Rodriguez-Molares, O. M. H. Rindal, O. Bernard, A. Nair, M. A. L. Bell, H. Liebgott, A. Austeng, and L. Løvstakken, "The ultrasound toolbox," in *2017 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2017, pp. 1–4.

[52] O. M. H. Rindal, S. Aakhus, S. Holm, and A. Austeng, "Hypothesis of improved visualization of microstructures in the interventricular septum with ultrasound and adaptive beamforming," *Ultrasound in Medicine & Biology*, vol. 43, no. 10, pp. 2494–2499, 2017.

[53] A. Rodriguez-Molares, O. M. H. Rindal, J. D'hooge, S.-E. Måsøy, A. Austeng, M. A. L. Bell, and H. Torp, "The generalized contrast-to-noise ratio: a formal definition for lesion detectability," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 67, no. 4, pp. 745–759, 2019.

[54] O. M. H. Rindal, A. Austeng, A. Fatemi, and A. Rodriguez-Molares, "The effect of dynamic range alterations in the estimation of contrast," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 66, no. 7, pp. 1198–1208, July 2019.

[55] A. Rodriguez-Molares, O. M. H. Rindal, J. D'hooge, S.-E. Måsøy, A. Austeng, and H. Torp, "The generalized contrast-to-noise ratio," in *2018 IEEE International Ultrasonics Symposium (IUS)*. IEEE, 2018, pp. 1–4.

[56] M. A. Lediju, M. J. Pihl, J. J. Dahl, and G. E. Trahey, "Quantitative assessment of the magnitude, impact and spatial extent of ultrasonic clutter," *Ultrasonic imaging*, vol. 30, no. 3, pp. 151–168, 2008.

[57] S. Vedula, O. Senouf, G. Zurakhov, A. Bronstein, O. Michailovich, and M. Zibulevsky, "Learning beamforming in ultrasound imaging," in *Proceedings of The 2nd International Conference on Medical Imaging with Deep Learning*, ser. Proceedings of Machine Learning Research, M. J. Cardoso, A. Feragen, B. Glocker, E. Konukoglu, I. Oguz, G. Unal, and T. Vercauteren, Eds., vol. 102. PMLR, 08–10 Jul 2019, pp. 493–511. [Online]. Available: <http://proceedings.mlr.press/v102/vedula19a.html>

[58] P. Jarosik, M. Byra, and M. Lewandowski, "Waveflow-towards integration of ultrasound processing with deep learning," in *2018 IEEE International Ultrasonics Symposium (IUS)*, 2018, pp. 1–3.

[59] D. Hyun, Y. L. Li, I. Steinberg, M. Jakovljevic, T. Klap, and J. J. Dahl, "An Open Source GPU-Based Beamformer for Real-Time Ultrasound Imaging and Applications," in *2019 IEEE International Ultrasonics Symposium (IUS)*, 2019, pp. 20–23.

[60] J. Zhang, Q. He, Y. Xiao, H. Zheng, C. Wang, and J. Luo, "Ultrasound image reconstruction from plane wave radio-frequency data by self-

supervised deep neural network," *Medical Image Analysis*, vol. 70, p. 102018, 2021.

[61] Z. Zhou, Y. Guo, and Y. Wang, "Ultrasound deep beamforming using a multiconstrained hybrid generative adversarial network," *Medical Image Analysis*, vol. 71, p. 102086, 2021.

[62] Y. Qi, Y. Guo, and Y. Wang, "Image quality enhancement using a deep neural network for plane wave medical ultrasound imaging," *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, 2020.

[63] R. P. Mathews and M. R. Panicker, "Towards fast region adaptive ultrasound beamformer for plane wave imaging using convolutional neural networks," *arXiv preprint arXiv:2106.07006*, 2021.

[64] J. Tang, B. Zou, C. Li, S. Feng, and H. Peng, "Plane-wave image reconstruction via generative adversarial network and attention mechanism," *IEEE Transactions on Instrumentation and Measurement*, 2021.

[65] L. Maier-Hein, M. Eisenmann, A. Reinke, S. Onogur, M. Stankovic, P. Scholz, T. Arbel, H. Bogunovic, A. P. Bradley, A. Carass *et al.*, "Why rankings of biomedical image analysis competitions should be interpreted with care," *Nature communications*, vol. 9, no. 1, pp. 1–13, 2018.



Dongwoon Hyun (Member, IEEE) received the B.S.E. and Ph.D. degrees in biomedical engineering from Duke University, Durham, NC, USA, in 2010 and 2017, respectively.

He is currently a Research Engineer with the Department of Radiology, Stanford University, Stanford, CA, USA. His current research interests include machine learning methods for beamforming, ultrasound molecular imaging, real-time software beamforming, and mathematical methods for image quality assessment.



Alycen Wiacek (Graduate Student Member, IEEE) received the B.S. degree in electrical and computer engineering (ECE) from Wayne State University, Detroit, MI, USA, in 2014, the M.S. degree in ECE from Oakland University, Rochester, MI, USA, in 2015, with a focus on signal processing, and the M.S.E. degree in ECE from Johns Hopkins University, Baltimore, MD, USA, in 2019. She is currently pursuing the Ph.D. degree in ECE at Johns Hopkins University, Baltimore, MD, USA. She is a 2021-

2022 ARCS Scholar. Her research interests include ultrasound imaging, photoacoustic imaging, coherence-based beamforming, breast imaging, machine learning, signal processing, and clinical translation.



Sobhan Goudarzi received his BSc degree from the University of Isfahan and the MASc degree from the Amirkabir University of Technology, Tehran, Iran. He is currently pursuing his PhD in electrical and computer engineering at IMPACT lab at Concordia University, Montreal, Canada. His research interests are biomedical signal and image processing, medical ultrasound imaging, and machine learning.



Sven Rothluebbers received the B.Sc. and M.Sc. degree in physics from University of Bremen, Bremen, Germany, with specializations on theoretical solid-state physics in 2009 and self-organization in complex systems in 2012, respectively. He joined the Fraunhofer Institute for Digital Medicine MEVIS in 2013 and mediri GmbH, Heidelberg, Germany, from 2014 to 2019. In 2018 he obtained the Dr. rer. nat. in physics from University of Bremen, Bremen, Germany, with a focus on motion tracking in

medical image data. Since 2019 he has been investigating multimodal ultrasound imaging and ultrasound image reconstruction with classical and machine learning methods at Fraunhofer MEVIS, with a current emphasis on applications in ultrasound thermometry.



Amir Asif (Senior Member, IEEE) received the M.Sc. and Ph.D. degrees in electrical and computer engineering from Carnegie Mellon University (CMU), Pittsburgh, PA, USA, in 1993 and 1996, respectively.

He is a Professor of Electrical Engineering and Computer Science at York University. He works in the area of statistical signal processing and communications. His current projects include distributed agent networks (autonomy and consensus in complex and contested environments); medical imaging (ultrasound elastography, brain-computer interfaces), data science (graph signal processing in social networks); and health management of mission-critical systems.

Dr. Asif has organized a number of IEEE conferences on signal processing theory and applications. He has received several distinguished awards, including the York University Faculty of Graduate Studies Teaching Award in 2008; the York President's University-Wide Teaching Award (Full-Time Senior Faculty Category) in 2008; and the Science and Engineering Teaching Excellence Award (Senior Faculty Category) from York's Faculty of Science and Engineering in 2006 and 2004, respectively. He sits on several boards of directors, including Research Canada and Making the Shift Inc., and has served as the Chair of the Research Committee of Engineering Deans Canada. He has served on the editorial boards of numerous journals and international conferences, including an Associate Editor for the IEEE TRANSACTIONS ON SIGNAL PROCESSING (2014–2018) and the IEEE SIGNAL PROCESSING LETTERS (2002–2006, 2009–2013). He is a member of the Professional Engineering Society of Ontario.



Klaus Eickel received his B.Sc. (2009) and M.Sc. (2011) in physics with focus on hadron physics at the Ruhr-University Bochum, Germany. From 2012 to 2015 he had a part-time position in the radiotherapy department at University Hospital Essen. In 2013 he joined the Fraunhofer Institute for Digital Medicine MEVIS, Bremen, Germany, and affiliated research group at University of Bremen, Germany. From 2015 to 2017 and from 2021 onwards he held a joint appointment with mediri GmbH, Heidelberg, Germany. He obtained the Dr. rer. nat. in physics (2019) from the University of Bremen in accelerated MR sequence development and reconstruction. His research interests are in deep-learning applied to medical imaging, specifically MR and ultrasound imaging. He holds a patent in deep-learning based MR image reconstruction.

Germany. He obtained the Dr. rer. nat. in physics (2019) from the University of Bremen in accelerated MR sequence development and reconstruction. His research interests are in deep-learning applied to medical imaging, specifically MR and ultrasound imaging. He holds a patent in deep-learning based MR image reconstruction.



Yonina C. Eldar (Fellow, IEEE) received the B.Sc. degree in physics and the B.Sc. degree in electrical engineering from Tel-Aviv University, Tel-Aviv, Israel, in 1995 and 1996, respectively, and the Ph.D. degree in electrical engineering and computer science from the Massachusetts Institute of Technology (MIT), Cambridge, MA, USA, in 2002.

She is currently a Professor with the Department of Mathematics and Computer Science, Weizmann Institute of Science, Rehovot, Israel.

She was previously a Professor with the Department of Electrical Engineering, Technion, where she held the Edwards Chair in Engineering. She is also a Visiting Professor with MIT, a Visiting Scientist with Broad Institute, and an Adjunct Professor with Duke University, Durham, NC, USA, and was a Visiting Professor with Stanford. She is the author of the book *Sampling Theory: Beyond Bandlimited Systems* and coauthor of four other books published by Cambridge University Press. Her research interests include the broad areas of statistical signal processing, sampling theory and compressed sensing, learning and optimization methods, and their applications to biology, medical imaging, and optics.

She is a member of the Israel Academy of Sciences and Humanities, an IEEE Fellow, and a EURASIP Fellow. She has received many awards for excellence in research and teaching, including the IEEE Signal Processing Society Technical Achievement Award, the IEEE/AESS Fred Nathanson Memorial Radar Award, the IEEE Kiyo Tomiyasu Award, the Michael Bruno Memorial Award from the Rothschild Foundation, the Weizmann Prize for Exact Sciences, and the Wolf Foundation Krill Prize for Excellence in Scientific Research. She is the Editor in Chief of Foundations and Trends in Signal Processing.



Jiaqi Huang received her B.S. degree in Engineering Science - Biomedical Systems from the University of Toronto, Toronto, ON, Canada in 2018 and her M.S.E. degree in 2020 in Biomedical Engineering at Johns Hopkins University, Baltimore, MD, USA with a focus on imaging and instrumentation. She is currently a Research and Development Engineer at Baylis Medical.



Massimo Mischi (Senior Member, IEEE) received the M.Sc. degree in electrical engineering from La Sapienza University, Rome, Italy, in 1999, and the Ph.D. degree from the Eindhoven University of Technology (TU/e), Eindhoven, The Netherlands, in 2004. In 2007, he was an Assistant Professor with the Electrical Engineering Department, TU/e. In 2011, he was an Associate Professor with TU/e and founded the Biomedical Diagnostics Research Laboratory, where he was involved in model-based quantitative analysis of

biomedical signals with applications ranging from electrophysiology to diagnostic imaging, with focus on ultrasound technology. He is currently a Full Professor with the Electrical Engineering Department, TU/e. He has co-authored over 300 peer reviewed publications, 13 patents, one book, and several book chapters. Prof. Mischi is a Board Member of the Imaging Section of the European Association of Urology, Secretary of the Dutch Society of Medical Ultrasound, and Chairman of the IEEE EMBS Benelux Chapter. He was a recipient of an STW VIDI Grant in 2009, ERC Starting Grant in 2011, and ERC Proof of Concept in 2019 for his research on angiogenesis imaging.



Hassan Rivaz (Senior Member, IEEE) received the B.Sc. degree from Sharif University of Technology, the M.A.Sc. degree from The University of British Columbia, and the Ph.D. degree from Johns Hopkins University. He holds the Research Chair in Medical Image Analysis at Concordia University, where he directs the IMPACT lab: Image Processing And Characterization of Tissue. His research interests are medical image analysis, machine learning, deep learning, elastography, quantitative ultrasound and beam-

forming.

Dr. Rivaz is an Associate Editor of IEEE TRANSACTIONS ON MEDICAL IMAGING and IEEE TRANSACTIONS ON ULTRASONICS, FERROELECTRICS AND FREQUENCY CONTROL. He is a member of the Organizing Committee of IEEE EMBC 2020 (Montreal, Canada), IEEE ISBI 2021 (Nice, France), and IEEE IUS 2023 (Montreal, Canada). He served as an Area Chair of MICCAI for 4 years since 2017. He co-organized two tutorials on advances in ultrasound imaging at IEEE ISBI 2018 and 2019. He also co-organized the CURIOUS 2018 and CURIOUS 2019 Challenges on registration of ultrasound and MRI in neurosurgery, and the CereVis 2018 Workshop on Cerebral Data Visualization, all in conjunction with MICCAI.



David Sinden received a B.Sc. from Imperial College, U.K., in 2003, then, in 2004, a M.Sc. from the University of Bath, U.K., both in applied mathematics. In 2008 he obtained a Ph.D. in nonlinear dynamics from University College London, U.K. He then held post-doctoral positions at University College London, U.K. and the Institute of Cancer Research, Sutton, U.K., before joining the National Physical Laboratory, Teddington, U.K. in 2014. Since 2019, he is a senior scientist at the Fraunhofer Institute for Digital Medicine

MEVIS, Bremen, Germany. His research interests are mathematical modelling applied to image-guided therapies. He is a member of the IEC technical committee 87 working group 6 – High Intensity Therapeutic Ultrasound.



Ruud J.G. van Sloun (Member, IEEE) received the B.Sc. and M.Sc. degrees (cum laude) in electrical engineering and the Ph.D. degree (cum laude) from the Eindhoven University of Technology, Eindhoven, The Netherlands, in 2012, 2014, and 2018, respectively. Since then, he has been an Assistant Professor with the Department of Electrical Engineering at the Eindhoven University of Technology and since January 2020 a Kickstart-AI fellow at Philips Research, Eindhoven. From 2019-2020 he was

also a Visiting Professor with the Department of Mathematics and Computer Science at the Weizmann Institute of Science, Rehovot, Israel. He is a NWO Rubicon laureate and received a Google Faculty Research Award in 2020. His current research interests include artificial intelligence and deep learning for front-end (ultrasound) signal processing, model-based deep learning, compressed sensing, ultrasound imaging, and probabilistic signal and image analysis.



Hannah Strohm received a B.Sc. in medical engineering in 2015 from Friedrich-Alexander University Erlangen-Nürnberg, Germany and a M.Sc. in electrical engineering from Hamburg University of Technology, Germany in 2018. She is currently pursuing her Ph.D. at the Fraunhofer Institute for Digital Medicine MEVIS, Bremen, Germany with a focus on the integration of data-driven methods into ultrasound reconstruction. Her research interests include ultrasound beamforming techniques, ultrasound thermometry, and deep learning methods.



Muyinatu A. Lediju Bell (Senior Member, IEEE) received the B.S. degree in mechanical engineering (minor in biomedical engineering) from the Massachusetts Institute of Technology, Cambridge, MA, USA, in 2006, and the Ph.D. degree in biomedical engineering from Duke University, Durham, NC, USA, in 2012. From 2009 to 2010, she conducted research abroad as a Whitaker International Fellow at The Institute of Cancer Research and Royal Marsden Hospital, Sutton, Surrey, U.K. From 2012 to 2016, she was a

postdoctoral fellow with the Engineering Research Center for Computer-Integrated Surgical Systems and Technology, Johns Hopkins University, Baltimore, MD, USA.

Dr. Bell is the John C. Malone Assistant Professor in the Department Electrical and Computer Engineering with a joint appointment in the Department of Biomedical Engineering and a secondary appointment in the Department of Computer Science at Johns Hopkins University, where she founded and directs the Photoacoustic and Ultrasonic Systems Engineering Laboratory. Her research interests include ultrasound and photoacoustic imaging, coherence-based beamforming, deep learning for ultrasound and photoacoustic image formation, image-guided surgery, robotics, and medical device design.

Dr. Bell received multiple awards, including the NSF CAREER Award in 2018, the NIH Trailblazer Award in 2018, MIT Technology Review's Innovator Under 35 Award in 2016, and the NIH K99/R00 Pathway to Independence Award in 2015. She currently serves as Associate Editor of the IEEE TRANSACTIONS ON MEDICAL IMAGING and Associate Editor in Chief of the IEEE TRANSACTIONS ON ULTRASONICS, FERROELECTRICS, AND FREQUENCY CONTROL. Dr. Bell was the lead organizer of the 2020 Challenge on Ultrasound Beamforming with Deep Learning.