

Northumbria Research Link

Citation: Morris, Robert, McHale, Glen, Dias, Tilak and Newton, Michael (2013) Embroidered Coils for Magnetic Resonance Sensors. *Electronics*, 2 (2). pp. 168-177. ISSN 2079-9292

Published by: MDPI

URL: <http://dx.doi.org/10.3390/electronics2020168>
<<http://dx.doi.org/10.3390/electronics2020168>>

This version was downloaded from Northumbria Research Link:
<http://nrl.northumbria.ac.uk/id/eprint/12415/>

Northumbria University has developed Northumbria Research Link (NRL) to enable users to access the University's research output. Copyright © and moral rights for items on NRL are retained by the individual author(s) and/or other copyright owners. Single copies of full items can be reproduced, displayed or performed, and given to third parties in any format or medium for personal research or study, educational, or not-for-profit purposes without prior permission or charge, provided the authors, title and full bibliographic details are given, as well as a hyperlink and/or URL to the original metadata page. The content must not be changed in any way. Full items must not be sold commercially in any format or medium without formal permission of the copyright holder. The full policy is available online: <http://nrl.northumbria.ac.uk/policies.html>

This document may differ from the final, published version of the research and has been made available online in accordance with publisher policies. To read and/or cite from the published version of the research, please visit the publisher's website (a subscription may be required.)

Article

Embroidered Coils for Magnetic Resonance Sensors

Robert H. Morris ^{1,*}, Glen McHale ², Tilak Dias ³ and Michael I. Newton ¹

¹ School of Science and Technology, Nottingham Trent University, Clifton Lane, Nottingham. NG11 8NS, UK; E-Mail: michael.newton@ntu.ac.uk

² School of Computing, Engineering & Information Sciences, Northumbria University. NE1 8ST, UK; E-Mail: glen.mchale@northumbria.ac.uk

³ School of Art and Design, Nottingham Trent University, Burton Street, Nottingham NG1 4BU, UK; E-Mail: tilak.dias@ntu.ac.uk

* Author to whom correspondence should be addressed; E-Mail: rob.morris@ntu.ac.uk; Tel.: +44-115-848-3123; Fax: +44-115-848-6636.

Received: 12 December 2012; in revised form: 22 January 2013 / Accepted: 29 March 2013 /

Published: 18 April 2013

Abstract: Magnetic resonance imaging is a widely used technique for medical and materials imaging. Even though the objects being imaged are often irregularly shaped, suitable coils permitting the measurement of the radio-frequency signal in these systems are usually made of solid copper. One problem often encountered is how to ensure the coils are both in close proximity and conformal to the object being imaged. Whilst embroidered conductive threads have previously been used as antennae in mobile telecommunications applications, they have not previously been reported for use within magnetic resonance. In this paper we show that an embroidered single loop coil can be used in a commercial unilateral nuclear magnetic resonance system as an alternative to a solid copper. Data is presented showing the determination of both longitudinal (T_1) and effective transverse (T_2^{eff}) relaxation times for a flat fabric coil and the same coil conformed to an 8 cm diameter cylinder. We thereby demonstrate the principles required for the wider use of fabric based conformal coils within nuclear magnetic resonance and magnetic resonance imaging.


Keywords: magnetic resonance; embroidered; high frequency coil; relaxation time

1. Introduction

The use of embroidered conductive thread to produce a range of radio frequency antenna systems has become popular since the late 1990s when conductive fabrics began to be used for wearable systems. Initially used for Direct Current to low frequency and for shielding applications [1], their obvious potential for higher frequency systems became clear in the early part of this century [2]. These systems are now becoming commonplace for use as GPS, Mobile Phone and Radio Frequency Identification (RFID) [3–7] antennas to which they are ideally suited. It should be noted however that regular washing of such conducting yarns does lead to degradation in the electrical properties [8]. An application which has, until now, remained unexplored is the use of conductive fiber coils in magnetic resonance imaging.

Pulsed nuclear magnetic resonance (NMR) and magnetic resonance imaging (MRI) are well established techniques most commonly associated with large scanners. In recent years the availability of low field strength (<1 Tesla) unilateral (single-sided) NMR probes [9–12], based on simple rare earth permanent magnets, has been accompanied by an increase in the number of low cost NMR consoles (the electronics used to drive them). Applications have also diversified as a result of more affordable hardware [13–15]. All pulsed magnetic resonance systems face the same challenge: a large power is needed to excite the sample (1–1000 W) whilst the collected signal is typically less than a micro-Watt. Figure 1 shows the elements required to obtain an NMR signal from a sample. For transmission, RF pulses are generated at low power and amplified to the required level to excite the sample when delivered to the NMR probe (containing an impedance matching circuit and sample coil). The small radio frequency signal produced by the sample is then induced into the same (or a closely placed) coil which is connected to a low noise preamplifier that produces a signal suitable for the RF detection stage allowing digital or analogue processing. A duplexer is used as a transmit receive switch to protect the preamp during transmission and to reduce noise by isolating the transmitter during reception.

Figure 1. Schematic diagram of a typical pulsed nuclear magnetic resonance (NMR) system showing components and impedance matching circuit.

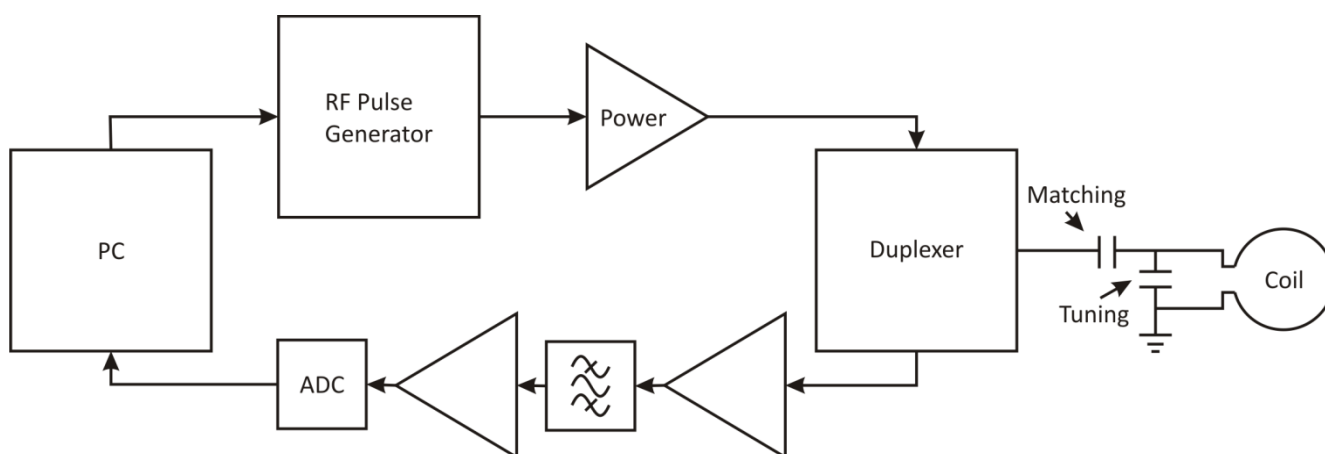


The NMR probe usually consists of a coil with a tuning capacitor in parallel with the coil and, a matching capacitor in series with the coil, allowing the probe to apply and receive high frequency

energy to and from a sample of interest in a magnetic field [16,17]. This is usually achieved with copper coils placed around the sample in rigid housings. Most often a single coil is used to both excite the sample and to collect the resultant signal, whilst for more sensitive studies separate coils are used. These can be made of copper on flexible substrates in order to decrease the separation between the sample and the coil as proximity and conformity of the coil are critical parameters in maximising the SNR. In this paper we present a fundamental demonstration of the principles of using an embroidered conductive fabric coil for magnetic resonance.

2. Experimental Section

A simple single loop coil of diameter 24.5 mm was produced using silver coated nylon yarn embroidered using a stitch length of 0.2 mm on a Barudan BEVT-Z1501CB digital embroidery machine modified to minimize the damage to the delicate yarn during application. This was embroidered onto a woven cotton fabric and protruded 1.1 mm either side of the cotton layer giving a coil resistance of 9.2Ω . A number of different designs were investigated however all these exhibited much higher resistance values (reducing the maximum achievable quality factor) and did not result in a sufficient impedance match at the required frequency. A photo of the selected design is shown in Figure 2 along with photographs of its use for measurements.

Figure 2. (a) Photograph of the embroidered coil; (b) The coil flat on the NMR MOUSE™; (c) Embroidered coil conformed to palm oil tub; (d) The coil and tub on the NMR MOUSE™ from the front, and (e) the side.

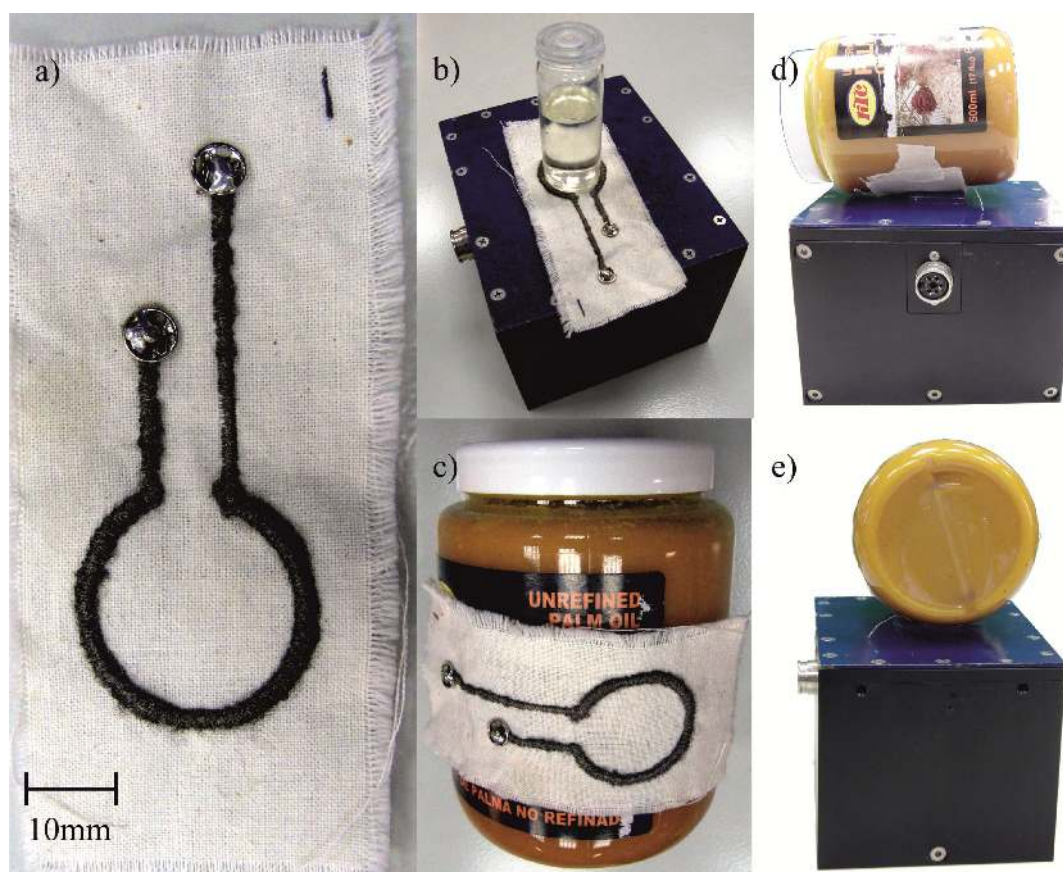

The coil, tuning and matching capacitors were connected to a network analyzer (Agilent E5061A) that scans through the frequency range of interest showing the resonant properties of the circuit. Figure 3 shows the data for the fabric coil with a broad resonance centered at 10.64 MHz. The commercial magnetic resonance instrument used in this work was the ACT (Aachen) profile NMR MOUSE™ [18] with a CAT-20 Apollo (Tecmag, Houston, TX, USA) console to provide pulse sequence generation and signal processing with a Tomco (Stepney, Australia) BT00250-Beta 250 W power amplifier. The instrument operates at a frequency of 10.64 MHz and uses the same coil for excitation and detection. The system is unilateral and provides a uniform magnetic field (which defines the sensitive volume being interrogated by the system), 5 mm above the top surface and with dimensions $5 \mu\text{m} \times 30 \text{ mm} \times 30 \text{ mm}$.

The resonance curve for the built in coil on the MOUSE™ is also shown in Figure 3. The much sharper resonance would be expected to deliver energy much more efficiently to the sample than the broader resonance of the fabric coil. For this particular application however, the broad resonance is advantageous in that changes in the shape of the coil when it conforms to the object being measured do not cause much variation in the tuning of the circuit. The loss in matching is predominantly due to the increased resistivity of the fabric coil compared to that of the NMR MOUSE™. It may be possible to improve this by using a different yarn although that has not been explored as part of this work. The Carr Purcell Meiboom Gill (CPMG) [19] sequence was used to measure T_2^{eff} , as is typical on unilateral instruments, with a saturation recovery sequence used for the determination of T1 [20]. The parameters used for these sequences are detailed in Table 1. Prior to these measurements a series of Carr Purcell Meiboom Gill (CPMG) sequences with increasing 90 degree pulse length were run to find the maximum signal and hence the optimum time for the 90 degree pulse; this was found to be 6000 ns and was significantly longer than the 4500 ns for the MOUSE™ coil (for the same RF transmit power of 250 W) as expected given the lower quality factor and the difference in the geometry of the coils.

Figure 3. The resonance curves for the fabric coil probe (red line) and the NMR MOUSE™ probe (blue line).

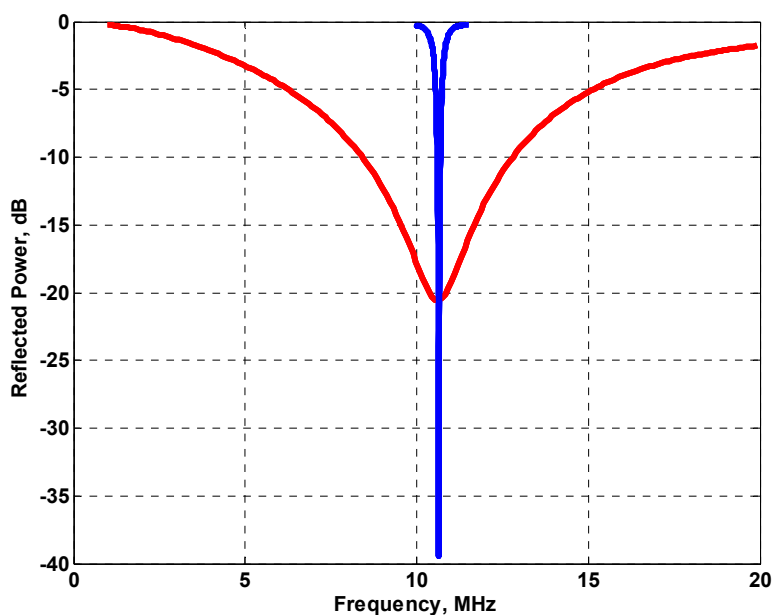


Table 1. Parameters used for MR measurements.

Parameters	Values
90° Pulse Length (Copper)	4500 ns
90° Pulse Length (fabric)	6000 ns
Echo Time	300 μ s
Repetition Time	600 ms
Number of Echoes	128
Dwell Time	1 μ s
Points per Echo Window	80

The longer pulse length will also result in a slight reduction in the volume of the selected slice due to the reduction in the bandwidth. The test samples used were sunflower oil and red palm oil. For investigating how well the fabric conforms to different surfaces and how this affects the measurements, a tube was used filled with red palm oil with a diameter of 8 cm. Wrapping the coil round the 8 cm tube, resulted in no measureable change in the frequency at which the minimum occurred in the resonance curve on the network analyzer. Even wrapping the coil as tightly as round a 2.5 cm tube resulted in a change in resonant frequency of less than 500 kHz which is a small change compared to the width of the resonance and thus would not require retuning. For the 2.5 cm tube, very little of the sample would be in the sensitive volume of the magnet due to the curvature of the sample so this is not presented. In the highly uniform field of a conventional MRI scanner however it would not show the reduced measurement volume that is experienced with a unilateral instrument.

3. Results and Discussion

The first eight spin echoes taken from a CPMG sequence are shown in Figure 4 with 1024 averages using the fabric coil (red) and the built in coil from the NMR MOUSE™ (blue). As is usual for this type of unilateral system, the first (Hahn) echo is significantly smaller than subsequent echo train as it is heavily influenced by diffusive motion. The signal is clearly much lower for the fabric coil which can be accounted for by the sharper resonance of the MOUSE™ coil resulting in more efficient generation and detection of the RF signal. In addition, the width of the echoes is significantly greater for the fabric coil. The SNRs of the two systems were estimated (using peak signal/standard deviation of surrounding noise for the real component of the 4th echo) as 17 and 61 for the fabric coil and the MOUSE™ coil respectively. Figure 5 shows the normalized NMR signal intensity for fabric coil for a 128 echo CPMG sequence using sunflower oil as the sample. By fitting an exponential curve to the data, values for the effective transverse relaxation time T_2^{eff} can be found. From the data in Figure 5, T_2^{eff} for sunflower oil is 58.1 ± 5.3 ms compared to 55.68 ± 2.5 ms for the inbuilt coil of the NMR MOUSE™. The error in the relaxation time has been determined from the exponential fit to the data. This demonstrates that a fabric coil can be used for measurements of relaxation time although it requires more averaging than the optimized commercial copper coil.

Figure 4. The first eight echoes produced by a CPMG sequence using (a) the fabric coil (red line) (b) the MOUSE™ coil (blue line).



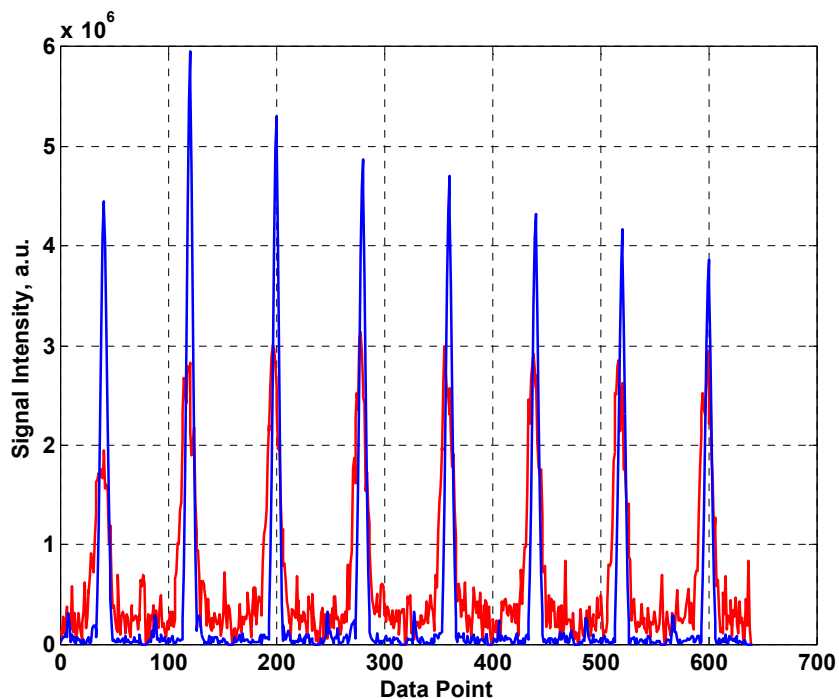


Figure 5. The normalized NMR signal intensity for the MOUSE™ coil (red circles) and fabric coil (blue squares) for a 128 echo CPMG sequence using sunflower oil as the sample.

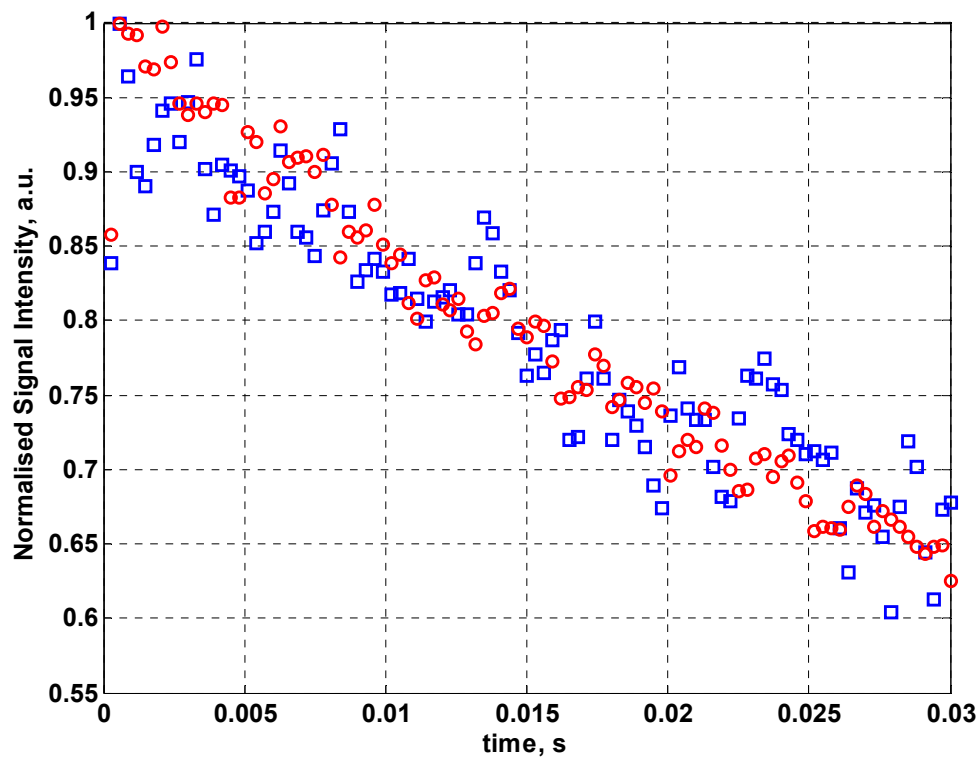

The fabric coil was then used to measure the relaxation times for red palm oil initially with a flat coil and then with it wrapped around an 8 cm diameter tube. Figure 6 shows the normalized signal intensity for a train of 128 echoes with 512 averages for a CPMG sequence for the flat fabric coil (squares) and the same coil wrapped round the 8 cm tube (circles). By fitting an exponential curve to the data, the flat fabric gives T_2^{eff} of 60.5 ± 2.8 ms, whilst wrapped round the 8 cm tube gives 55.8 ± 2.8 ms. To better demonstrate the variation in signal quality between the coil flat and conformed to a cylinder, Figure 7 shows the first four spin echoes produced for the fabric coil lying flat on the MOUSETM and conformed to the red palm oil tube (8 cm in diameter), this results in a minor loss in signal due to the change in geometry. The thin slice of magnetic homogeneity prevents us from seeing an improvement in the fill factor of the coil (the ratio of the sample volume of interest to the sensitive volume of the coil) which would likely negate this effect in a traditional MRI scanner.

Figure 6. The normalized NMR signal intensity for 128 echo CPMG sequence with 512 averages for red palm oil using flat fabric coil (red circles) and the fabric coil wrapped round the 8 cm tube (blue squares).

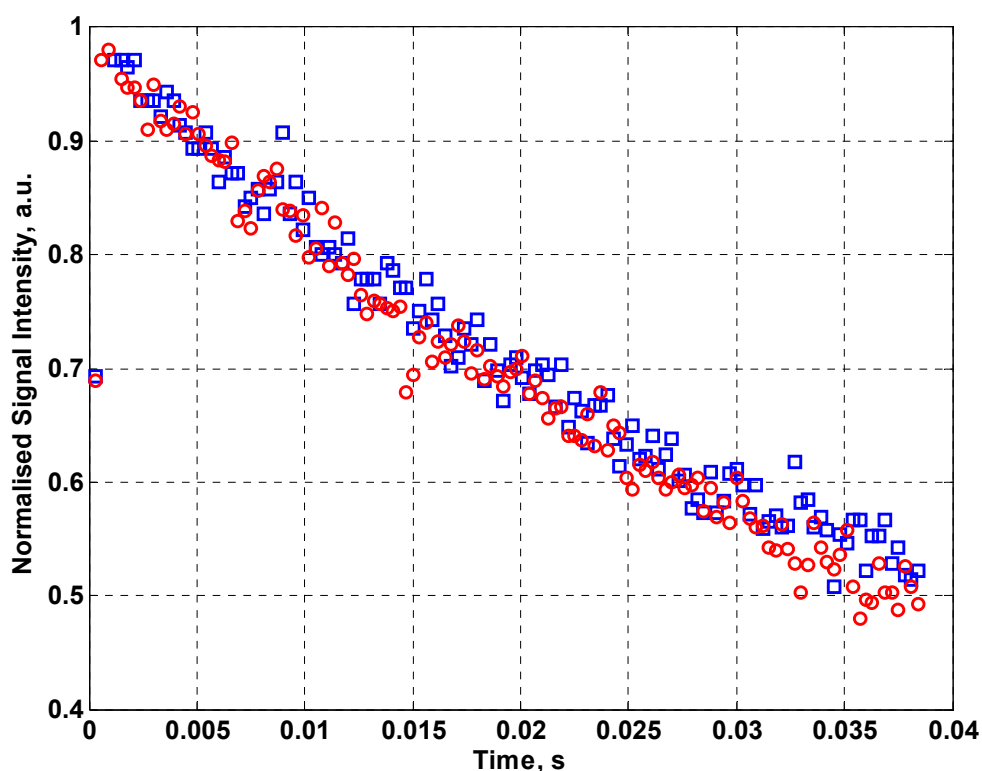

In addition to measuring T_2^{eff} , increasing repetition times were used to determine T_1 for the red palm oil and used a 128 echo train and 512 averages with the normalized data presented in Figure 8. The flat fabric (squares) gives T_1 of 100.6 ± 0.8 ms, whilst wrapped around the 8 cm tube (circles) gives 103.6 ± 0.8 ms. Given that sunflower oil and red palm oil are natural materials with some spatial variation expected in measured relaxation times, the values of T_1 and T_2^{eff} are within the expected experimental measurement range.

Figure 7. Raw spin echoes comparing the fabric coil flat (blue) and conformed (red) to an 8 cm cylinder.


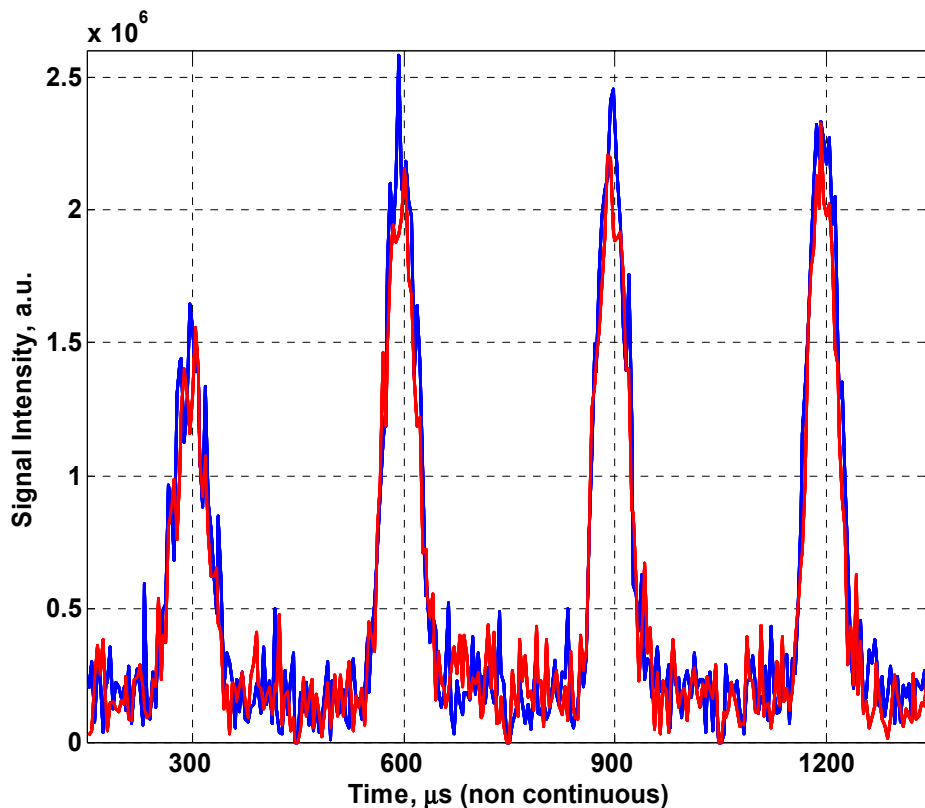


Figure 8. Normalized data for a saturation recovery sequence for the red palm oil used a 128 echo train and 512 averages. Data for the flat fabric coil is shown as red circles whilst the fabric coil wrapped round the 8 cm tube is shown as blue squares.

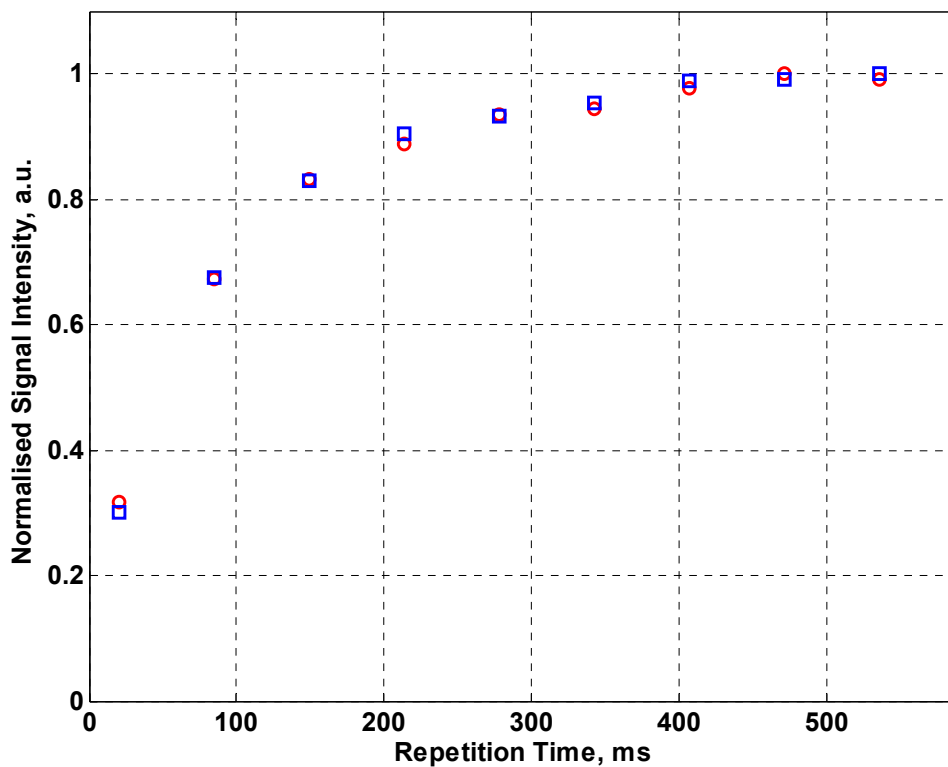

4. Conclusions

We have demonstrated the ability to use an embroidered coil as a substitute for a traditional copper coil in an MR system. The measured signal levels are smaller than the commercial instrument due to the lower Q factor of the coil which therefore requires more averaging to achieve the same SNR. The higher coil resistance results in the poorer quality factor of the coil and is ultimately responsible for the reduction of SNR in comparison to the copper coil. By using a more conductive yarn than that which we have used, using a thicker thread, changing the stitch pattern, or producing a different coil geometry, it should be possible to reduce this resistance to the point at which the achievable increase in fill factor improves the SNR in comparison to a copper coil. However, even with the current yarn, the ability to embroider such coils on textiles (flexible substrates) will allow this same technique to be applied to samples in which it is desirable to have a soft conformable coil such as cranial imaging or elastomer based limb coils within a medical magnetic resonance imaging scanner or as a low cost disposable technology. We have demonstrated for the first time that it is possible to perform a magnetic resonance experiment using an embroidered coil.

Acknowledgments

We gratefully acknowledge the UK Engineering and Physical Sciences Research Council for support under grant (EP/I016414/1).

References

1. Guy, A.W.; Chung-Kwang, C.; McDougall, J.A.; Sorensen, C. Measurement of shielding effectiveness of microwave-protective suits. *IEEE Trans. Microw. Theory Tech.* **1987**, *35*, 984–994
2. Massey, P.J. GSM fabric antenna for mobile phones integrated within clothing. *Proc. IEEE Antennas Propag. Soc. Int. Symp.* **2001**, *3*, 452–455.
3. Locher, I.; Klemm, M.; Kirstein, T.; Troster, G. Design and characterization of purely textile patch antennas. *IEEE Trans. Adv. Packag.* **2006**, *29*, 777–788.
4. Hertleer, C.; Tronquo, A.; Rogier, H.; van Langenhove, L. The use of textile materials to design wearable microstrip patch antennas. *Text. Res. J.* **2008**, *78*, 651–658.
5. Yang, L.; Vyas, R.; Rida, A.; Pan, J.; Tentzeris, M.M. Wearable RFID-Enabled Sensor Nodes for Biomedical Applications. In Proceedings of the 58th Electronic Components and Technology Conference, Lake Buena Vista, FL, USA, 27–30 May 2008; pp. 2156–2159.
6. Kaivanto, E.K. Wearable circularly polarized antenna for personal satellite communication and navigation. *IEEE Trans. Antennas Propag.* **2011**, *12*, 4490–4496.
7. Lilja, J. Design and manufacturing of robust textile antennas for harsh environments. *IEEE Trans. Antennas Propag.* **2012**, *9*, 4130–4140.
8. Varnaitė, S.; Katunskis, J. Influence of washing on the electric charge decay of fabrics with conductive yarns. *Fibres Text. East. Eur.* **2009**, *17*, 69–75.
9. Kleinberg, R.L.; Sezginer, A.; Griffin, D.D. Novel NMR apparatus for investigating an external sample. *J. Magn. Reson.* **1992**, *97*, 466–485.

10. Eidmann, G.; Savelsberg, R.; Blumler, P.; Blumich, B. The NMR MOUSE, a mobile universal surface explorer. *J. Magn. Reson., Ser. A* **1996**, *122*, 104–109.
11. Manz, B.; Coya, A.; Dykstrac, R.; Ecclesa, C.D.; Hunterd, M.W.; Parkinsond, B.J.; Callaghand, P.T. A mobile one-sided NMR sensor with a homogeneous magnetic field: The NMR-MOLE. *J. Magn. Reson.* **2006**, *183*, 25–31.
12. García-Naranjo, J.C.; Mastikhin, I.V.; Colpitts, B.G.; Balcom, B.J. A unilateral magnet with an extended constant magnetic field gradient. *J. Magn. Reson.* **2010**, *207*, 337–344.
13. Blümich, B.; Casanova, F. Mobile NMR. In *Modern Magnetic Resonance Part I*; Springer: Dordrecht, The Netherlands, 2006; pp. 369–377.
14. Van Landeghem, M.; Danieli, E.; Perlo, J.; Blümich, B.; Casanova, F. Low-gradient single-sided NMR sensor for one-shot profiling of human skin. *J. Magn. Reson.* **2012**, *215*, 74–84.
15. Geya, Y.; Kimura, T.; Fujisaki, H.; Terada, Y.; Kose, K.; Haishi, T.; Gemma, H.; Sekozawa, Y. Longitudinal NMR parameter measurements of Japanese pear fruit during the growing process using a mobile magnetic resonance imaging system. *J. Magn. Reson.* **2013**, *226*, 45–51.
16. Callaghan, P.T. *Principles of Nuclear Magnetic Resonance Microscopy*; Oxford University Press: Oxford, UK, 1993.
17. Fukushima, E.; Roeder, S.B.W. *Experimental Pulse Nuclear Magnetic Resonance: A Nuts and Bolts Approach*; Westview Press: Boulder, CO, USA, 1981.
18. Blumich, B.; Blumler, P.; Eidmann, G.; Guthausen, A.; Haken, R.; Schmitz, U.; Saito, K.; Zimmer, G. The NMR-mouse: construction, excitation, and applications. *Magn. Reson. Imaging.* **1998**, *16*, 479–484.
19. Meiboom, S.; Gill, D. Modified spin-echo method for measuring nuclear relaxation times. *Rev. Sci. Instrum.* **1958**, *29*, 688–691.
20. Blumich, B. *NMR Imaging of Materials*; Oxford University Press: Oxford, UK, 2004.

© 2013 by the authors; licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution license (<http://creativecommons.org/licenses/by/3.0/>).