







Graphdiyne-modified TiO₂ nanofibers with osteoinductive and enhanced photocatalytic antibacterial activities to prevent implant infection

Rui Wang ^{1,2,5}, Miusi Shi ^{1,5}, Feiyan Xu ^{3,4}, Yun Qiu¹, Peng Zhang¹, Kailun Shen¹, Qin Zhao ¹, Jiaguo Yu ^{3,4}✉ & Yufeng Zhang ^{1,2}✉

Titanium implants have been widely used in bone tissue engineering for decades. However, orthopedic implant-associated infections increase the risk of implant failure and even lead to amputation in severe cases. Although TiO₂ has photocatalytic activity to produce reactive oxygen species (ROS), the recombination of generated electrons and holes limits its antibacterial ability. Here, we describe a graphdiyne (GDY) composite TiO₂ nanofiber that combats implant infections through enhanced photocatalysis and prolonged antibacterial ability. In addition, GDY-modified TiO₂ nanofibers exert superior biocompatibility and osteoinductive abilities for cell adhesion and differentiation, thus contributing to the bone tissue regeneration process in drug-resistant bacteria-induced implant infection.

¹State Key Laboratory Breeding Base of Basic Science of Stomatology (Hubei-MOST) and Key Laboratory of Oral Biomedicine, Ministry of Education, School and Hospital of Stomatology, Wuhan University, 430079 Wuhan, PR China. ²Medical Research Institute, School of Medicine, Wuhan University, 430071 Wuhan, PR China. ³Foshan Xianhu Laboratory of the Advanced Energy Science and Technology Guangdong Laboratory, Xianhu Hydrogen Valley, 528200 Foshan, PR China. ⁴State Key Laboratory of Advanced Technology for Material Synthesis and Processing, Wuhan University of Technology, Luoshi Road 122#, 430070 Wuhan, PR China. ⁵These authors contributed equally: Rui Wang, Miusi Shi. ✉email: yujaguo93@whut.edu.cn; zyf@whu.edu.cn

Since the early 1970s, titanium (Ti) and Ti-alloy implants have been widely applied in orthopedics and dentistry due to their benign biocompatibility, chemical stability, and mechanical properties^{1,2}. However, orthopedic implant-associated infections mainly caused by *Staphylococcus aureus* (*S. aureus*) delay the healing process and lead to bone loss, requiring extensive surgical intervention, and long-term antibiotic therapy³. Repeated antibiotic treatment increases the possibility of drug resistance (40% of pathogenic *S. aureus* are methicillin-resistant forms)⁴. These infections often lead to implant failure, which requires implant replacements and causes chronic and/or relapsing disease^{3,5}. In addition to causing pain and financial loss in further treatment, severe infections might induce amputation or life-threatening sepsis⁶.

Current studies to optimize bone implants mainly focus on surface modification or changing topological features to promote stem cell differentiation and induce bone regeneration^{7–11}. However, the antibacterial ability of the implants should also be taken into consideration. Theoretically, TiO₂ as a photocatalytic material can produce reactive oxygen species (ROS) to kill bacteria under UV irradiation¹², while the recombination of generated electrons and holes reduces the photocatalytic performance of TiO₂ and restricts its practical antibacterial effects¹³. Recently, researchers have loaded antibiotics, metal nanoparticles, and other antimicrobial elements onto TiO₂ surfaces for antibacterial applications^{13–16}. However, the bacterial resistance arising from antibiotic application and the potential cytotoxicity of metal nanoparticles limit their clinical applications. Therefore, an ideal titanium implant should have features of a controllable antibacterial surface based on steady long-term tissue regeneration guidance properties.

As a new member of 2D carbon-based nanomaterials, graphdiyne (GDY) has been predicted to be the most stable diacetylenic carbon allotrope¹⁷. It is composed of 18-C hexagon units with benzene rings connected by butadiyne linkages ($-C\equiv C-C\equiv C-$). Compared with graphene, the particular *sp* and *sp*² hybridized carbon atoms of GDY endow the latter with a unique electronic structure and superior electrical conductivity, which are highly beneficial for electron transfer and enhance the catalytic effects of metals and their oxides^{18–23}. In addition, GDY and its derivatives exhibit great stability and biocompatibility in some *in vivo* studies^{24–26}, thus displaying favorable biological properties in biosensing and cancer therapy. Oxidative GDY alone was also reported to have antibacterial effect under visible light through ROS generation, direct contact and good dispersion²⁷. In addition, graphene, the most investigated allotrope of GDY, possesses favorable osteogenic capability, indicating that GDY also has osteoinductive potential²⁸. In view of the aforementioned advantages, GDY is an ideal material to coordinate the dual functions of TiO₂ implants with both tissue regeneration properties and antibacterial effects.

In this study, we synthesize a TiO₂/graphdiyne composite (TiO₂/GDY) to improve its bioactivity. By changing the surface charges of GDY sheets and TiO₂ nanofibers, we successfully assemble GDY onto TiO₂ by electrostatic force. TiO₂/GDY nanofibers exhibit excellent photocatalytic performance with increased photocatalytic ROS production. The abundant generated ROS induce cellular component oxidation and bacterial cell wall perforation, which lead to membrane leakage, structural destruction, and eventual bacterial death. Furthermore, the antibacterial effect of TiO₂/GDY is prolonged with surprising sustained ROS release that prevents Methicillin-resistant *Staphylococcus aureus* (MRSA) biofilm formation. In addition, GDY enhances the biocompatibility of TiO₂ nanofibers and exhibits the adsorption of osteoinductive components *in vitro*, thus promoting cell proliferation and osteoinduction abilities.

Mouse orthopedic implant infection models further demonstrate the excellent sterilization and bone regeneration effects of TiO₂/GDY nanofibers. Due to their great multilevel properties, TiO₂/GDY nanofibers can be applied as an ideal scaffold or surface modification strategy for titanium implants to prevent implant infections and promote bone tissue regeneration.

Results

Characterization and photocatalytic properties of TiO₂/GDY. First, we used transmission electron microscopy (TEM) to show the microstructure of the prepared TiO₂/GDY. The TEM image confirms that the TiO₂ nanofibers and GDY were successfully self-assembled and that the diameter of the nanofibers was ~150 nm (Fig. 1a). Then, we used Raman spectroscopy to confirm the molecular component of TiO₂/GDY. As shown in Fig. 1b, four main peaks in red from 144.3 to 638.5 cm⁻¹ represent TiO₂, while the two peaks of 1409.7 and 1606.8 cm⁻¹ magnified in blue are ascribed to the aromatic bonds, the C–C triple bonds and their conjugate bond neighbors of GDY²⁹.

The photocatalytic activity of TiO₂/GDY and TiO₂ nanofibers was measured through a rhodamine B (RhB) degradation assay. RhB belongs to xanthene dyes, a class of stable fluorescent dyes that can be degraded by the photocatalytic effect of TiO₂ through photobleaching and N-desulfurization³⁰. After the TiO₂/GDY or TiO₂-mixed RhB solution was irradiated with ultraviolet (UV) light (365 nm, 2 W cm⁻²) for 60 min, the solution became paler in color, and its absorbance decreased (Fig. 1c). According to the variations in absorption peaks and area under the curve, the RhB photodegradation with TiO₂/GDY was faster than that with TiO₂ due to the capability of electron separation of GDY (Fig. 1d, e). Conversely, pure RhB irradiated under UV light barely degraded. Furthermore, the electron spin resonance (ESR) spectra show that the signals of ·OH, ·O₂⁻, 1O₂, and ·OOH derived from TiO₂/GDY were stronger than those from TiO₂ under UV irradiation, demonstrating that the ROS (·OH, ·O₂⁻, 1O₂, and ·OOH) generation ability of TiO₂ nanofibers was significantly enhanced after GDY assemblage (Fig. 1f and Supplementary Fig. 1). Also, photocatalytic TiO₂/GDY produced more H₂O₂ than TiO₂, and maintained a relative high concentration level in at least 60 min after Xe lamp irradiation (Supplementary Fig. 2). In addition, the contact angle of TiO₂/GDY was 15°, which was much smaller than that of TiO₂ (49°) (Fig. 1g).

Morphology and viability of cells on TiO₂/GDY. To investigate the biocompatibility of nanofibers during bone regeneration, murine-derived osteoblast-like MC3T3-E1 cells were used for *in vitro* evaluation. The cells were cultured with TiO₂/GDY or TiO₂ for 24 h, and then the cytoskeletons were stained with fluorescein isothiocyanate (FITC)-phalloidin to observe the cell morphology. Compared with those cultured with TiO₂, cells on TiO₂/GDY nanofibers tended to aggregate and adhere more. The attached cells exhibited more spreading, filopodia extension and intercellular contacts than did the normal cultured cells in the control group (Fig. 2a). The cell area calculation also showed that the cells on TiO₂/GDY was more spreading than on TiO₂ (Supplementary Fig. 3a). The SEM images indicate that cells could adhere to both TiO₂ and TiO₂/GDY. However, their adhesion and spreading were flatter and tighter on TiO₂/GDY than on TiO₂ (Fig. 2b). As shown in the illustration (Fig. 2c), cells tended to spread on TiO₂/GDY for the expansive contact area, and the increased hydrophilicity of the surface was attributed to GDY. In addition, there were more cells adhered on TiO₂/GDY than on TiO₂ (Supplementary Fig. 3b).

The live/dead staining and CCK-8 assays indicated that TiO₂/GDY barely led to cell death and inhibited cell proliferation

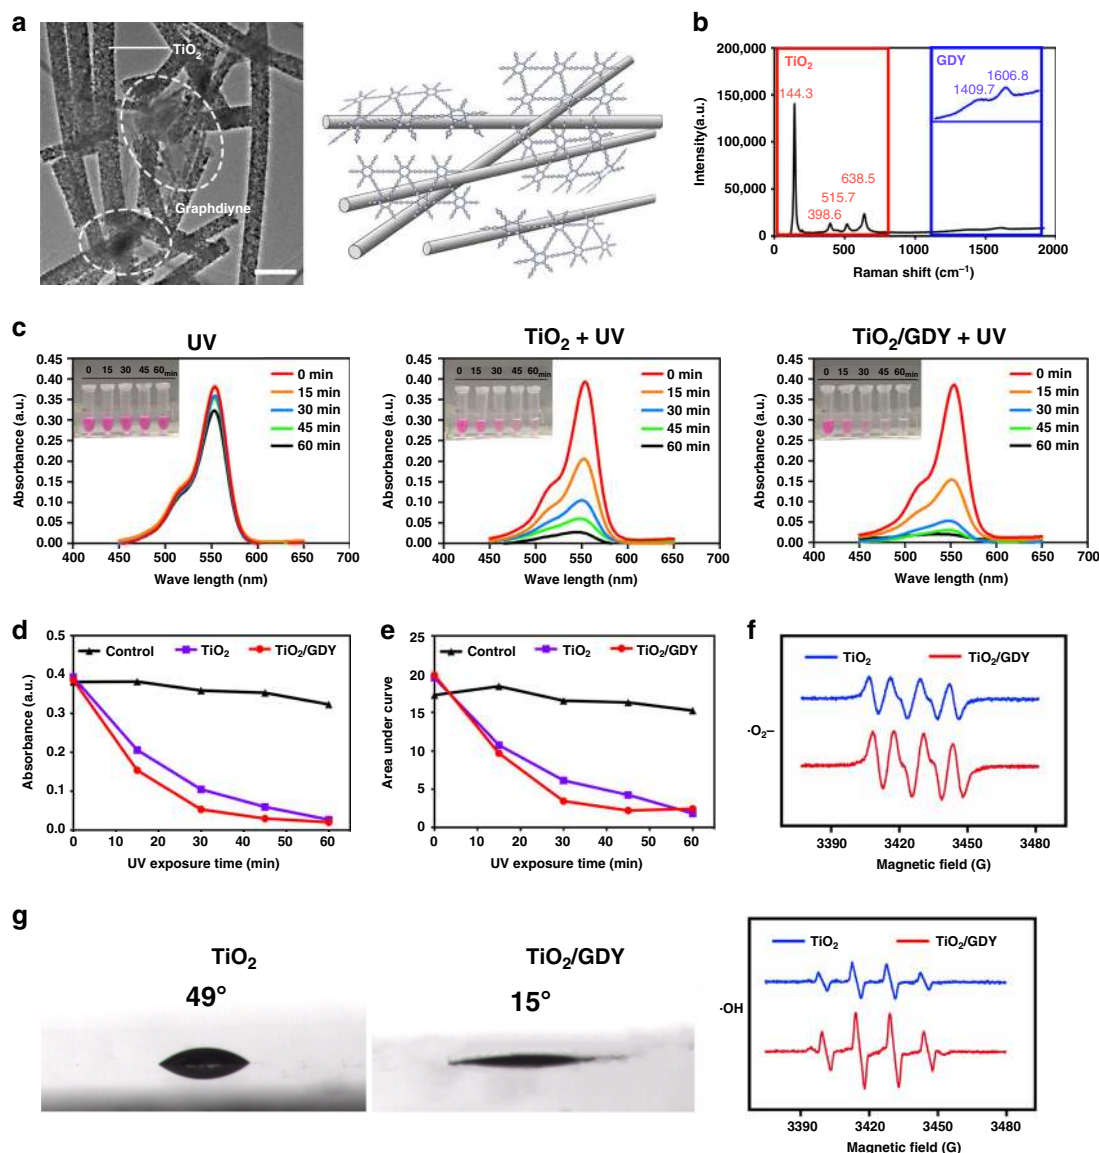


Fig. 1 Characterization and photocatalytic properties of TiO₂/GDY. **a** Transmission electron microscopy image of TiO₂/GDY ($n = 3$ separate materials) and illustration of the TiO₂/GDY structure (right). **b** Raman spectra of TiO₂/GDY. The main peaks of TiO₂ are shown in the red box, and the magnified peaks of GDY are shown in blue. **c** Absorption curves and photos of rhodamine B degradation by TiO₂ and TiO₂/GDY photocatalysis under UV irradiation for different times (0, 15, 30, 45, and 60 min). **d** Trends in the absorbance peaks of the RhB curves at each UV exposure time point. **e** Areas under the absorption curves at each time point. **f** Electron spin resonance for •OH (below) and •O₂⁻ (above) generation after TiO₂ (blue) and TiO₂/GDY (red) were induced by UV. **g** Contact angle measurements of TiO₂ and TiO₂/GDY nanofibers. Source data of **b–f** are provided as a Source Data file.

(Fig. 2d–f). TiO₂/GDY produced few dead cells (red) with or without UV irradiation, while TiO₂ nanofibers induced cell death without UV irradiation and caused a significant rise with UV irradiation (Fig. 2d, e; Supplementary Fig. 4). The CCK-8 assay on TiO₂/GDY with different GDY weight ratios revealed that TG0.5 used in this research showed good biocompatibility even at high concentrations (Supplementary Fig. 5). In summary, these results demonstrated that TiO₂/GDY exhibited favorable cell adhesion and biocompatible characteristics that contributed to cell proliferation and migration on the scaffold for bone regeneration.

Photocatalytic antibacterial effects of TiO₂/GDY in vitro. According to recent statistics, nearly 40% of *S. aureus*-caused orthopedic implant-associated infections are methicillin-resistant forms, and the constant rise of new resistance mechanisms

increases the difficulties of infectious disease treatment^{4,31}. Thus, we used MRSA to explore the antibacterial ability of TiO₂/GDY and develop a drug-resistant bacterium-associated implant infection model. Standard plate counting assay results showed that after pretreatment with the nanofibers and irradiation with UV, the number of live bacteria decreased significantly. The number of colonies of the TiO₂/GDY + UV group reduced by 98% compared to that of the group not treated with UV (Fig. 3a, b). In particular, TG0.5 exhibited the best antibacterial effect among various GDY proportions of nanofibers (Supplementary Fig. 6). Moreover, we compared the oxide graphene (GO) assembled TiO₂ nanofibers (TiO₂/GO) with TiO₂/GDY. It revealed that the colonies in photocatalytic TiO₂/GO treated group were twice as much as in photocatalytic TiO₂/GDY group and were much bigger, indicating TiO₂/GDY nanofibers got better sterilization effect after UV irradiation. Colonies in GO + UV and GDY + UV group were

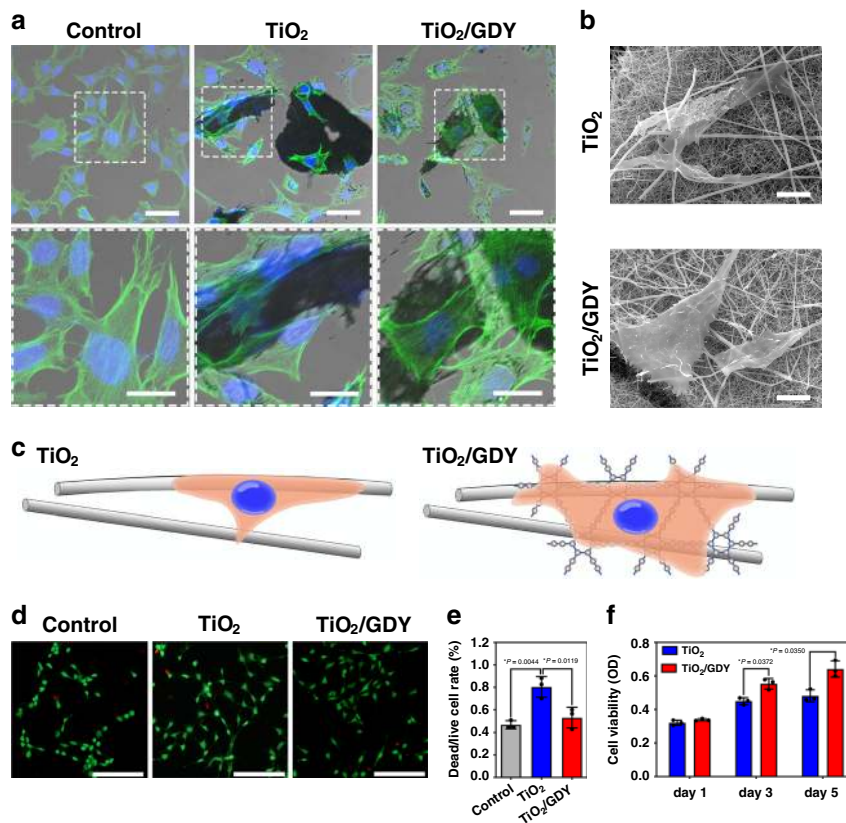


Fig. 2 Cell morphology and viability of TiO₂/GDY and TiO₂. **a** Cytoskeleton staining of MC3T3-E1 cells with FITC-tagged phalloidin (green) and DAPI (blue) after co-culturing with TiO₂ or TiO₂/GDY nanofibers for 24 h; scale bar = 50 μm (above); 25 μm (below) ($n = 3$ independent experiments). **b** SEM images showing the MC3T3-E1 cell morphology on nanofibers (scale bar = 10 μm). ($n = 3$ independent experiments). **c** Illustration of the states of cell adhesion on different nanofibers. **d** Live/dead staining with calcein AM (green) for live cells and PI (red) for dead and apoptotic MC3T3-E1 cells cultured with nanofibers (scale bar = 50 μm). **e** Ratio of PI- and calcein AM-stained positive cells quantitated from the live/dead stain. ($n = 3$). **f** Cell proliferation assay for MC3T3-E1 cells cultured with TiO₂ or TiO₂/GDY nanofibers for 1, 3, and 5 days. The data of **e**, **f** are shown as the mean ± S. D., error bars = Standard Deviation ($n = 3$ independent experiments, one-way ANOVA was applied for statistical analysis, * $p < 0.05$; ** $p < 0.01$). Source data of **e**, **f** are provided as a Source Data file.

slightly higher than PBS + UV group, as a result, the effects of GO or GDY alone were also excluded (Supplementary Fig. 7).

Because biofilm formation plays a pivotal role in the pathogenesis of implant infections³, we then investigated the biofilm eradication effect of TiO₂/GDY. By performing a live/dead staining assay on MRSA biofilms after photocatalytic treatments, we found that TiO₂/GDY after UV irradiation destroyed approximately 76% of the biofilm (Fig. 3c). The ratio of dead cells to live cells in the TiO₂/GDY + UV group was 4 times higher than that in the TiO₂ + UV group (Fig. 3d). Next, we investigated whether photocatalytic TiO₂/GDY could also prevent biofilm formation. After pretreatment with photocatalysis, MRSA cells were cultured for 24 h on slides and fixed for SEM scanning and crystal violet staining. SEM images of the TiO₂/GDY + UV group show a few single colonies, while those of other groups present several clusters with multiple colonies. The semiquantitative evaluation by crystal violet staining also revealed that TiO₂/GDY + UV group got the least biofilm formation (Fig. 3e, Supplementary Fig. 8). Furthermore, in the magnified SEM images, pits are observed on the photocatalysis-treated group, especially in TiO₂/GDY with UV irradiation. We attributed those pits to the cell wall perforation caused by ROS³².

Then, we detected the intracellular ROS production capacity of TiO₂/GDY-treated bacteria by a fluorescent ROS probe (DCFH-DA). As shown in Fig. 3f, g, GDY modification increased ROS generation in MRSA under UV irradiation compared with that in

other groups. In addition, ROS release after photocatalysis treatment was sustained for at least 60 min in the TiO₂/GDY + UV group (Fig. 3f). The above results proved that photocatalyst TiO₂/GDY could not only damage existing biofilms but also prevent biofilm formation. The SEM scanning of single bacteria at 0, 1 h after photocatalytic treatment indicated that the TiO₂/GDY + UV treatment destroyed the cell structure of MRSA (Supplementary Fig. 9a). Due to the small amount of ROS generation by near-UV irradiation, PBS + UV treatment also induced cell wall perforation but not as severe as TiO₂/GDY + UV. Moreover, the decrease of intracellular adenosine triphosphate (ATP) generation of TiO₂/GDY + UV group indicating that the cell metabolism was disrupted (Supplementary Fig. 9b).

Osteogenic effect of TiO₂/GDY and TiO₂ in vitro. To study the osteoinductive properties of the nanofibers in vitro, MC3T3-E1 cells were treated with TiO₂/GDY or TiO₂ nanofibers and cultured for 14 days. Alkaline phosphatase (ALP) is the most widely recognized biochemical marker for osteoblast activity during osteogenic differentiation³³. The ALP staining assay showed that the TiO₂/GDY-treated group exhibited a high ALP level (Fig. 4a, b). Alizarin Red S (ARS) staining revealed that the TiO₂/GDY-treated MC3T3-E1 cells had nearly twofold more calcium deposition and mineralization nodules than did the TiO₂ group (Fig. 4a, c). As comparison, GDY showed a slightly increase in ALP expression than GO, which contributed to the better osteoinductive ability of GDY-assembled

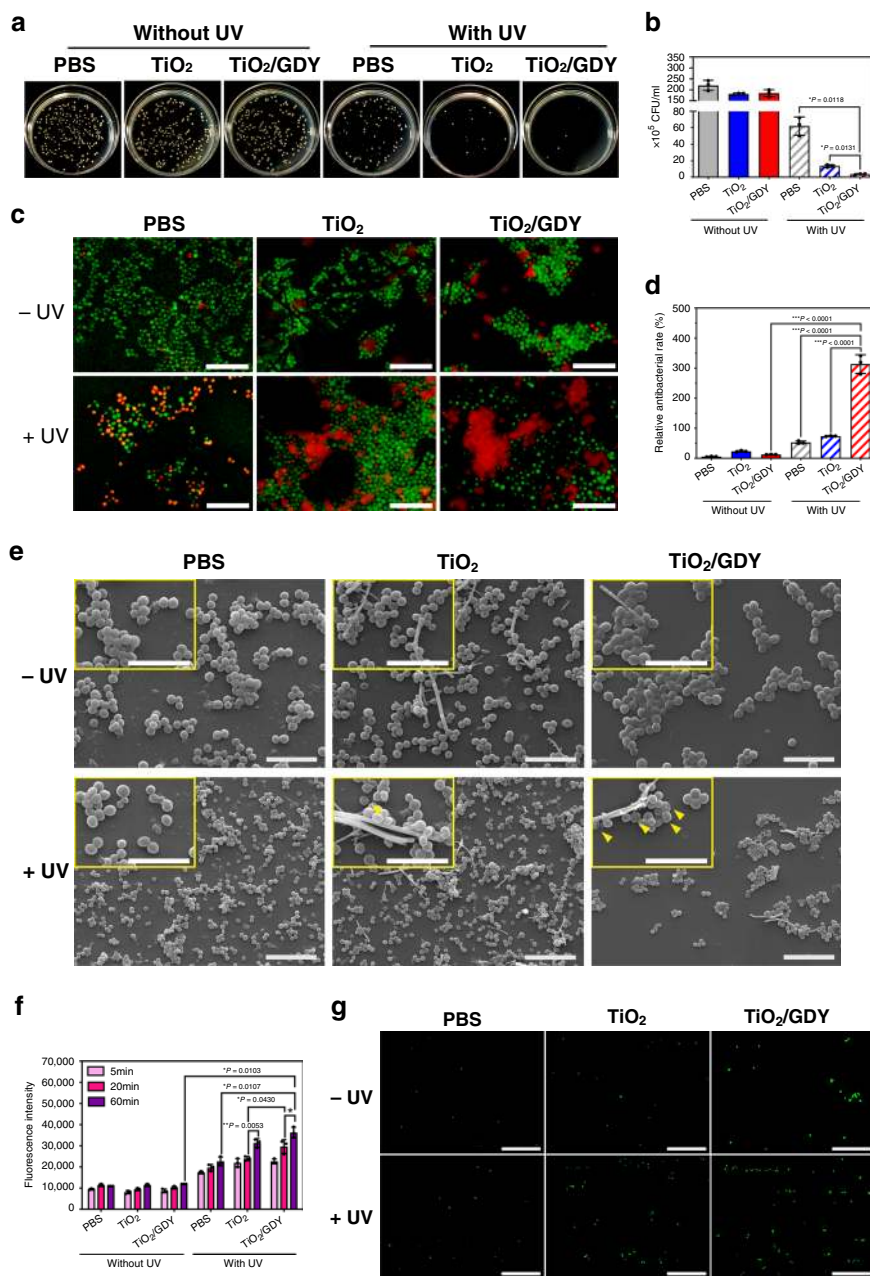


Fig. 3 Photocatalytic antibacterial effects of TiO_2/GDY and TiO_2 in vitro. MRSA were treated with TiO_2 , TiO_2/GDY or PBS, with or without UV (365 nm , 2 W cm^{-1}) irradiation. **a**, **b** Photos of agar plates and quantitative analysis of bacterial colonies. **c** Live/dead stained images of MRSA biofilms with photocatalytic treatment (scale bar = $10\ \mu\text{m}$). **d** Semiquantification of the live/dead staining for the ratio of PI- and calcein AM-stained areas. **e** SEM images of MRSA biofilms after exposure to photocatalytic treatment with nanofibers; yellow arrowheads in the magnified inset images indicate holes on the bacterial surface; scale bar = $5\ \mu\text{m}$ (upper), $10\ \mu\text{m}$ (below). **f** Quantitative analysis of radical oxygen species (ROS) in MRSA 5, 20, and 60 min after photocatalytic treatment. **g** Fluorescence images of ROS in bacteria for 24 h (FITC-tagged probes); scale bar = $100\ \mu\text{m}$. The data of **b**, **d** and **f** are shown as the mean \pm S. D., error bars = Standard Deviation ($n = 3$ independent experiments, one-way ANOVA was applied in **b**, **d**, and multiple t test was applied in **f** for statistical analysis, $*p < 0.05$; $**p < 0.01$; $***p < 0.001$). Source data of **b**, **d**, **f** are provided as a Source Data file.

TiO_2 . In addition, the pretreating of UV irradiation on materials has no significant effect on cell osteogenic differentiation (Supplementary Fig. 10).

Studies have shown that graphene has the ability to preconcentrate osteoinducers such as dexamethasone and β -glycerophosphate to promote osteogenic differentiation³⁴. Therefore, we asked whether GDY modification acted in the same mechanism. We determined the capacities of TG0.5, TG0.25, and TiO_2 nanofibers to load dexamethasone by UV spectrophotometry. The adsorption isotherms showed that TG0.5 had the highest amount

of dexamethasone adsorption after 1 day of incubation (Fig. 4d). The adsorbed dexamethasone can induce the expression of proteins and enzymes required during bone differentiation, thus leading to increased mineral deposition³⁵. These results confirmed that TiO_2/GDY nanofibers were equipped with outstanding osteoinductive properties and deserve to be an ideal implant material for bone regeneration. ALP, Osteocalcin (OCN), Osterix (OSX), and Collagen 1a (Col1a) are all osteogenetic markers in early stage of bone remodeling^{36,37}. Real time-qPCR assay revealed that both TiO_2/GO and TiO_2/GDY could enhance the

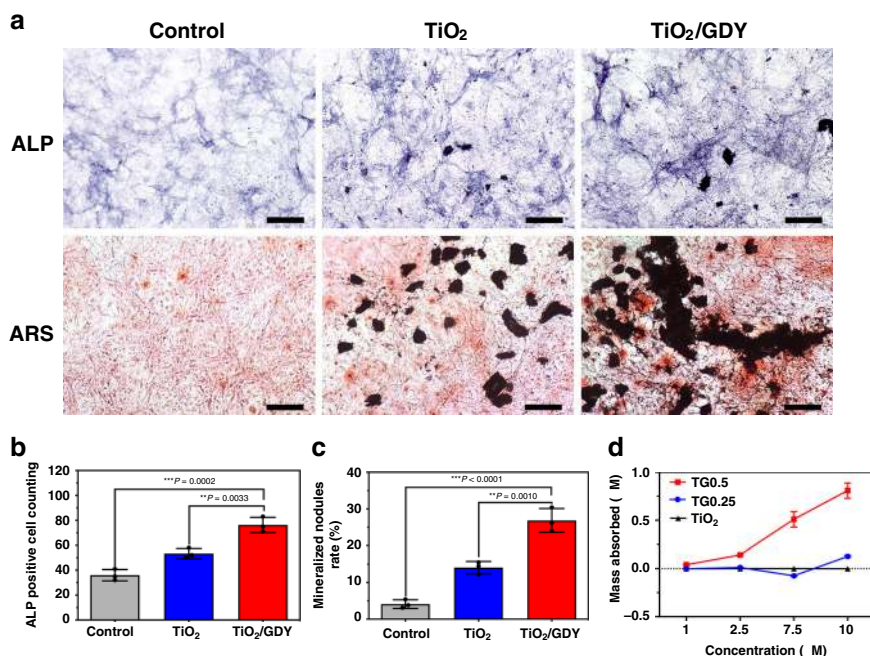


Fig. 4 Osteogenic effect of TiO₂/GDY and TiO₂ in vitro. MC3T3-E1 cells were cultured with TiO₂, TiO₂/GDY or PBS under osteogenic induction. **a** Alkaline phosphatase activity (upper labeled ALP) and Alizarin Red S staining (lower labeled ARS) on day 14. **b, c** Semiquantitative analysis of ALP activity and ARS staining. **d** Loading capacity of dexamethasone on TiO₂/GDY (TG0.25, TG0.5) and TiO₂ nanofibers for 24 h. Scale bar = 100 μm. The data are shown as the mean ± S.D., error bars = Standard Deviation (*n* = 3 independent experiments). One-way ANOVA was applied for statistical analysis in **b, c** (**p* < 0.05; ***p* < 0.01; ****p* < 0.001). Source data of **b–d** are provided as a Source Data file.

expression of osteogenesis factors which promoted osteoblast differentiation. While the TiO₂/GDY treatment showed a better enhancement on ALP expression (Supplementary Fig. 11), which was also convinced by the ALP staining.

Antibacterial and osteogenic effects of TiO₂/GDY in vivo. After confirming the antibacterial and osteoinductive properties of TiO₂/GDY in vitro, we then established implant-associated infection models to verify the nanofibers' in vivo therapeutic effects. Five days after surgery, we counted the bacterial colonies in the grinding fluid of the implanted femur. Plate counting results showed that there was 85% less MRSA in TiO₂/GDY + UV-treated femurs than in the PBS group, better than GO + UV, GDY + UV, TiO₂/GO + UV, and TiO₂ + UV group (Fig. 5a, b; Supplementary Figs. 12, 13), which indicated that TiO₂/GDY could effectively inhibit bacterial infection with UV irradiation under the condition of MRSA contamination during implantation.

To explore the in vivo cell compatibility of nanofibers, we scanned the implanted nanofibers by SEM 5 days after implantation (Fig. 5c). Consistent with the in vitro observations, cells appeared to attach firmly on the surface of the GDY-assembled nanofibers. Then, we used hematoxylin–eosin (H&E) staining to reveal the pathological features of femur infections. Figure 5d shows that the PBS, PBS + UV and TiO₂ + UV groups all had significant infected and necrotic zones (orange dotted lines) in the bone defect area, while the TiO₂/GDY + UV group showed minimal inflammatory cell infiltration. Furthermore, the TiO₂/GDY + UV group had the widest new bone regeneration area (blue dotted lines, Fig. 5d and Supplementary Figs. 14 and 15). Immunohistochemical assays on the expression of the osteogenesis marker osteopontin (OPN) revealed many OPN-positive cells in the TiO₂/GDY-implanted femurs (Fig. 5d and Supplementary Fig. 14). The results above all confirmed that TiO₂/GDY provided a good osteoinductive microenvironment

in vivo. In contrast, without UV irradiation, the femurs barely exhibited new bone formation and were filled with infectious tissue (Supplementary Fig. 14a), which proved the vital role of the antibacterial process during bone infections.

Four weeks after surgery, we conducted Masson staining to evaluate the bone regeneration status. The PBS group still had an unhealed hole and chronic infection with necrotic tissue in the bone marrow (Fig. 5e). However, the bone defect implanted with TiO₂/GDY was completely healed with the generation of large amounts of new bone (blue staining in dashed boxes). In comparison, the bone masses of the PBS + UV and TiO₂ + UV groups were inadequate, and the process of bone regeneration was very slow (Supplementary Fig. 16). H&E staining images also exhibit the bone remodeling levels of different groups (Supplementary Fig. 17). Both GDY + UV and GO + UV group got great new bone formation surrounded the implants but there were still unhealed bone defects. We attributed this to the insufficient bactericidal effects and non-supporting structure in the absence of TiO₂ nanofibers. In addition, organs in mice were collected and observed with H&E staining for histological toxicity evaluation (Supplementary Fig. 18). There was no significant difference between nanofiber-implanted groups and the PBS control group. It reveals that the systematic toxicity of nanofibers could be neglected. Taken together, the in vivo studies verified the combined outstanding bactericidal and osteogenic properties of TiO₂/GDY in implant-associated infections.

Discussion

Implant device-associated infections are a series of typical complications affecting the prognosis of orthopedic surgery. Titanium implants may become loose and displaced with delayed healing afterwards. Furthermore, bacteria spreading within the entire body lead to local bone loss, amputation, systemic inflammation, and even sepsis^{3,5,6}. Although TiO₂ itself has a certain degree of antibacterial effects when induced by UV light, the effects are

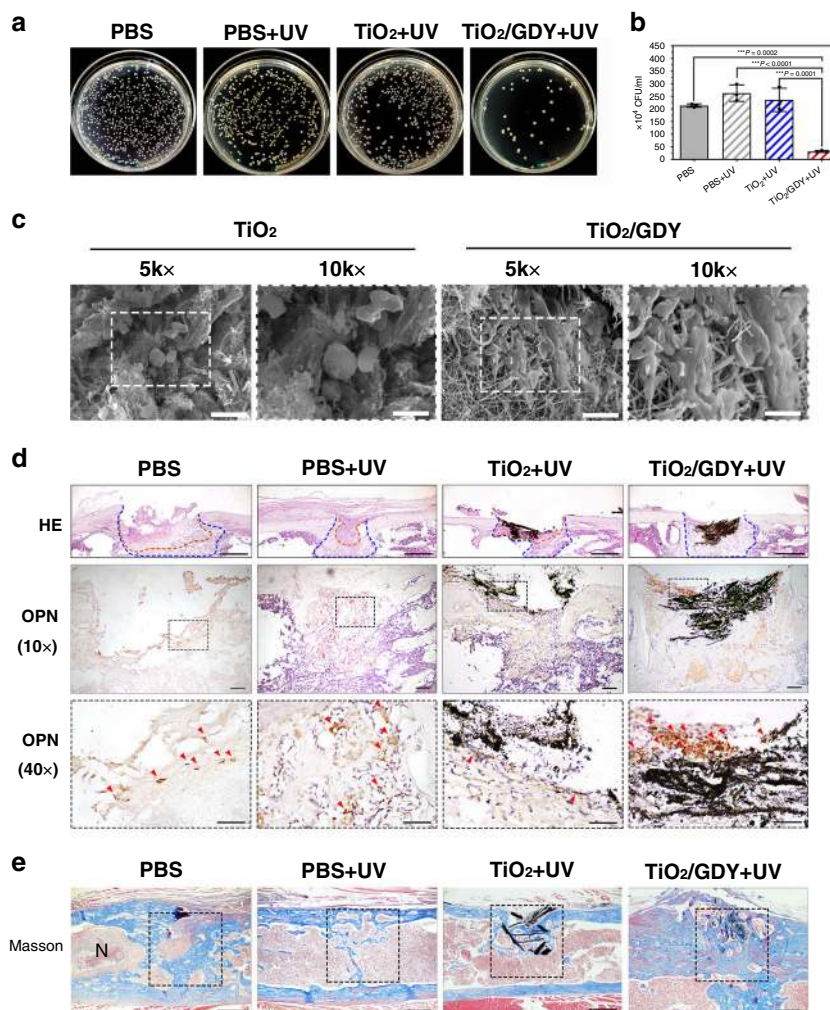


Fig. 5 Antibacterial and osteogenic effects of TiO₂/GDY in vivo. **a, b** Photographs and quantitative analysis of the bacterial colonies of the infected femurs treated with TiO₂, TiO₂/GDY, or PBS as a control, with UV irradiation (365 nm, 2 W cm⁻¹, 5 min). The data are shown as the mean ± S.D., error bars = Standard Deviation (*n* = 3 biological independent samples, one-way ANOVA was applied for statistical analysis, **p* < 0.05; ***p* < 0.01; ****p* < 0.001). **c** SEM images of the mouse femur tissues with TiO₂ or TiO₂/GDY nanofiber implantation after 5 days, with ×5000 (left) and ×10,000 (right) magnification, scale bar = 10 μm (left), 5 μm (right). (*n* = 3 biological independent samples). **d** H&E staining and immunohistochemical staining of infected tissues after 5 days. Orange dotted lines in the H&E images represent infectious and necrotic areas; between the orange and blue dotted lines are new bone formation areas (scale bar = 500 μm). OPN 40×: scale bar = 50 μm; OPN 10×: scale bar = 100 μm, and red arrowheads point out OPN-positive osteoblasts. (*n* = 3 biological independent samples). **e** Masson staining for bone formation after 4 weeks (scale bar = 500 μm). “N” in the PBS image represents the necrotic tissue in the bone marrow. (*n* = 3 biological independent samples.) Source data of (b) are provided as a Source Data file.

limited since the photocatalytic effect of TiO₂ alone is extremely transient^{12,38}. Researchers have introduced antibiotics and metal nanoparticles onto titanium implant scaffolds to enhance bacteriostatic efficacy, but these studies still exhibit various drawbacks^{14,15}. In this study, we changed the zeta potential of TiO₂ nanofibers to positive and the charge of a novel two-dimensional carbon-based nanomaterial, GDY, to negative to synthesize a GDY-combined TiO₂ heterojunction to enhance the photocatalytic effect^{39,40}. Further, our previous XPS results indicated that GDY contained oxyfunctional groups, such as C–OH and C=O²³. After the composites were calcined at 350 °C for 2 h, a strong interaction was produced between TiO₂ and GDY due to their chemical action, hydrogen bonding and van der Waals force. This results in the composites with high structure stability in vivo experiments.

The TEM image and chemical bond analysis of the Raman spectra illustrated that the TiO₂/GDY compound was successfully synthesized with a GDY sheet attached to the surface of TiO₂ nanofibers. TiO₂/GDY maintained the nanostructure with a large

specific surface area and a porous network. In addition to its typical application as an orthopedic implant material, TiO₂ is also a widely developed semiconductor metal oxide with photocatalytic performance⁴¹. With UV irradiation, electrons are excited from the valence band to the conduction band, producing electron–hole pairs. Free electrons migrate to the surface of TiO₂ and participate in redox reactions, producing ROS such as hydroxyl radicals, superoxide anions, and hydrogen peroxide (H₂O₂)¹². However, the high recombination rate of electrons and holes in TiO₂ restrains its photocatalytic antibacterial effect. Studies have been conducted to improve the photocatalytic efficiency of TiO₂, such as by reducing the particle size⁴², modifying the nanoscale surface, and doping with Cd or other elements^{43–45}. As the only two-dimensional carbon nanomaterial containing both *sp* and *sp*² hybrid carbon atoms, GDY has a rigid carbon mesh and a natural band gap, which result in a large specific surface area and high hole mobility^{22,23,40,46}. The superior conductive GDY assemblage made the free electrons generated on TiO₂ under UV irradiation easily adsorb on the surface of GDY,

thereby reducing the recombination rate and intensifying the photocatalytic performance. As evidence, RhB degraded more rapidly by photocatalytic TiO₂/GDY than by pure TiO₂. In addition, the generation of ROS including ·OH, ·O₂⁻, 1O₂, ·OOH, and H₂O₂ was also detected through ESR and ferric ion titration method. Oxidative cellular damage or oxidative stress occurs when the oxidation ability of ROS overpowers that of antioxidants in the living organisms. If the balance between the generation and the detoxification of ROS is disturbed due to oxidative stress, the viability of the cells would decrease. ROS inhibit bacteria through interference of bacteria metabolism, cell wall proliferation and induction of DNA damage^{47,48}. For example, hydroxyl radicals can attach to cell walls and consequently cause cell destruction through the rapid release of potassium ions or the oxidation and degradation of intracellular CoA enzyme^{12,49}. On SEM images in this research, pits were found on the bacterial surface with photocatalytic treatment (Fig. 3e). After 1 h UV irradiation, bacterial structure was destroyed (Supplementary Fig. 9a). In addition, as ATP is the essential energy source of cell metabolism generated from respiratory action, the lowest ATP level in TiO₂/GDY + UV group exhibited that the bacterial metabolism was significantly inhibited (Supplementary Fig. 9b).

A primary problem of medical device-associated infections, biofilms are responsible for the persistence of implant infections and are a source of bacterial dissemination to other sites in the body^{3,50}. In this study, the biofilm staining assay of MRSA demonstrated that TiO₂/GDY nanofibers could not only effectively eliminate bacteria in the mature biofilms but also inhibit biofilm formation (Fig. 3c, e). In the implant-associated infection models, no local necrotic infection area was observed in femurs implanted with UV-irradiated TiO₂/GDY where the bone tissue was well repaired (Fig. 5d). Although TiO₂/GDY did not exhibit remarkable improvement in the photocatalytic antibacterial effect compared to that exhibited by TiO₂ nanofibers *in vitro*, the combined characteristics of TiO₂/GDY made it much more efficient for *in vivo* treatment.

In the antibacterial experiment, a low dose of near-ultraviolet light (365 nm, 2 W cm⁻¹) was applied within a short time. Because near-ultraviolet light has a sterilization effect by damaging DNA and generating ROS⁵¹, the group with UV irradiation alone showed a certain antibacterial effect *in vitro*. However, the bactericidal effect of low-dose UV light alone was far lower than the synergistic effect with nanofibers. In addition, the cell viability assay showed no cytotoxicity of TiO₂/GDY on eukaryotes under irradiation, indicating favorable biocompatibility of the TiO₂/GDY treatment. The sterilization effect of oxygen radical (such as: ·OH, ·O₂⁻, 1O₂, ·OOH) is transient in general. However, the produced H₂O₂ has long lifetime and continuous bactericidal effect after the UV was turned off⁵². Therefore, it is not surprising that a sustained antibacterial effect was observed after employment. For *in vivo* application, we treated MRSA-contaminated nanofibers with UV irradiation before implantation to completely eliminate pathogens and avoid unnecessary tissue damage caused by UV irradiation.

In addition to antibacterial properties, ideal tissue engineering scaffolds with great osteoinductive properties are also required. GDY-based quantum dots were reported to be a potential new fluorescence reagent for imaging and theranostics, which exhibited high biocompatibility and bioactivity both *in vitro* and *in vivo*⁵³. It has been reported that the high surface energy of a hydrophilic surface can strengthen the interaction with cells and proteins in the early stage of tissue regeneration⁵⁴. Carbon-based nanomaterials have been composited as an effective strategy to improve membrane surface hydrophilicity^{55–57}. Accordingly, GDY-assembled TiO₂ nanofibers showed improved

hydrophilicity (Fig. 1g). This is due to the hydrophilic functional groups linked to the *sp* and *sp*² hybridized carbon atoms of GDY²⁴. In addition, the 2D and porous structure of GDY contributes to water diffusion²³. The scaffold material surface with high hydrophilicity favors cell adhesion and proliferation. The cytoskeleton staining, SEM images and cell proliferation assays showed that TiO₂/GDY nanofibers were beneficial to cell adhesion and proliferation (Fig. 2). The SEM results of the implant materials *in vivo* further verified the excellent guidance property of TiO₂/GDY for cell adhesion (Fig. 5c). Although MRSA might tend to adhere to the nanofibers, ROS produced on the materials through photocatalytic effects can effectively eliminate the bacteria in an instant.

In addition, GDY-assembled TiO₂ nanofibers exhibited improved biocompatibility. The SEM images and live/dead staining of osteoblasts reveal that TiO₂ nanofibers alone were cytotoxic to some extent, leading to abnormal cell morphology and membrane perforation (Fig. 2a, b). With a kind of high aspect ratio nanostructure, TiO₂ nanofibers were reported to initiate incomplete cell phagocytosis, raise the expression of inflammatory cytokines, and promote the oxidative stress of cells to cause apoptosis^{58,59}. GDY as a kind of two-dimensional polymers, is flexible and scan cover the surface of TiO₂ nanofibers. As a result, it could improve the interaction between TiO₂ nanofibers and biological tissues. In addition, due to the unique conjugate π bond system and conjugate diacetylene bond, GDY has been shown to have a long-term scavenging effect on intracellular free radicals⁶⁰. However, our results revealed that photocatalytic TiO₂/GDY still produced significant ROS generation and sterilization effects. We inferred that the free radical scavenging effect of the GDY component in the nanofibers was nearly negligible compared with the robust photocatalytic effect under irradiation in a very short time. In contrast, during the long-term implantation period in bone tissues, the free radical scavenging property made the nanofibers less cytotoxic than pure TiO₂. As a result, TiO₂/GDY not only has photocatalytic antibacterial effects on ROS production but also possesses long-term tissue regeneration guidance properties.

Studies have revealed that the expression of osteogenic genes increases on more hydrophilic surfaces⁶¹. In addition, some carbon-based nanomaterials, such as graphene, could promote osteogenic differentiation through protein or osteoinductive component adsorption⁶². In this research, GDY assemblage improved the surface hydrophilicity of nanofibers and increased the absorption of small molecules due to the conjugated π bond system. With the increased ratio of GDY in the TiO₂/GDY compound, the adsorption of dexamethasone, a main effective molecule for osteogenic differentiation, became stronger. In the implant-associated infection model, the TiO₂/GDY-implanted group showed a significant increase in OPN expression on the fifth day and exhibited the richest new bone formation on the fourth week after implantation *in vivo*. Due to the negative potential of GDY surface, it would be beneficial to calcium deposition⁶³. In addition, GDY nanosheets possess a high surface area, suggesting that they have a better drug loading capacity⁶⁴. These indicated that the specific structure of GDY significantly improved the osteoinductive ability of TiO₂ nanofibers. In the early stage of osteogenesis, progenitors differentiating into mature-osteoblasts requires varies of transcription factors, including Runx2 and Osterix. Then the differentiated osteoblasts will activate Col1 and OCN genes to secrete matrix such as collagen fibrils. During late stage of mineralization, OCN has a high affinity toward bone and extracellular matrix to induce the calcium deposition. Meanwhile, ALP is able to hydrolyze pyrophosphates (PPi) to generate inorganic orthophosphates (Pi), which participate well in phosphorus metabolism and late biomineralization^{36,37}. The enhanced expressions of Col1a, OCN,

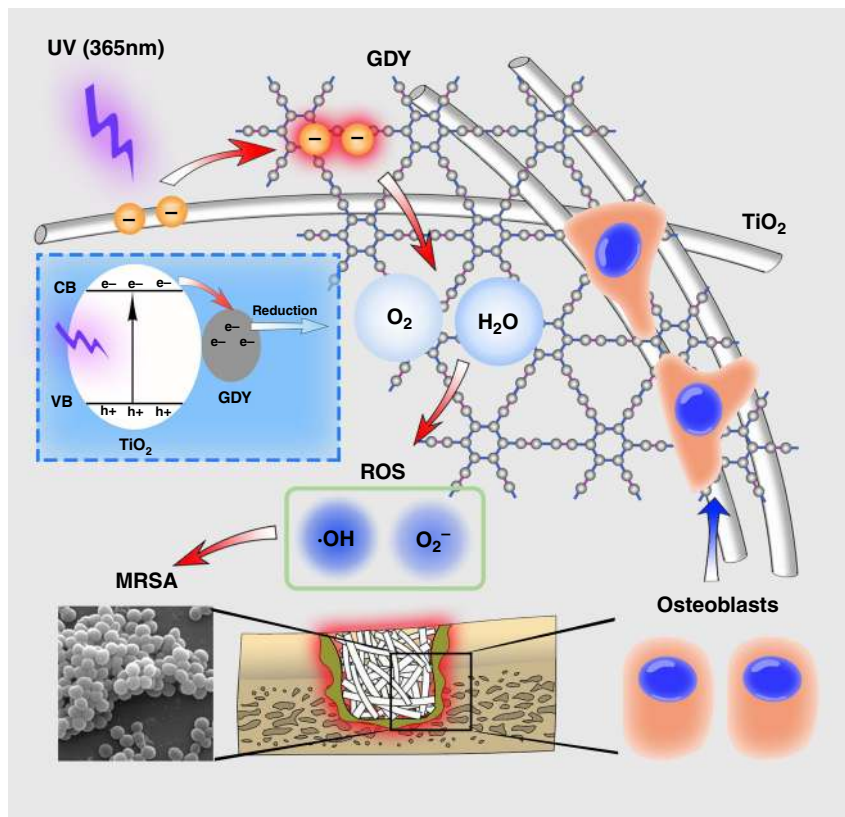


Fig. 6 Schematic of the dual function of TiO₂/GDY in orthopedic implant infection. On the one hand, electrons transferred from UV (365 nm)-irradiated TiO₂ nanofibers to GDY resulted in more reactive oxygen species generation for sterilization. On the other hand, osteoblasts tended to adhere to the nanofibers due to the great biocompatibility of GDY. The blue dashed box exhibits the free electron generation and transfer in TiO₂/GDY. “e⁻” in the blue dashed box represents negative electron, while “h⁺” represents positive hole.

OSX, and ALP indicate that TiO₂/GDY could improve osteoblast differentiation and bone mineralization (Supplementary Fig. 11).

In conclusion, we prepared GDY-assembled TiO₂ nanofibers to intensify their photocatalytic antibacterial effect and long-term osteoinductive ability (Fig. 6). With UV irradiation, the free electrons from the photocatalytic-activated TiO₂ transferred to GDY surface and had longer lifetime, so that the activated state of TiO₂ was prolonged with more ROS (including oxygen radical and hydrogen peroxide) generation for sterilization (red arrows). On the other hand, GDY-assembled TiO₂ nanofibers showed great biocompatibility to promote cell adhesion and bone tissue regeneration (blue arrows). Our study not only provided a difunctional TiO₂/GDY nanofiber as an ideal bone implant but also suggested an effective modification strategy for titanium implants to prevent implant device-associated infections.

Methods

Materials preparation. First, 4 g of tetrabutyl titanate (TBT) and 1.5 g of Polyvinyl pyrrolidone (PVP, $M_w = 1.3 \times 10^6$) were added to a mixed solution of ethanol (20 g) and acetic acid (4 g) under magnetic stirring for 5 h. Then, the obtained transparent pale-yellow solution was transferred into a 20 mL syringe. The voltage of electrospinning setup and the feeding rate of solution was 20 kV and 2.5 mL h⁻¹, respectively. The distance of needle-to-static collector was 10 cm. The collected TiO₂ fiber precursor was heat-treated at 550 °C for 2 h in air to fabricate TiO₂ nanofibers.

GDY used in this work was provided by Institute of Chemistry, Chinese Academy of Science⁶⁵. A zeta potential analyzer was used to measure the zeta potential of TiO₂ and GDY in water at pH 4, which are +15.1 mV and -19.2 mV, respectively. Typically, TiO₂ nanofibers (200 mg) were dispersed in water at pH = 4, then, magnetically stirred for 1 h at room temperature. Meanwhile, 10 mg of GDY was dispersed in a mixture solution of water (30 mL) and ethanol (60 mL) under sonication irradiation for 2 h. Afterwards, a certain amount of GDY solution was added into the TiO₂ suspension by stirring vigorously for 1 h. TiO₂ and GDY were electrostatically self-assembled. Subsequently, the solvents were removed. the

obtained composites were calcined at 350 °C for 2 h. The *x* in “TG_{*x*}” represents the added GDY weight ratio. The TiO₂/GDY applied in the following experiments was the typical TG 0.5.

Material characterization and photocatalytic properties. The microstructure of TiO₂/GDY was characterized by TEM (Titan G2 60-300). The molecular structure was detected by Raman spectroscopy (Renishaw Co. RM1000). The surface contact angles of TiO₂/GDY and TiO₂ nanofibers were detected by a contact angle meter (Powereach[®] JC2000C1).

A RhB degradation assay was carried out to detect the photocatalytic activity of TiO₂/GDY and TiO₂ nanofibers. 1 mL of 8 μg mL⁻¹ RhB solution and 100 μg of photocatalysts (TiO₂/GDY or TiO₂) were added into ep tubes and exposed to 365 nm UV light (2 W cm⁻² for up to 60 min) (Yinzhū, UVEC-4II, China). Each sample was centrifuged for 5 min at 1000 × *g*. The absorbance of the supernatants was detected by an UV spectrophotometer (SOPTOP, UV2800, China).

The ability of TiO₂/GDY and TiO₂ nanofibers to generate ·OH and ·O₂⁻ was respectively measured in water and methanol under 300 W Xe lamp irradiation using ESR (Bruke, emx nano) at room temperature and 5,5-Dimethyl-1-Pyrroline N-oxide (DMPO) as spin trapping reagent. For measuring the generation of 1O₂ and ·OOH, 2,2,6,6-tetramethyl-piperidine (TEMP) and DMPO were used as trapping reagent. The measurement was performed in water using ESR (Bruke, a300) at room temperature. The generation of H₂O₂ was characterized by ferric ion titration method. Fifteen milligrams of photocatalysts were suspended in 15 mL of H₂O and ultrasonicated for 5 min. The suspension was firstly bubbled with high-purity O₂ for 30 min and irradiated with 300 W Xe lamp for 3 h. The H₂O₂ concentration was measured every 1 h. After turning off the light, H₂O₂ level was also tested continuously in 30 and 60 min.

Cell morphology and viability. The murine-derived osteoblast-like cells MC3T3-E1 were cultured in α-minimal essential medium (Hyclone, Thermo Fisher Scientific Inc.) supplemented with 10% FBS (FBS, Gibco) and maintained at 37 °C in 5% CO₂ and 95% air in a humidified incubator.

The MC3T3-E1 cells were incubated on confocal dishes at a density of 6 × 10⁴ cell per dish with 20 μg mL⁻¹ TiO₂/GDY or TiO₂ nanofibers for 24 h. After washed with phosphate buffered saline (PBS) solution, cells were fixed with 4% paraformaldehyde (PFA) for 10 min at room temperature. Removed PFA and washed with PBS, then cells were permeabilized with -20 °C acetone for 5 min.

The F-actin and nuclei were stained with FITC Phalloidin (Yeasen, 40735ES75) and DAPI, respectively and observed by laser scanning confocal microscope (LSCM, Leica-LCS-SP8-STED). 25 of random adhered cell areas of each group were calculated through Image J. Adhered cell number was analyzed by DAPI staining of cell nucleuses.

For SEM scanning, MC3T3-E1 cells were seeded on 24-well cell culture plates at a density of 2×10^4 cells per well with $20 \mu\text{g mL}^{-1}$ TiO₂/GDY or TiO₂ nanofibers and incubated for 24 h. After washing with PBS, cells were fixed with 2.5% glutaraldehyde overnight at 4 °C. The samples were washed 3 times with water, then freeze-dried. Followed by sputter coated with gold, samples were observed by SEM (TESCAN VEGA 3 LMU) with an accelerating voltage of 20 kV and a working distance of 11.7 mm.

The live/dead staining assay was carried out with Calcein-AM/PI Double Stain Kit (Yeasen, 40747ES80). In brief, cells were seeded onto glass coverslips in 24-well cell culture plates at a density of 2×10^4 cells per well. $20 \mu\text{g mL}^{-1}$ TiO₂/GDY or TiO₂ nanofibers were added to cells without UV irradiation, received UV (365 nm , 2 W cm^{-2}) irradiation together with cells, or received UV irradiation before addition. After 24 h incubation, the glass coverslips were rinsed with 1 × Assay Buffer for 3 times. Afterwards, the coverslips were incubated with $2 \mu\text{M}$ Calcein-AM and $1 \mu\text{M}$ propidium iodide (PI) in 1 × Assay Buffer for 15 min at 37 °C. Images were taken using a fluorescence microscope (Zeiss Axio Imager A2). The numbers of live and dead cells were counted by Image J.

Cell proliferation was evaluated by the cell counting kit-8 (CCK-8) assay. MC3T3-E1 cells were seeded in 96-well cell culture plate with 5×10^3 cells per well and incubated overnight for attachment. Then cells were exposed to various concentrations of TiO₂/GDY or TiO₂ nanofibers from 1 to $50 \mu\text{g mL}^{-1}$. At the time points of 1, 3, 5-day incubation, cells were incubated with the CCK-8 agent (Dojindo, Japan) diluted 1:10 with culture medium for 2 h. Then the absorbances were measured by a microplate reader scanning at 450 nm (PowerWave XS2, BioTek, Winoski, VT, USA). The assays were implemented triplicated with three independent experiments.

Antibacterial properties in vitro. MRSA USA 300 were cultured in an aerobic environment in LB broth at 37 °C. The bacterial suspension was diluted to 10^9 colony forming units (CFU mL⁻¹) for experimental use after measuring the absorbance at 600 nm using the UV spectrophotometer.

For bacterial standard plate counting assay, MRSA cells were prepared in 20 mL liquid LB medium into 10^9 CFU mL⁻¹ and then added with various ratios of TiO₂/GDY, TiO₂, TiO₂/GO ($100 \mu\text{g mL}^{-1}$), GO, GDY ($50 \mu\text{g mL}^{-1}$) or PBS as control. After 1 h incubation, cells were irradiated with UV (365 nm , 2 W cm^{-2}) for 5 min, then 25 μL bacterial suspensions were spread onto LB agar plates. The images were taken, and the colonies were counted using Image J software after 24 h incubation.

The property of biofilm destruction by photocatalysis was determined through live/dead staining. Five hundred microliters 10^9 CFU mL⁻¹ MRSA suspensions were seeded onto 10% Poly-L-Lysine pretreated glass coverslips and incubated 24 h to obtain biofilms in advance. TiO₂/GDY or TiO₂ nanofibers were added onto the biofilms with UV irradiation for 5 min. Then the live/dead staining was carried out with Calcein-AM/PI Double Stain Kit. The glass coverslips were rinsed with 1 × Assay Buffer for 3 times. Afterwards, the coverslips were incubated with $2 \mu\text{M}$ Calcein-AM and $1 \mu\text{M}$ propidium iodide (PI) in 1 × Assay Buffer for 15 min at 37 °C. Images were taken using a fluorescence microscope (Zeiss Axio Imager A2). The numbers of live and dead cells were counted by Image J.

The effect on the bacterial biofilm formation was investigated through SEM scanning. 10^9 CFU mL⁻¹ MRSA cells were mixed with $100 \mu\text{g mL}^{-1}$ TiO₂/GDY or TiO₂ nanofibers and exposed to UV for 5 min. Five hundred microliters bacterial suspensions were seeded onto a 10% Poly-L-Lysine pretreated glass coverslip and incubated 24 h to form bacterial biofilm. Then the biofilms were washed with PBS and fixed with 2.5% glutaraldehyde overnight at 4 °C. The samples were washed 3 times with water, then freeze-dried. Followed by sputter coated with gold, samples were observed by SEM (TESCAN VEGA 3 LMU) with an accelerating voltage of 20 kV and a working distance of 10.5 mm.

Crystal violet staining was carried out for semi-amount evaluation of biofilm formation. 10^9 CFU mL⁻¹ MRSA cells were mixed with $100 \mu\text{g mL}^{-1}$ TiO₂/GDY or TiO₂ nanofibers and exposed to UV (2 mW cm^{-2}) for 5 min. Ten microliters bacterial suspensions were added to 100 μL LB medium in 96-well plate. After 24 h incubation in 37 °C, the biofilms were rinsed and fixed with 4% of PFA for 10 min. Then crystal violet (Servicebio, China) was added 50 μL per well. After 20 min incubation in room temperature, removed the dye liquor and rinsed with ddH₂O.

Ethyl alcohol was added 100 μL per well for dissolution. Absorbance at 590 nm of each well was measured after 20 min shaking (Molecular Devicesmd, spectramax i3x).

ROS generation in MRSA was tested using a ROS assay kit (Beyotime, China). MRSA cells (10^9 CFU mL⁻¹) were loaded with the fluorescence probe (DCFH-DA) in 37 °C for 20 min. Then the bacteria were incubated with $100 \mu\text{g mL}^{-1}$ TiO₂/GDY or TiO₂ nanofibers and exposed to UV for 5 min. The fluorescence intensity of DCF, denoted the intracellular ROS generation, was measured 5, 20, 60 min after UV irradiation (Molecular Devicesmd, spectramax i3x). Images of fluorescence were observed using the fluorescence microscope (Zeiss Axio Imager A2).

10^9 CFU mL⁻¹ MRSA cells were incubated with $100 \mu\text{g mL}^{-1}$ TiO₂/GDY or TiO₂ nanofibers and exposed to UV for 5 min. ATP levels evaluation was carried out in accordance with the manufacturer's protocol (Promega, G8320). For bacterial structure observation, 10^9 CFU mL⁻¹ MRSA cells were incubated with $100 \mu\text{g mL}^{-1}$ TiO₂/GDY or TiO₂ nanofibers and exposed to UV for 1 h. Cells were fixed and observed with SEM 0, 1 h after treatment.

Osteogenesis properties in vitro. MC3T3-E1 cells were cultured in 24-well plates at a density of 5×10^4 cells per well. After 24 h incubation, the culture medium was replaced by the osteogenic differentiation media consisting of 10 mM of β-glycerophosphate, 10 nM of dexamethasone and 0.2 mM of L-ascorbic acid 2-phosphate (Sigma-Aldrich). Then $20 \mu\text{g mL}^{-1}$ of TiO₂/GDY, TiO₂/GO or TiO₂ nanofibers, $10 \mu\text{g mL}^{-1}$ of GDY or GO were added into the culture medium. Medium was changed every 2–3 days. After 14 days of culture, ALP staining was performed by an ALP staining kit (Beyotime, China) and the positive cells were counted by the Image J software.

ARS staining was carried out on day 14 after osteoinduction. Using 95% alcohol to fix cells for 10 min at room temperature. Cells were stained with 2% ARS at pH of 4.1 for 30 min in 37 °C. Then washed the cells with ddH₂O for 3 times. The stained mineralized nodules were observed under a light microscope. Semiquantitative analysis of ARS staining was implemented with Image J software by measuring the red staining areas.

Real time-qPCR assay on ALP, OCN, OSX, Col1a mRNA expression was conducted to explore osteogenesis property. MC3T3-E1 cells were cultured on $10 \mu\text{g mL}^{-1}$ of GO, GDY, TiO₂/GO, TiO₂/GDY or PBS, then cultured in osteogenic differentiation media for 7 days. Total RNA from cultured cells was extracted. After reverse transcription, Real time-qPCR analysis was performed for detection of gene transcriptional levels. The amount of mRNA was normalized to GAPDH. The primer sequences were shown in Table 1.

Loading capacity. To determine the loading capacity of the nanofibers, dexamethasone (Aladdin, China) with concentrations ranging from 1 to 10 μM were prepared in phosphate buffer. Each concentration of the solution (0.5 mL) was mixed with TiO₂/GDY 0.5, TiO₂/GDY 0.25 and TiO₂ nanofibers (1 mg mL^{-1} , 0.5 mL) separately, and vortexed in a shaker for equilibration at room temperature. After 24 h, the mixtures were centrifuged ($12,000 \times g$, 5 min) to collect the supernatant for spectrophotometric measurement. The adsorption isotherm of dexamethasone was obtained using UV-vis spectroscopy (SOPTOP, UV2800, China).

In vivo implant infection model. All animal surgical procedures were approved by the Ethics Committee for Animal Research of Wuhan University in China. The mouse implant infection model was operated on Kunming mice (8-week-old, female). MRSA prepared for infection were in mid-exponential grown phase of 10^7 CFU mL⁻¹. After anesthesia with isoflurane, the hindlimb of mice were shaved and disinfected with povidone iodine and alcohol. A small incision was made on the lateral aspect along the femur. The femur was exposed with blunt dissection. A cortical bone defect in 1-mm diameter was made close to the lower end of femur by trephination with MANI needle. Meanwhile, MRSA (1×10^7 CFU mL⁻¹) infected $100 \mu\text{g}$ of TiO₂/GDY, TiO₂, TiO₂/GO nanofibers or $50 \mu\text{g}$ of GDY or GO were implanted into the defect on femur and then received UV (365 nm , 2 W cm^{-2}) irradiation for 90 s or not. Afterwards, carefully sutured and closed muscle fasciae and skin. Five days and 4 weeks after surgery, the femurs were harvested after euthanasia by sodium pentobarbital. The samples were ground in sterile PBS (5 mL) for standard plate counting or fixed in 4% PFA for 24 h at room temperature for histomorphological study. Three animal samples were operated for each experiment per group.

Table.1 Real time-qPCR primer sequences.

Genes	Primer sequences (F/R)
Alp	GCTGATCATTCCCACGTTTT/CTGGGCCTGGTAGTTGTTGT
Ocn	AAGCAGGAGGGCAATAAGGT/TTTGTAGCGGCTTCAAGC
Osx	CAACCTGCTAGAGATCTGAG/TGCAATAGGAGAGAGCGA
Col1a	TGGCAAAGACGGACTCAAC/GGCAGGAAGCTGAAGTCATAA
Gapdh	GTGAAGGTCGGTGTGAACGG/TCCTGGAAGATGGTGTATGGG

Histomorphological analysis. H&E staining and Masson staining were carried out for histomorphological analysis. Fixed femur samples were decalcified in 10% EDTA for 4 weeks and changed twice a week. Decalcified samples were dehydrated with alcohol gradient and embedded in paraffin. Serial sections in 4 μ m thickness were mounted on slides. Samples were deparaffinized and rehydrated before subjected to H&E staining (MXB, China) and Masson staining (MXB, China) in accordance with the manufacturer's protocol. The quantitative analysis of Masson staining was performed by the Image J software on 5 regions of interest.

For immunohistochemical staining, slices were incubated with the primary antibody of OPN (Santa cruz, sc-21742, 1:100) overnight at 4 °C and then stained with immunohistochemical kit (MXB, China) according to manufacturer's protocol. The images were visualized by the light microscope. The quantitative analysis was performed by counting positive cells in 5 of the observed areas with Image J software.

Statistical analysis. All data were presented as means with standard deviations (SD). The significance analysis between two groups was tested with ANOVA and t test with GraphPad Prism software (6.0).

Reporting summary. Further information on research design is available in the Nature Research Reporting Summary linked to this article.

Data availability

Source data that support the findings of this study are available in Figshare with the identifier <https://doi.org/10.6084/m9.figshare.12715457>. Source data underlying Figs. 1b–f, 2e, f, 3b, d, f, 4b–d, 5b and Supplementary Figs. 1, 2, 3, 4b, 5, 6b, 7b, 8, 9b, 11, 12b, 13b, 14b, 16 are provided with this paper. All data pertaining to this work is available from the corresponding author upon reasonable request. Source data are provided with this paper.

Received: 29 December 2019; Accepted: 7 August 2020;

Published online: 08 September 2020

References

- Limo, M. J. et al. Interactions between metal oxides and biomolecules: from fundamental understanding to applications. *Chem. Rev.* **118**, 11118–11193 (2018).
- Sollazzo, V. et al. Anatase coating improves implant osseointegration in vivo. *J. Craniofac. Surg.* **18**, 806–810 (2007).
- Arciola, C. R., Campoccia, D. & Montanaro, L. Implant infections: adhesion, biofilm formation and immune evasion. *Nat. Rev. Microbiol.* **16**, 397–409 (2018).
- Li, B. & Webster, T. J. Bacteria antibiotic resistance: New challenges and opportunities for implant-associated orthopedic infections. *J. Orthop. Res.* **36**, 22–32 (2018).
- Darouiche, R. O. Treatment of infections associated with surgical implants. *N. Engl. J. Med.* **350**, 1422–1429 (2004).
- Lebeaux, D., Ghigo, J. M. & Beloin, C. Biofilm-related infections: bridging the gap between clinical management and fundamental aspects of recalcitrance toward antibiotics. *Microbiol. Mol. Biol. R.* **78**, 510–543 (2014).
- Dumitriu, C. et al. Electrospun TiO₂ nanofibers decorated Ti substrate for biomedical application. *Mater. Sci. Eng. C.* **45**, 56–63 (2014).
- Bai, L. et al. A multifaceted coating on titanium dictates osteoimmunomodulation and osteo/angio-genesis towards ameliorative osseointegration. *Biomaterials* **162**, 154–169 (2018).
- Jung, H. S. et al. Surface modification of multipass caliber-rolled Ti alloy with dexamethasone-loaded graphene for dental applications. *ACS Appl. Mater. Interfaces* **7**, 9598–9607 (2015).
- Zheng, S. et al. Poly-L-lysine coated PLGA/Poly (amino Acid) modified hydroxyapatite porous scaffolds as efficient tissue engineering scaffolds for cell adhesion, proliferation, and differentiation. *N. J. Chem.* **43**, 9989–10002 (2019).
- Qiu, J. et al. TiO₂ nanorod array constructed nanotopography for regulation of mesenchymal stem cells fate and the realization of location-committed stem cell differentiation. *Small* **12**, 1770–1778 (2016).
- Laxma Reddy, P. V., Kavitha, B., Kumar Reddy, P. A. & Kim, K. H. TiO₂-based photocatalytic disinfection of microbes in aqueous media: a review. *Environ. Res.* **154**, 296–303 (2017).
- Anandan, S. et al. Superhydrophilic graphene-loaded TiO₂ thin film for self-cleaning applications. *ACS Appl. Mater. Interfaces* **5**, 207–212 (2013).
- Jia, Z. et al. Bioinspired anchoring AgNPs onto micro-nanoporous TiO₂ orthopedic coatings: Trap-killing of bacteria, surface-regulated osteoblast functions and host responses. *Biomaterials* **75**, 203–222 (2016).
- Han, J. et al. Sustained release vancomycin-coated titanium alloy using a novel electrostatic dry powder coating technique may be a potential strategy to reduce implant-related infection. *BioSci. Trends* **11**, 346–354 (2017).
- Li, M. et al. Toward a molecular understanding of the antibacterial mechanism of copper-bearing titanium alloys against staphylococcus aureus. *Adv. Healthc. Mater.* **5**, 557–566 (2016).
- Zuo, Z. C. & Li, Y. L. Emerging electrochemical energy applications of graphdiyne. *Joule* **3**, 899–903 (2019).
- Kuang, P., He, M., Zou, H., Yu, J. & Fan, K. OD/3D MoS₂-NiS₂/N-doped graphene foam composite for efficient overall water splitting. *Appl. Catal. B* **254**, 15–25 (2019).
- Jin, Z. et al. Graphdiyne:ZnO nanocomposites for high-performance UV photodetectors. *Adv. Mater.* **28**, 3697–3702 (2016).
- Zhang, X. et al. Pristine graphdiyne-hybridized photocatalysts using graphene oxide as a dual-functional coupling reagent. *Phys. Chem. Chem. Phys.* **17**, 1217–1225 (2015).
- Xue, Y. et al. Extraordinarily durable graphdiyne-supported electrocatalyst with high activity for hydrogen production at all values of pH. *ACS Appl. Mater. Interfaces* **8**, 31083–31091 (2016).
- Xu, Q. et al. Photocatalytic H₂ evolution on graphdiyne/g-C₃N₄ hybrid nanocomposites. *Appl. Catal. B* **255**, 117770 (2019).
- Kuang, P. et al. Graphdiyne: a superior carbon additive to boost the activity of water oxidation catalysts. *Nanoscale Horiz.* **3**, 317–326 (2018).
- Liu, J., Chen, C. & Zhao, Y. Progress and prospects of graphdiyne-based materials in biomedical applications. *Adv. Mater.* **31**, e1804386 (2019).
- Hu, X. et al. A difunctional regeneration scaffold for knee repair based on aptamer-directed cell recruitment. *Adv. Mater.* **29**, 1605235 (2017).
- Li, S. et al. Graphdiyne materials as nanotransducer for in vivo photoacoustic imaging and photothermal therapy of tumor. *Chem. Mater.* **29**, 6087–6094 (2017).
- Zhang, Y. et al. 2D graphdiyne oxide serves as a superior new generation of antibacterial agents. *iScience* **19**, 662–675 (2019).
- Gu, M. et al. Is graphene a promising nano-material for promoting surface modification of implants or scaffold materials in bone tissue engineering? *Tissue Eng. Part B* **20**, 477–491 (2014).
- Zhang, S. Q. et al. Raman spectra and corresponding strain effects in graphyne and graphdiyne. *J. Phys. Chem. C.* **120**, 10605–10613 (2016).
- Madras, T. A. G. Photocatalytic degradation of rhodamine dyes with nano-TiO₂. *Ind. Eng. Chem. Res.* **46**, 7–14 (2007).
- Kullar, R., Sakoulas, G., Deresinski, S. & van Hal, S. J. When sepsis persists: a review of MRSA bacteraemia salvage therapy. *J. Antimicrob. Chemother.* **71**, 576–586 (2016).
- Cabiscol, E., Tamarit, J. & Ros, J. Oxidative stress in bacteria and protein damage by reactive oxygen species. *Intern. Microbiol.* **3**, 3–8 (2000).
- Yin, C. et al. Setd7 and its contribution to boron-induced bone regeneration in boron-mesoporous bioactive glass scaffolds. *Acta Biomater.* **73**, 522–530 (2018).
- Lee, W. C. et al. Origin of enhanced stem cell growth and differentiation on graphene and graphene oxide. *ACS Nano* **5**, 7334–7341 (2011).
- Oshina, H. et al. Effects of continuous dexamethasone treatment on differentiation capabilities of bone marrow-derived mesenchymal cells. *Bone* **41**, 575–583 (2007).
- Hankenson, K. D., Gagne, K. & Shaughnessy, M. Extracellular signaling molecules to promote fracture healing and bone regeneration. *Adv. Drug. Deliv. Rev.* **94**, 3–12 (2015).
- Hankenson, K. D., Zimmerman, G. & Marcucio, R. Biological perspectives of delayed fracture healing. *Injury* **45**(Suppl 2), S8–S15 (2014).
- Tan, A. W. et al. Enhanced in vitro angiogenic behaviour of human umbilical vein endothelial cells on thermally oxidized TiO₂ nanofibrous surfaces. *Sci. Rep.* **6**, 21828 (2016).
- Low, J., Yu, J., Jaroniec, M., Wageh, S. & Al-Ghamdi, A. A. Heterojunction photocatalysts. *Adv. Mater.* **29**, 1601694 (2017).
- Xu, F. et al. Graphdiyne: a new photocatalytic CO₂ reduction cocatalyst. *Adv. Funct. Mater.* **29**, 1904256 (2019).
- Reddy, P. A. et al. Recent advances in photocatalytic treatment of pollutants in aqueous media. *Environ. Int.* **91**, 94–103 (2016).
- Lin, X. et al. Toxicity of TiO₂ nanoparticles to *Escherichia coli*: effects of particle size, crystal phase and water chemistry. *PLoS ONE* **9**, e110247 (2014).
- Karunakaran, C., Vijayabalan, A., Manikandan, G. & Gomathisankar, P. Visible light photocatalytic disinfection of bacteria by Cd–TiO₂. *Catal. Commun.* **12**, 826–829 (2011).
- Zheng, L., Hu, K., Teng, F. & Fang, X. Novel UV–visible photodetector in photovoltaic mode with fast response and ultrahigh photosensitivity employing Se/TiO₂ nanotubes heterojunction. *Small* **13**, 1602448 (2017).
- Si, Y. et al. Daylight-driven rechargeable antibacterial and antiviral nanofibrous membranes for bioprotective applications. *Sci. Adv.* **4**, eaar5931 (2018).
- Huang, C. et al. Progress in research into 2D graphdiyne-based materials. *Chem. Rev.* **118**, 7744–7803 (2018).

47. Brynildsen, M. P., Winkler, J. A., Spina, C. S., MacDonald, I. C. & Collins, J. J. Potentiating antibacterial activity by predictably enhancing endogenous microbial ROS production. *Nat. Biotechnol.* **31**, 160–165 (2013).
48. Kim, S. Y. et al. Antibacterial strategies inspired by the oxidative stress and response networks. *J. Microbiol.* **57**, 203–212 (2019).
49. Courtney, C. M. et al. Potentiating antibiotics in drug-resistant clinical isolates via stimuli-activated superoxide generation. *Sci. Adv.* **3**, e1701776 (2017).
50. Masters, E. A. et al. Evolving concepts in bone infection: redefining “biofilm”, “acute vs. chronic osteomyelitis”, “the immune proteome” and “local antibiotic therapy”. *Bone Res.* **7**, 1–18 (2019).
51. Gao, Q. & Garcia-Pichel, F. Microbial ultraviolet sunscreens. *Nat. Rev. Microbiol.* **9**, 791–802 (2011).
52. Zheng, L. et al. Highly selective photocatalytic production of H₂O₂ on sulfur and nitrogen co-doped graphene quantum dots tuned TiO₂. *Appl. Catal. B* **239**, 475–484 (2018).
53. Min, H. et al. Synthesis and imaging of biocompatible graphdiyne quantum dots. *ACS Appl. Mater. Interfaces* **11**, 32798–32807 (2019).
54. Wubneh, A., Tsekoura, E. K., Ayranci, C. & Uludag, H. Current state of fabrication technologies and materials for bone tissue engineering. *Acta Biomater.* **80**, 1–30 (2018).
55. Rahimpour, A. et al. Novel functionalized carbon nanotubes for improving the surface properties and performance of polyethersulfone (PES) membrane. *Desalination* **286**, 99–107 (2012).
56. Wang, J. et al. Construction of TiO₂@graphene oxide incorporated antifouling nanofiltration membrane with elevated filtration performance. *J. Membr. Sci.* **533**, 279–288 (2017).
57. Vatanpour, V., Madaeni, S. S., Moradian, R., Zinadini, S. & Astinchap, B. Fabrication and characterization of novel antifouling nanofiltration membrane prepared from oxidized multiwalled carbon nanotube/polyethersulfone nanocomposite. *J. Membr. Sci.* **375**, 284–294 (2011).
58. Allegri, M. et al. Shape-related toxicity of titanium dioxide nanofibres. *PLoS ONE* **11**, e0151365 (2016).
59. Ramkumar, K. M. et al. Oxidative stress-mediated cytotoxicity and apoptosis induction by TiO₂ nanofibers in HeLa cells. *Eur. J. Pharm. Biopharm.* **81**, 324–333 (2012).
60. Xie, J. et al. Graphdiyne nanoparticles with high free radical scavenging activity for radiation protection. *ACS Appl. Mater. Interfaces* **11**, 2579–2590 (2019).
61. Calciolari, E., Hamlet, S., Ivanovski, S. & Donos, N. Pro-osteogenic properties of hydrophilic and hydrophobic titanium surfaces: Crosstalk between signalling pathways in vivo models. *J. Periodontal Res.* **53**, 598–609 (2018).
62. Nayak, T. R. et al. Graphene for controlled and accelerated osteogenic differentiation of human mesenchymal stem cells. *ACS Nano* **5**, 4670–4678 (2011).
63. Bodhak, S., Bose, S. & Bandyopadhyay, A. Role of surface charge and wettability on early stage mineralization and bone cell-materials interactions of polarized hydroxyapatite. *Acta Biomater.* **5**, 2178–2188 (2009).
64. Jin, J. et al. Graphdiyne nanosheet-based drug delivery platform for photothermal/chemotherapy combination treatment of cancer. *ACS Appl. Mater. Interfaces* **10**, 8436–8442 (2018).
65. Guo, S. et al. Graphdiyne-promoted highly efficient photocatalytic activity of graphdiyne/silver phosphate pickering emulsion under visible-light irradiation. *ACS Appl. Mater. Interfaces* **11**, 2684–2691 (2019).

Acknowledgements

We acknowledge the Medical Research Center for Structural Biology in Wuhan University School of Basic Medical Sciences for the LSCM images, the large-scale instrument and equipment sharing foundation of Wuhan University for the Raman spectra and the School of Chemistry and Chemical Engineering in Huazhong University of Science & Technology for contact angle testing. This work was supported by the National Key R&D Program of China (2018YFC1105300), the National Natural Science Foundation of China (81771050, 81570954, 51932007, 51961135303 and U1705251), and the Innovative Research Funds of Foshan Xianhu Laboratory of the Advanced Energy Science and Technology Guangdong Laboratory (XHD2020-001).

Author contributions

Zhang’s lab contributed to the discovery of the dual function of TiO₂/GDY and performed the characterization test of materials, in vivo and in vitro experiments on antibacterial and osteoinduction properties. Yu’s lab implemented the material synthesis, conducted TEM, and directed ESR assay. Y.Z. and J.Y. raised the project and guided the research design, R.W., M.S., and Q.Z. contributed to the research design, R.W., F.X., Y.Q., P.Z., and K.S. performed experiment and collected data. R.W. and M.S. wrote the paper.

Competing interests

The authors declare no competing interests.

Additional information

Supplementary information is available for this paper at <https://doi.org/10.1038/s41467-020-18267-1>.

Correspondence and requests for materials should be addressed to J.Y. or Y.Z.

Peer review information *Nature Communications* thanks Alideertu Dong, Lorenzo Drago and the other anonymous reviewer(s) for their contribution to the peer review of this work.

Reprints and permission information is available at <http://www.nature.com/reprints>

Publisher’s note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons license, and indicate if changes were made. The images or other third party material in this article are included in the article’s Creative Commons license, unless indicated otherwise in a credit line to the material. If material is not included in the article’s Creative Commons license and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this license, visit <http://creativecommons.org/licenses/by/4.0/>.

© The Author(s) 2020