

Durham Research Online

Deposited in DRO:

17 March 2017

Version of attached file:

Accepted Version

Peer-review status of attached file:

Peer-reviewed

Citation for published item:

Ward, E. N. and Pal, R. (2017) 'Image scanning microscopy : an overview.', *Journal of microscopy*, 266 (2). pp. 221-228.

Further information on publisher's website:

<https://doi.org/10.1111/jmi.12534>

Publisher's copyright statement:

This is the accepted version of the following article: Ward, E. N. and Pal, R. (2017), Image scanning microscopy: an overview. *Journal of Microscopy*. 266(2): 221-228, which has been published in final form at <https://doi.org/10.1111/jmi.12534>. This article may be used for non-commercial purposes in accordance With Wiley Terms and Conditions for self-archiving.

Additional information:

Use policy

The full-text may be used and/or reproduced, and given to third parties in any format or medium, without prior permission or charge, for personal research or study, educational, or not-for-profit purposes provided that:

- a full bibliographic reference is made to the original source
- a [link](#) is made to the metadata record in DRO
- the full-text is not changed in any way

The full-text must not be sold in any format or medium without the formal permission of the copyright holders.

Please consult the [full DRO policy](#) for further details.

AN OVERVIEW OF IMAGE SCANNING MICROSCOPY

Edward N Ward, Robert Pal.

Correspondence to: Robert Pal, Department of Chemistry, Durham University, Lower Mountjoy, South Road, Durham DH1 3LE. Tel: 01913342102 Email: robert.pal@durham.ac.uk

Summary

For almost a century, the resolution of optical microscopy was thought to be limited by Abbé's law describing the diffraction limit of light. At the turn of the millennium, aided by new technologies and fluorophores, the field of optical microscopy finally surpassed the diffraction barrier: a milestone achievement that has been recognised by the 2014 Nobel Prize in Chemistry. Many super-resolution methods rely on the properties of the fluorophores to improve resolution, posing significant limitations on biological imaging. Structured Illumination Microscopy (SIM) is one branch of super-resolution microscopy that requires no special properties of the fluorophores, making it more versatile than other techniques. Since its introduction in biological imaging, SIM has proven to be a popular tool in the biologist's arsenal for following biological interaction and probing structures of nanometre scale. SIM continues to see much advancement in design and implementation, including the development of Image Scanning Microscopy (ISM) which uses single point-spread functions (PSFs) as the excitation pattern. This review aims to give a brief overview of the SIM and ISM processes and developments in the image reconstruction process. Drawing from this, and incorporating more recent achievements in light shaping (such as pattern scanning, phase modulation, and super-resolution beam shaping), this study hopes to suggest potential future directions for this ever-expanding field.

Lay Description

The resolving ability of a light microscope is limited by the diffraction of light. This resolution barrier can be broken in a number of ways: by using the properties of the fluorophores; localising sparsely emitting fluorophores; or by using patterned illumination. ISM is a technique that uses grid patterns of diffraction-limited spots to achieve super-resolution. This review discusses the theory of the technique and its limitations, and suggests potential future directions.

Background

Fluorescence microscopy stands out as possibly the most ubiquitous tool in biological imaging. However, this versatile technique suffers from a critical barrier in resolution which limits its potential to study samples at the nanometre scale. First formalised in 1873 by Ernst Abbé, this resolution barrier is dependent on the wavelength of light and the numerical aperture of the imaging system; itself a function of the refractive index of the imaging media and the angle of light that can be received from the focal plane of the objective lens. (Abbé 1873) For visible light and a high-quality objective, this typically limits resolution to ~200nm in the lateral plane and ~700nm in the axial direction. The Laser Scanning Confocal Microscope (LSCM) was the first microscope to reach this resolution barrier and has become the most widespread imaging tool in biological imaging. The key advantage of the LSCM is a pinhole in the optical path to reject out-of-focus light, allowing structures to be studied in 3D by imaging only a single focal plane.

Super-resolution microscopy (nanoscopy) is a more recent development to the field of fluorescence microscopy, and describes any imaging technique capable of breaking Abbé's diffraction limit. To date, there has been a vast number of nanoscopic techniques conceived, and innumerable examples of new discoveries resulting from these techniques. So far, the highest resolution methods exploit the properties of the fluorophores to achieve an increase in resolution. The Single-Molecule Localisation Microscopy (SMLM) techniques – Photo-Activation Localisation Microscopy (Betzig et al. 2006) and Stochastic Optical Reconstruction Microscopy (Rust et al.

2006) – give the highest resolutions. Stimulated Emission Depletion (STED) microscopy also harnesses unique properties of fluorophores: a doughnut-shaped depletion beam travels along the same path as a classical excitation beam – identical to that used in LSCM – and acts to reduce the effective size of the excitation spot. (Hell & Wichmann 1994)

SIM describes any sub-diffraction technique that involves the use of patterned excitation.

(Although structured illumination imaging is possible without fluorescent response, this review will be limited to its application in fluorescence microscopy.) The first examples of SIM involved the use of opposing objectives focused onto the same focal plane. (Gustafsson et al. 1995; Hell et al. 1994) In this configuration, it is possible to generate standing waves or interference patterns in the axial plane with periods shorter than the axial resolution of the objectives. This has the effect of reducing the thickness of the plane illuminated, increasing axial resolution. Lateral increase necessitates the use of laterally patterned excitation and was first achieved at the turn of the millennium. (Heintzmann & Cremer 1999; Gustafsson 2000) Since then, it has taken off as one of the key methods in nanoscopy. The great advantages of SIM are that it is compatible with any fluorophore and that it uses only modest excitation power. This allows biologists to continue using their existing protocols and facilitates live-cell imaging.

Theory of super-resolution SIM

For any point, \vec{r} , in an image recorded from a wide-field microscope, the intensity, $D(\vec{r})$ is given by

$$D(\vec{r}) = (S(\vec{r}) \cdot E(\vec{r})) \otimes PSF(\vec{r}) .$$

For the proper description of a wide-field microscope, the case of incoherent illumination is assumed throughout. (Goodman 2004) $S(\vec{r})$ is the structure or distribution of fluorophores in the sample; $E(\vec{r})$ is the excitation light amplitude; and $PSF(\vec{r})$ is the detection point-spread function. \otimes denotes the mathematical convolution operation which has the effect of blending two functions.

The PSF of the system can be conceived as the result in the image plane of an infinitesimal

emitter in the sample plane. It also represents the smallest volume to which light can be focused. When considering the resolution limit of an imaging system, it is easier to consider the associated frequency space. Taking the Fourier transform of the function converts the intensity distribution from real to frequency space:

$$\tilde{D}(\vec{k}) = \tilde{S}(\vec{k}) \otimes \tilde{E}(\vec{k}) \cdot OTF(\vec{k}) .$$

The tildes denote the Fourier transforms of the component functions, and the convolution and product have been swapped according to the mathematical definition of a convolution. The Optical Transfer Function, $OTF(\vec{k})$, is the direct Fourier transform of the PSF. In frequency space, higher spatial frequencies correspond to a better-resolved image. The OTF of an imaging system acts as low-pass filter, cutting off high spatial frequencies. The general SIM process is shown in Figure 1.

In the simplest case of 2D SIM, a striped sinusoidal pattern is used and the function $E(\vec{r})$ becomes

$$E(\vec{r}) = E_0(1 + \cos(\vec{k}_0 \cdot \vec{r} + \varphi)).$$

Here, the vector \vec{k}_0 describes the frequency and direction of the pattern, and φ is the phase. When substituting this into the previous equation we get:

$$\tilde{D}(\vec{k}) = E_0[\tilde{S}(\vec{k}) + 0.5\tilde{S}(\vec{k} + \vec{k}_0)e^{i\varphi} + 0.5\tilde{S}(\vec{k} - \vec{k}_0)e^{-i\varphi}].$$

Looking at this, the detected Fourier spectrum is now a linear superposition of three zones of the frequency space of the sample structure. To extract the extra information, it is necessary to move the new frequency components to their correct place in the final image spectrum. This is achieved by capturing three separate images with different illumination pattern phases to isolate each sampled region of frequency space. The extra frequency information can then be assigned to its correct place in frequency space. Since the frequency components are only shifted in the direction of \vec{k}_0 , it is necessary to repeat this process at three directions of illumination pattern to achieve isotropic resolution increase. SIM is particularly sensitive to movement of the sample and to changes in its fluorescent response while these pictures are being acquired. As such, these images must be captured in quick succession and with a suitably low illumination intensity to minimise sample drift and photo-bleaching.

There have been a number of improvements to this core SIM implementation. Of particular note is Saturated SIM (SSIM) (Gustafsson 2005) which achieves a theoretically unlimited resolution by using the non-linear response of fluorophores at high excitation intensities. Above a certain intensity threshold, the fluorescent response saturates. This is seen as a 'levelling off' in the sinusoidal to a square pattern. This square pattern introduces higher spatial frequencies into the excitation pattern, allowing for sampling of a greater region of the object's frequency space. To extract these extra frequencies, more phase shifts are required for each direction of pattern, extending acquisition time. However, while excellent resolution is achievable, the increased imaging time and the higher excitation power are normally incompatible with live-cell imaging. SSIM is also very susceptible to photo-bleaching, as any difference in response between excitation patterns results in artefacts after image reconstruction.

Image scanning microscopy

One of the more recent advancements in SIM has been ISM which was achieved in 2010 by Müller and Enderlein, (Müller & Enderlein 2010) despite having been previously described some years earlier. (Sheppard 1988) The underlying principle of ISM can be understood as extracting the inherent super-resolution information from a LSCM. The origin of this extra information can be conceptualised in two different ways. The first description is based on the idea of the overlap of excitation and emission PSFs in a confocal microscope; (Sheppard 1988; Sheppard et al. 2013) the second sought to describe this as a SIM technique. (Müller & Enderlein 2010) In a scanning microscope, a diffraction-limited spot is raster scanned across the sample and the image is built up in a pixel-by-pixel fashion. This means that, for every point in the scan, the excitation pattern is the excitation PSF. By definition, the Fourier transform of this diffraction-limited spot contains all the spatial frequencies permitted by the objective. As with all patterned illumination, the spatial frequency components of the sample are mixed with those of the excitation pattern, meaning high spatial frequencies of the sample are moved into the range of the detection OTF. In the case of the point-scanning microscope, the highest frequency component of the excitation pattern is the

cut-off frequency of the excitation OTF. This means that the maximum spatial frequency moved into the supported region of the detection OTF is double that which is usually gathered.

In a LSCM, some of this super-resolution information can be collected simply by closing the pinhole. However, in practice, the large amount of light rejected by a smaller pinhole reduces the Signal-to-Noise Ratio (SNR) to prohibitively low levels. ISM works by recovering this lost super-resolution information. The optical configuration required to achieve ISM on a scanning microscope is relatively simple and involves recording the signal that passes through the pinhole on an array detector and capturing an image at every scan position. The simplest way to recover a final super-resolution image is pixel reassignment, shown in Figure 4. (Sheppard et al. 2013) In practice, pixel reassignment is relatively simple to accomplish. For each scan position, the image acquired is shrunk by some factor, and added to a running-total image, centred at the scan position of the beam. The degree of shrinking is based on several factors, including the Stoke's shift of the fluorophores used. After a complete picture has been reconstructed, further resolution enhancement can be achieved by Fourier re-weighting. It should be noted that this pixel reassignment technique has also been achieved all-optically – without the need for complicated post-processing – by Roth et al. (Roth et al. 2013) and more recently with a modified spinning disc microscope (Azuma & Kei 2015) for faster acquisition.

Developments of ISM

From these early steps, ISM has undergone significant improvement towards a more robust microscopic technique. The first hurdle to overcome was the extended acquisition time associated with all scanning methods, and even further exaggerated in ISM. Since the light gathered is spread out over a camera, the signal recorded on the array detector is weaker, and longer pixel dwell times are required. This means there is a total image acquisition time of at least 25 seconds for a modest $4\mu\text{m} \times 4\mu\text{m}$ field of view. This can be greatly reduced if more than one excitation spot is used simultaneously and the whole Field of View (FOV) is recorded, analogous with spinning disc microscopy. This was first accomplished by York et al. who used a Digital Micro-mirror Device

(DMD) to illuminate the sample in a process they termed Multifocal Structured Illumination Microscopy (MSIM). (York et al. 2012) Using the DMD, they reported speeds of up to 1Hz for a $50\mu\text{m} \times 50\mu\text{m}$ FOV: a significant improvement on the scanning method, now offering a temporal resolution suitable for basic live-cell imaging. However, since MSIM employs wide-field detection, the optical sectioning capability is lost. This can, in part, be recovered through the process of 'digital pinholing'. To achieve this, the location of the excitation spots in each of the raw images is determined and a mask is then applied around this point, rejecting light gathered on surrounding pixels. This has the effect of partially removing light from outside the focal plane. An alternative approach to retaining optical sectioning while using multiple excitation spots has also been demonstrated by Schulz et al., who combined a spinning-disc microscope with a microsecond pulsed laser. (Schulz et al. 2013)

As well as speeding up the process, lately there have been substantial advances in the image reconstruction process. Newer reconstruction procedures for ISM have focused on using Maximum-Likelihood Deconvolution (MLD) algorithms. Put simply, MLD is an iterative process that maximises the probability that an estimated sample structure will generate the images acquired under the illumination patterns used. The classical diffraction-limited image is taken as the initial estimate of the sample. The computer then predicts the fluorescent response of the estimated sample to each illumination pattern. From the differences between the acquired and predicted images, an update step is calculated and applied to the initial estimate to generate a new estimate. The process is then repeated either until the update step reaches a predefined minimum, or until a user-defined iteration limit is reached. The most popular MLD algorithms are joint Richardson-Lucy (jRL) deconvolution (Ingaramo et al. 2014; Ströhl & Kaminski 2015) and pattern-illuminated Fourier Ptychography. (Dong et al. 2014) The difference between these is the way in which the update step is calculated, and the relative strengths of these methods and the mathematical background has recently been reviewed excellently by Chakrova et al. (Chakrova et al. 2016) MLD has been shown to outperform pixel reassignment in terms of both resolution improvement and signal-to-noise ratio. This is in part because MLD can be tuned to account for

one or more of the different types of noise associated with image acquisition, specifically: Poisson noise originating from the low photon counts; and Gaussian noise originating from the readout noise of the camera. This is in contrast to pixel reassignment where, rather than being suppressed, noise is amplified during image reconstruction. MLDs also negate the need to apply Fourier re-weighting onto the image after reconstruction and may, under certain circumstances, improve resolution beyond ISM alone by estimating super-resolution information from predefined knowledge of the sample. (Heintzmann 2007) A final key advantage of MLDs is that they are able to extract SI information in situations where the direct reconstruction process is not known. In fact, MLD can even be implemented in cases where the illumination pattern is unknown, (Mudry et al. 2012) though these methods are generally outperformed by using known illumination patterns. (N.Chakrova, B.Rieger 2015) Pixel reassignment, however, is based on the underlying assumption that the emission and detection PSFs are scaled versions of each other, and as such is resultantly applicable in very specific circumstances.

Limitations

As with all techniques, ISM has its limitations. These are particularly apparent when compared to other nanoscopic methods. Since the structured illumination information comes from a diffraction-limited pattern, it is limited to only a twofold resolution increase in the lateral plane; this is no improvement over simpler forms of SIM which use a striped pattern. Furthermore, scanning ISM requires much greater acquisition time than LSCM or SIM. Multi-spot ISM offers an improvement to temporal resolution but, unless it is operated on a spinning disc microscope, it loses the confocality offered by scanning systems. Total internal reflection excitation and axially-patterned excitation (Gustafsson et al. 2008) have allowed other forms of SIM to avoid this issue and achieve super-resolution in all three directions, something not yet possible with ISM.

Precise knowledge of the excitation pattern is also imperative to MSIM in both applying digital pinholes and in image reconstruction. The effects of this are particularly apparent when imaging deeper into tissues or in highly-scattering samples, where aberrations and noise produce

reconstruction artefacts in the final image. This has proven problematic in practical applications of ISM, where the pattern must either be determined by regularly calibrating the system using a test slide (York et al. 2012; Schulz et al. 2013) or by computationally identifying the excitation pattern post-acquisition. (Ströhl & Kaminski 2015; McGregor et al. 2015) Both of these techniques have their limitations: calibrating the system is a time-consuming step, and is ineffective if the sample has greatly different optical properties to the test slide; determining the pattern post-acquisition adds another step to an already computationally intensive technique; and, depending on the algorithm used, reconstruction can break down in patterned or sparsely fluorescing samples. (McGregor et al. 2015) Combining MSIM with two-photon excitation has been demonstrated to reduce the effects of scattering samples and may offer one solution to this issue. (Wawrzusin et al. 2014)

Future directions of ISM

Despite these shortfalls, ISM is an ever-developing method and shows great potential as a super-resolution technique. A significant limitation to ISM is the relatively small increase in resolution it affords. Since the resolution increase in ISM is achieved by the frequency components of the focal spot, introducing higher-than-classically-allowed spatial frequencies into the excitation spot would allow for a better than twofold gain in resolution. One promising direction is merging the fields of PSF engineering and ISM. PSF engineering involves altering an optical system in such a way as to generate a non-classical excitation or detection PSF. (Fang et al. 2015) The most prominent example of PSF engineering is the generation of the doughnut-shaped depletion beam used in 2D STED nanoscopy. (Hell & Wichmann 1994) To create this doughnut shape, a spiral phase is imparted to the beam, generating an intensity minimum at the centre of the focal spot. Crucially, the size of this dark region is not diffraction-limited, and as such, preventing fluorescence outside of this central region results in an effective excitation PSF that is considerably smaller than in LSCM. ISM on a scanning STED microscope was recently demonstrated by Laporte et al., (Laporte et al. 2014) who used pixel reassignment to give a 1.25x improvement in resolution over standalone STED nanoscopy. However, it may be possible to extract SI information from a

microscope when using only the doughnut-shaped excitation spot. Since the width of the central dark spot is sub-diffraction, there are higher spatial frequencies in the doughnut spot than a diffraction-limited Gaussian PSF. Figures 5E and 5F show an example of simulated MSIM data when using arrays of doughnut PSFs. The sub-diffraction structure of the excitation PSFs has given a clear improvement in resolution over MSIM using a Gaussian spot pattern. Laporte et al. also attempted to build on the SSIM method and take advantage of saturation of fluorophores within a single excitation spot. As in SSIM, saturation of fluorophores leads to an effectively flat-topped PSF, containing high spatial frequencies. While theoretically possible, this method proved unsuccessful, since the intensity of these high frequency components was too low to be detectable.

Other efforts to bring PSF engineering into ISM have aimed to improve the axial resolution. RESCH (REfocusing after SCanning using a Helical phase engineering) is one such technique that operates in a similar manner to scanning ISM. (Jesacher et al. 2015; Roeder et al. 2016) As with ISM, the signal from a point-scanning microscope is collected on a camera in the place of a point detector. However, in RESCH, the phase of the collected light is modulated by a SLM in such a way that axial information is encoded into the image captured on the camera. By sampling different regions of the camera image, the fluorescence at different focal planes can be simultaneously measured from a single scan. Using this method to achieve optical sectioning allows for a better axial resolution than confocal microscopy. Combining RESCH with MLD brings some of the lateral resolution increase of ISM and, in simulations, the combination has been shown to produce a 20% increase in resolution in all three directions when compared to confocal microscopy. (Roeder et al. 2016) Although this is only a modest improvement, and some way off a practical technique, this is still an area of ongoing research.

As well as in instrument design, there is significant room for improvement in the image reconstruction process. Currently, the choice of algorithm results in very different reconstructed images, and choosing the right method for a particular application is a complex – and at times,

Reference	(Cox & Sheppard 2004)	(Hell & Wichmann 1994; Liu et al. 2012)	(Rust et al. 2006; Hess et al. 2006)	(Gustafsson 2000)	(Shao et al. 2011)	(Gustafsson 2005)	(Müller & Enderlein 2010)	(York et al. 2012; Wawrzusin et al. 2014)
-----------	-----------------------	---	--------------------------------------	-------------------	--------------------	-------------------	---------------------------	---

† Can exceed 150 μm if combined with multi-photon excitation

References

- Abbé, E., 1873. Beiträge zur Theorie des Mikroskops und der mikroskopischen Wahrnehmung. *Arkiv. Mikroskop. Anat.*, (4), pp.413–468.
- Azuma, T. & Kei, T., 2015. Super-resolution spinning-disk confocal microscopy using optical photon reassignment. *Optics Express*, 23(11), p.15003.
- Betzig, E. et al., 2006. Imaging intracellular fluorescent proteins at nanometer resolution. *Science (New York, N. Y.)*, 313(September), pp.1642–1645.
- Booth, M. et al., 2015. Aberrations and adaptive optics in super-resolution microscopy. *Microscopy*, 64(4), pp.251–261.
- Chakrova, N., Rieger, B. & Stallinga, S., 2016. Deconvolution methods for structured illumination microscopy. *Journal of the Optical Society of America A*, 33(7), p.B12.
- Cox, G. & Sheppard, C.J.R., 2004. Practical Limits of Resolution in Confocal and Non-Linear Microscopy. *Microscopy Research and Technique*, 63(1), pp.18–22.
- Débarre, D. et al., 2008. Adaptive optics for structured illumination microscopy. *Optics Express*, 16(13), p.9290.
- Dong, S. et al., 2014. High-resolution fluorescence imaging via pattern-illuminated Fourier ptychography. *Optics express*, 22(17), pp.20856–70.
- Fang, Y. et al., 2015. Resolution and contrast enhancements of optical microscope based on point spread function engineering. *Frontiers of Optoelectronics*, 8(2), pp.152–162.
- Goodman, J.W., 2004. *Introduction to Fourier Optics, Third Edition*, Roberts and Company.
- Gustafsson, M.G., 2000. Surpassing the lateral resolution limit by a factor of two using structured illumination microscopy. *Journal of microscopy*, 198(January), pp.82–87.
- Gustafsson, M.G.L., 2005. Nonlinear structured-illumination microscopy: wide-field fluorescence imaging with theoretically unlimited resolution. *Proceedings of the National Academy of Sciences of the United States of America*, 102(37), pp.13081–13086.
- Gustafsson, M.G.L. et al., 2008. Three-dimensional resolution doubling in wide-field fluorescence microscopy by structured illumination. *BIOPHYSICAL JOURNAL*, 94(12), pp.4957–4970.
- Gustafsson, M.G.L., Agard, D.A. & Sedat, J.W., 1995. Sevenfold improvement of axial resolution in 3D widefield microscopy using two objective lenses. In T. Wilson & C. J. Cogswell, eds. pp. 147–156.
- Heintzmann, R., 2007. Estimating missing information by maximum likelihood deconvolution. *Micron*, 38(2), pp.136–144.
- Heintzmann, R. & Cremer, C.G., 1999. Laterally modulated excitation microscopy: Improvement of resolution by using a diffraction grating. In I. J. Bigio et al., eds. pp. 185–196.
- Hell, S.W. et al., 1994. Confocal microscopy with an increased detection aperture: type-B 4Pi confocal microscopy. *Optics letters*, 19(3), p.222.
- Hell, S.W. & Wichmann, J., 1994. Breaking the diffraction resolution limit by stimulated emission: stimulated-emission-depletion fluorescence microscopy. *Optics Letters*, 19(11), p.780.
- Hess, S.T., Girirajan, T.P.K. & Mason, M.D., 2006. Ultra-High Resolution Imaging by Fluorescence Photoactivation Localization Microscopy. *Biophysical Journal*, 91(11), pp.4258–4272.
- Ingaramo, M. et al., 2014. Richardson-Lucy Deconvolution as a General Tool for Combining Images with Complementary Strengths. *ChemPhysChem*, 15(4), pp.794–800.
- Jesacher, A., Ritsch-Marte, M. & Piestun, R., 2015. Three-dimensional information from two-dimensional scans: a scanning microscope with postacquisition refocusing capability. *Optica*,

2(3), p.210.

- Kim, B. & Naemura, T., 2015. Blind Depth-variant Deconvolution of 3D Data in Wide-field Fluorescence Microscopy. *Scientific reports*, 5(9894), p.9894.
- Laporte, G.P.J. et al., 2014. Resolution enhancement in nonlinear scanning microscopy through post-detection digital computation. *Optica*, 1(6), p.455.
- Liu, Y. et al., 2012. Achieving $\lambda/10$ resolution CW STED nanoscopy with a Ti:Sapphire oscillator. *PLoS ONE*, 7(6).
- McGregor, J.E., Mitchell, C. a. & Hartell, N. a., 2015. Post-processing strategies in image scanning microscopy. *Methods*, 88, pp.28–36.
- Mudry, E. et al., 2012. Structured illumination microscopy using unknown speckle patterns. *Nature Photonics*, 6(5), pp.312–315.
- Müller, C.B. & Enderlein, J., 2010. Image scanning microscopy. *Physical Review Letters*, 104(19), pp.1–4.
- N.Chakrova, B.Rieger, S.S., 2015. Studying different illumination patterns for resolution improvement in fluorescence microscopy. *Optics Express*, 23(24), pp.24692–24701.
- Preza, C. & Conchello, J.-A., 2004. Depth-variant maximum-likelihood restoration for three-dimensional fluorescence microscopy. *Journal of the Optical Society of America. A, Optics, image science, and vision*, 21(9), pp.1593–601.
- Roider, C. et al., 2016. Deconvolution approach for 3D scanning microscopy with helical phase engineering. *Optics Express*, 24(14), p.15456.
- Roth, S. et al., 2013. Optical photon reassignment microscopy (OPRA). *Optical Nanoscopy*, 2(1), p.5.
- Rust, M.J., Bates, M. & Zhuang, X., 2006. Sub-diffraction-limit imaging by stochastic optical reconstruction microscopy (STORM). *Nature methods*, 3(10), pp.793–795.
- Schulz, O. et al., 2013. Resolution doubling in fluorescence microscopy with confocal spinning-disk image scanning microscopy. *Proceedings of the National Academy of Sciences of the United States of America*, 110(52), pp.21000–5.
- Shaevitz, J.W. & Fletcher, D. a, 2007. Enhanced three-dimensional deconvolution microscopy using a measured depth-varying point-spread function. *Journal of the Optical Society of America. A, Optics, image science, and vision*, 24(9), pp.2622–2627.
- Shao, L. et al., 2011. Super-resolution 3D microscopy of live whole cells using structured illumination. *NATURE METHODS*, 8(12), p.1044+.
- Sheppard, C.J.R., 1988. Super-resolution in confocal imaging. *Optik*, 80(2), pp.53–54.
- Sheppard, C.J.R., Mehta, S.B. & Heintzmann, R., 2013. Superresolution by image scanning microscopy using pixel reassignment. *Optics letters*, 38(15), pp.2889–92.
- Ströhl, F. & Kaminski, C.F., 2015. A joint Richardson—Lucy deconvolution algorithm for the reconstruction of multifocal structured illumination microscopy data. *Methods and Applications in Fluorescence*, 3(1), p.14002.
- Wang, G. et al. eds., 2015. *Algorithms and Architectures for Parallel Processing*, Cham: Springer International Publishing.
- Wawrzusin, P. et al., 2014. Two-photon excitation improves multifocal structured illumination microscopy in thick scattering tissue. *Proceedings of the National Academy of Sciences of the United States of America*, 111(14), pp.5254–9.
- York, A.G. et al., 2012. Resolution doubling in live, multicellular organisms via multifocal structured illumination microscopy. *Nature methods*, 9(7), pp.749–754.

Figures

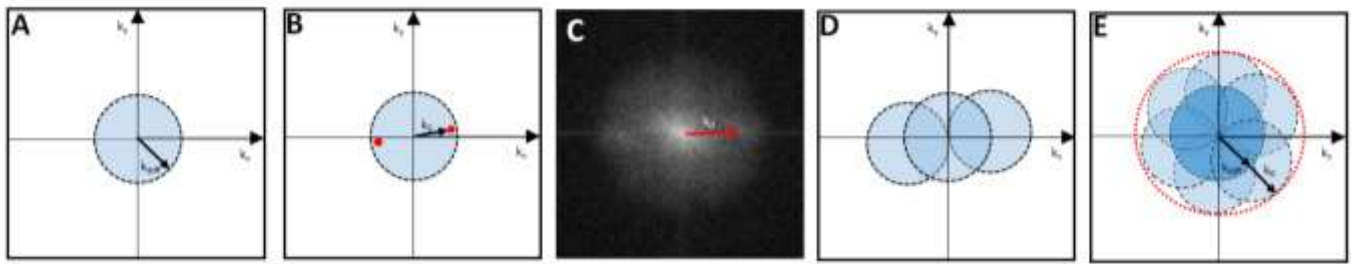


Figure 1. SIM methodology visualised in frequency space. A: In diffraction-limited imaging, only a small region (blue circle) of frequency space can be observed. This region is defined by a cut-off frequency proportional to the resolution limit. B: Under striped-pattern illumination, the frequency components of the excitation pattern are chosen to be as close to the diffraction limit as possible, to maximise resolution increase. The observed region of frequency space now contains frequency components from outside the supported region. C: Real image data of B. D: After shifting the phase of the pattern, the different regions of frequency space can be isolated and moved into the correct place in the image. E: Repeating the process for multiple directions of pattern allows for resolution increase in all directions. The new frequency cut-off is shown by the red circle.

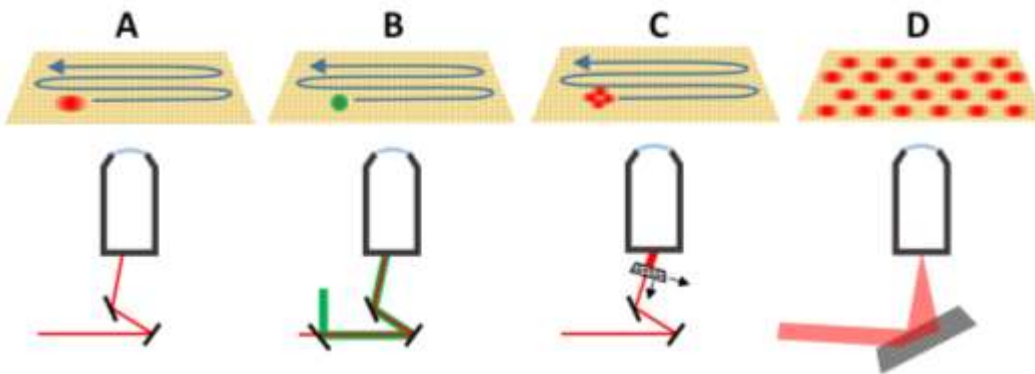


Figure 2. Illumination methods in optical microscopy. A: Confocal scanning microscope. Two scan mirrors guide the beam across the sample, building up the image pixel-by-pixel. B: STED microscopy. A spiral phase plate generates a doughnut-shaped depletion beam (green) which is scanned coaxially with a Gaussian excitation beam by a pair of scan mirrors. The effective excitation spot (shown in red) is smaller than that of a LSCM. C: Phase modulation nanoscopy. An oscillating diffraction grating is placed after the scan mirrors to generate a cluster of excitation spots in the focal plane. D: SIM or MSIM. A SLM is used to generate patterns at the focal plane.

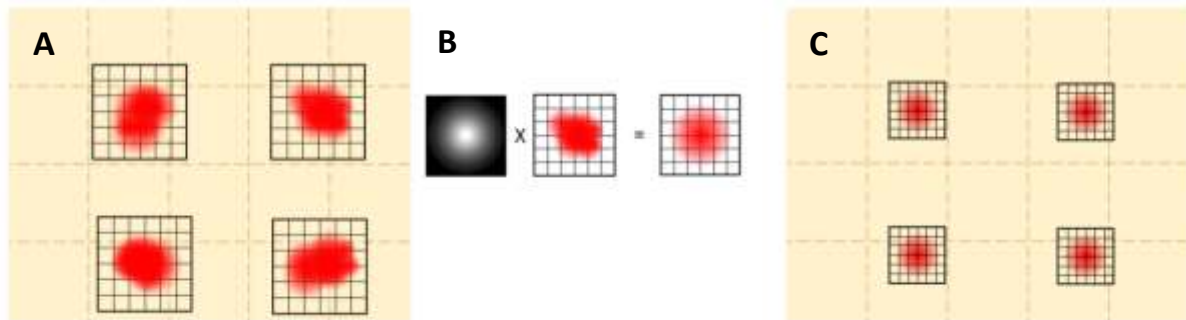


Figure 3. Pixel reassignment of MSIM data. A: Raw image captured under a particular illumination pattern. The location of the excitation spots is determined and this region of the image is extracted. B: Multiplication with a Gaussian mask removes some out-of-focus blur. C: The resulting image of the excited region of the sample is shrunk and added into a final image.

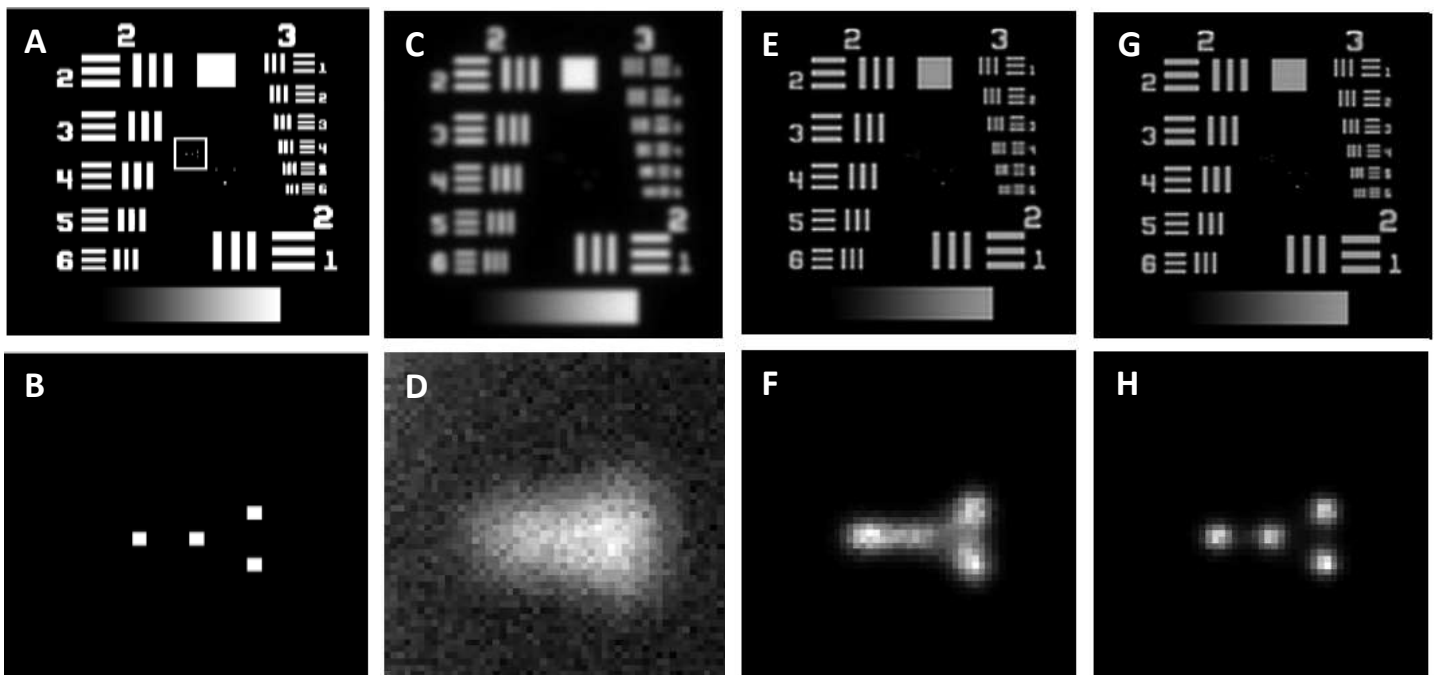


Figure 4. jRL deconvolution of simulated ISM data. A: 500 x 500 pixel resolution target. Square shows the magnified region with a cluster of point sources. B: Magnified 25 x 25 pixel view showing cluster of point sources. C&D: Simulated diffraction-limited image. E&F: ISM using the classical excitation. G&H: ISM with STED doughnut PSFs only.