


REVIEW

Open Access



# Management of the thrombotic risk associated with COVID-19: guidance for the hemostasis laboratory

M. Hardy<sup>1,2</sup>, T. Lecompte<sup>3</sup>, J. Douxfils<sup>4,5</sup>, S. Lessire<sup>2</sup>, J. M. Dogné<sup>4</sup>, B. Chatelain<sup>1</sup>, S. Testa<sup>6</sup>, I. Gouin-Thibault<sup>7</sup>, Y. Gruel<sup>8</sup>, R. L. Medcalf<sup>9</sup>, H. ten Cate<sup>10</sup>, G. Lippi<sup>11</sup> and F. Mullier<sup>1\*</sup> 

## Abstract

Coronavirus disease 2019 (COVID-19) is associated with extreme inflammatory response, disordered hemostasis and high thrombotic risk. A high incidence of thromboembolic events has been reported despite thromboprophylaxis, raising the question of a more effective anticoagulation. First-line hemostasis tests such as activated partial thromboplastin time, prothrombin time, fibrinogen and D-dimers are proposed for assessing thrombotic risk and monitoring hemostasis, but are vulnerable to many drawbacks affecting their reliability and clinical relevance. Specialized hemostasis-related tests (soluble fibrin complexes, tests assessing fibrinolytic capacity, viscoelastic tests, thrombin generation) may have an interest to assess the thrombotic risk associated with COVID-19. Another challenge for the hemostasis laboratory is the monitoring of heparin treatment, especially unfractionated heparin in the setting of an extreme inflammatory response. This review aimed at evaluating the role of hemostasis tests in the management of COVID-19 and discussing their main limitations.

**Keywords:** Thrombosis, D-dimers, Anticoagulation, COVID-19, Coagulopathy, Hemostasis, Fibrinolysis, Heparin, Thrombin generation, Viscoelastic tests

## Introduction

Since the beginning of the coronavirus infectious disease 2019 (COVID-19) pandemic in December 2019, increasing data have supported a major thrombotic risk, which could explain a substantial part of morbidity and mortality associated with this infection. The first observations in China reported a marked increase in plasma D-dimers, associated with unfavorable prognosis and enhanced thrombotic risk [1, 2]. A recent meta-analysis demonstrated an association between several inflammatory biomarkers (such as C-reactive protein (CRP), procalcitonin, interleukin (IL-6) and ferritin) with COVID-19 severity [3]. There is a cross-talk between

inflammation and coagulation as inflammation leads to coagulation activation, and coagulation also affects inflammatory activity [4, 5]. Although heparin at prophylactic doses appears to be effective in reducing mortality in severe COVID-19 patients [6], several studies reported a considerably high incidence of venous and even arterial thromboembolic events (deep vein thrombosis, pulmonary embolism or in situ thrombosis in the pulmonary arteries; arterial thromboses in the systemic circulation) despite thromboprophylaxis, thus raising the issue of increasing anticoagulant doses [7–14]. This approach has been suggested by several groups of experts for patients at higher thrombotic risk [15–19]. However, this suggestion has not been endorsed by other expert groups or societies [20–23]. Prospective trials are currently in progress to try to answer this question.

\* Correspondence: [mullierfrancois@gmail.com](mailto:mullierfrancois@gmail.com)

<sup>1</sup>Université catholique de Louvain, CHU UCL Namur, Namur Thrombosis and Hemostasis Center (NTHC), Hematology Laboratory, Yvoir, Belgium  
Full list of author information is available at the end of the article



© The Author(s). 2020 **Open Access** This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>. The Creative Commons Public Domain Dedication waiver (<http://creativecommons.org/publicdomain/zero/1.0/>) applies to the data made available in this article, unless otherwise stated in a credit line to the data.

The features and specificities of hemostasis disorders associated with COVID-19 are partially known only. In general, severe pulmonary inflammation (acute respiratory distress syndrome (ARDS)) is associated with a significant thrombotic risk, the main mechanisms of which include (i) local expression of tissue factor (TF) on mononuclear cells, its accumulation and release following endothelial damage, which subsequently initiates coagulation initiation and thrombin generation, (ii) as well as inhibition of fibrinolysis in response to the cytokine storm (TNF $\alpha$ , IL-1, IL-6) [24–26]. IL-1 and TNF- $\alpha$  are also the main cytokines responsible for the impairment of endogenous anticoagulant pathways [27]. Increase in von Willebrand factor (vWF), FVIII and fibrinogen plasma levels was also observed [28]. Regarding fibrinolysis, an initial and transient increase of tissue plasminogen activator (tPA) has been described in severe acute inflammatory states, rapidly followed by a sustained release of PAI-1 by the endothelium [28], the extend of the latter being associated with a worse outcome [29]. Accordingly, t-PA and PAI-1 levels were increased at ICU admission in ARDS patients in a recent study, whether COVID-19 or not [30]. Levels of thrombin activatable fibrinolysis inhibitor (TAFI) and protein C inhibitor were also found to be significantly elevated in the bronchoalveolar fluid of patients with interstitial lung disease when compared to healthy controls, which could also add to the hypofibrinolysis observed [31, 32]. However, this hypothesis seems at odds with the marked increase in plasma D-dimers observed in COVID-19 patients. This needs to be further investigated in patients with COVID-19.

Other biomarkers of *in vivo* activation of blood coagulation such as soluble fibrin complexes may also be informative in assessing the thrombotic risk, but their usefulness remains to be established. In this article, we will be using the term ‘D-dimers’ to designate the (soluble) fibrin degradation products containing the motif ‘D-dimers’ and that of soluble fibrin complexes (SFC) to designate complexes containing one or more fibrin monomers associated with two fibrinogen molecules or with fibrinogen (or even fibrin) degradation products (Table 1).

Endothelial activation by inflammatory cytokines (with secretion of von Willebrand factor, factor VIII and PAI-1) and dysfunction could also contribute to the prothrombotic state observed in COVID-19 patients [33]. Previous studies identified possible direct infection of endothelial cells by SARS-CoV-2 with endothelialitis [34] and increased circulatory endothelial cells, an indicator of endothelial damage [35]. As in many severe inflammatory states, thrombotic microangiopathy (TMA) may develop secondary to acquired deficiency of ADAMTS13 and subsequent increase in large von

Willebrand factor multimers [27, 36]. In COVID-19, signs of localized pulmonary TMA were observed with typical microvascular platelet-rich thrombi identified in small vessels of the lungs and other organs. Von Willebrand factor antigen and activity were reported to be elevated and ADAMTS13 levels to be decreased, although remaining higher than 10% [27, 36, 37]. However, schistocytes were not identified on blood smears, signs of hemolysis were absent and platelet count was higher than expected in this condition [27].

With limited solid data available, many questions remain unanswered regarding underlying mechanisms but also stratification and management of thrombotic risk, including the level of anticoagulation and the duration of treatment. Some first-line hemostasis tests (i.e., activated partial thromboplastin time (APTT), prothrombin time (PT), fibrinogen, D-dimers, platelet count) are easy to perform, widespread and relatively inexpensive, but have also significant drawbacks, which should be clearly considered in guiding clinical management. The reliability of D-dimers, especially at very high values, as well as the respective role of anti-Xa activity and APTT for monitoring therapy with unfractionated heparin (UFH), will be discussed in the following parts of this article. The indications and limitations of tests available in the hemostasis laboratory are summarized in Table 2.

### Hemostasis assessment in the laboratory

COVID-19 is frequently associated with hemostasis disturbances (often referred to as “coagulopathy”, even if many if not all aspects of hemostasis can be affected), which significantly enhance the risk of thrombosis, and in particular venous thrombosis. Several studies have found an association between increased plasma D-dimers values and unfavorable prognosis in COVID-19 [1]. Different thresholds have been proposed for stratifying the risk of mortality (i.e. between 1000 or 3000 ng/mL [38, 39]), most often according to retrospective, methodologically weak studies, with limited statistical power. D-dimers at hospital admission could also be predictive of thromboembolic events [2, 11, 14, 40, 41]. However, in the presence of significant pulmonary inflammation, such as in severe COVID-19, fibrin deposits can occur within alveoli and pulmonary extravascular space, which has been confirmed in COVID-19 patients in autopsies series [42]. The lysis of those deposits could also contribute to the rise of D-dimers, which are thus not specific of intravascular fibrin formation [43, 44].

Nevertheless, the measurement of plasma D-dimers has been put forward by some expert groups as a laboratory criterion, along with clinical data, for stratifying COVID-19 patients according to their thrombotic risk, and to consider adjusted anticoagulation intensity. For example, the working group on perioperative hemostasis

**Table 1** Definition of D-dimers, fibrin monomers, fibrinogen degradation products and fibrin degradation products

Entity	Definition	Antigenic definition (what is recognized by the antibodies of the immunoassay – immunogen that was used to obtain the antibodies in the animal)
<b>Degradation products containing the ‘D-dimers’ motif (fibrin degradation products)</b>	Soluble molecular assemblies produced by the action of plasmin on polymerized fibrin stabilized by factor XIIIa, hence comprising the ‘D-dimers’ motif	Two ‘D’ nodules of two adjacent fibrin monomers in the fibrin network, covalently linked by factor XIIIa
<b>Soluble fibrin complexes</b>	Complexes formed of at least one fibrin monomer associated with fibrinogen molecules, but also fibrinogen or even fibrin degradation products – those complexes are soluble in plasma	desAA-fibrin (fibrinogen from which fibrinopeptides A have been removed)
<b>Fibrinogen degradation products</b>	Molecules produced by the action of plasmin on fibrinogen (when there systemic fibrinolysis occurs)	Nodule ‘D’ or ‘E’ of fibrinogen: present on fibrinogen and their degradation products; fibrinogen must therefore be eliminated beforehand so as not to be measured

(GIHP stands for “Groupe d’Intérêt en Hémostasie Périopératoire” in French) with the French group of studies on hemostasis and thrombosis (GFHT, stands for “Groupe Français d’Étude sur l’Hémostasie et la Thrombose”) considered patients with plasma D-dimers levels > 3000 ng/mL as having a very high thromboembolic risk, and hence might benefit from increased doses of heparin [15]. In patients at high risk of thromboembolism, other authors also recommended continuing thromboprophylaxis after hospital discharge for a maximum of 45 days after individual assessment of the benefit/risk balance [45]. However, the variability between methods for measuring D-dimers raises questions about the use of a fixed threshold [46, 47]; an increased plasma D-dimers concentration with ongoing thromboprophylaxis should give consideration of the administration of higher doses of anticoagulants, and to the active search for thrombotic event.

The most seriously affected individuals (non-survivors and those admitted to intensive care), also have slightly longer PT than patients with more favorable prognosis [48, 49]. APTT is generally proportionally less prolonged than PT, probably due to an increase in plasma concentration of factor VIII, which is an acute phase reactant [48, 49]. A low platelet count at admission (i.e., < 200 × 10<sup>9</sup>/L), along with a further decline during hospital stay, has also been associated with increased risk of death [50–52].

In the majority of patients, hemostasis disorders associated with COVID-19 do not evolve towards disseminated intravascular coagulation (DIC), the diagnostic criteria of which include, according to the International Society on Thrombosis and Haemostasis (ISTH), a reduction in platelet count and fibrinogen levels associated with an increase in PT and markers of fibrin formation, or ‘fibrin-related markers’ (D-dimers or SFC, the former being the most used in Europe) [49, 53]. Among laboratory criteria, hypofibrinogenemia (< 1 g/L) is a late criterion and hence a poorly sensitive one, which can only be

found in less than 50% of cases [54]. This observation can be explained by enhanced liver production of fibrinogen in response to systemic inflammatory response, which is hence effective to maintain normal plasma concentrations even in concomitance with consumption coagulopathy. A shortening of PT has also been reported in up to 30% of patients with COVID-19, which has been explained with increased fibrinogen concentration in plasma [55]. In this setting, the early identification of consumption coagulopathy can therefore be jeopardized, so that longitudinal monitoring of these parameters, at least in more severe patients admitted to the ICU, would be necessary to identify early changes that would indicate the onset of DIC.

Monitoring every 48 h the plasma concentration of PT, fibrinogen, D-dimers and platelet count has been proposed for continuously assessing the thrombotic risk and identifying timely alerts on possible venous thrombotic events, as reflected by markedly increasing concentrations of D-dimers within 24–48 h [15, 27]. An increase in the plasma D-dimers in patients with anticoagulant therapy may also warrant an increase in anticoagulation intensity, after weighting thrombotic and hemorrhagic risks, although there is no clinical evidence yet to support such D-dimers based dose adjustments.

However, the relevance of the utilization of D-dimers levels to tailor thromboprophylaxis in COVID-19 patients has been questioned, as plasma D-dimers levels could depend more on the lysis of extra-vascular rather than intra-vascular fibrin deposits [43, 44]. This would be consistent with the observation that SFC levels, which are thought to only depend on intra-vascular fibrin deposition, remain low in most COVID-19 patients despite high D-dimer levels [30]. Additional biomarkers of in vivo enhanced thrombin generation, such as SFC, may thus provide some additional useful information for managed care of COVID-19 [56]. SFC could also be an earlier marker of DIC than D-dimers, of which the concentration increases only after clot lysis has begun [56].

**Table 2** Indications and limitations of tests available in the hemostasis laboratory

	Main Limitations	Indications in COVID-19					
		Evaluation of the thrombotic risk	Screening of thromboembolic events	Prognosis: disease severity	Diagnosis of DIC	Detection of HIT	Monitoring of unfractionated heparin
<b>Platelet count</b>	Many causes of thrombocytopenia in the critically ill patient			X	X	X	
<b>APTT</b>	Major influence of preanalytical step Differences of APTT reagents in their sensitivity to unfractionated heparin, lupus anticoagulant and inflammatory syndrome					X (*)	X
<b>Prothrombin Time</b>	Influence of the preanalytical step Influence of fibrinogen level				X		
<b>Fibrinogen (Clauss)</b>	Lack of sensitivity for the diagnosis of DIC (mostly in infectious/inflammatory setting)	X		X	X		
<b>D-dimers</b>	Possibility of interference of direct thrombin inhibitors with some reagents Decreased analytical performances in high D-dimers values Production dependent on the fibrinolytic activity Cut-offs non commutable between reagents	X	X	X	X		
<b>Soluble fibrin complexes (AKA 'Fibrin monomers')</b>	Preliminary validation only Not evaluated in COVID-19 Cut-offs non commutable between the reagents		X		X		
<b>Fibrinolysis capacity tests</b>	Fibrinolysis is assessed in non-physiological conditions Large array of methods Not evaluated in COVID-19	X		X			
<b>Anti-Xa activity</b>	Inter-reagent variability Influence of presence/absence of exogenous AT in the reagent Expensive Only available 24 h a day 7 days a week in a fraction centers						X
<b>Viscoelastic tests</b>	Not evaluated in COVID-19 Lack of standardization between instruments and centers Expensive	X		X			X
<b>Thrombin generation assays</b>	Not evaluated in COVID-19 High sensitivity to heparins Limited availability in clinical practice Expensive	X					

(\*) Heparin resistance can be due to HIT.

Note: the assessment of the in vivo effect of (any) anticoagulant treatment could be assisted with the monitoring of fibrin-related markers (D-dimers; fibrin monomers)

Measurement of plasma SFCs has therefore been proposed as an option besides that of D-dimers in the diagnostic scores for DIC proposed by the ISTH and the Japanese society of Thrombosis Hemostasis (JSTH) [57, 58]. However, the diagnostic thresholds vary considerably from one kit to another (two kits are available to the best of our knowledge: STA-Liatest FM® kit (Stago, Asnières-sur-Seine, France) and Nanopia SF (Sekisui Medical, Japan)), and there is a lack of extensive clinical validation [59, 60]. For instance, The STA-Liatest FM® kit (Stago, Asnières-sur-Seine) uses a monoclonal antibody (F405) specific for fibrin monomers. This antibody is produced using desAA-fibrin as immunogen in the presence of an anti-polymerization peptide (Gly-Pro-Arg-Pro, GPRP) [61]. Regarding desAA-fibrin, it is the result of an enzymatic cleavage of purified fibrinogen by the action of batroxobin (reptilase), with the release of fibrinopeptides A only; under those conditions, factor XIIIa cannot have any role, thus there is no 'D-dimer' motif. The evaluation of laboratory performance by an external quality control (EQA performed by ProBioQual) showed an inter-laboratory imprecision (coefficient of variation; CV) of ~30% for the three levels of controls tested. The half-life of SFC is slightly shorter than that of D-dimers (i.e., <6 h), depending on the clinical context though (size and range of molecules produced, fibrinolytic activity and so forth) [62]. The half-life is hence longer than that of fibrinopeptides A and B (3–5 min), thrombin-antithrombin complexes (TAT; 10–15 min) and prothrombin fragments 1 + 2 (90 min) [63], so that is less dependent on the time of blood collection, considering that activation of coagulation cannot be a continuous, steady process. Nevertheless, the influence of the time elapsed between thrombosis onset, blood collection, and measurement, as well as the potential influence of anticoagulants remain to be studied [56]. For all assays, in particular for fibrinopeptides and TAT, the influence of preanalytical artifacts (thrombin formed during blood collection and processing) should be considered [56]. At this stage, additional evidence is needed to define the incremental clinical value of SFC over D-dimers in COVID-19 hemostasis monitoring.


#### **Limitations of measurement of the plasma concentration of D-dimers**

Even if the usefulness of D-dimer testing in the management of COVID-19 patients remains uncertain, some expert groups suggested the use of this parameter together with clinical variables to stratify patients according to their thrombotic risk and determine thromboprophylaxis intensity accordingly [15–19]. This implies that test results shall be timely and reliable, and accurate threshold values need to be defined according

to the specific clinical context and the immunoassay used.

Soluble fibrin degradation products containing the D-dimer motif constitute a heterogeneous set of molecules produced during degradation of polymerized fibrin network, which has been previously covalently cross-linked by activated factor XIII. This explains differences observed between fibrinogen and fibrin degradation products (FDP), the former being generated by degradation of fibrinogen from the fibrinolytic system (Fig. 1) [58]. A large inter-laboratory variability has been reported for the measurement of the plasma D-dimers concentration, which mostly reflects the different assay methodologies, the different mix of antibodies with variable antigenic specificity, the individual calibration and the variation of measuring units [64–66]. The lack of internationally certified calibrators and quality controls also challenges to achieve better degree of universal harmonization. The large inter-individual variability (depending among others on renal function), is a further source of uncertainty in test results interpretation. A diagnostic threshold that has been validated within a specific clinical setting, using a certain assay, cannot be translated to different analytical conditions and different clinical settings [67]. The diagnostic thresholds shall hence be validated according to the method used and for the intended diagnostic purpose. Most of the available D-dimers assays have also been developed to have the best reproducibility around the threshold value used for excluding deep vein thrombosis and/or pulmonary embolism, which is usually around 500 ng/mL. Therefore, their performance at higher values, such as those proposed for initiating high dose anticoagulation in COVID-19 patients (i.e., over 3000 ng/mL), is probably suboptimal and would need to be assessed in order to avoid the use of inaccurate results in these patients. For example, external quality controls performed with moderately elevated D-dimers samples (target value 4000 ng/mL FEU) identified method-specific D-dimers means ranging from 470 to 10,150 ng/mL FEU (all methods coefficient of variation: 23%) [68]. As a possible solution, the threshold values of plasma D-dimers could be adjusted based on assay methodology. For example, for DIC diagnosis according to the ISTH definition, the appropriate D-dimer cut-off value for 2 points ranged from 3500 ng/mL to 6500 ng/mL, depending on the reagents used [69].

The potential impact of many preanalytical variables on measurement of plasma D-dimers should also be considered, as this test is vulnerable to the excessive presence of free hemoglobin in plasma, and becomes virtually uninterpretable when the plasma free hemoglobin concentration is over 30 g/L [70]. Hyperlipemia, hyperbilirubinemia or a high concentration of immunoglobulins

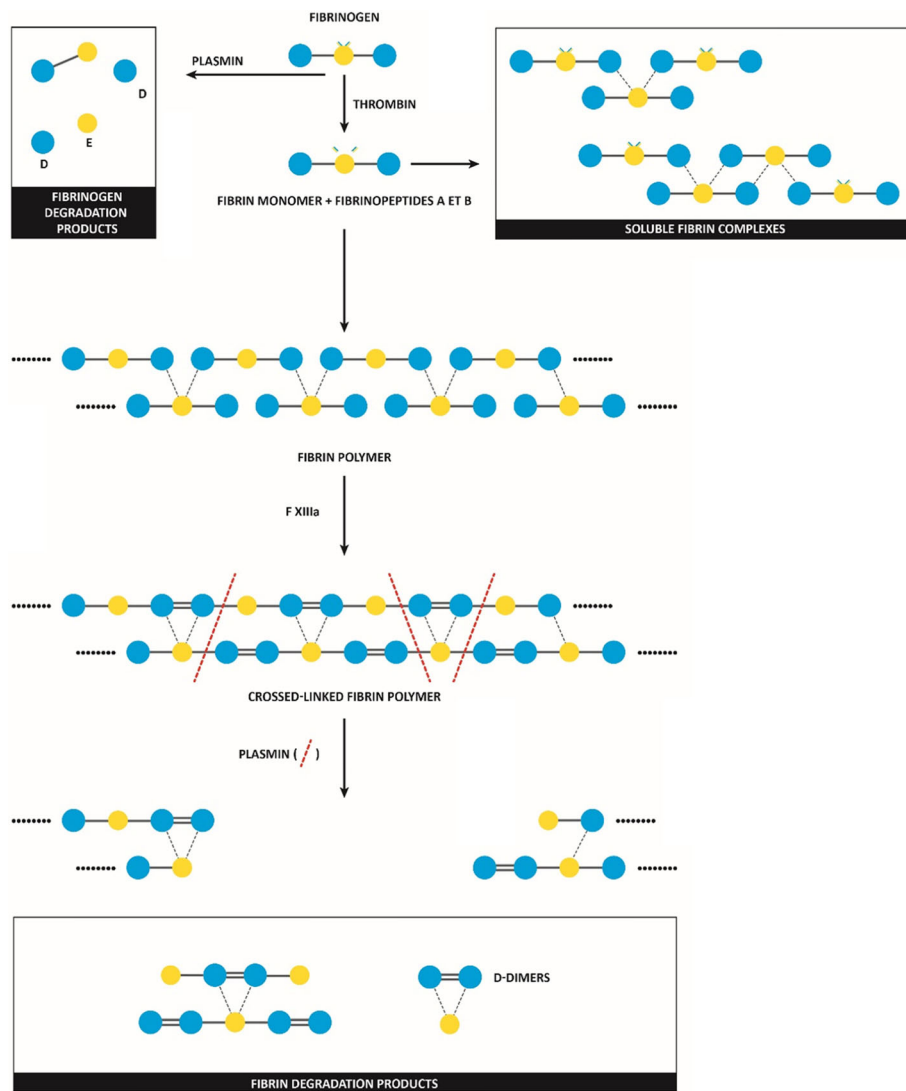

**Fig. 1** Mechanisms of production of: D-dimers, fibrin monomer, fibrinogen degradation products and fibrin degradation products. Fibrinogen is composed of two lateral regions “D” and one central region “E” connected by coiled coils: the formula is D-E-D. Fibrinopeptides A and B located at the N-termini of A-alpha and B-beta chains (x2) on the E region are cleaved from fibrinogen by thrombin, resulting in the production of a fibrin monomer (FM). FMs are highly reactive and if locally formed and concentrated, quickly interact with one another by to form a two-stranded fibrin polymer. These polymers then aggregate laterally to make fibers (not shown). Activated factor XIII covalently crosslinks adjacent D regions (belonging to two fibrin monomers), which tightens the fibrin strand, increases clot stiffness, and makes it more resistant to degradation by plasmin. Other crosslinks also occur, not shown here for simplicity’s sake. The physical state is a gel - such polymerized structures are no longer soluble. During fibrinolysis, plasmin can cleave fibrin polymers between adjacent D and E regions, but cannot separate covalently linked D regions. This produces fibrin degradation products of different size, containing the ‘D-dimer’ motif, and when small enough are soluble. FM can escape in the fluid plasma phase, the more so if formed in a disseminated manner (systemic thrombin generation), and then quickly binds to fibrinogen molecules, or fibrinogen degradation products, bringing the polymerization process to an end; they hence remain soluble because they are small enough. These compounds are known as ‘soluble fibrin complexes’ (SFC). In the presence of hyperfibrinolysis (systemic, disseminated), PAI-1 (plasminogen activator inhibitor) and alpha2-antiplasmin can be overwhelmed, and uninhibited plasmin can diffuse in the plasma fluid phase; under those conditions, plasmin can also cleave fibrinogen molecules, resulting in fibrinogen degradation products production. ‘FDP’ may refer to both fibrinogen and fibrin degradation products

can also generate a bias in the measurement, though the influence of these conditions has been less studied [70]. However, it has to be considered in the context of COVID-19 due to the high concentration of immunoglobulins measured in some of these patients 2 weeks after the symptom onset [71].

**Laboratory investigation of fibrinolysis**

Many of the methods available for the study of fibrinolysis have significant drawbacks. Fibrinolysis assays are technically challenging, time consuming and cannot be easily automated, thus explaining their underuse in clinical laboratories. Under physiological circumstances,

fibrinolysis takes many hours or days to develop in healthy blood after clotting, and this is indeed a major limitation for rapidly assessing the 'global fibrinolysis capacity' (GFC). The accelerated (albeit remaining long) assessment of fibrinolysis needs prior removal of inhibitors or the addition of tPA to initiate plasmin generation, complicating our appraisal of what is going on in vivo. Plasma-based systems, for example, where clotting and lysis may be easily monitored with turbidimetric assessment, need tPA to accelerate the reaction [72]. Alternatively, euglobulin may be prepared from plasma, thus lowering the concentration of fibrinolytic inhibitors (including PAI-1 and antiplasmin) [73, 74].

Individual components of the fibrinolytic system can also be measured. Although interesting evidence is emerging especially for PAI-1 in COVID-19 [30], its measurement is limited by large inter-laboratory variability, which is attributable to the different assay methodology, antigenic specificity of the antibodies, the lack of internationally certified calibrators and quality controls, as well as to the many measuring units that can be used for reporting data.

Interestingly, PAI-1 follows a circadian rhythm in humans, with a morning peak (around 8 AM) independent from the sleep pattern [75, 76]. The time-interval between blood collection and analysis, the anticoagulant used in sample tubes and storage temperature are other variables that are known to have an impact on plasma PAI-1 measurement [77–79].

A weak stability at room temperature of the plasma used for assessing fibrinolysis (and especially PAI-1) has been occasionally described, whilst hemolysis (with release of cell free hemoglobin and other intracellular components) may contribute to produce an inhibitory effect on some fibrinolysis assays [80]. The contact phase (i.e., activated factor XII) also stimulates fibrinolysis through conversion of single chain urokinase-type plasminogen activator (scu-PA) in uPA [81]. Therefore, standardization of preanalytical and analytical steps is of utmost importance for obtaining accurate and reliable results of most fibrinolysis assays.

Regarding viscoelastic tests, ROTEM and TEG currently lack sensitivity to disordered fibrinolysis but there is still room for improvement [82].

As some extracellular vesicles are able to facilitate plasmin generation, it would be interesting to assess the contribution of such vesicle-dependent fibrinolytic activity in COVID-19 [83, 84].

### Viscoelastic tests

Viscoelastic tests (VETs) are "global" hemostasis tests evaluating mechanical properties of the clot as it forms and lyses. The most frequent used VETs comprise thromboelastography (TEG) and rotational

thromboelastometry (ROTEM). These commercial assays are embedded in the care for critically ill patients in many institutions, in particular for guiding transfusion management in patients at high risk of bleeding. In general, these assays are sensitive to detect hypocoagulability related to consumption of coagulation factors like fibrinogen, but hypercoagulability can also be detected. Indeed, increased clot firmness has been associated with occurrence of venous thromboembolism (VTE) in various clinical settings [85–91], and has hence been proposed for evaluating the thrombotic risk associated with SARS-CoV-2 infection.

In COVID-19 patients, whole blood rotational thromboelastometry (ROTEM) has been able to detect accelerated clot formation and increased clot strength, persisting for at least 5 days [92]. Similar findings were reported by other groups using ROTEM and Quantra instruments, with both elevated platelets and fibrinogen contribution to clot strength [93, 94]. Increased heparin prophylaxis dose was associated with attenuation of fibrinogen contribution to clot strength and fibrinogen level, although lacking control conditions, this may have been a chance finding. Data regarding fibrinolysis evaluation in COVID-19 using VETs is sparser; hypofibrinolysis has been identified in one study [95], although another could not confirm this result [92]. Only one study evaluated the association between clinical outcomes and VETs parameters in COVID-19. The authors identified that the lack of clot lysis at 30 min on citrated kaolin TEG with heparinase was associated with VTE, whereas increased clot strength was not [95]. The combination of absence of lysis at 30 min with D-dimers levels >2600 ng/mL was also strongly associated with VTE and with the need for dialysis [95]. Nonetheless, the place of VETs in the management of COVID-19 deserves further evaluation.

When using VETs, some drawbacks have to be considered. First, these tests are generally poorly sensitive to platelet function and mild fibrinolysis disorders [96, 97], and their sensitivity to fibrinogen levels is quite variable depending on the test methodology [98]. Second, even if considered as being global tests, they do not evaluate the contribution of endothelium, whose dysfunction likely contributes to COVID-19 associated hemostasis disturbances [34]. Moreover, similarly to D-dimers and SFC, correlation between methods is moderate, and inter-laboratory variation is high [99], but probably improving with introduction of new methods (ROTEM Sigma<sup>®</sup>, TEG6S<sup>®</sup> and Quantra<sup>®</sup>). Regarding preanalytical conditions, the time-interval between blood collection and VET [100, 101], anticoagulants and/or additives used in sample tubes [102, 103], over or underfilling of blood tubes [104], hemolysis [105] and hematocrit [106–108] can influence the test results. Pneumatic tubes transport

systems (PTS) may also exert little influence on test results, depending on acceleration forces of the local system [109–112]. Therefore, this effect should be evaluated locally when utilization of PTS is considered for blood sampled for VETs. Finally, the accuracy of these tests for bleeding management or thrombotic risk stratification has not been validated in any hyperinflammatory context. Caution is therefore required when using VETs in COVID-19 patients, and further studies are needed to precise their added value in the management of these patients.

#### Thrombin generation assay

Thrombin generation assays (TGA) enable an integrative approach of coagulation. Commercial assays include Technothrombin® TGA kit from Technoclone and Calibrated Automated Thrombogram® (CAT) and ST-Genesia® from Stago Diagnostica [113, 114]. While TGA may be used to detect hypercoagulability, the frequent use of heparin/low molecular weight heparin (LMWH) in hospitalized COVID-19 patients could make this test relatively unsuitable for evaluating hypercoagulability. Modification of the TGA conditions, i.e. by adding polybrene or heparinase as neutralizing agent [115], could be of interest to eliminate heparin. However, data has not been reported yet in COVID-19 patients. Of note, pre-analytical variables and choice of the reference plasma to normalize the result also have important impact on TGA measurement and must be controlled in order to reduce the variability of measurement [116].

#### Anticoagulation - laboratory monitoring

Due to the high thrombotic risk associated with this infection, systematic antithrombotic prophylaxis should be administered and to date, parenteral administration of a heparin preparation is the preferred procedure in the hospital setting.

#### Choice of anticoagulant

LMWH is recommended as first-line therapy for the prophylaxis of VTE in hospitalized COVID-19 patients [15, 20, 117, 118]. Direct oral anticoagulants (DOACs) or vitamin K antagonists, are not recommended because of the risk of drug interactions, among others with some antiviral drugs, the expected broad fluctuation in plasma concentrations (for DOACs), especially in patients at higher risk of rapid clinical deterioration, and because of the late onset of anticoagulation and higher risk of bleeding with VKA [119]. Heparin, and especially the long heparin chains, was reported to also exhibit anti-inflammatory activity in addition to the anticoagulant effect, by binding and neutralizing inflammatory cytokines and acute phase proteins, while potentially exerting a protective effect on endothelium [120]. It also interferes with neutrophils recruitment into tissue and

impairs neutrophil function by inhibiting the activity of the neutrophil protease's human leukocyte elastase and cathepsin G, which can promote inflammation [121, 122]. It has also been hypothesized that heparin may hinder the interaction between the virus and the host cell through non-specific ionic bond, and thus may contribute to decrease the rate of infected cells [120, 123]. However, we do not yet know precisely to what extent heparin is clinically effective in this infection.

Compared to UFH, LMWH has better bioavailability after subcutaneous administration and longer duration of action, allowing daily administration in one or two injections. No regular laboratory monitoring is necessary for treatment with LMWH because of the predictable anticoagulant activity after administration of doses adjusted to body weight on the one hand, and the lack of formal association demonstrated between laboratory tests results and clinical efficacy or complications on the other [124]. However, a single anti-Xa activity measurement can be proposed in case of administration of high or intermediate doses in a patient with moderate renal impairment, with a BMI < 18 kg/m<sup>2</sup> or > 30 kg/m<sup>2</sup>, or during pregnancy, mainly to rule out drug accumulation [125]. In the event of increased doses in patients at enhanced thrombotic risk, measurement of anti-Xa activity is also recommended 4 h after the third dose to exclude accumulation. The anti-Xa value must be based on a calibration curve with the specific heparin type and interpretation of test result must also be made for the same compound; e.g. with therapeutic doses of enoxaparin, the mean peak concentration observed is 1.2 IU/mL. This measurement can be repeated for example in case of renal function impairment.

UFH is only recommended in case of severe renal failure (creatinine clearance according to Cockcroft-Gault equation < 30 mL/min), extracorporeal membrane oxygenation (ECMO) [15] or significant bleeding risk (shorter half-life than LMWHs, easier neutralization by protamine) [126]. The risk of heparin-induced thrombocytopenia (HIT) is also much higher with UFH [127]. Regular laboratory monitoring during anticoagulation is necessary because of the high inter- and intra-individual variability in the anticoagulant response [125].

#### Laboratory monitoring of unfractionated heparin treatment

Adjustment is thought to be required because of high inter and intra-individual variability. Historically, adjustment of UFH dosage was based on APTT. The measurement is performed 4 to 6 h after initiation and any dose change, and once a day at least, to reach a target APTT ratio between 1.5 and 2.5. This therapeutic target dates from work in 1972 and has never been confirmed in large clinical studies [128]. Since then, the number of



reagents used for the APTT has exponentially increased, the sensitivity of which is very different both to heparin and biological interference (including several proteins of the acute phase) [129–131]. Therefore, calculation of the APTT ratio corresponding to an anti-Xa activity between 0.3 and 0.7 IU/mL would be recommended for each analyzer and each new batch of reagents. This calculation should best be performed with plasma samples from patients treated with UFH because the use of plasma spiked with UFH gives less relevant results due to the influence of the metabolism of heparin *in vivo* and its bioavailability [132]. For some reagents, the relationship between heparin levels and APTT is linear, but this can change in case of significant inflammation [133]. Most importantly, APTT is very dependent on pre-analytical conditions. Among others, platelet factor 4 (PF4) released by activated platelets during inadequate sampling procedure or prolonged delay before centrifugation can neutralize part of the heparin, leading to a risk of underestimating its activity [134].

Several biological parameters can cause a prolongation of the APTT (e.g. high CRP, presence of lupus anticoagulants, coagulation factors deficiency, high plasma concentration in FDPs which oppose the polymerization of fibrin) or its shortening (e.g. increased plasma concentration of acute phase proteins such as FVIII and fibrinogen) [63, 135, 136]. The influence of these parameters will also depend on assay methodology, the type of reagents, and has a high inter-individual and intra-individual (i.e., during hospitalization) variability [137, 138]. For these reasons, the GFHT advises against the use of APTT for monitoring treatment with UFH [133]. Moreover, the use of APTT is problematic when this test is prolonged prior to initiation of UFH treatment (for example, in case of lupus anticoagulants or coagulation factors deficiency); anti-Xa target should also consider the etiology of this prolongation when clinically relevant (i.e. defects with a bleeding risk).

In COVID-19, the increased plasma concentrations of fibrinogen and FVIII can cause a shortening of APTT (observed in 16% of affected patients) [55], and this may lead to underestimating the anticoagulant effect of heparin. This situation can contribute to excess heparin dosing, enhancing the bleeding risk, and underlines the importance of collecting a basal APTT value before anticoagulation. This can be problematic in some settings, e.g. in the ICU, where patients are frequently transferred with anticoagulation already started at intermediate or therapeutic doses [13]. Conversely, APTT prolongation may be related to the transient increased levels of antiphospholipid antibodies, a situation encountered during viral infections [139], including COVID-19 [10, 140–143], or when CRP is high [138], thus leading to a risk of heparin underdosage. Lupus anticoagulant

screening can also be falsely positive in the presence of variables prolonging clotting time of tests used for its screening (for example, elevated CRP or presence of anticoagulants, among which heparin) [143–146]. The APTT may also be prolonged in the presence of DIC (which is relatively rare in COVID-19). In this situation, its measurement by means of an optical system may become uninterpretable: an immediate and gradual decrease in light transmittance can be observed even before clot formation due to the presence of a complex between CRP and very low density lipoproteins in the presence of calcium [147], thus rendering the measurement unreliable [148]. Therefore, mechanical methods are advisable in this circumstance, where measurement anti-Xa activity may even be the best choice.

Thus, heparin monitoring with aPTT may be challenging in COVID-19 patients due to the hyper-inflammatory status of the patient. Indeed, the high fibrinogen and factor VIII levels, the interference of CRP (depending on the reagents used) and also the potential presence of antiphospholipid antibodies may affect the aPTT. Therefore, anti-Xa activity seems more suitable to monitor UFH treatment in these patients and more generally in ICU patients for the very same reasons. However, there are several caveats here as well. First, FXa is not the essential target of UFH. Its inhibition is studied under very artificial conditions: in the fluid phase (and not within the prothrombinase complex formed on a phospholipid surface) and in a calcium-depleted medium. The *in vivo* inhibitory activity of UFH is indeed three times stronger towards FIIa than FXa [149]. This difference is further artificially increased *in vitro* by use of low calcium concentrations in the assay mixture: the anti-Xa activity was halved under these conditions, compared to physiological concentrations of calcium, but the effect of low calcium on anti-IIa activity is more limited [149]. Having mentioned that, a good correlation exists *in vitro* between anti-Xa and anti-IIa activities, thus enabling the use of the former test to assess the effect of heparin therapy. The anti-Xa assay consists of measuring *in vitro* the residual activity on a chromogenic substrate specific for FXa added to citrated plasma. Compared to APTT, this test has the advantage of being less vulnerable to biological interference (possible interference of free hemoglobin and bilirubin in case of significant elevation [150]) and less dependent on pre-analytical conditions - with the notable exception of PF4 released *in vitro* by platelets. Even if the validity of anti-Xa activity of UFH in the presence of an important inflammatory syndrome has not been formally established (or for that matter under any circumstances), this measure will be less impacted in this context, particularly if the reagents contain antithrombin (AT). However, it is not advisable to use kits with exogenous AT to avoid overestimation of anticoagulant activity in case of AT deficiency, with risk of heparin underdosing. The plasma

concentration of AT can indeed decrease in case of sepsis [151]. Only few data are available on the sensitivity of kits without exogenous AT to changes in plasma AT concentration [152]. Some reagents also contain dextran sulfate, which will displace heparin from its non-specific binding (including PF4). Particularly, the influence of PF4 released by activated platelets is therefore minimized, which is favorable for limiting the impact of pre-analytical conditions on test result, but problematic when the concentration of PF4 is actually high in vivo. Unlike a 'global' test like APTT, the measurement of anti-Xa activity is insensitive to fluctuations in the underlying hemostatic state (for example, coagulation factor defect following hemorrhage or DIC), which should prompt an adjustment in therapeutic targets to the clinical context and the possible identification of such defects. Finally, significant variability in heparin sensitivity has been reported between the different commercial kits [153–156].

The therapeutic range in terms of anti-Xa activity is considered between 0.3 and 0.7 IU/mL [125]. These values are derived from the work of 1972 that was previously mentioned. It was hence inferred from the APTT target to be reached for secondary prevention of VTE. The bottom line is that it lacks validation for the same reasons [157]. The application and interpretation of these tests in a hyperinflammatory context also raises important questions. Given the very high thrombotic risk described or suspected in some subgroups of patients, the GIHP suggested narrowing the target of anti-Xa activity in the upper zone, to 0.5–0.7 IU/mL, for those at the highest thromboembolic risk [15]. This increase in dosage, not supported by objective data, remains debated [20–23], whilst ongoing prospective, multicenter clinical trials aim at addressing this question. In addition to the selection of patients who could potentially benefit from increased doses of anticoagulants, the question of treatment duration is a major one. The resolution of the inflammatory syndrome should be accompanied by a reduction in the thrombotic risk, thus exposing the patient to excessive anticoagulation and risk of bleeding when higher doses of heparin are maintained. However, no firm recommendation on duration and intensity of COVID-19 anticoagulation can be made at this time.

In patients receiving UFH, a laboratory resistance to the anticoagulant effect of heparin, arbitrarily defined by failure to reach the therapeutic target despite the administration of doses > 1.5 times usual doses, which are about 400 to 600 U/kg/24 h [158, 159], is frequently observed in COVID-19 [13, 160], and adds to the clinical resistance previously outlined (occurrence of thrombotic events under well-conducted drug thromboprophylaxis). The hyperinflammatory context could also explain part of this observation. Indeed, UFH is able to non-specifically bind several acute phase proteins as well as

activated endothelial cells and platelets, thus limiting its anticoagulant activity [161, 162]. The administration of an initial bolus of UFH is therefore needed to saturate non-specific fixation [163]. The increased plasma concentration of fibrinogen and FVIII will also contribute to generate heparin resistance when the effect is monitored with the APTT, which is less likely to be observed when anti-Xa activity is used. Acquired AT deficiency by consumption or production defects (negative protein of the acute phase) could also contribute to the heparin resistance observed in some COVID-19 patients [151], especially those most seriously affected [10, 49], but in most patients it does not justify the prescription of AT concentrates. To the best of our knowledge there is one single prospective interventional study on UFH monitoring in case of laboratory heparin resistance. In this study, the utilization of anti-Xa activity instead of aPTT permitted to avoid UFH dosage escalation with similar clinical outcomes [164]. Whether this holds true for COVID-19 patients remains to be established. When heparin resistance is suspected based on APTT values, UFH shall be administered according to the anti-Xa activity [165]. The advantages and limitations of APTT vs anti-Xa for UFH monitoring are summarized in Table 3.

#### Diagnosis of heparin-induced thrombocytopenia (HIT)

A final aspect of heparin monitoring is screening for HIT. A platelet count should be performed before administering the first injection of heparin, if possible, or as soon as possible thereafter. In the COVID-19 setting, it is reasonable to monitor the platelet count regularly between the 4th and the 14th day following the initiation of heparin therapy (once or twice a week in case of LMWH treatment, two to three times a week during UFH treatment), then once a week until the end of the first month of therapy. The development of thrombocytopenia ( $< 100 \times 10^9/L$ ) or the rapid decrease in platelet count (especially if  $\geq 50\%$  in less than 24 h) should then suggest the diagnosis of HIT [166]. However, especially in the presence of acute inflammation and infection, other etiologies may explain a decrease in platelet count. Therefore, a systematic evaluation of clinical probability of diagnosis allows better identification of patients in whom the occurrence of this complication must be suspected, and for whom laboratory work-up for HIT antibodies is indicated. This evaluation is generally performed with the 4Ts' score, much studied [167, 168] [159], despite its limitations, particularly in more complex situations such as those encountered in ICU (no consensus on the drugs responsible for thrombocytopenia, many other causes of thrombocytopenia, very high negative predictive value but not absolute (e.g. thrombosis in the absence of thrombocytopenia), insufficient data on platelet count, weak agreement in the determination of the 4th criteria (other causes of thrombocytopenia)) [166, 169, 170].

**Table 3** Main advantages and limitations of APTT and anti-Xa activity for UFH treatment laboratory monitoring

	Advantages	Limits
<b>APTT</b>	<ul style="list-style-type: none"> <li>- largely available, low cost</li> <li>- sensitive to clinically relevant changes of coagulation (coagulation proteins increases or deficiencies)</li> </ul>	<ul style="list-style-type: none"> <li>- numerous interferences; optical methods can be unreliable in case of DIC</li> <li>- heparin sensitivity is highly reagent dependent</li> <li>- APTT prolongation target needs to be established for each new batch of reagents</li> <li>- APTT before UFH needed</li> <li>- clinically irrelevant changes, or of dubious clinical relevance</li> </ul> <p>APTT prolonged with:</p> <ul style="list-style-type: none"> <li>• presence of antiphospholipid antibodies (viral infections)</li> <li>• high CRP (depending on the reagent)</li> <li>• high plasma levels in FDPs</li> </ul> <p>APTT shortened with:</p> <ul style="list-style-type: none"> <li>• preanalytical (e.g., heparin/EDTA contamination, under-filling, delayed centrifugation, hypertriglyceridemia, hyperbilirubinemia)</li> <li>• preanalytical (e.g., prolonged venous stasis, vigorous mixing, coagulation of the sample, PF4)</li> <li>• high factor VIII levels</li> </ul>
<b>Anti-Xa activity</b>	<ul style="list-style-type: none"> <li>- less vulnerable to biological interferences</li> <li>- no requirement for measurement before UFH administration</li> </ul>	<ul style="list-style-type: none"> <li>- preanalytical interferences: PF4*; free hemoglobin and bilirubin if significant elevation</li> <li>- insensitive to fluctuations in the underlying coagulation state (i.e., coagulation factor increases or defects), of potential clinical relevance</li> <li>- AT deficiency (e.g. in sepsis): risk of heparin underdosing with kits containing exogenous AT; sensitivity to endogenous AT not evaluated with kits that do not contain exogenous AT</li> <li>- variability in reagents composition (AT, dextran...)</li> <li>- therapeutic range poorly defined</li> <li>- not validated in hyperinflammatory states</li> <li>- less available, more expensive</li> </ul>

\*PF4 released by activated platelets during poor sampling technique will neutralize UFH, leading to an underestimation of its activity  
 AT antithrombin, APTT activated partial thromboplastin time, UFH unfractionated heparin, PF4 platelet factor 4; CRP C-reactive protein, DIC disseminated intravascular coagulation, FDP fibrinogen and fibrin degradation products; FVIII factor VIII.

In case of strong suspicion, or as soon as the antibodies are identified, treatment with heparin should be stopped and replaced by a direct thrombin inhibitor (DTI; argatroban, bivalirudin) or by danaparoid sodium. Of note, the presence of a DTI can lead to underestimation of plasma fibrinogen concentrations by inhibition of the thrombin present in Clauss' reagent [171]. This interference will vary depending on the thrombin concentration used in the reagent [172, 173]. To a lesser extent, interference may also exist in the presence of high concentration of UFH (0.6 to 2.0 IU/mL, depending on the reagent), which would exceed the neutralization capacities of the reagent used, or in the presence of high concentration of FDPs (> 100–130 µg/mL) [173].

### Conclusion

SARS-CoV-2 (COVID-19) infection is associated with a laboratory prothrombotic state and a high incidence of thrombosis. The follow-up of COVID-19 patients by

hemostasis testing could be pivotal, both in terms of risk evaluation and therapeutic monitoring, though the limitations of the tests used must always be acknowledged. Longitudinal studies are needed to clarify which parameters are the most relevant in terms of thrombotic risk assessment and how to use them for patients' management (clinical implications, optimal cut-offs, frequency of measurement, etc.). Measuring anti-Xa activity is recommended to guide UFH treatment, although this assay is not without drawbacks. Whichever the test used, the attitude adopted must fit local analytical conditions. Additional studies are needed to gain knowledge on the complex, variable and changing disturbances of hemostasis in COVID-19 patients and its interactions with the proinflammatory and infectious status of these patients.

### Acknowledgements

The authors would like to thank Axel Bailly for the conception of the figure.

**Ethical approval and consent to participate**

Not applicable.

**Availability of supporting data**

Not applicable.

**Authors' contributions**

All authors contributed to the literature review. M.H., T.L., H.T.C., G.L. and F.M. drafted the manuscript. All authors reviewed the manuscript for critical content and approved the final version.

**Funding**

This work was supported by the Fonds National de la Recherche Scientifique: 'Anticoagulation fibrinolysis COVID19' (reference: 40002796).

**Consent for publication**

Not applicable.

**Competing interests**

The authors declare no competing interest.

**Author details**

<sup>1</sup>Université catholique de Louvain, CHU UCL Namur, Namur Thrombosis and Hemostasis Center (NTHC), Hematology Laboratory, Yvoir, Belgium. <sup>2</sup>Université catholique de Louvain, CHU UCL Namur, Namur Thrombosis and Hemostasis Center (NTHC), Anesthesiology Department, Yvoir, Belgium. <sup>3</sup>Département de Médecine, Hôpitaux Universitaires de Genève, service d'angiologie et d'hémostase et Faculté de Médecine Geneva Platelet Group (GpG), Université de Genève, Geneva, Suisse, Switzerland. <sup>4</sup>Pharmacy Department, University of Namur, Namur Thrombosis and Hemostasis Center (NTHC), Namur, Belgium. <sup>5</sup>Qualiblood s.a, Namur, Belgium. <sup>6</sup>Haemostasis and Thrombosis Center, Cremona Hospital, Cremona, Italy. <sup>7</sup>Département d'Hématologie Biologique, INSERM, CIC 1414 (Centre d'Investigation Clinique de Rennes), Université de Rennes, CHU de Rennes, Rennes, France. <sup>8</sup>Laboratoire d'Hématologie-Hémostase, CHRU de Tours, Hôpital Trousseau, Tours, France. <sup>9</sup>Australian Centre for Blood Diseases, Monash University, Melbourne, Victoria, Australia. <sup>10</sup>Department of Internal Medicine, Cardiovascular Research Institute (CARIM), Maastricht University Medical Center, Maastricht, the Netherlands. <sup>11</sup>Section of Clinical Biochemistry, University of Verona, Verona, Italy.

Received: 2 June 2020 Accepted: 21 July 2020

Published online: 07 September 2020

**References**

- Lippi G, Favaloro EJ. D-dimer is associated with severity of coronavirus disease 2019: a pooled analysis. *Thromb Haemost.* 2020;120(5):876–8.
- Cui S, Chen S, Li X, Liu S, Wang F. Prevalence of venous thromboembolism in patients with severe novel coronavirus pneumonia. *J Thromb Haemost.* 2020;18(6):1421–4.
- Zeng F, Huang Y, Guo Y, Yin M, Chen X, Xiao L, et al. Association of inflammatory markers with the severity of COVID-19: a meta-analysis. *Int J Infect Dis.* 2020;96:467–74.
- Iba T, Levy JH. Inflammation and thrombosis: roles of neutrophils, platelets and endothelial cells and their interactions in thrombus formation during sepsis. *J Thromb Haemost.* 2018;16(2):231–41.
- Levi M, Poll T. Coagulation in patients with severe sepsis. *Semin Thromb Hemost.* 2015;41(1):9–15.
- Tang N, Bai H, Chen X, Gong J, Li D, Sun Z. Anticoagulant treatment is associated with decreased mortality in severe coronavirus disease 2019 patients with coagulopathy. *J Thromb Haemost.* 2020;18(5):1094–9.
- Klok FA, Kruijff M, van der Meer NJM, Arbous MS, Gommers D, Kant KM, et al. Incidence of thrombotic complications in critically ill ICU patients with COVID-19. *Thromb Res.* 2020;191:145–7.
- Middeldorp S, Coppens M, van Haaps TF, Foppen M, Vlaar AP, Muller MCA, et al. Incidence of venous thromboembolism in hospitalized patients with COVID-19. *J Thromb Haemost.* 2020. Online ahead of print. <https://doi.org/10.1111/jth.14888>.
- Thomas WJ, Johnston A, Symington E, Robinson M, Shears K, Lavinio A, Bessera M. Thrombotic complications of patients admitted to intensive care with COVID-19 at a teaching hospital in the United Kingdom. *Thromb Res.* 2020;191:76–7.
- Helms J, Tacquard C, Severac F, Leonard-Lorant I, Ohana M, Delabranche X, et al. High risk of thrombosis in patients with severe SARS-CoV-2 infection: a multicenter prospective cohort study. *Intensive Care Med.* 2020;46(6):1089–98.
- Poissy J, Goutay J, Caplan M, Parmentier E, Duburcq T, Lassalle F, et al. Pulmonary Embolism in COVID-19 Patients: Awareness of an Increased Prevalence. *Circulation.* 2020. Online ahead of print. <https://doi.org/10.1161/CIRCULATIONAHA.120.047430>.
- Klok FA, Kruijff M, van der Meer NJM, Arbous MS, Gommers D, Kant KM, et al. Confirmation of the high cumulative incidence of thrombotic complications in critically ill ICU patients with COVID-19: an updated analysis. *Thromb Res.* 2020;191:148–50.
- Beun R, Kusadasi N, Sikma M, Westerink J, Huisman A. Thromboembolic events and apparent heparin resistance in patients infected with SARS-CoV-2. *Int J Lab Hematol.* 2020;42(Suppl 1):19–20.
- Artifoni M, Danic G, Gautier G, Gicquel P, Boutolle D, Raffi F, et al. Systematic assessment of venous thromboembolism in COVID-19 patients receiving thromboprophylaxis: incidence and role of D-dimer as predictive factors. *J Thromb Thrombolysis.* 2020;50(1):211–6.
- Susen S, Tacquard CA, Godon A, Mansour A, Garrigue D, Nguyen P, et al. Prevention of thrombotic risk in hospitalized patients with COVID19 and hemostasis monitoring: proposals from the French working group on perioperative Haemostasis (GHIP) the French Society on thrombosis and Haemostasis (GFHT), in collaboration with the French Society for Anaesthesia and Intensive Care (SFAR). *Crit Care.* 2020;24(1):364.
- Casini A, Alberio L, Angelillo-Scherrer A, Fontana P, Gerber B, Graf L, et al. Thromboprophylaxis and laboratory monitoring for in-hospital patients with COVID-19 – a Swiss consensus statement by the working party hemostasis. *Swiss Med Wkly.* 2020;150:w20247.
- Gesellschaft für Thrombose- und Hämostaseforschung (GTH). Empfehlungen zur Thromboseprophylaxe bei SARS-CoV-2 (COVID-19). 2020. Available from: <http://gth-online.org/wp-content/uploads/2020/04/Aktualisierte-GTH-Empfehlungen-COVID-19-1.pdf> [Accessed 2 June 2020].
- Oudkerk M, Buller HR, Kuijpers D, van Es N, Oudkerk SF, McCloud TC, et al. Diagnosis, prevention, and treatment of thromboembolic complications in COVID-19: report of the National Institute for public health of the Netherlands. *Radiology.* 2020;201629.
- Zhai Z, Li C, Chen Y, Gerotziafas G, Zhang Z, Wan J, et al. Prevention and treatment of venous thromboembolism associated with coronavirus disease 2019 infection: a consensus statement before guidelines. *Thromb Haemost.* 2020;120(6):937–48.
- Thachil J, Tang N, Gando S, Falanga A, Cattaneo M, Levi M, et al. ISTH interim guidance on recognition and management of coagulopathy in COVID-19. *J Thromb Haemost.* 2020;18(5):1023–6.
- American Society for Hematology (ASH). COVID-19 and VTE/Anticoagulation: Frequently Asked Questions. 2020. Available from: <https://www.hematology.org/covid-19/covid-19-and-vte-anticoagulation> [Accessed 2 June 2020].
- Marietta M, Ageno W, Artoni A, De Candia E, Gresele P, Marchetti M, et al. COVID-19 and haemostasis: a position paper from Italian society on thrombosis and Haemostasis (SISIT). *Blood Transfus.* 2020;18(3):167–9.
- Hunt B, Retter A, McClintock C. Practical guidance for the prevention of thrombosis and management of coagulopathy and disseminated intravascular coagulation of patients infected with COVID-19. 2020. Available from: <https://thrombosisuk.org/downloads/T&H%20and%20COVID.pdf> [Accessed 2 June 2020].
- Frantzeskaki F, Armaganidis A, Orfanos SE. Immunothrombosis in acute respiratory distress syndrome: Cross talks between inflammation and coagulation. *Respiration.* 2017;93(3):212–25.
- Schultz MJ, Haitsma JJ, Zhang H, Slutsky AS. Pulmonary coagulopathy as a new target in therapeutic studies of acute lung injury or pneumonia - a review. *Crit Care Med.* 2006;34(3):871–7.
- Kowalewski M, Fina D, Slomka A, Raffa GM, Martucci G, Lo Coco V, et al. COVID-19 and ECMO: the interplay between coagulation and inflammation - a narrative review. *Crit Care.* 2020;24(1):205.
- Levi M, Thachil J, Iba T, Levy JH. Coagulation abnormalities and thrombosis in patients with COVID-19. *Lancet Haematol.* 2020;7(6):e438–40.
- Voss R, Matthias FR, Borkowski G, Reitz D. Activation and inhibition of fibrinolysis in septic patients in an internal intensive care unit. *Br J Haematol.* 1990;75(1):99–105.
- Prabhakaran P, Ware LB, White KE, Cross MT, Matthay MA, Olman MA. Elevated levels of plasminogen activator inhibitor-1 in pulmonary edema

- fluid are associated with mortality in acute lung injury. *Am J Physiol Lung Cell Mol Physiol.* 2003;285(1):L20–8.
30. Masi P, Hékimian G, Lejeune M, Chommeloux J, Desnos C, Pineton De Chambrun M, et al. Systemic Inflammatory Response Syndrome is a Major Contributor to COVID-19-Associated Coagulopathy: Insights from a Prospective Single-Center Cohort Study. *Circulation.* 2020. Online ahead of print. <https://doi.org/10.1161/CIRCULATIONAHA.120.048925>.
  31. Fujimoto H, Gabazza EC, Hataji O, Yuda H, D'Alessandro-Gabazza CN, Nakano M, et al. Thrombin-activatable fibrinolysis inhibitor and protein C inhibitor in interstitial lung disease. *Am J Respir Crit Care Med.* 2003;167(12):1687–94.
  32. Whyte CS, Morrow GB, Mitchell JL, Chowdhary P, Mutch NJ. Fibrinolytic abnormalities in acute respiratory distress syndrome (ARDS) and versatility of thrombolytic drugs to treat COVID-19. *J Thromb Haemost.* 2020;18(7):1548–55.
  33. Marchandot B, Sattler L, Jesel L, Matsushita K, Schini-Kerth V, Grunebaum L, et al. COVID-19 related coagulopathy: a distinct entity? *J Clin Med.* 2020;9(6):E1651.
  34. Varga Z, Flammer AJ, Steiger P, Haberecker M, Andermatt R, Zinkernagel AS, et al. Endothelial cell infection and endotheliitis in COVID-19. *Lancet.* 2020; 395(10234):1417–8.
  35. Khider L, Gendron N, Goudot G, Chocron R, Hauw-Berlemont C, Cheng C, et al. Curative anticoagulation prevents endothelial lesion in COVID-19 patients. *J Thromb Haemost.* 2020. Online ahead of print. <https://doi.org/10.1111/jth.14968>.
  36. Huisman A, Beun R, Sikma M, Westerink J, Kusadasi N. Involvement of ADAMTS13 and von Willebrand factor in thromboembolic events in patients infected with SARS-CoV-2. *Int J Lab Hematol.* 2020. Online ahead of print. <https://doi.org/10.1111/ijlh.13244>.
  37. Morici N, Bottiroli M, Fumaçalli R, Marini C, Cattaneo M. Role of von Willebrand Factor and ADAMTS-13 in the Pathogenesis of Thrombi in SARS-CoV-2 Infection: Time to Rethink. *Thromb Haemost.* 2020. Online ahead of print. <https://doi.org/10.1055/s-0040-1713400>.
  38. Zhou F, Yu T, Du R, Fan G, Liu Y, Liu Z, et al. Clinical course and risk factors for mortality of adult inpatients with COVID-19 in Wuhan, China: a retrospective cohort study. *Lancet.* 2020;395(10229):1054–62.
  39. Yin S, Huang M, Li D, Tang N. Difference of coagulation features between severe pneumonia induced by SARS-CoV2 and non-SARS-CoV2. *J Thromb Thrombolysis.* 2020. Online ahead of print. <https://doi.org/10.1007/s11239-020-02105-8>.
  40. Al-Samkari H, Karp Leaf RS, Dzik WH, Carlson JC, Fogarty AE, Waheed A, et al. COVID and Coagulation: Bleeding and Thrombotic Manifestations of SARS-CoV2 Infection. *Blood.* 2020. Online ahead of print. <https://doi.org/10.1182/blood.202006520>.
  41. Chen S, Zhang D, Zheng T, Yu Y, Jiang J. DVT incidence and risk factors in critically ill patients with COVID-19. *J Thromb Thrombolysis.* 2020. Online ahead of print. <https://doi.org/10.1007/s11239-020-02181-w>.
  42. Fox SE, Akmatbekov A, Harbert JL, Li G, Brown JQ, Vander Heide RS. Pulmonary and Cardiac Pathology in African American Patients With COVID-19: An Autopsy Series From New Orleans. *Lancet Respir Med.* 2020. Online ahead of print. [https://doi.org/10.1016/S2213-2600\(20\)30243-5](https://doi.org/10.1016/S2213-2600(20)30243-5).
  43. Thachil J. All those D-dimers in COVID-19. *J Thromb Haemost.* 2020. Online ahead of print. <https://doi.org/10.1111/jth.14939>.
  44. Hunt BJ, Levi M. Re The source of elevated plasma D-dimer levels in COVID-19 infection. *Br J Haematol.* 2020. Online ahead of print. <https://doi.org/10.1111/bjh.16907>.
  45. Bikdeli B, Madhavan MV, Jimenez D, Chuich T, Dreyfus I, Driggin E, et al. COVID-19 and thrombotic or thromboembolic disease: implications for prevention, antithrombotic therapy, and follow-up. *J Am Coll Cardiol.* 2020; 75(23):2950–73.
  46. Stang LJ. D-dimer and fibrinogen/fibrin degradation products. *Methods Mol Biol.* 2013;992:415–27.
  47. Longstaff C, Adcock D, Olson JD, Jennings I, Kitchen S, Mutch N, et al. Harmonisation of D-dimer - a call for action. *Thromb Res.* 2016;137:219–20.
  48. Chen T, Wu D, Chen H, Yan W, Yang D, Chen G, et al. Clinical characteristics of 113 deceased patients with coronavirus disease 2019: retrospective study. *BMJ.* 2020;368:m1091.
  49. Tang N, Li D, Wang X, Sun Z. Abnormal coagulation parameters are associated with poor prognosis in patients with novel coronavirus pneumonia. *J Thromb Haemost.* 2020;18(4):844–7.
  50. Liu Y, Sun W, Guo Y, Chen L, Zhang L, Zhao S, et al. Association between platelet parameters and mortality in coronavirus disease 2019: Retrospect Cohort Stud. *Platelets.* 2020: 1–7.
  51. Lippi G, Plebani M, Henry BM. Thrombocytopenia is associated with severe coronavirus disease 2019 (COVID-19) infections: a meta-analysis. *Clin Chim Acta.* 2020;506:145–8.
  52. Page MJ, Pretorius E. A champion of host defense: a generic large-scale cause for platelet dysfunction and depletion in infection. *Semin Thromb Hemost.* 2020;46(3):302–19.
  53. Taylor FB Jr, Toh CH, Hoots WK, Wada H, Levi M. Scientific subcommittee on disseminated intravascular coagulation of the international society on T, et al. towards definition, clinical and laboratory criteria, and a scoring system for disseminated intravascular coagulation. *Thromb Haemost.* 2001; 86(5):1327–30.
  54. Levi M, Toh CH, Thachil J, Watson HG. Guidelines for the diagnosis and management of disseminated intravascular coagulation. British Committee for Standards in Haematology. *Br J Haematol.* 2009;145(1):24–33.
  55. Chen N, Zhou M, Dong X, Qu J, Gong F, Han Y, et al. Epidemiological and clinical characteristics of 99 cases of 2019 novel coronavirus pneumonia in Wuhan, China: a descriptive study. *Lancet.* 2020; 395(10223):507–13.
  56. Refaai MA, Riley P, Mardovina T, Bell PD. The clinical significance of fibrin monomers. *Thromb Haemost.* 2018;118(11):1856–66.
  57. Wada H, Takahashi H, Uchiyama T, Eguchi Y, Okamoto K, Kawasugi K, et al. The approval of revised diagnostic criteria for DIC from the Japanese society on thrombosis and hemostasis. *Thromb J.* 2017;15:17.
  58. Asakura H, Takahashi H, Uchiyama T, Eguchi Y, Okamoto K, Kawasugi K, et al. Proposal for new diagnostic criteria for DIC from the Japanese society on thrombosis and hemostasis. *Thromb J.* 2016;14:42.
  59. Brionne-François M, Geara C, Riviere M, Gautier P, Davy JB, Le Querrec A, et al. Etude prospective de l'utilisation des monomères de fibrine dans le calcul du score diagnostique de CIVD de l'ISTH (Poster). 33e congrès de la Société Française d'Hématologie (SFH); Paris. 2016.
  60. Westerlund E, Woodhams BJ, Eintrei J, Soderblom L, Antovic JP. The evaluation of two automated soluble fibrin assays for use in the routine hospital laboratory. *Int J Lab Hematol.* 2013;35(6):666–71.
  61. Hamano A, Tanaka S, Takeda Y, Umeda M, Sakata Y. A novel monoclonal antibody to fibrin monomer and soluble fibrin for the detection of soluble fibrin in plasma. *Clin Chim Acta.* 2002;318(1–2):25–32.
  62. Dempfle CE. The use of soluble fibrin in evaluating the acute and chronic hypercoagulable state. *Thromb Haemost.* 1999;82(2):673–83.
  63. Lutze G, Naumann C. Useful Facts about Coagulation: Questions/answers ; [general Principles, Clinical Aspects/treatment, Preanalytical/analytical Aspects]: Roche Diagnostics; 2004.
  64. Madoiwa S, Kitajima I, Ohmori T, Sakata Y, Mimuro J. Distinct reactivity of the commercially available monoclonal antibodies of D-dimer and plasma FDP testing to the molecular variants of fibrin degradation products. *Thromb Res.* 2013;132(4):457–64.
  65. Lippi G, Cervellin G, Franchini M, Favaloro EJ. Biochemical markers for the diagnosis of venous thromboembolism: the past, present and future. *J Thromb Thrombolysis.* 2010;30(4):459–71.
  66. Favaloro EJ, Thachil J. Reporting of D-dimer data in COVID-19: some confusion and potential for misinformation. *Clin Chem Lab Med.* 2020;58(8): 1191–9.
  67. Hatada T, Wada H, Kawasugi K, Okamoto K, Uchiyama T, Kushimoto S, et al. Analysis of the cutoff values in fibrin-related markers for the diagnosis of overt DIC. *Clin Appl Thromb Hemost.* 2012;18(5):495–500.
  68. Olson JD, Cunningham MT, Higgins RA, Eby CS, Brandt JT. D-dimer: simple test, tough problems. *Arch Pathol Lab Med.* 2013;137(8):1030–8.
  69. Suzuki K, Wada H, Imai H, Iba T, Thachil J, Toh CH, et al. A re-evaluation of the D-dimer cut-off value for making a diagnosis according to the ISTH overt-DIC diagnostic criteria: communication from the SSC of the ISTH. *J Thromb Haemost.* 2018;16(7):1442–4.
  70. Favresse J, Lippi G, Roy PM, Chatelain B, Jacqmin H, Ten Cate H, et al. D-dimer: Preanalytical, analytical, postanalytical variables, and clinical applications. *Crit Rev Clin Lab Sci.* 2018;55(8):548–77.
  71. Tre-Hardy M, Blairon L, Wilmet A, Beukinga I, Malonne H, Dogne JM, et al. The role of serology for COVID-19 control: Population, kinetics and test performance do matter. *J Infect.* 2020. Online ahead of print. <https://doi.org/10.1016/j.jinf.2020.05.019>.
  72. Pieters M, Philippou H, Undas A, de Lange Z, Rijken DC, Mutch NJ, et al. An international study on the feasibility of a standardized combined plasma clot turbidity and lysis assay: communication from the SSC of the ISTH. *J Thromb Haemost.* 2018;16(5):1007–12.

73. Glassman A, Abram M, Baxter G, Swett A. Euglobulin lysis times: an update. *Ann Clin Lab Sci*. 1993;23(5):329–32.
74. Cohen W, Alessi MC. Temps de lyse. *EMC Biologie médicale*. 2012;7(3):1–3.
75. Scheer FA, Shea SA. Human circadian system causes a morning peak in prothrombotic plasminogen activator inhibitor-1 (PAI-1) independent of the sleep/wake cycle. *Blood*. 2014;123(4):590–3.
76. Budkowska M, Lebiecka A, Marcinowska Z, Wozniak J, Jastrzebska M, Dolegowska B. The circadian rhythm of selected parameters of the hemostasis system in healthy people. *Thromb Res*. 2019;182:79–88.
77. Eriksson E, Tengborn L, Risberg B. The effect of various anticoagulant/antiplatelet mixtures on determination of plasminogen activator inhibitor, platelet proteins and hemostasis parameters. *Thromb Haemost*. 1989;61(3):511–6.
78. Paramo JA, de Boer A, Colucci M, Jonker JJ, Collen D. Plasminogen activator inhibitor (PA-inhibitor) activity in the blood of patients with deep vein thrombosis. *Thromb Haemost*. 1985;54(3):725.
79. Juhan-Vague I, Alessi MC, Fossat C, Declerck PJ, Kruihof EK. Plasma determination of plasminogen activator inhibitor 1 antigen must be performed in blood collected on antiplatelet/anticoagulant mixture. *Thromb Haemost*. 1987;58(4):1096.
80. Mertens JC, Claesen K, Leenaerts D, Sim Y, Lambear AM, Hendriks D. Inhibition of the procarboxypeptidase U (proCPU, TAFI, proCPB2) system due to hemolysis. *J Thromb Haemost*. 2019;17(6):878–84.
81. Amiral J, Seghatchian J. The contact system at the crossroads of various key patho- physiological functions: update on present understanding, laboratory exploration and future perspectives. *Transfus Apher Sci*. 2019;58(2):216–22.
82. Scarlatescu E, Juffermans NP, Thachil J. The current status of viscoelastic testing in septic coagulopathy. *Thromb Res*. 2019;183:146–52.
83. Cointe S, Harti Souab K, Bouriche T, Vallier L, Bonifay A, Judicone C, et al. A new assay to evaluate microvesicle plasmin generation capacity: validation in disease with fibrinolysis imbalance. *J Extracell Vesicles*. 2018;7(1):1494482.
84. Vallier L, Cointe S, Lacroix R, Bonifay A, Judicone C, Dignat-George F, et al. Microparticles and fibrinolysis. *Semin Thromb Hemost*. 2017;43(2):129–34.
85. Harahsheh Y, Duff OC, Ho KM. Thromboelastography predicts thromboembolism in critically ill Coagulopathic patients. *Crit Care Med*. 2019;47(6):826–32.
86. McCrath DJ, Cerboni E, Frumento RJ, Hirsh AL, Bennett-Guerrero E. Thromboelastography maximum amplitude predicts postoperative thrombotic complications including myocardial infarction. *Anesth Analg*. 2005;100(6):1576–83.
87. Gary JL, Schneider PS, Galpin M, Radwan Z, Munz JW, Achor TS, et al. Can Thromboelastography predict venous thromboembolic events in patients with severe extremity trauma? *J Orthop Trauma*. 2016;30(6):294–8.
88. Cotton BA, Minei KM, Radwan ZA, Matijevic N, Pivalizza E, Podbielski J, et al. Admission rapid thromboelastography predicts development of pulmonary embolism in trauma patients. *J Trauma Acute Care Surg*. 2012;72(6):1470–5.
89. Brill JB, Badiee J, Zander AL, Wallace JD, Lewis PR, Sise MJ, et al. The rate of deep vein thrombosis doubles in trauma patients with hypercoagulable thromboelastography. *J Trauma Acute Care Surg*. 2017;83(3):413–9.
90. Coleman JR, Kay AB, Moore EE, Moore HB, Gonzalez E, Majercik S, et al. It's sooner than you think: blunt solid organ injury patients are already hypercoagulable upon hospital admission - results of a bi-institutional, prospective study. *Am J Surg*. 2019;218(6):1065–73.
91. Dai Y, Lee A, Critchley LA, White PF. Does thromboelastography predict postoperative thromboembolic events? A systematic review of the literature. *Anesth Analg*. 2009;108(3):734–42.
92. Pavoni V, Giansello L, Pazzi M, Stera C, Meconi T, Frigieri FC. Evaluation of coagulation function by rotation thromboelastometry in critically ill patients with severe COVID-19 pneumonia. *J Thromb Thrombolysis*. 2020. Online ahead of print. <https://doi.org/10.1007/s11239-020-02130-7>.
93. Ranucci M, Ballotta A, Di Dedda U, Bayshnikova E, Dei Poli M, Resta M, et al. The procoagulant pattern of patients with COVID-19 acute respiratory distress syndrome. *J Thromb Haemost*. 2020;18(7):1747–51.
94. Spiezia L, Boscolo A, Poletto F, Cerruti L, Tiberio I, Campello E, et al. COVID-19-related severe hypercoagulability in patients admitted to intensive care unit for acute respiratory failure. *Thromb Haemost*. 2020;120(6):998–1000.
95. Wright FL, Vogler TO, Moore EE, Moore HB, Wohlaer MV, Urban S, et al. Fibrinolysis Shutdown Correlates to Thromboembolic Events in Severe COVID-19 Infection. *J Am Coll Surg*. 2020. Online ahead of print. <https://doi.org/10.1016/j.jamcollsurg.2020.05.007>.
96. Raza I, Davenport R, Rourke C, Plattton S, Manson J, Spoor C, et al. The incidence and magnitude of fibrinolytic activation in trauma patients. *J Thromb Haemost*. 2013;11(2):307–14.
97. Ranucci M, Baryshnikova E. Sensitivity of viscoelastic tests to platelet function. *J Clin Med*. 2020;9(1):189.
98. Ranucci M, Di Dedda U, Baryshnikova E. Trials and tribulations of viscoelastic-based determination of Fibrinogen concentration. *Anesth Analg*. 2020;130(3):644–53.
99. Chitlur M, Sorensen B, Rivard GE, Young G, Ingerslev J, Othman M, et al. Standardization of thromboelastography: a report from the TEG-ROTEM working group. *Haemophilia*. 2011;17(3):532–7.
100. Camenzind V, Bombeli T, Seifert B, Jamnicki M, Popovic D, Pasch T, et al. Citrate storage affects Thromboelastograph analysis. *Anesthesiology*. 2000;92(5):1242–9.
101. Zambruni A, Thalheimer U, Leandro G, Perry D, Burroughs AK. Thromboelastography with citrated blood: comparability with native blood, stability of citrate storage and effect of repeated sampling. *Blood Coagul Fibrinolysis*. 2004;15(1):103–7.
102. Wasowicz M, Srinivas C, Meineri M, Banks B, McCluskey SA, Karkouti K. Technical report: analysis of citrated blood with thromboelastography: comparison with fresh blood samples. *Can J Anaesth*. 2008;55(5):284–9.
103. Gilman EA, Koch CD, Santrach PJ, Schears GJ, Karon BS. Fresh and citrated whole-blood specimens can produce different thromboelastography results in patients on extracorporeal membrane oxygenation. *Am J Clin Pathol*. 2013;140(2):165–9.
104. Haas T, Spielmann N, Cushing M. Impact of incorrect filling of citrate blood sampling tubes on thromboelastometry. *Scand J Clin Lab Invest*. 2015;75(8):717–9.
105. Tang N, Jin X, Sun Z, Jian C. Effects of hemolysis and lipemia interference on kaolin-activated thromboelastography, and comparison with conventional coagulation tests. *Scand J Clin Lab Invest*. 2017;77(2):98–103.
106. Spiezia L, Radu C, Marchioro P, Bertini D, Rossetto V, Castelli M, et al. Peculiar whole blood rotation thromboelastometry (Rotem) profile in 40 sideropenic anaemia patients. *Thromb Haemost*. 2008;100(6):1106–10.
107. Ogawa S, Szlam F, Bolliger D, Nishimura T, Chen EP, Tanaka KA. The impact of hematocrit on fibrin clot formation assessed by rotational thromboelastometry. *Anesth Analg*. 2012;115(1):16–21.
108. Solomon C, Rahe-Meyer N, Schoch H, Ranucci M, Gorlinger K. Effect of hematocrit on fibrin-based clot firmness in the FIBTEM test. *Blood Transfus*. 2013;11(3):412–8.
109. Glas M, Mauer D, Kassas H, Volk T, Kreuer S. Sample transport by pneumatic tube system alters results of multiple electrode aggregometry but not rotational thromboelastometry. *Platelets*. 2013;24(6):454–61.
110. Amann G, Zehntner C, Marti F, Colucci G. Effect of acceleration forces during transport through a pneumatic tube system on ROTEM(R) analysis. *Clin Chem Lab Med*. 2012;50(8):1335–42.
111. Le Quellec S, Paris M, Nougier C, Sobas F, Rugeri L, Girard S, et al. Pre-analytical effects of pneumatic tube system transport on routine haematology and coagulation tests, global coagulation assays and platelet function assays. *Thromb Res*. 2017;153:7–13.
112. Nissen PH, Wulff DE, Torring N, Hvas AM. The impact of pneumatic tube transport on whole blood coagulation and platelet function assays. *Platelets*. 2018;29(4):421–4.
113. Kintigh J, Monagle P, Ignjatovic V. A review of commercially available thrombin generation assays. *Res Pract Thromb Haemost*. 2018;2(1):42–8.
114. Douxfils J, Morimont L, Bouvy C, de Saint-Hubert M, Devalet B, Devroye C, et al. Assessment of the analytical performances and sample stability on ST Genesis system using the STG-DrugScreen application. *J Thromb Haemost*. 2019;17(8):1273–87.
115. Carlo A, Arnaud E, Woodhams BJ. The use of polybrene for heparin neutralization in the thrombin generation test. Boston: Poster presented at XXII Isth Congress & 55th Annual SSC Meeting; 2009.
116. Loeffen R, Kleinegriss MC, Loubele ST, Pluijmen PH, Fens D, van Oerle R, et al. Preanalytic variables of thrombin generation: towards a standard procedure and validation of the method. *J Thromb Haemost*. 2012;10(12):2544–54.
117. Alhazzani W, Lim W, Jaeschke RZ, Murad MH, Cade J, Cook DJ. Heparin thromboprophylaxis in medical-surgical critically ill patients: a systematic review and meta-analysis of randomized trials. *Crit Care Med*. 2013;41(9):2088–98.

118. Lim W, Meade M, Lauzier F, Zarychanski R, Mehta S, Lamontagne F, et al. Failure of anticoagulant thromboprophylaxis: risk factors in medical-surgical critically ill patients\*. *Crit Care Med*. 2015;43(2):401–10.
119. Testa S, Prandoni P, Paoletti O, Morandini R, Tala M, Dellanoce C, et al. Direct oral anticoagulant plasma levels' striking increase in severe COVID-19 respiratory syndrome patients treated with antiviral agents: the Cremona experience. *J Thromb Haemost*. 2020;18(6):1320–3.
120. Thachil J. The versatile heparin in COVID-19. *J Thromb Haemost*. 2020;18(5):1020–2.
121. Wakefield TW, Greenfield LJ, Rolfe MW, DeLucia A 3rd, Strieter RM, Abrams GD, et al. Inflammatory and procoagulant mediator interactions in an experimental baboon model of venous thrombosis. *Thromb Haemost*. 1993;69(2):164–72.
122. Tichelaar YI, Kluin-Nelemans HJ, Meijer K. Infections and inflammatory diseases as risk factors for venous thrombosis. A systematic review. *Thromb Haemost*. 2012;107(5):827–37.
123. Vicenzi E, Canducci F, Pinna D, Mancini N, Carletti S, Lazzarin A, et al. Coronaviridae and SARS-associated coronavirus strain HSR1. *Emerg Infect Dis*. 2004;10(3):413–8.
124. Bounameaux H, de Moerloose P. Is laboratory monitoring of low-molecular-weight heparin therapy necessary? *No J Thromb Haemost*. 2004;2(4):551–4.
125. Garcia DA, Baglin TP, Weitz JI, Samama MM. Parenteral anticoagulants: antithrombotic therapy and prevention of thrombosis, 9th ed: American College of Chest Physicians Evidence-Based Clinical Practice Guidelines. *Chest*. 2012;141(2 Suppl):e245–435.
126. Dolovich LR, Ginsberg JS, Douketis JD, Holbrook AM, Cheah G. A meta-analysis comparing low-molecular-weight heparins with unfractionated heparin in the treatment of venous thromboembolism: examining some unanswered questions regarding location of treatment, product type, and dosing frequency. *Arch Intern Med*. 2000;160(2):181–8.
127. Martel N, Lee J, Wells PS. Risk for heparin-induced thrombocytopenia with unfractionated and low-molecular-weight heparin thromboprophylaxis: a meta-analysis. *Blood*. 2005;106(8):2710–5.
128. Basu D, Gallus A, Hirsh J, Cade J. A prospective study of the value of monitoring heparin treatment with the activated partial thromboplastin time. *N Engl J Med*. 1972;287(7):324–7.
129. Gouin-Thibault I, Martin-Toutain I, Peynaud-Debayle E, Marion S, Napol P, Alhenc-Gelas M, et al. Monitoring unfractionated heparin with APTT: a French collaborative study comparing sensitivity to heparin of 15 APTT reagents. *Thromb Res*. 2012;129(5):666–7.
130. Cuker A, Raby A, Moffat KA, Flynn G, Crowther MA. Interlaboratory variation in heparin monitoring: lessons from the quality management program of Ontario coagulation surveys. *Thromb Haemost*. 2010;104(4):837–44.
131. Marlar RA, Clement B, Gausman J. Activated partial Thromboplastin time monitoring of unfractionated heparin therapy: issues and recommendations. *Semin Thromb Hemost*. 2017;43(3):253–60.
132. Bain B, Forster T, Sleight B. Heparin and the activated partial thromboplastin time—a difference between the in-vitro and in-vivo effects and implications for the therapeutic range. *Am J Clin Pathol*. 1980;74(5):668–73.
133. Gouin-Thibault I LT, Sie P, Siguret V. Anticoagulants usuels : maniemnt et gestion des complications. In: *Encyclopédie Médico-Chirurgicale Akos (traité de Médecine)* 2013.
134. Levine SP, Sorenson RR, Harris MA, Knieriem LK. The effect of platelet factor 4 (PF4) on assays of plasma heparin. *Br J Haematol*. 1984;57(4):585–96.
135. Mischke R, Wolling H. Influence of fibrinogen degradation products on thrombin time, activated partial thromboplastin time and prothrombin time of canine plasma. *Haemostasis*. 2000;30(3):123–30.
136. Vandiver JW, Vondracek TG. Antifactor Xa levels versus activated partial thromboplastin time for monitoring unfractionated heparin. *Pharmacotherapy*. 2012;32(6):546–58.
137. Erdem-Eraslan L, Hens JJH, van Rossum AP, Frasa MAM, Keuren JFW. Inter-individual variability in phospholipid-dependent interference of C-reactive protein on activated partial thromboplastin time. *Br J Haematol*. 2018;183(4):681–3.
138. Devreese KM, Verfaillie CJ, De Bisschop F, Delanghe JR. Interference of C-reactive protein with clotting times. *Clin Chem Lab Med* 2015; 53(5): e141–5.
139. Uthman IW, Gharavi AE. Viral infections and antiphospholipid antibodies. *Semin Arthritis Rheum*. 2002;31(4):256–63.
140. Bowles L, Platton S, Yartey N, Dave M, Lee K, Hart DP, et al. Lupus Anticoagulant and Abnormal Coagulation Tests in Patients with Covid-19. *N Engl J Med*. 2020. Online ahead of print. <https://doi.org/10.1056/NEJMc2013656>.
141. Harzallah I, Debliguis A, Drenou B. Lupus anticoagulant is frequent in patients with Covid-19. *J Thromb Haemost*. 2020. Online ahead of print. <https://doi.org/10.1111/jth.14867>.
142. Zhang Y, Xiao M, Zhang S, Xia P, Cao W, Jiang W, et al. Coagulopathy and Antiphospholipid antibodies in patients with Covid-19. *N Engl J Med*. 2020; 382(17):e38.
143. Connell NT, Battinelli EM, Connors JM. Coagulopathy of COVID-19 and antiphospholipid antibodies. *J Thromb Haemost*. 2020. Online ahead of print. <https://doi.org/10.1111/jth.14893>.
144. Sangle NA, Rodgers GM, Smock KJ. Prevalence of heparin in samples submitted for lupus anticoagulant testing. *Lab Hematol*. 2011;17(1):6–11.
145. De Kesel PMM, Devreese KMJ. The effect of unfractionated heparin, enoxaparin, and danaparoid on lupus anticoagulant testing: can activated carbon eliminate false-positive results? *Res Pract Thromb Haemost*. 2020; 4(1):161–8.
146. Favresse J, Lardinois B, Sabor L, Devalet B, Vandepapeliere J, Braibant M, et al. Evaluation of the DOAC-stop(R) procedure to overcome the effect of DOACs on several thrombophilia screening tests. *TH Open*. 2018;2(2):e202–e9.
147. Toh CH, Samis J, Downey C, Walker J, Becker L, Brufatto N, et al. Biphasic transmittance waveform in the APTT coagulation assay is due to the formation of a Ca(++)-dependent complex of C-reactive protein with very-low-density lipoprotein and is a novel marker of impending disseminated intravascular coagulation. *Blood*. 2002;100(7):2522–9.
148. Sevenet PO, Depasse F. Clot waveform analysis: where do we stand in 2017? *Int J Lab Hematol*. 2017;39(6):561–8.
149. Hemker HC, Béguin S. The activity of heparin in the presence and absence of Ca2+ ions; why the anti-Xa activity of LMW heparins is about two times overestimated. *Thromb Haemost*. 1993;70(04):717–8.
150. Kostousov V, Nguyen K, Hundalani SG, Teruya J. The influence of free hemoglobin and bilirubin on heparin monitoring by activated partial thromboplastin time and anti-Xa assay. *Arch Pathol Lab Med*. 2014;138(11):1503–6.
151. White B, Perry D. Acquired antithrombin deficiency in sepsis. *Br J Haematol*. 2001;112(1):26–31.
152. Newall F. Anti-factor Xa (anti-Xa) assay. *Methods Mol Biol*. 2013;992:265–72.
153. Depasse F, Gilbert M, Goret V, Rolland N, Samama MM. Anti-Xa monitoring: inter-assay variability. *Thromb Haemost*. 2000;84(6):1122–3.
154. Uprichard J, Manning RA, Laffan MA. Monitoring heparin anticoagulation in the acute phase response. *Br J Haematol*. 2010;149(4):613–9.
155. Hollestelle MJ, van der Meer FJM, Meijer P. Quality performance for indirect Xa inhibitor monitoring in patients using international external quality data. *Clin Chem Lab Med*. 2020. Online ahead of print. <https://doi.org/10.1515/cclm-2020-0130>.
156. Smahi M, De Pooter N, Hollestelle MJ, Toulon P. Monitoring unfractionated heparin therapy. Lack of standardization of anti-Xa activity reagents. *J Thromb Haemost*. 2020. Online ahead of print. <https://doi.org/10.1111/jth.14969>.
157. Eikelboom JW, Hirsh J. Monitoring unfractionated heparin with the aPTT: time for a fresh look. *Thromb Haemost*. 2006;96(5):547–52.
158. Guermazi S, Znazen R. Resistance to curative treatment by unfractionated heparin. *Rev Med Interne*. 2009;30(4):331–4.
159. Marchetti M, Barelli S, Zermatten MG, Monnin-Respen F, Matthey-Guirao E, Nicolas N, et al. Rapid and accurate Bayesian diagnosis of heparin-induced thrombocytopenia. *Blood*. 2020;135(14):1171–84.
160. White D, MacDonald S, Bull T, Hayman M, de Monteverde-Robb R, Sapsford D, et al. Heparin resistance in COVID-19 patients in the intensive care unit. *J Thromb Thrombolysis*. 2020. Online ahead of print. <https://doi.org/10.1007/s11239-020-02145-0>.
161. Young E, Podor TJ, Venner T, Hirsh J. Induction of the acute-phase reaction increases heparin-binding proteins in plasma. *Arterioscler Thromb Vasc Biol*. 1997;17(8):1568–74.
162. Young E, Venner T, Ribau J, Shaughnessy S, Hirsh J, Podor TJ. The binding of unfractionated heparin and low molecular weight heparin to thrombin-activated human endothelial cells. *Thromb Res*. 1999;96(5):373–81.
163. Finley A, Greenberg C. Review article: heparin sensitivity and resistance: management during cardiopulmonary bypass. *Anesth Analg*. 2013;116(6):1210–22.
164. Levine MN, Hirsh J, Gent M, Turpie AG, Cruickshank M, Weitz J, et al. A randomized trial comparing activated thromboplastin time with heparin

- assay in patients with acute venous thromboembolism requiring large daily doses of heparin. *Arch Intern Med.* 1994;154(1):49–56.
165. Hirsh J, Raschke R. Heparin and low-molecular-weight heparin: the seventh ACCP conference on antithrombotic and thrombolytic therapy. *Chest.* 2004; 126(3 Suppl):188S–203S.
166. Gruel Y, De Maistre E, Pouplard C, Mullier F, Susen S, Rouillet S, et al. Diagnosis and management of heparin-induced thrombocytopenia. *Anaesth Crit Care Pain Med.* 2020;39(2):291–310.
167. Cuker A, Gimotty PA, Crowther MA, Warkentin TE. Predictive value of the 4Ts scoring system for heparin-induced thrombocytopenia: a systematic review and meta-analysis. *Blood.* 2012;120(20):4160–7.
168. Lo GK, Juhl D, Warkentin TE, Sigouin CS, Eichler P, Greinacher A. Evaluation of pretest clinical score (4 T's) for the diagnosis of heparin-induced thrombocytopenia in two clinical settings. *J Thromb Haemost.* 2006;4(4): 759–65.
169. Crowther M, Cook D, Guyatt G, Zytaruk N, McDonald E, Williamson D, et al. Heparin-induced thrombocytopenia in the critically ill: interpreting the 4Ts test in a randomized trial. *J Crit Care.* 2014;29(3):470 e7–15.
170. Linkins LA, Bates SM, Lee AY, Heddle NM, Wang G, Warkentin TE. Combination of 4Ts score and PF4/H-PaGIA for diagnosis and management of heparin-induced thrombocytopenia: prospective cohort study. *Blood.* 2015;126(5):597–603.
171. Maier CL, Barker NA, Sniecinski RM. Falsely low fibrinogen levels in COVID-19 patients on direct thrombin inhibitors. *Anesth Analg.* 2020. Online ahead of print. <https://doi.org/10.1213/ANE.0000000000004949>.
172. Ranucci M. Fibrinogen Levels in COVID-19 Patients and Their Measure Under Direct Thrombin Inhibitors. *Anesth Analg.* 2020. Online ahead of print. <https://doi.org/10.1213/ANE.0000000000004950>.
173. Stang LJ, Mitchell LG. Fibrinogen. *Methods Mol Biol.* 2013;992:181–92.

## Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

**Ready to submit your research? Choose BMC and benefit from:**

- fast, convenient online submission
- thorough peer review by experienced researchers in your field
- rapid publication on acceptance
- support for research data, including large and complex data types
- gold Open Access which fosters wider collaboration and increased citations
- maximum visibility for your research: over 100M website views per year

**At BMC, research is always in progress.**

Learn more [biomedcentral.com/submissions](https://biomedcentral.com/submissions)

