

University of Warwick institutional repository: <http://go.warwick.ac.uk/wrap>

This paper is made available online in accordance with publisher policies. Please scroll down to view the document itself. Please refer to the repository record for this item and our policy information available from the repository home page for further information.

To see the final version of this paper please visit the publisher's website. Access to the published version may require a subscription.

Author(s): Christopher D. Claxton and Richard C. Staunton

Article Title: Measurement of the point-spread function of a noisy imaging system

Year of publication: 2008

Link to published article:

<http://dx.doi.org/10.1364/JOSAA.25.000159>

Publisher statement: This paper was published in Journal Optical Society America A and is made available as an electronic reprint with the permission of OSA. The paper can be found at the following URL on the OSA website:

<http://www.opticsinfobase.org/abstract.cfm?URI=josaa-25-1-159> .

Systematic or multiple reproduction or distribution to multiple locations via electronic or other means is prohibited and is subject to penalties under law..

Measurement of the Point Spread Function of a Noisy Imaging System.

Christopher D. Claxton,¹ and Richard C. Staunton^{2,*}

¹*School of Engineering, University of Warwick, Coventry, CV4 7AL, UK*

²*School of Engineering, University of Warwick, Coventry, CV4 7AL, UK*

*Corresponding author: R.C.Staunton@warwick.ac.uk

Citation: C. D. Claxton and R. C. Staunton, "Measurement of the point-spread function of a noisy imaging system," *J. Opt. Soc. Am. A* **25**, 159-170 (2008)

This paper was published in the Journal of the Optical Society of America A, and is made available as an electronic reprint with the permission of OSA. The paper can be found at the following URL on the OSA website: <http://www.opticsinfobase.org/abstract.cfm?URI=josaa-25-1-159> . Systematic or multiple reproduction or distribution to multiple locations via electronic or other means is prohibited and is subject to penalties under law.

Abstract: The averaged point spread function (PSF) estimation of an image acquisition system is important for many computer vision applications, including edge detection and depth from defocus. The paper compares several mathematical models of the PSF and presents an improved measurement technique that enabled sub-pixel estimation of 2-D functions. New methods for noise suppression and uneven illumination modelling were incorporated. The PSF was computed from an ensemble of edge spread function measurements. The Generalized Gaussian was shown to be an 8 times better fit to the estimated PSF than the Gaussian and a 14 times better fit than the pillbox model. © 2007 Optical Society of America

OCIS codes: 110.2970, 110.4850, 220.4840, 350.4600, 150.5670, 220.2560.

1 INTRODUCTION

The research reported concerns mathematical modelling and practical measurement of the Point Spread Function (PSF) of focused and defocused image acquisition systems, such as digital TV cameras. This measure of image blur can be utilised to optimize image processing functions such as edge detection [1-3] and Depth From Defocus (DFD) depth estimation [4-11]. An image acquisition system typically consists of optical components (such as lenses and apertures) and electronic components (such as the 2-D CCD array, anti-aliasing and communication circuits). Each of the components in the optical and electronic paths can be considered as spatial low-pass filters. Considering the system in the terminology of system theory, the transfer functions of each of its components can be estimated and then all combined to find the overall transfer function. Alternatively, and the approach taken in this work, the transfer function for the entire system can be measured. Typically, input signals are provided in the

form of bar patterns, point sources or step edges. For entire system measurement, the output signal is the captured digital image.

The Fourier transform of the PSF is the Optical Transfer Function (OTF), and both measures have been widely used to characterize systems. The lens can be thought of as a 2-D low-pass filter with a spatial cut-off frequency that is limited by diffraction and aberration effects. The 2-D array samples the image and also includes low-pass filtering as the individual sensor elements have a finite area required for low light operation. Together the elements tile the image plane. As a simple model, charge generated by a photon at a point in an element will distribute evenly across the tile [12]. The sampled value is then proportional to the accumulated charge from all the photons converted in the element during the acquisition phase and since the previous sample was acquired. The CCD is read by a raster scanning process [12]. Here the charge in each of the elements is transferred to vertical columns of shift registers. In turn these shift into a horizontal register and are

shifted to an analogue charge-to-voltage converter and then further electronics that provide, nominally, 1-D signal processes such as low-pass filtering and digitization. The low-pass filtering provided by the lens is necessary as it acts as an anti-aliasing filter for the image discretization. CCD elements require a relatively large area for the camera to work well at low light levels, and this finite area limits the high-frequency response.

PSF measurements can be limited by the Nyquist frequency of the discretization in the acquisition system, however an averaging and accumulation process was researched to overcome this [2,13,14]. This process required a knife or step edge to be imaged, i.e. this is not a general technique for all images. The image was of a blurred step and several edge-spread functions (ESF) were estimated along the length of the edge. The ESFs were then each registered to a reference point and accumulated to form a super-resolution ESF that contained frequency information above the Nyquist limit of the sampling grid. The PSF is more useful than the ESF for DFD measurement and image simulation as it can be directly convolved with an input image to estimate the output image [2,6,9]. The PSF is obtained by differentiating the ESF, however, even low levels of noise in the ESF can result in high levels of noise in the PSF and render it unusable. The source of the noise is in the imaging system's sensors and electronics. In this research it was found that both digital and inexpensive analogue TV cameras had too poor a signal-to-noise ratio (SNR) for the previous PSF measurement techniques to work reliably.

In this paper we compare research into several methods to both reduce the noise in the ESF estimation and to accurately model usable PSFs for the acquisition system. In Section 2 we review PSF measurement techniques and describe how a super-resolution ESF, and eventually a PSF is computed from an ensemble of low-resolution measurements. In Section 3 we examine the theoretical PSF models that result from consideration of both geometric and diffraction optics. In Section 4 we describe improvements to the traditional super-resolution PSF measurement technique that involve:- (i) Compensation for non-uniform illumination within the light box used to produce the test images; (ii) A regularized numerical differentiation process to limit noise in the computed PSF; (iii) Models of the ESF that have been developed and used to compute PSFs that have then been compared with the theoretical models described in Section 2. Fitting the correct ESF model to the measured data is key to obtaining accurate PSFs for the system. Section 5 presents the experimental results from both focused and defocused systems. Specific 1-D results have been used to

demonstrate problems with noise in the ESF estimation, and bias to the PSF when non-uniform illumination remains uncompensated. Then the results of ESF fitting experiments have been reported and discussed. Finally 2-D PSF plots have been produced for the most successful fitting methods. Section 6 provides conclusions.

2 MEASUREMENT TECHNIQUES

Here we have proposed PSF measurement of the whole system, however methods exist to measure individual PSFs for each component. These can then be combined to give the overall PSF. Lasers have been used to measure the PSFs of individual pixels within the CCD array [15,16]. These are a function of wavelength, and so a complete characterization is lengthy and complex. However the PSF for the array is spatially variant and widely used in image restoration. Classically, images of sinusoidal gratings have been used for OTF lens measurements. When a

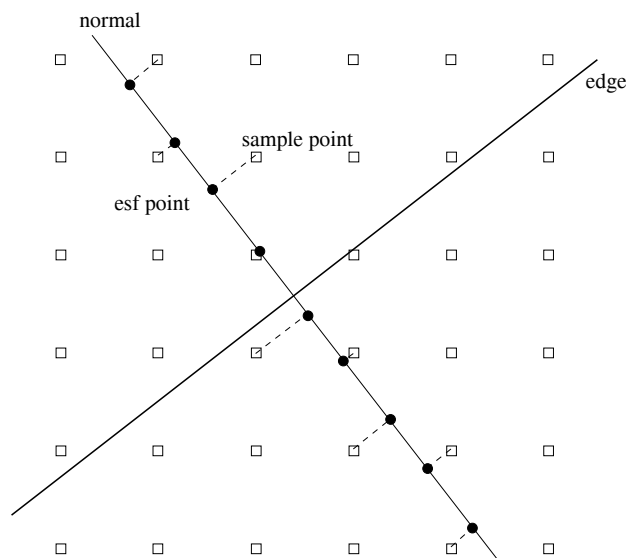


Fig. 1. Migration of samples onto the ESF

focal plane array (FPA) images the grating the discretization means that the FPA must be moved relative to the image to give minimum and maximum MTF curves [17]. Sinusoidal laser interference patterns have been used by Marchywka and Socker [18], and laser speckle techniques can also be employed [19]. The main limitation of lasers is the monochromatic light. Spatial domain techniques have been used to measure the PSF of the lens. A scanned point source can be used to obtain a 2D PSF containing local blur and aberration information up to the Nyquist limit of the FPA. A 2D unit intensity step, known as a knife-edge can be easily produced

experimentally, using a lightbox. Differentiating the response of the lens, the ESF, gives the PSF.

The knife-edge technique can be extended to acquisition system measurement. If the system contains a FPA then undersampling effects cause errors in the PSF estimation due to aliasing. In practice PSF information beyond the Nyquist limit of the array is often required. Reichenbach *et al.* [13] solved the problem by using many ESF profiles to create a super-resolution image of a 1D edge. Tzannes and Mooney [14] fitted a sum of three Fermi-Dirac

functions to the edge to reduce the noise during differentiation to obtain the PSF, and Staunton [2] extended the technique to measure the ESF for many differently angled edges to produce a 2D PSF and MTF. At edge angles other than 0 or 90 degrees, a resampling of the data was performed to obtain the discrete ESFs along normals to the edge. A normal was set and then the closest samples to it projected on to it from a direction parallel to the edge as shown by the dashed lines in Fig. 1. The sampled values were then not equally spaced along the normal, but this

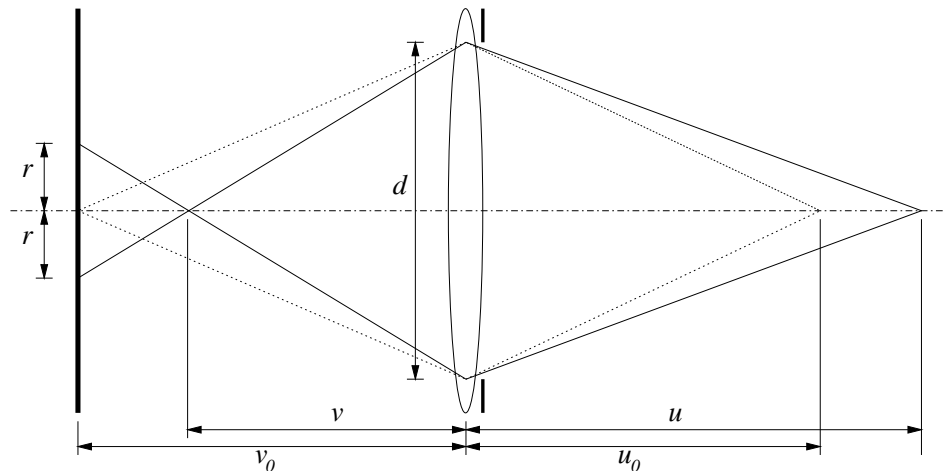


Fig. 2. Simple model of the optical system with the image plane on the left.

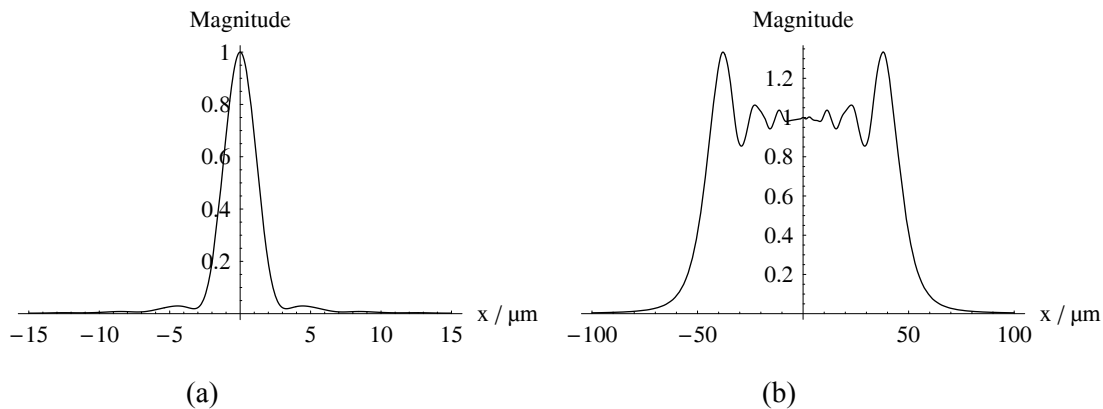


Fig. 3. Normalized-magnitude PSFs for a 16mm, f4 lens. (a) Focused. (b) Defocused.

was irrelevant to the following super-resolution stage. To understand the super-resolution stage used in [2,13,14], consider an edge oriented close to zero degrees, but not actually at zero. The edge cuts each pixel along its length so that part of the pixel is brightly illuminated, and part is dark. The sampled

value for each pixel along the edge is proportional to the averaged illumination throughout the pixel. Each sampled value along the edge is therefore different. In the same way each of the many ESFs located at the pixels along the edge comprises differently sampled values. These low-resolution ESFs are then registered

with one another and assembled to form a single high resolution ESF that is resampled onto typically a 0.1 pixel grid.

The proposed knife-edge technique is simple to perform, but the PSF measurements are averaged along the length of the edge. Such an average is advantageous for shift invariant models used in processes such as edge detector testing [2], depth from defocus [6], or image simulation, but may be disadvantageous for processes that require models of lens aberrations in addition to spherical aberration, such as may be required for image restoration [20]. These may require space variant estimation of the PSF.

3 THEORETICAL PSF MODELS

A Geometrical Optics

Pentland [4] showed that for the simple defocused optical system shown in Fig. 2, and assuming geometrical optics, the PSF is a pillbox shape with a blur circle radius given by

$$r = \frac{v_o u - F(v_o + u)}{2fu}, \quad (1)$$

where v_o is the distance between the lens and the CCD, u is the depth of the object, F is the focal length of the lens and f is the f-number, which is defined as $f = F/d$, where d is the diameter of the aperture. The distance u_o is the distance at which an object would appear in focus on the image plane.

B Diffraction Approach

The PSF $h(\mathbf{x})$ of a focused lens that is subject to diffraction effects and with optical aberrations as a function $\theta(\mathbf{x})$, but neglecting sampling due to the FPA, is given by [21] as

$$h(\mathbf{x}) = \left| \int A(\xi) e^{j\theta(\xi)} e^{-j\frac{2\pi}{\lambda F} \xi \mathbf{x}} d\xi \right|^2 \quad (2)$$

where \mathbf{x} is a position vector, $A(\xi)$ is the aperture function, λ is the wavelength of light and F is the focal length of the lens. Out-of-focus blurring can be modelled as a quadratic aberration of the form

$$\theta(\mathbf{x}) = \frac{\pi}{\lambda} \left(\frac{1}{u} + \frac{1}{v} - \frac{1}{F} \right) |\mathbf{x}|^2 \quad (3)$$

where u is the distance between the object and the lens, and v is the distance between the FPA and the

lens. Substituting (3) into (2), assuming polychromatic light with equal intensities between wavelengths λ_1 and λ_2 , and the aperture function, $A(\xi)$, to be a circle, radius r , then in 1D the PSF becomes

$$h(x) = \int_{\lambda_1}^{\lambda_2} \left| \int_{-r}^{+r} e^{-j\frac{\pi}{\lambda} \left(\frac{2}{F} \xi x - \left(\frac{1}{u} + \frac{1}{v} - \frac{1}{F} \right) |\xi|^2 \right)} d\xi \right|^2 d\lambda \quad (4)$$

Fig. 3(a) shows a PSF expected for a focused system where only diffraction is present. The polychromatic light is modelled as white light with equal intensity components in the range 400 to 700 nm. The PSF looks similar to a Gaussian. Fig. 3(b) shows a PSF for a defocused 16mm lens where the camera is focused at 0.464m and the point source is at 0.8m. The PSF has been flattened out and made to look more like a pillbox function.

4 IMPROVEMENTS TO EDGE SPREAD FUNCTION ESTIMATION

In this research the knife-edge technique was employed and this section firstly considers an improvement to Staunton's [2] algorithm that incorporates the effect of non-uniform illumination of the lightbox. Without noise the ESF could be differentiated to yield the PSF, but differentiating a noisy function amplifies the noise. In this paper models of the ESF are developed from several PSF models and then compared. A regularized numerical differentiation process is proposed.

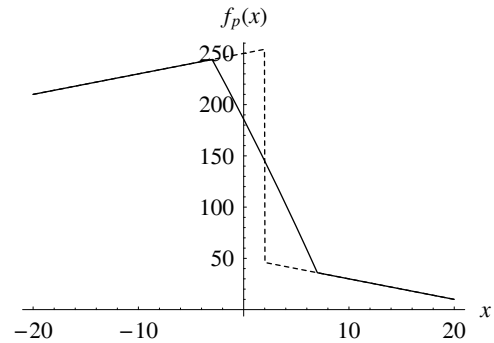


Fig. 4. ESF with a pillbox PSF where $\sigma = 5$ (solid) and the ideal step edge (dashed)

A Compensation for Non-Uniform Illumination

An ideal brightness step changes abruptly from one constant brightness level to the other. Experimentally a light box was employed with a knife-edge to approximate the step, however, in practice the brightness of each region was significantly non-

uniform. This resulted in erroneous PSFs. We propose a new model that retains the abrupt transition, but allows each region to have a linear change in intensity as a function of spatial position. As an example, shown by the dotted trace in Fig. 4, both the bright and darker areas of this particular light box increase in intensity towards the knife-edge. However other linear illumination field conditions can also be modelled by this scheme. The modified step was given by

$$s(x) = (m_1x + c_1)u(x + x_0) + (m_2x + c_2)u(x - x_0) \quad (5)$$

$$g_p(x) = \begin{cases} m_1x + c_1 & x - x_0 < -\sigma \\ \frac{1}{4\sigma} [-(2c_1 + m_1(x + x_0 - \sigma))(x - x_0 - \sigma) + (x - x_0 + \sigma)(2c_2 + m_2(x + x_0 + \sigma))] & -\sigma \leq x - x_0 \leq \sigma \\ m_2x + c_2 & \sigma < x - x_0 \end{cases} \quad (7)$$

where x_0 is the location of the transition [22]. An example of the ESF for a PSF with a blur circle radius $\sigma = 5$ is shown in Fig. 4 where the original step is shown with a dotted line.

Note that there are two sharp transitions in the resulting ESF. A pillbox PSF would result if the lens passed every spatial frequency, however, due to diffraction it is known that this is not possible and a smoother PSF will result.

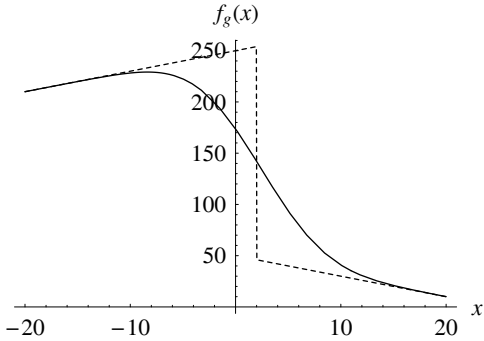


Fig. 5. ESF when the PSF is a Gaussian with $\sigma = 5$ (solid line) and unevenly illuminated ideal step edge (dashed line).

C ESF Modelled as a Sum of Fermi-Dirac Functions

Tzannes and Mooney [14] fitted a sum of three Fermi-Dirac functions to the ESF. Their technique resulted in a smoothed transition across the edge. In general form the sum of N Fermi-Dirac functions for modelling the ESF is

where $u(x)$ is the unit step function, c_1 and c_2 are the brightness of the upper and lower regions and m_1 and m_2 are the gradients of the brightness.

B ESF Assuming a Pillbox PSF

For a defocused lens under geometrical optics the PSF is a pillbox and given by

$$h_p(x) = \frac{1}{2\sigma} [u(x + \sigma) - u(x - \sigma)] \quad (6)$$

where σ is the radius of the pillbox, and hence the blur circle. The ESF assuming a pillbox PSF and using (5) becomes

$$g_{FD}(x) = \sum_{i=1}^N \left(\frac{a_i}{1 + \exp\left\{\frac{x - b_i}{c_i}\right\}} \right) + d \quad (8)$$

where constants a_i have been added to normalize the intensity, b_i to set the centre point, c_i to control the gradient and d to account for the non-zero brightness of the lowest level. In order to recover the PSF the ESF must be differentiated, which is given by [22] as

$$h_{FD}(x) = \frac{\partial g_{FD}(x)}{\partial x} = - \sum_{i=1}^N \left(\frac{a_i \exp\left\{\frac{x - b_i}{c_i}\right\}}{c_i \left(1 + \exp\left\{\frac{x - b_i}{c_i}\right\}\right)^2} \right) \quad (9)$$

However a problem with this model is that it cannot readily take into account the non-uniform illumination in a way that allows the step and the PSF to be separated. The PSFs determined experimentally were consequently non-symmetrical, as shown for example in Figure 10.

D ESF Assuming a Gaussian PSF

The Gaussian PSF is the most frequently assumed model found in the literature on defocused lenses and this is partly due to its simplicity. A 1D Gaussian with a standard deviation σ and centered at $x = \bar{x}$ is then given by

$$h_g(x) = \frac{1}{\sqrt{2\pi}\sigma} \exp\left\{-\frac{1}{2} \frac{(x - \bar{x})^2}{\sigma^2}\right\}. \quad (10)$$

The ESF assuming a Gaussian PSF and a step edge with non-uniform illumination is given by [22]

$$g_g(x) = \frac{1}{2} \left[-(m_1 + m_2) \sigma \sqrt{\frac{2}{\sigma}} \exp\left(-\frac{(x-\bar{x})^2}{2\sigma^2}\right) + (m_1 x + c_1) \left(1 - \operatorname{erf}\left(\frac{(x-\bar{x})}{\sigma\sqrt{2}}\right)\right) + (m_2 x + c_2) \left(1 + \operatorname{erf}\left(\frac{(x-\bar{x})}{\sigma\sqrt{2}}\right)\right) \right] \quad (11)$$

where $\operatorname{erf}(\cdot)$ is the error function, defined as

$$\operatorname{erf}(x) = \frac{2}{\sqrt{\pi}} \int_0^x \exp(-t^2) dt. \quad (12)$$

If the ideal step with non-uniform illumination as shown in Fig. 4 is defocused with a Gaussian ($\sigma = 5$, $\bar{x} = 0$) then the ESF is as shown in Fig. 5.

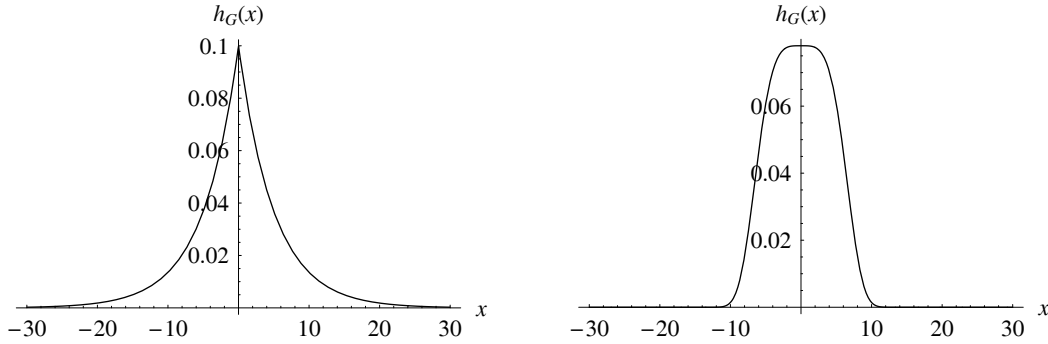


Fig. 6. Generalized Gaussian PSFs where (left) ($p = 1$, $\sigma = 5$) and (right) ($p = 4$, $\sigma = 5$)

E ESF Assuming a Generalized Gaussian PSF

The Generalized Gaussian function [23] is being proposed here as a model of the PSF of a defocused lens. Along with the mean \bar{x} and the standard deviation σ , the power p of the function is required. The function can take the form of a Gaussian when the power $p = 2$ and a pillbox when $p = \infty$, and thus encompasses both of the frequently used models of defocus. The Generalized Gaussian is

$$h_G(x) = \frac{1 - \frac{1}{p}}{2\sigma \Gamma\left(\frac{1}{p}\right)} \exp\left\{-\frac{1}{p} \frac{|x - \bar{x}|^p}{\sigma^p}\right\} \quad (13)$$

where $\Gamma(\cdot)$ is the Gamma function and $|\cdot|$ represents the modulus. The term before the exponential ensures the function has unit area. Two Generalized Gaussian functions are presented in Fig. 6, where $p=1$ (eg for a lens in focus), and $p=4$ (eg defocused).

The ESF, assuming a step edge with non-uniform illumination and a Generalized Gaussian PSF, is given by the convolution of (11) with (13). A closed form, algebraic solution could not be found so the convolution integral was evaluated numerically. The ESF is given by [22] as

$$g_G(x) = \frac{1 - \frac{1}{p}}{2\sigma \Gamma\left(\frac{1}{p}\right)} \int_{x-x_0}^{\infty} \exp\left\{-\frac{1}{p} \frac{|\xi|^p}{\sigma^p}\right\} \{m_1(x - \xi) + c_1\} d\xi + \frac{1 - \frac{1}{p}}{2\sigma \Gamma\left(\frac{1}{p}\right)} \int_{-\infty}^{x-x_0} \exp\left\{-\frac{1}{p} \frac{|\xi|^p}{\sigma^p}\right\} \{m_2(x - \xi) + c_2\} d\xi \quad (14)$$

Using the PSFs shown in Fig. 6 and the ideal step with non-uniform illumination the resulting ESFs are shown in Fig. 7.

F Regularized Numerical Differentiation

In order to recover the PSF from the super-resolution Edge Spread Function (ESF) the response must be differentiated and as the data is discrete, finite-difference approximations must be employed. However the ESF is noisy and both two and five point numerical differentiation were found to give poor results. Chartrand [24] considered the problem of finding the derivative of a function when the underlying function is noisy and has a discontinuity in the derivative. The solution proposed uses total-variation regularization where the derivative of a

function $y(x)$ defined on the closed interval $[0, L]$ is the minimizer of the function

$$Y(u) = \alpha \int_0^L |u'(x)| dx + \frac{1}{2} \int_0^L \left| \int_0^x u(z) dz - y(x) \right|^2 dx \quad (15)$$

where $u'(x)$ is the first derivative of the function $y(x)$ and α is a regularization term that weights the first term, a penalty term, against the second term, the data fidelity term.

The total variation suppresses the noise without removing discontinuities in the derivative. The appeal of this approach is that a pillbox PSF has two finite discontinuities and this method ensures that they can be recovered and that additionally noise suppression is achievable. The main problem is the choice of the regularization parameter α as it affects the derivative produced.

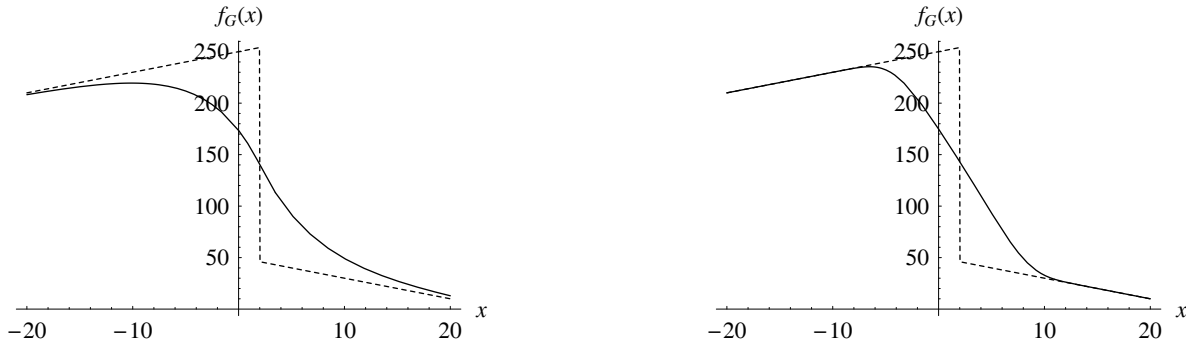


Fig. 7. The ideal steps (dashed lines) and the ESFs (solid lines) assuming Generalized Gaussian PSFs with (left) ($p = 1, \sigma = 5$) and (right) ($p = 4, \sigma = 5$)



Fig. 8. An example of the windowed image

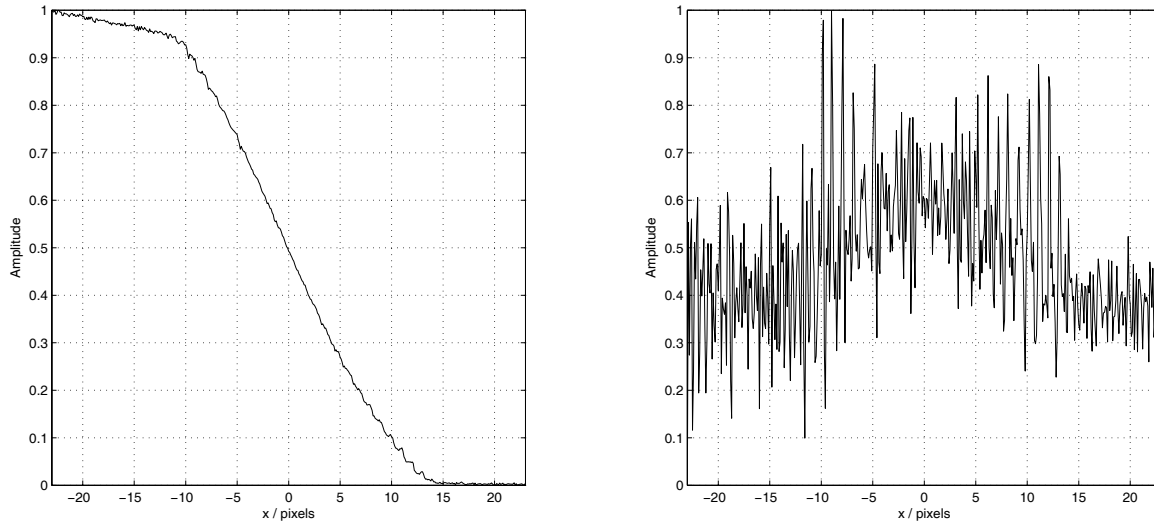


Fig. 9. Five-point numerical differentiation results for f2.8, $z=0.725m$, angle=0 degrees with ESF shown on the left and the PSF on the right

5 EXPERIMENTAL RESULTS, FOCUSED AND DEFOCUSED SYSTEMS

A The PSF Recovery Algorithm

Initially a knife-edge was setup on a lightbox so that it was angled with a slight offset to a row of pixels in the FPA. Its image was windowed (51 x 500 pixels) as shown in Fig. 8. Individual ESFs along the edge therefore contained 51 samples from black to white. This width was sufficient even for defocused lens measurements.

The sampled ESFs were normalized to remove non-uniform illumination along the direction of the edge. Next the central brightness positions of the ESFs were estimated using a cubic fit and the ESFs aligned to these. This alignment resulted in the samples being displaced relative to each other. The super-resolution edge was created by averaging the pixel intensities within sub-pixel bins to give a ten times resolution improvement. Having

obtained the mean ESF for a given distance, f-number and knife-edge angle it was necessary to find the PSF. The methods examined were:- Five-point numerical differentiation; Regularized numerical differentiation using Chartrand's algorithm; Regularized numerical differentiation using Chartrand's algorithm followed by a fit of the resulting PSF to a Generalized Gaussian function; Fitting the ESF to a sum of Fermi-Dirac functions [14]; Fitting the ESF to a defocused step assuming even illumination and a Gaussian PSF; Fitting the ESF to a defocused step where the illumination is assumed to have a linear dependence on position and a Gaussian PSF; Fitting the ESF to a defocused step assuming even illumination and a Generalized Gaussian PSF; Fitting the ESF to a defocused step where the illumination is assumed to have a linear dependence on position and a Generalized Gaussian PSF. In this section results for a 24mm photographic lens fitted to a Basler A631fc color camera are presented when the lightbox was 0.725m from the camera.

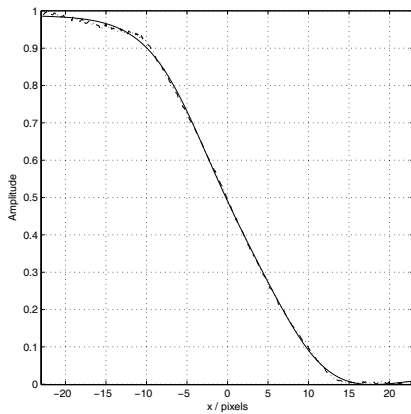


Fig. 10. The actual ESF (dashed line) and Fermi-Dirac fitted ESF (solid line) results for f/2.8,

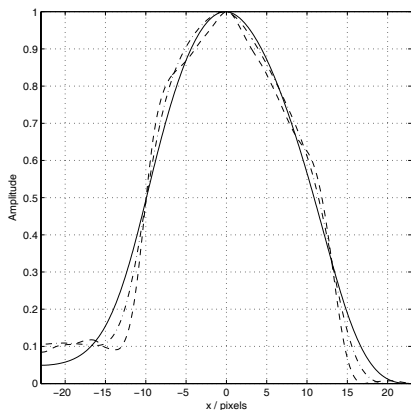
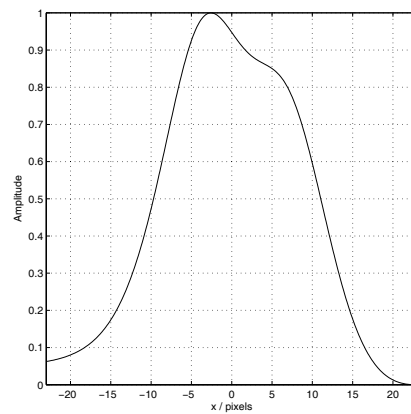


Fig. 11. Regularized numerical differentiation results (right) for $\alpha = 10$ (dashed), $\alpha = 100$ (dash-dot) and $\alpha = 1000$ (solid)

B Specific 1D Results

The results from the five-point numerical differentiation in Fig. 9 show that although the ESF looks fairly smooth, the noise is swamping the underlying PSF, thus making this approach unusable without further processing.

When the measured ESF was fitted to a sum of Fermi-Dirac functions, as shown in Fig. 10, the ESF appeared to have a good fit, however the PSF neither had symmetry or a single peak. These are properties expected of a physical PSF.

C Regularized Numerical Differentiation

In order to determine the optimum regularization parameter α , a series of simulations were performed. Both pillbox and Gaussian PSFs were used to defocus an ideal step. Three levels of noise were added with SNRs of 20 (high noise), 25, and 30 (low noise) dB, and then the ESF was differentiated using Chartrand's algorithm

[24]. The MSE was employed as a distance measure between the actual PSF and the result of the numerical differentiation. The value: $\alpha = 1000$ was optimum for the

SNR = 20 dB case, while $\alpha = 100$ was optimum for 25 and 30 dB. These values were employed in the modelling

Table 1. MSE results for $f/2.8$ as a function of the depth to the light box

Method	Mean Square Error (MSE) / 10^{-3}				
	0.414m	0.491m	0.569m	0.647m	0.725m
Fermi-Dirac	25.2	29.2	34.3	28.3	26.1
Generalized Gaussian without I.C.	10.3	7.37	9.03	5.58	6.45
Generalized Gaussian with I.C.	7.91	5.92	7.95	4.99	6.01
Gaussian without I.C.	64.6	51.1	64.9	68.2	70.2
Gaussian with I.C.	47.6	43.4	55.0	51.1	48.5
Pillbox without I.C.	130.0	90.9	90.7	86.0	85.5
Pillbox with I.C.	102.0	70.3	72.4	70.8	68.3

of real ESFs. An example is shown in Fig. 11 where we have taken the low noise case because it illustrates a problem with the method in that it could not take into account non-uniform illumination and produced non-symmetric PSFs.

The remaining fitting methods produced PSFs with less noise and better symmetry, and so were processed further to give 2D results.

Table 2. Mean MSE results for all three apertures from best to worst

Method	Average MSE / 10^{-3}
Generalized Gaussian with Illumination Correction	5.04
Generalized Gaussian without Illumination Correction	6.93
Sum of three Fermi-Dirac functions	26.7
Gaussian with Illumination Correction	42.5
Gaussian without Illumination Correction	56.7
Pillbox with Illumination Correction	72.0
Pillbox without Illumination Correction	97.6

D Edge Spread Function Fitting Experiments

The ESFs were fitted to the various functions for a range of distances. The results for aperture $f2.8$ are displayed in Table 1. It shows the MSE of the fit as an average for all angles tested, which were -80 to +90 degrees in 10-degree intervals. The plane in-focus was at 0.414m in front of the lens.

The results show that the error assuming a pillbox PSF decreases for increasing defocusing, which was expected from the diffraction-based optics theory in Section 3. The MSEs of the fits using Generalized Gaussian, Gaussian

and pillbox models are lower when the non-uniform illumination was taken into account. The experiment was repeated for f -numbers of $f4$ and $f5.6$. In Table 2, the summarized results for all apertures show that the Generalized Gaussian with illumination correction has resulted in the lowest MSE, thus giving the best fit to the data. The pillbox model produced the worst results with a MSE about 14 times greater than that of the Generalized Gaussian. The MSE of the Gaussian fell almost half way between the Generalized Gaussian and the pillbox.

E Results assuming Gaussian and Generalized Gaussian PSFs

Images of the knife-edge were obtained in 1mm increments over a 30cm depth range for angles of -80 to +90 degrees in 10-degree increments. Each image gave a single mean ESF and that ESF was fitted assuming both Gaussian and Generalized Gaussian PSFs, as derived in Section 4. The PSFs were found to be very nearly circularly symmetric and so the following results are given for the x direction only. Fig. 12 shows the standard deviation of both the Gaussian and Generalized Gaussian as a function of distance for three different f -numbers tested. The plots appear to be smooth and increase monotonically, except for the Gaussian at the maximum distance tested for $f2.8$. Being more robust with increasing depth, the Generalized Gaussian is considered a better model for use with DFD [22].

The Generalized Gaussian PSF has two parameters, the standard deviation σ and the power p . When the power as a function of depth was plotted it was found to be noisier than σ as shown in Fig. 13.

F Two-dimensional PSFs

Complete 2D-PSFs are presented below assuming pillbox, Gaussian and Generalized Gaussian PSF models for two depths, corresponding to the furthest and closest positions tested. The non-uniform illumination improvement was

used. Figs. 14 to 16 show the PSFs for a distance, $z = 0.725\text{m}$, between the camera and the lightbox for an aperture of $f/2.8$.

The Gaussian PSF model shown in Fig. 14 is for a defocused lens, and is clearly circularly symmetric. The

fit has resulted in a smooth contour plot. The Generalized Gaussian PSF model shown in Fig. 15 appears to be a cross between the Gaussian and a pillbox. The fit has

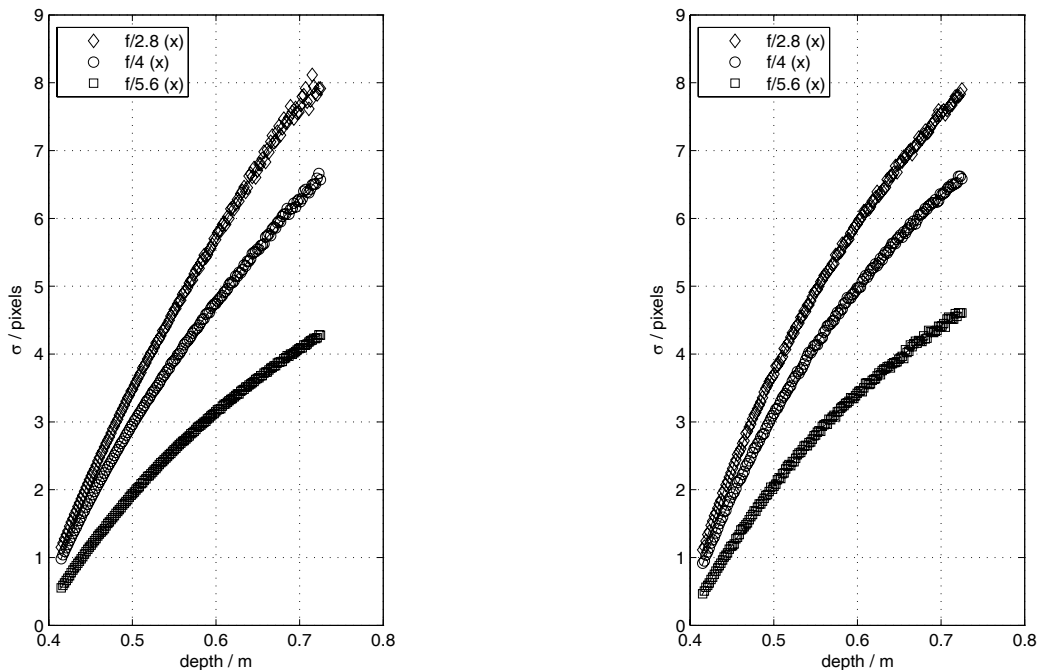


Fig. 12: Standard deviation against depth when fitting (left) a Gaussian PSF and (right) a Generalized Gaussian PSF

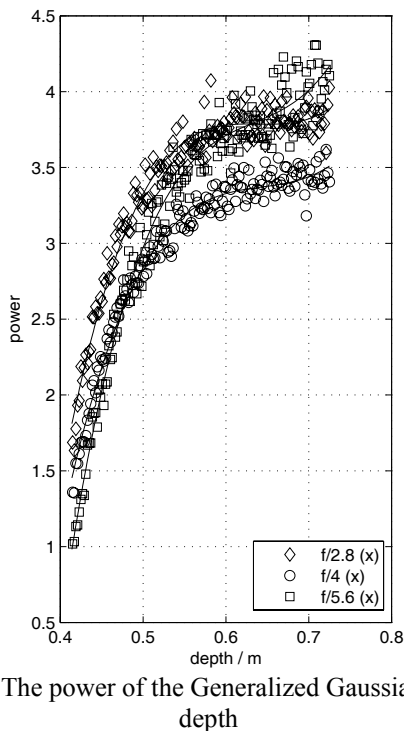


Fig. 13: The power of the Generalized Gaussian against depth

resulted in a contour plot that is less smooth than for the Gaussian, which is probably due to noise in the ESFs and increased complexity of the function due to it having more parameters than all the other models. The pillbox model, Fig. 16, has resulted in a reasonably circular PSF. Figs. 17 to 19 show the PSFs for $z = 0.414\text{m}$, the in focus case. Note the change of x and y axis scales in Figs. 17 to 19. Now all three models have less circularly symmetry and have a maximum spread at approximately 45 degrees to the x axis. The power of the Generalized Gaussian is less than two, and so the function is more pointed than that for the Gaussian.

G Discussion

The goodness-of-fit of the Generalized Gaussian PSF is exemplified by the results of Table 3. Where the non-uniform illumination model was employed, the fit was between 9 and 16 times better than using a Gaussian PSF. The Gaussian PSF has a faster roll-off when the camera is very defocused compared to that using the Generalized Gaussian because the power of the Generalized Gaussian increases with defocus, making it more pillbox in shape, as highlighted in Fig. 20.

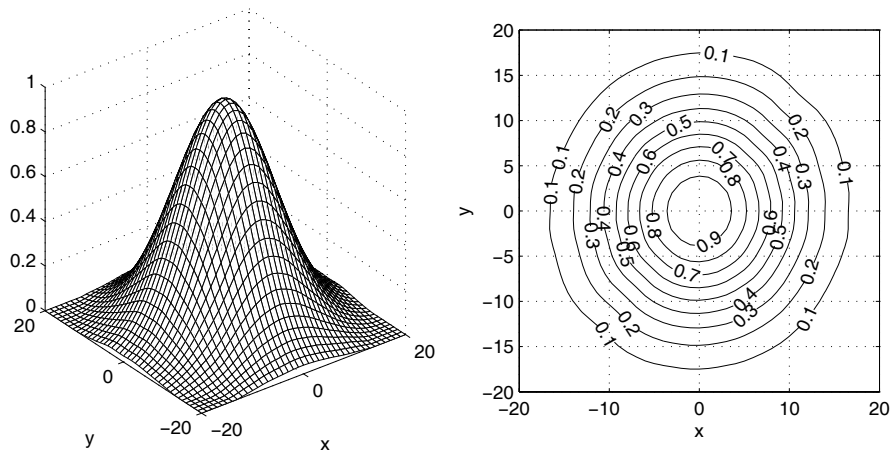


Fig. 14: 2D PSF assuming a Gaussian model for $z = 0.725\text{m}$ and $f2.8$ where x and y are in pixels

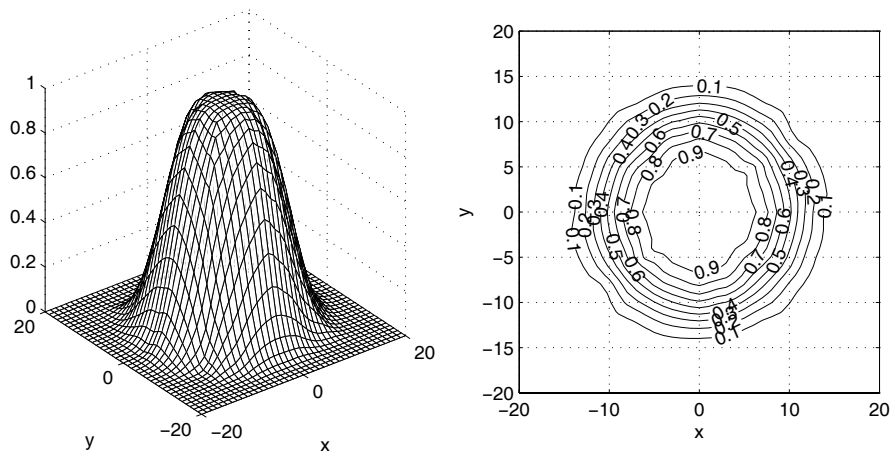


Fig. 15: 2D PSF assuming a Generalized Gaussian model for $z = 0.725\text{m}$ and $f2.8$ where x and y are in pixels

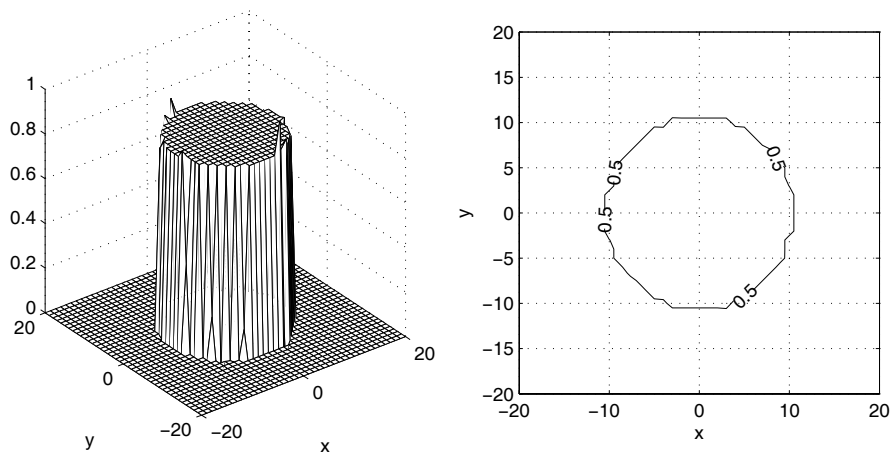


Fig. 16: 2D PSF assuming a Pillbox model for $z = 0.725\text{m}$ and $f2.8$ where x and y are in pixels

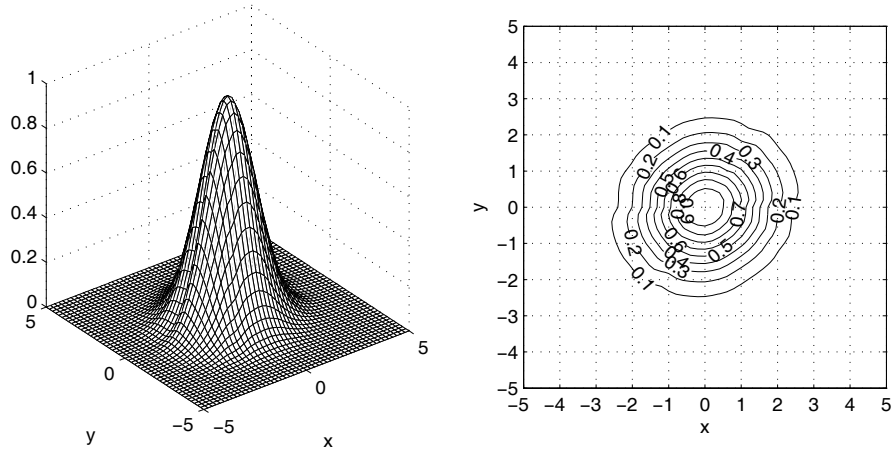


Fig. 17: 2D PSF assuming a Gaussian model for $z = 0.414\text{m}$ and $f2.8$ where x and y are in pixels

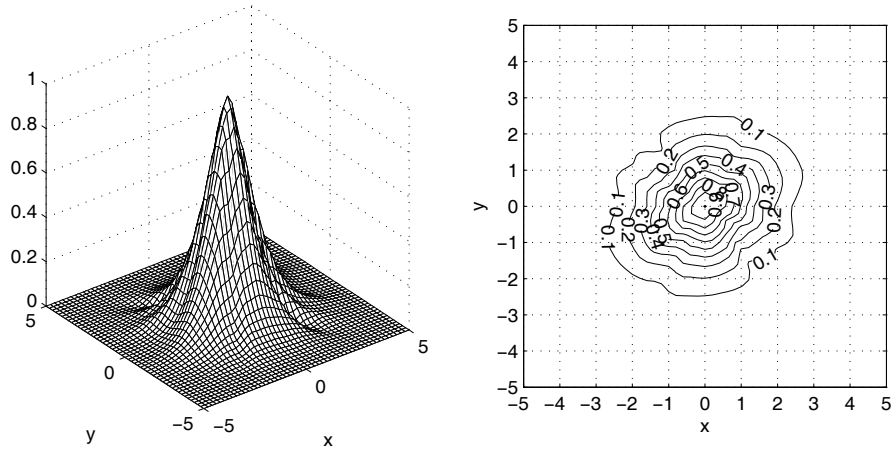


Fig. 18: 2D PSF assuming a Generalized Gaussian model for $z = 0.414\text{m}$ and $f2.8$ where x and y are in pixels

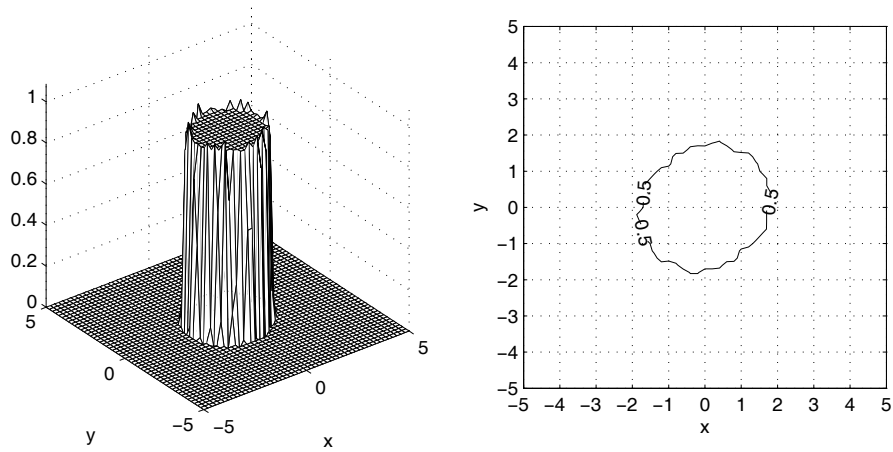


Fig. 19: 2D PSF assuming a Pillbox model for $z = 0.414\text{m}$ and $f2.8$ where x and y are in pixels

Table 3. The average MSE for each method

		Average Mean Square Error (MSE) / 10^{-3}		
		f/2.8	f/4	f/5.6
Method, direction				
Gaussian, direction	x-	31.7	21.9	23.3
Gaussian, direction	y-	46.1	27.3	23.7
Generalized Gaussian, x-direction		2.20	1.67	1.42
Generalized Gaussian, y-direction		4.99	2.44	1.87

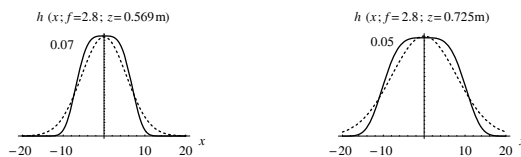


Fig. 20: Comparison between PSFs for the Gaussian (dashed line) and Generalized Gaussian (solid line)

6 CONCLUSION

We have reported improvements to an easily performed super-resolution, but averaged, PSF estimation method that enables it to be used for focused and defocused lenses and with noise generated within the camera. The method involved the initial accumulation of a super-resolution ESF. Previously the calculation of the PSF from the ESF could give both noisy and distorted results.

Distortions were attributed to non-uniform illumination of the knife-edge test object. Where a model of the illumination could be incorporated into the computation of the PSF, symmetrical functions resulted.

Previously noise in the ESF was amplified when it was differentiated to form the PSF. We researched a regularized numerical differentiation that greatly reduced the noise. However changes to the value of the regularization parameter chosen resulted in varying distortions of the PSF. The method was not constrained by any assumption of an underlying model of the ESF or PSF, but in practice, it was found to be outperformed by methods that did.

Several widely used models of the PSF were investigated including the pillbox and Gaussian, together with the use

of Fermi-Dirac fitting functions. A Generalized Gaussian that incorporated both pillbox, Gaussian, and a continuum of models in between, through the choice of a parameter, was also used to model the PSF. The corresponding models for the ESF were derived from these as reported in the paper. The results showed that the MSE of the fit using the Generalized Gaussian performed best across the range of distances and f-numbers tested and that it was 8 times better than the Gaussian model and 14 times better than the pillbox model. Pillbox and Gaussian models are often assumed in DFD work and this research has shown that both are sub-optimum. Finally, 1D PSFs for various knife-edge angles were combined to form 2D PSFs.

REFERENCES

1. R.G. White and R.A. Schowengerdt, "Effect of point spread functions on precision step edge measurement", *J. Opt. Soc. Am. A-Optics* **11**, 2593-2603 (1994).
2. R.C. Staunton, "Edge operator error estimation incorporating measurements of CCD TV camera transfer function", *IEE P-Vis. Image Sign.* **145**, 229-235 (1998).
3. R.C. Staunton, "Detected edge evaluation using measured acquisition system parameters", *Pattern Recogn. Lett.* **26**, 1609-1619 (2005).
4. A. Pentland, "A new sense for depth of field," *IEEE T. Pattern Anal.* **9**, 523-531 (1987).
5. M. Subbarao and N. Gurumoorthy, "Depth recovery from blurred edges," *In Proceedings of IEEE Conference on Computer Vision and Pattern Recognition* (IEEE, 1988), pp. 498-503.
6. J. Ens and P. Lawrence, "An investigation of methods for determining depth from focus," *IEEE T. Pattern Anal.* **15**, 97-108 (1993).
7. M. Subbarao and G. Surya, "Depth from defocus: a spatial domain approach," *Int. J. Comput. Vis.* **13**, 271-294, (1994).
8. A.N. Rajagopalan and S. Chaudhuri, "A variational approach to recovering depth from defocused images," *IEEE T. Pattern Anal.* **19**, 1158-1164 (1997).
9. M. Watanabe and S. Nayar, "Rational Filters for Passive Depth from Defocus," *Int. J. Comput. Vis.* **27**, 203-225 (1998).
10. Li-Ma and R. C. Staunton, "Integration of multiresolution image segmentation and neural networks for object depth recovery", *Pattern Recogn.* **38**, 985-996 (2005).
11. P. Favaro and S. Soatto, "A geometric approach to shape from defocus" *IEEE T. Pattern Anal.* **27**, 406-417 (2005).

12. D.K. Schroder, *Advanced MOS Devices* (Addison Wesley, 1987).
13. S.E. Reichenbach, S.K. Park and R. Narayanswamy, "Characterizing digital image acquisition devices", *Opt. Eng.* **30**, 170-177, (1991).
14. A.P. Tzannes and J.M. Mooney, "Measurement of the modulation transfer function of infrared cameras", *Opt. Eng.* **34**, 1808-1817 (1995).
15. D. Kavaldjiev and Z. Ninkov, "Influence of nonuniform charge-coupled device pixel response on aperture photometry", *Opt. Eng.* **40**, 162-169 (2001).
16. G. Boreman and E.L. Dereniak, "Method for measuring modulation transfer-function of charge-coupled-devices using laser speckle", *Opt. Eng.* **25**, 148-150 (1986).
17. J.C. Feltz and M.A. Karim "Modulation transfer-function of charge-coupled-devices", *Appl. Optics* **29**, 717-722 (1990).
18. M. Marchywka and D.G. Socker, "Modulation transfer-function measurement technique for small-pixel detectors", *Appl. Optics* **31**, 7198-7213 (1992).
19. A. Daniels, G.D. Boreman and A.D. Ducharme, "Random transparency targets for modulation transfer-function measurement in the visible and infrared regions", *Opt. Eng.* **34**, 860-868 (1995).
20. A. Rosenfeld and A. C. Kak, *Digital picture processing*, **1**, (Academic, 1982).
21. T.J. Schultz, "Multiframe image restoration", in *Handbook of Image and Video Processing*, A. Bovik ed. (Academic, 2000), pp. 175-189.
22. C.D. Claxton, "Colour Depth-from-defocus incorporating experimental point spread function measurements", (Ph.D. dissertation, Univ. Warwick, Coventry, U.K. Jan 2007).
23. A. Tarantola, *Inverse problem theory: Methods for data fitting and model parameter estimation*, (Elsevier, 1987).
24. R. Chartrand, "Numerical differentiation of noisy, nonsmooth data," <http://math.lanl.gov/Research/Publications/Docs/chartrand-2005-numerical.pdf>