

OPEN ACCESS

Operation and performance of the ICARUS T600 cryogenic plant at Gran Sasso underground Laboratory

To cite this article: M. Antonello *et al* 2015 *JINST* **10** P12004

View the [article online](#) for updates and enhancements.

Related content

- [The CNGS neutrino beam](#)
G Giacomelli
- [Performance study of the new light collection system for the ICARUS T600 detector](#)
A. Falcone and ICARUS Collaboration
- [Long Term Operation of a CW Doubly Resonant Optical Parametric Oscillator](#)
Takeshi Ikegami, Sergey Slyusarev, Shin-ichi Ohshima *et al.*

Recent citations

- [ICARUS: perspective for sterile neutrino search at FermiLab](#)
Alberto Guglielmi
- [ICARUS status and near future](#)
Filippo Varanini
- [ICARUS status and near future](#)
Filippo Varanini

Operation and performance of the ICARUS T600 cryogenic plant at Gran Sasso underground Laboratory

The ICARUS collaboration

M. Antonello,^a P. Aprili,^a B. Baibussinov,^b F. Boffelli,^c A. Bubak,^d E. Calligarich,^c N. Canci,^a S. Centro,^b A. Cesana,^e K. Cieřlik,^f D.B. Cline,^{g,1} A.G. Cocco,^h A. Dabrowska,^f A. Dermenev,ⁱ J.M. Disdier,^p A. Falcone,^c C. Farnese,^b A. Fava,^b A. Ferrari,^j D. Gibin,^b S. Gninenko,ⁱ A. Guglielmi,^b M. Haranczyk,^f J. Holeczek,^d A. Ivashkin,ⁱ M. Kirsanov,ⁱ J. Kisiel,^d I. Kochanek,^d J. Lagoda,^k S. Mania,^d A. Menegolli,^c G. Meng,^b C. Montanari,^c S. Otwinowski,^g P. Picchi,^l F. Pietropaolo,^b P. Plonski,^m A. Rappoldi,^c G. L. Raselli,^c M. Rossella,^c C. Rubbia,^{a,j} P. R. Sala,ⁿ A. Scaramelli,ⁿ E. Segreto,^a F. Sergiampietri,^o D. Stefan,ⁿ R. Sulej,^k M. Szarska,^f M. Terrani,^e M. Torti,^c F. Varanini,^b S. Ventura,^b C. Vignoli,^{a,2} H.G. Wang,^g X. Yang,^g A. Zalewska,^f A. Zani^c and K. Zaremba^m

^aINFN – Laboratori Nazionali del Gran Sasso, Assergi, Italy

^bUniversità di Padova e INFN, Padova, Italy

^cUniversità di Pavia e INFN, Pavia, Italy

^dInstitute of Physics, University of Silesia, Katowice, Poland

^eINFN e Politecnico di Milano, Milano, Italy

^fH.Niewodniczański Institute of Nuclear Physics, Kraków, Poland

^gDepartment of Physics, UCLA, Los Angeles, U.S.A.

^hUniversità Federico II di Napoli e INFN, Napoli, Italy

ⁱInstitute for Nuclear Research of the Russian Academy of Sciences, Moscow, Russia

^jCERN, Geneva, Switzerland

^kNational Centre for Nuclear Research, Otwock, Świerk, Poland

^lINFN Laboratori Nazionali di Frascati, Frascati, Italy

^mInstitute for Radioelectronics, Warsaw Univ. of Technology, Warsaw, Poland

ⁿINFN Sezione di Milano, Milano, Italy

^oUniversità di Pisa e INFN, Pisa, Italy

^pLuca Scarcia Company, Italy

E-mail: chiara.vignoli@lngs.infn.it

¹Deceased.

²Corresponding author.

ABSTRACT: ICARUS T600 liquid argon time projection chamber is the first large mass electronic detector of a new generation able to combine the imaging capabilities of the old bubble chambers with an excellent calorimetric energy measurement. After the three months demonstration run on surface in Pavia during 2001, the T600 cryogenic plant was significantly revised, in terms of reliability and safety, in view of its long term operation in an underground environment. The T600 detector was activated in Hall B of the INFN Gran Sasso Laboratory during spring 2010, where it was operated without interruption for about three years, taking data exposed to the CERN to Gran Sasso long baseline neutrino beam (CNGS) and cosmic rays. In this paper the T600 cryogenic plant is described in detail together with the commissioning procedures that lead to the successful operation of the detector shortly after the end of the filling with liquid argon. Overall plant performance and stability during the underground run are discussed. Finally, the decommissioning procedures, carried out about six months after the end of the CNGS neutrino beam operation, are reported.

KEYWORDS: Time projection Chambers (TPC); Noble liquid detectors (scintillation, ionization, double-phase); Large detector systems for particle and astroparticle physics; Cryogenic detectors

ARXIV EPRINT: [1504.01556](https://arxiv.org/abs/1504.01556)

Contents

1	Introduction	1
2	Overview of the ICARUS T600 liquid argon TPC	2
2.1	The T600 underground location at LNGS	3
2.2	The T600 cryogenic plant	5
2.3	ICARUS T600 safety and monitoring equipment	10
3	Commissioning	11
3.1	Vacuum phase	12
3.2	Cooling phase	13
3.3	LAr filling phase	14
3.4	Detector commissioning and LAr re-circulation and purification start-up	16
4	Cryogenic plant operation and performance	17
5	Decommissioning	22
6	Conclusions	22

1 Introduction

The ICARUS T600 liquid argon time projection chamber (LAr-TPC) [1] is the largest LAr imaging detector ever built with a total argon mass of ~ 760 t. It was located at the INFN Gran Sasso underground Laboratory (LNGS) with a coverage of 1400 meters of rock. The operational principle of the LAr-TPC [2] is based on the possibility, in highly purified LAr, to transport free electrons from ionizing tracks practically undistorted by a uniform electric field over macroscopic distances. A suitable set of electrodes (wires) placed at the end of the drift path continuously sense and record the signals induced by the drifting electrons. This provides simultaneous projective views of the same event, allowing precise three-dimensional imaging capability [3] and high resolution calorimetric measurements. The design and assembly of the ICARUS T600 LAr-TPC relied on industrial support and represents the application of concepts matured in laboratory tests to the kton scale.

The T600 was smoothly and safely operated from May 2010 to June 2013, taking data on the CERN to Gran Sasso (CNGS) neutrino beam with extremely high argon purity, stability and detector live-time [1]. It also acted as underground observatory recording cosmic ray and atmospheric neutrino events. The T600 detector has a unique role since it is presently the largest physics grade operational LAr-TPC and it will remain so for several years to come. It represents the state of the art and it marks a milestone in the practical realization of any future larger scale LAr detector. The successful run of the ICARUS T600 LAr-TPC, which allowed performing a sensitive search for $\nu_\mu \rightarrow \nu_e$ oscillations [4, 5], demonstrates the enormous potential of this detection technique. The procedures that brought to the activation and operation of the T600 cryogenic plant in an

underground environment open the way to larger detector masses (up to tens of ktons) as foreseen by several new neutrino and rare event physics projects.

The ICARUS T600 detector was moved to CERN in 2014 for overhauling. It is expected to be put again in operation at FNAL exposed to the short baseline Booster neutrino beam [6], for a definitive clarification of the observed neutrino anomalies [4, 7, 8] hinting at the presence of a new “sterile” neutrino state. It will also collect a large sample ($\geq 10^6$) of neutrino interactions from the NuMI beam in the few GeV energy domain relevant to the future long baseline experiment [9], allowing detailed study of any event topology and precise tuning of the reconstruction tools. The foreseen LAr program may also pave the way to ultimate realization of the multi kton detector with the precise measurement of the visible energies of both hadron and electron showers and of the muon momentum [9–13].

In this paper the T600 cryogenic plant is described in details together with all the underground infrastructures, as well as the main phases of the ICARUS T600 commissioning, which allowed collecting cosmic ray and CNGS neutrino events soon after the detector filling with ultra-pure LAr. Steady state operation is reported focusing on the stability and reliability of the plant. The decommissioning phase is also described.

2 Overview of the ICARUS T600 liquid argon TPC

The ICARUS T600 plant [14] consists of a large cryostat split into two identical, adjacent “modules” with internal dimensions 3.6 (width) \times 3.9 (height) \times 19.6 (length) m^3 and filled with ~ 760 tons of ultra-pure liquid argon.

Each module houses two TPC’s separated by a common cathode, with a drift length of 1.5 m. Ionization electrons, abundantly produced by charged particles along their path, are drifted under uniform electric field ($E_D = 500$ V/cm) towards the TPC anode made of three parallel wire planes, 3 mm apart, facing the drift volume. A total of 53248 wires are deployed, with 3 mm pitch, oriented on each plane at a different orientation (0° , $+60^\circ$, -60°) with respect to the horizontal direction. Wires are made of AISI 304 V stainless steel with a diameter of 150 μm and maximum length of 9.42 m for the horizontal wires or 3.77 m for the inclined ones. The wire-frame mechanics is based on the innovative concept of variable geometry design consisting in movable and spring-loaded frames to set the proper tension of the wires after installation for precise detector geometry and planarity, to compensate for possible over-stress during the cooling-down and liquid argon filling phases and to counteract the flexibility of the frame. This design demonstrated its reliability, since none of the wires broke and no damages at the wire chamber structure occurred during the 2001 test run, the transport of the two modules from Pavia INFN Laboratory to LNGS, the installation movements on site, the commissioning phase at LNGS and all the successive operations.

By appropriate voltage biasing, the first two wire planes (“Induction-1” and “Induction-2”) provide signals in non-destructive way; finally the ionization charge is collected and measured on the last plane (“Collection”). The relative time of each ionization signal, combined with the electron drift velocity information ($v_D \sim 1.6$ mm/ μs), provides the position of the track along the drift coordinate. Combining the wire coordinate on each plane at a given drift time, a three-dimensional image of an ionizing event can be reconstructed with the remarkable resolution of about 1 mm³.

A special feed-through flange¹ for the wire signals has been adopted in the T600 detector. It is based on multilayer printed circuit boards where the electrical contacts are ensured by blind holes realized staggering successive printed circuit boards (PCB) layers. The absence of through-going holes ensures perfect tightness for Ultra High Vacuum (UHV) applications. This design was successfully tested in the WARP experiment [15] at LNGS showing high reliability. A set of 96 flanges, holding 576 channels each, was installed on the T600 during detector reassembly at LNGS.

The electronic chain was designed to allow continuous read-out, digitization and independent waveform recording of signals from each wire of the TPC. Organized in 96 crates placed on top of the detector cryostat, it provided wire biasing, hosted the front-end amplifiers and performed 16:1 channel multiplexing and 10-bit ADC digitization at 400 ns sampling time per channel. The electronic noise achieved with the custom designed low noise front-end was ~ 1500 electrons r.m.s. to be compared with ~ 15000 free electrons² produced by minimum ionizing particles in the 3 mm wire pitch ($S/N \sim 10$).

The absolute time of the ionizing events was provided by the prompt VUV (128 nm) scintillation light emitted in liquid argon (~ 5000 photons/mm for minimum ionizing particles²) and measured through arrays of Photo Multiplier Tubes (PMTs) coated with VUV sensitive wavelength-shifter (Tetra-Phenyl-Butadiene, TPB), placed in LAr behind the wire planes. The PMT system, used also for internal trigger purposes [16], allowed for a precise measure of neutrino velocity with CNGS beam [17, 18].

Liquid argon purity is a key issue for the LAr-TPC. LAr electronegative impurities (mainly H_2O , O_2 , CO_2) must be kept at a very low concentration level (less than 0.1 ppb), to allow “unperturbed” drift of ionization electrons from the point of production to the wire planes. To this purpose the ICARUS Collaboration developed a successful technique based on the use of commercial filters, carefully selected among the many availabilities on the market and operated directly on liquid and the adoption of ultra high vacuum materials and techniques. The commissioning procedures included an initial vacuum phase followed at regime by the continuous argon re-circulation and purification of both the liquid bulk and the top gas phase.

Additional details on the T600 detector design and construction can be found in [14]; initial detector operation and performance at LNGS exposed to CNGS neutrino beam and cosmic rays are described in [1].

2.1 The T600 underground location at LNGS

The ICARUS T600 plant and its dedicated technical infrastructures were installed in the Northern-end side of the Hall B at the LNGS underground Laboratory (figure 1, figure 2). The final design of the apparatus was compliant with requirements on safety, anti-seismic prescriptions and reliability for long time operation in a confined underground experimental area at 1400 m depth with the access in the middle of the 10.5 km long highway tunnel. Additional restrictions came from the LNGS Laboratory location inside a National Park and from the proximity of a public aqueduct.

The T600 plant occupied about 10×22 m² surface, while the whole “ICARUS Area” in the Hall B was $15 \times 42,5$ m². This area contained a dedicated service structure surrounding the T600 (about

¹Proprietary technology from INFN.

²Free electrons and photons yields include electron-ion recombination in LAr at $E = 500$ V/cm.



Figure 1. The ICARUS T600 plant in the Northern side of the Hall B at LNGS. Ladders to access the intermediate and the top levels are visible in the front together with the 3 m high wall that separates the T600 area from the rest of Hall B. Cabinets with the readout electronics are installed at the intermediate level. At the top level, the two 30 m³ cryogenic storage tanks and the additional electronic equipment (HV supply, PMT electronics, trigger system, etc.) are also visible. The cryogenic equipment (nitrogen and argon pumps, cryocoolers, etc.) is located on the rear side of the T600, at the Northern end of the Hall B.

11 × 36 m²) organized in three levels (floor level, 5 and 10 m height) in order to maximize the use of available space in the semi-cylindrical hall. It hosted two 30 m³ horizontal cryogenic liquid storages (top level), the nitrogen re-liquefaction apparatus (rear floor) and most of the ICARUS auxiliary systems. The ICARUS Area was served by the two Hall B cranes (40 t and 5 t). The apparatus was placed on 28 dampers to fulfill the seismic requirements. The earthquake occurred in the Gran Sasso region in 2009 did not produce any effect on the T600 empty detector and the already operational N₂ re-liquefaction plant. The ICARUS Area, adequately equipped with a fine grid of sensors to promptly detect any presence of cryogenic liquids, oxygen deficiency, temperature decrease, fire and smoke, was separated from the rest of the Hall B by means of a 3 m high wall. A distributed fast extraction aspiration from ground to protect plant and personnel in case of cryogenic liquid and cold gas spillages was also installed. Most of the infrastructures and auxiliary systems were specifically developed for the T600 operation at LNGS, such as redundant power supply sources and distribution systems, uninterrupted power supply for cryogenic plant and detector control systems, upgraded and redundant cooling water system and the nitrogen re-liquefaction plant.

The ICARUS Control Room, which hosted all the data acquisition systems and the remote controls of the cryogenic plant and of the detector, was located on the Southern side of the Hall B.

2.2 The T600 cryogenic plant

To achieve the physics goals of the ICARUS experiment, the T600 design had to fulfill several strict requirements in terms of detector mechanics precision and stability, electric noise, argon purity and cryogenic plant performance and reliability. The main technical specifications for the T600 cryogenic plant were:

- an extremely high liquid argon purity in terms of residual contamination of electronegative molecules such as water, oxygen and carbon dioxide (better than 0.1 part per billion) to allow ionization electrons drifting over long distances (1.5 m);
- a fast cooling of the whole detector from room to liquid Ar temperature to minimize outgassing and obtain a good initial liquid argon purity while guaranteeing a temperature gradient $\Delta T < 50$ K on the wire-chamber structures and $\Delta T < 120$ K on the cold vessels, as required by the mechanical design of the detector [14];
- a very high temperature uniformity in steady state conditions ($\Delta T < 1$ K in the whole liquid argon volume) to guarantee the uniformity of the electron drift velocity even without forced LAr re-circulation;
- low and stable thermal losses to reduce operation costs and minimize the power request in emergency situations;
- a full redundancy of the relevant elements to guarantee uninterrupted and stable operation over several years in the underground environment;
- no microphonic noise introduced on detector by cryogenic plant dynamic components operation;
- a cryogenic liquid containment that meets the prescribed safety requirements;
- an availability of spare components to guarantee long term operation.

The common denominator of the whole ICARUS T600 construction was the partnership with industry based on the achievements and technical developments from the long ICARUS R&D experience with different prototypes [19–21] and the use of commercial solutions available on the market, when possible. Industry involvement was crucial in order to perform the scaling-up of the technology from the laboratory prototypal scale to the kton one. In particular the T600 cryostat design and construction were carried out in strict collaboration with Air Liquide Italia Service (ALIS) Company.³

Some upgrades and improvements in the cryogenic plant were introduced after the 2001 surface test run [14] for the long term operation at LNGS. In particular new solutions for cooling and insulation systems were adopted [22]. Schematic views of the T600 plant at LNGS are shown in figure 2 and figure 3. In the rest of the paper we describe in details only the relevant innovations of the cryogenic plant while for the unchanged components we refer to [14].

³www.airliquide.it.

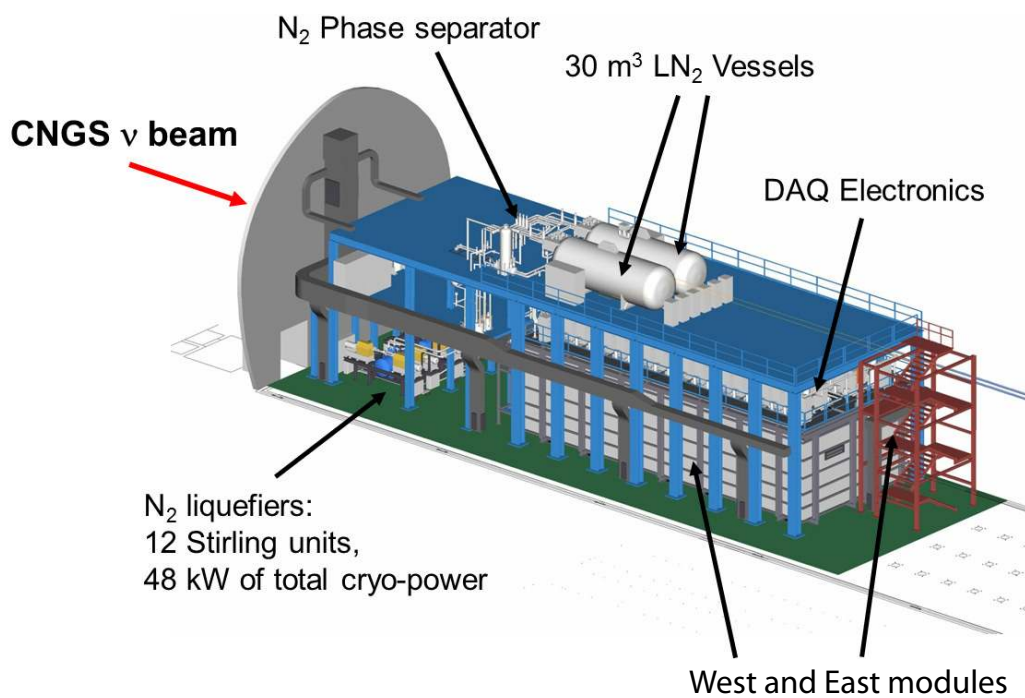


Figure 2. Schematic view of the ICARUS T600 plant in the Hall B at LNGS.

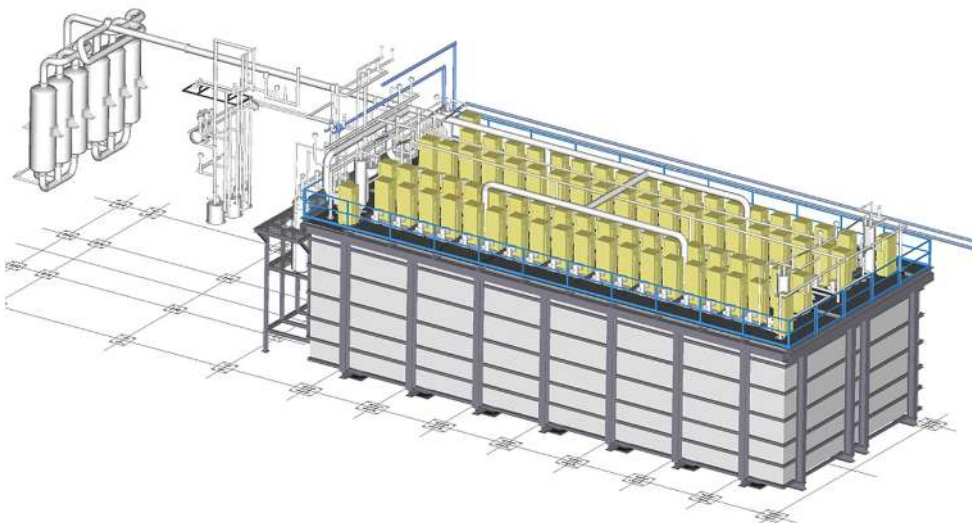


Figure 3. Schematic view of the T600 cryostat with representation of the electronic racks and gaseous argon re-circulation systems on the top, the liquid nitrogen circulation pumps and liquid argon re-circulation systems in the rear side. The safety equipment is visible: the vent line with the electrical heater connected to all the possible exhausts and the collecting pipes from the T600 modules and insulation vessel safety disks to the six passive heater system.

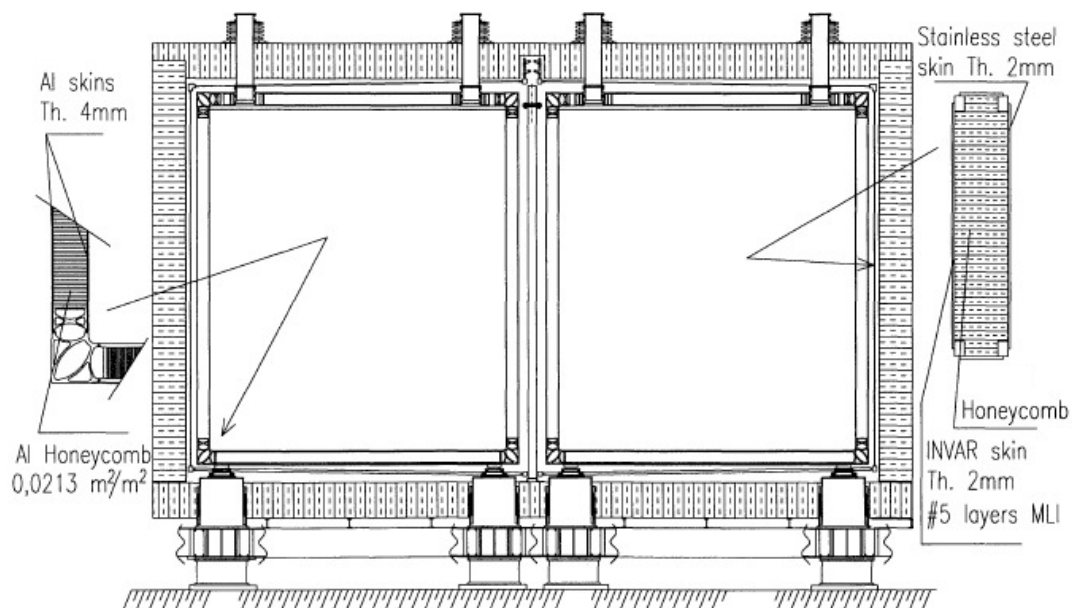


Figure 4. Vertical cross section of the ICARUS T600 cryostat.

The two T600 modules were independent from the point of view of LAr containment and purification plants (figure 4) while the nitrogen cooling system and the thermal insulation were common to both. The two modules were aluminum parallelepiped containers, each one with an internal volume of 275 m^3 and $4.2 \text{ h} \times 3.9 \text{ w} \times 19.91 \text{ m}^3$ external dimensions. They had the maximum size allowed for transportation into the LNGS underground laboratory. In the following they will be referred as West module — the one already commissioned in 2001 in Pavia and widely characterized [23–28] — and East module (the CNGS beam was arriving from the North, figure 2). Each cold vessel was realized with 150 mm thick panels (3.9 m long and 2 m wide) made of aluminum honeycomb glued between two Al skins and to extruded profiles at the borders. The external and internal skins acted as double cryogenic containment. The honeycomb was filled with dry nitrogen gas, except during the vacuum phase when it was also evacuated to avoid stresses on the internal skin. This unconventional vessel solution was adopted mainly for lightness request for transportability and rigidity request to stand stresses during the evacuation phase and the overall LAr and detector weight during steady state [14].

The T600 thermal insulation was a single vessel surrounding the two modules and designed to behave as an additional container for safety in case of cryogenic liquid spillages. Insulation vessel walls, with the exception of the roof, were made of metallic boxes filled with insulating honeycomb panels (0.4 m thick made of Nomex™ or equivalent material) and super-insulation layers placed on the internal (cold) surface [22]. The outer skins of the boxes were made of stainless steel while the inner and side skins were of Pernifer™ to avoid thermal shrinking. Each box was designed to be operated in vacuum to reduce gas conduction and convection (limited by the honeycomb cell geometry but still present due to residual gas) while radiative losses were suppressed by the super-insulation layers, resulting in an overall heat load around 10 W/m^2 . They were intended to be evacuated only once down to 10^{-4} mbar and then kept in static vacuum conditions by means

of getter pumps. However various difficulties introduced by the large wall dimensions together with an excessive outgassing (mainly water) of the internal honeycomb surface were faced during the construction and mounting of the insulation vessel preventing to reach the nominal design parameters.⁴ As a consequence, during cryostat operation, insulation walls were maintained under dynamic evacuation and their internal pressure was continuously monitored for safety reasons.

Holes for pipes and for cables' chimneys were all located on the ceiling of the insulation. The tightness of the insulation vessel was ensured by dedicated bellows installed around the pass-through pipes and chimneys (figure 4).

An external metallic cage mechanically coupled to the anti-seismic shock-absorbers reinforced the insulation box to guarantee stress distribution in case of internal overpressure. It also supported all the weight of the electronic racks present on the T600 top.

A cooling shield for nitrogen circulation was placed between the insulation vessel and the aluminum cold containers to intercept the residual heat losses through the insulation walls thus avoiding the boiling of the LAr bulk [22]. Circulation of 2-phase nitrogen, with its latent heat, was chosen instead of under-cooled single phase liquid with much lower specific heat, as used in Pavia test run. This new solution allowed using lower power circulation pumps and guaranteed fast cooling-down phase with thermal gradients within specification. Moreover it forced de-stratification of LAr during normal operation maintaining uniform and stable temperature in the LAr bulk. For safety reasons the cooling shield was designed to operate also with gravity driven liquid nitrogen circulation ensuring cooling even in case of total lack of electric power.

In order to reach and maintain the required LAr purity, each T600 module was equipped with two gas and one liquid re-circulation systems to purify gas phase and liquid bulk respectively. A schematic view of all the argon and nitrogen cryogenic circuits is shown in figure 5.

The gas re-circulation units collected Ar gas (GAr) from the chimneys hosting the read-out cables and the feed-through flanges. GAr on the T600 top is warm and dirtier with respect to the liquid, as it is in contact with hygroscopic plastic cables and it could be polluted by possible small leaks due to the presence of several joints on each chimney. The gas was re-condensed and then dropped into a liquid nitrogen cooled OxisorbTM filter placed below the re-condenser. Finally the purified LAr flowed back into the LAr bulk just below the liquid/gas interface. The re-condenser was fed with liquid nitrogen at the temperature required for efficient re-condensation of the argon gas, by means of liquid nitrogen (LN₂) forced circulation. The system also acted as detector pressure stabilizer during steady state operation. The argon re-circulation rate was kept at the rate of 25 GAr Nm³/h/unit.

The re-circulation in liquid phase was instead devoted to massively purify LAr and to reach and maintain the highest purity level after the cryostat filling and, in addition, to rapidly restore argon purity in case of accidental pollution during the detector operation. Each LAr re-circulation system extracted LAr at about 2 m below the surface on the 4 m height sides of the T600 modules and injected it on the opposite side, 20 m apart, close to the module floor, through a horizontal pierced pipe that ensured a uniform distribution over the vessel width. Each system was equipped with an immersed cryogenic pump (ACD CRYO AC-32 centrifugal pump) placed inside an independent dewar. From

⁴A mechanical instability problem occurred during evacuation of the Northern insulation wall, causing some domino effects. The North wall was repaired and its internal honeycomb replaced on-site with four closed-cell DivinycellTM 0.1 m thick layers. After this event the North and East insulation walls were left at about ambient pressure.

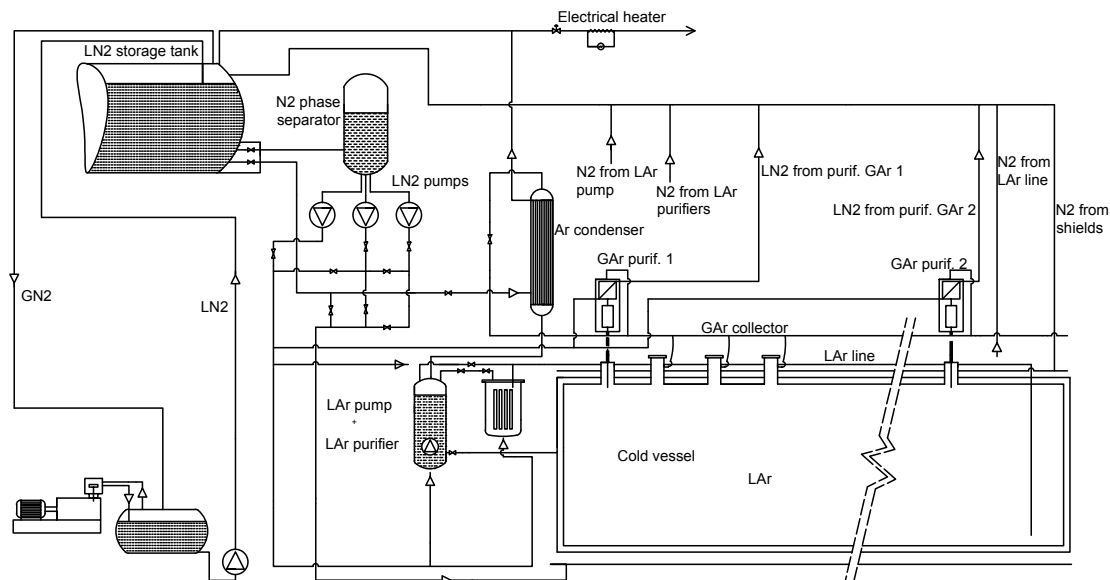


Figure 5. Schematic view of the ICARUS T600 cryostat with argon and nitrogen circuits including the implementation of the system to operate in full gravity-driven mode even for GAr re-condensers.

the pumps reservoir, the circulated LAr passed through a battery of four Oxisorb/Hydrosorb™ filter cartridges (connected in parallel) and was then re-injected into the detector volume. Each set of filters had a nominal O₂ absorption capacity exceeding 200 normal liters, sufficient to purify a module starting from standard commercial liquid argon (O₂ concentration \approx 0.5 ppm). The nominal re-circulation rate was \approx 2 m³/h, resulting from the pump throughput and the filter battery impedance, and corresponding to a full volume re-circulation in about six days. Liquid nitrogen was used to cool the pump vessel, purifier cartridges and all the Ar transfer lines.

Three external motor Barber Nichols BNCP-51B-000 centrifugal pumps were installed to circulate liquid nitrogen inside the T600 cryostat circuits. One was dedicated to the cooling shield and one to the argon re-circulation systems, while the third one was redundant and ready to start in case of need. Each pump was located inside an independent cryostat fed by gravity from the nitrogen phase separator connected to the main liquid nitrogen storage on the top of the supporting structure. One more extra spare pump was present on site.

The two-phase nitrogen returning from cryostat screens and from the gas and liquid Ar re-circulation systems was sent back to the two 30 m³ liquid nitrogen storage tanks⁵ on the top of the ICARUS service structure. For safety reasons related to the long term underground operation the T600 nitrogen circuit was designed to work in closed loop by means of a dedicated nitrogen re-liquefaction plant. Emergency operation in open circuit was also possible and easily handled in case of prolonged stops of the system provided that liquid nitrogen reservoir was maintained through periodic refill by trucks.

The nitrogen re-liquefaction plant was dimensioned to cover the nominal total cold power required for the whole ICARUS T600 plant with at least 50% margin, determined by the design

⁵In steady state conditions both the 30 m³ reservoirs were dedicated to nitrogen storage (filled up to about 80 %), while during commissioning one was used for liquid argon.

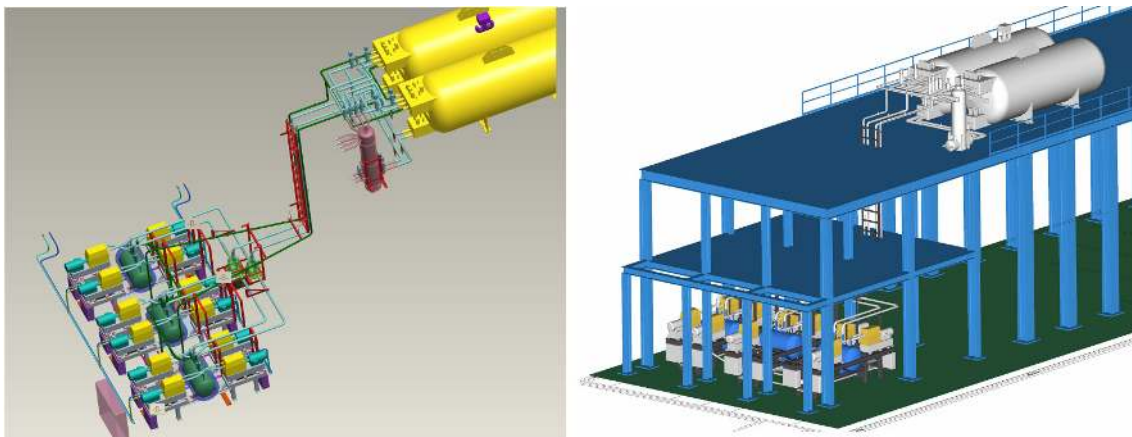


Figure 6. Schematic view of the ICARUS T600 LN₂ re-liquefaction system plant composed by the 12 cryo-generators installed on the Hall B floor and the two storage tanks on the top of the ICARUS supporting structure. A dedicated 2 t crane was installed above the skids to ease cryocooler maintenance.

heat load through the insulation (including the heat input through joints, cryostat feet and cables), the foreseen nitrogen consumption for the cooling screen (circulation pump and distribution lines included) and the Ar gas and liquid Ar re-circulation and purification systems.

The implemented plant consisted of twelve Stirling⁶ Cryogenics BV SPC-4 (4-cylinder) cryocoolers,⁷ based on the “reverse Stirling thermodynamic cycle”, delivering 4.1 kW of cold power each at 84 K with a nominal efficiency of 10.4% (each unit requires 45 kW power for its electrical motor). This system was organized in 3 skids, each one composed by 4 cryocoolers and one 1 m³ reservoir for liquid LN₂ (figure 6).

During steady state the liquid nitrogen tank pressure was kept stable by the re-liquefaction system: the typical working pressure was ≈ 2.1 bar abs (corresponding to about 84.5 K temperature) in order to maintain liquid argon at about 87.5 K with an overpressure of about 100 mbar. Nitrogen gas present in the two 30 m³ LN₂ storage tanks was re-condensed in the 1 m³ reservoirs and then injected in one of the two 30 m³ storage tanks by means of a redundant cryogenic transfer pump (Barber Nichols external motor centrifugal pump BNCP-68-M1 model).

All units operated independently, automatically switching on/off to keep the nitrogen pressure at any given set-point thus delivering the actual cold power needed by the system. This design provided large flexibility in delivering cold power because of its intrinsic factorization; in addition it featured further advantages such as less critical maintenance stops (one unit at a time) without interference with the continuous cooling demand, electrical consumption minimization and easy plant expansion.

2.3 ICARUS T600 safety and monitoring equipment

The ICARUS T600 detector was equipped with several intrinsic safety systems to prevent and confine liquid and gas spillage. Each T600 module was protected by two ADAREGTM magnetic

⁶www.stirlingcryogenics.com.

⁷At the time of the commissioning only ten cryocoolers were installed. The system was later upgraded to guarantee larger redundancy.

disks opening at an internal relative pressure of 0.45 bar and closing when the relative pressure drops below 0.4 bar. Three manual valves were also installed on three different feed-through chimneys to lower the pressure. The volume between the insulation vessel and the two T600 modules was monitored by temperature sensors and protected by two safety magnetic disks and one safety valve. Similarly the aluminum honeycomb walls of the T600 modules were monitored and protected against pressure increase. All the possible exhausts were collected into a vent line, warmed up through a 50 kW electrical heater (or passive heaters in case of lack of electrical power) and conveyed to the ventilation extraction port.

The mechanical deformations of the two T600 modules, i.e. the insulation and inner walls and the wire chamber displacement, and the correlated pressures were continuously monitored during the whole critical phases of evacuation, cooling and filling with liquid Ar, through dedicated sensors. A set of platinum resistors allowed monitoring internal and external temperatures. The liquid Ar level was monitored by carbon resistors acting as level probes.

The whole T600 plant (argon purification and nitrogen circulation systems) and the nitrogen cryocoolers, were equipped with two local and independent control systems based on widely employed industrial devices (Allen-Bradley for the T600 cryogenic plant and Hitachi for the cryocoolers). A high level of redundancy was achieved with automatic intervention to guarantee the maximum operational continuity. All the plant parameters of the T600 cryostat were handled by PLCs (Programmable Logic Controllers). Automatic process control was developed in order to promptly react to any parameter change or emergency.

A common interface based on a SCADA server (iFix Intellution installed on an industrial PC) was also available for higher level remote supervision to record and store all the relevant parameters and events and to issue alarms and automatic notifications. It was interfaced with the general LNGS underground Safety Control Room.

During normal operation, about 7,000 m³/h of air were inlet in the south side of Hall B and extracted (from bottom and top) in the north side, to maintain a slight overpressure with respect to the rest of the Laboratory. In case of “cryogenic emergency” the extraction system in the Hall B was set to create an under-pressure with respect to the rest of the Laboratory. An emergency system, made of a large number of pipes connected to the main Hall B air extraction system, was installed to exhaust gas from the floor of the ICARUS area.

The electrical power supply dedicated to the operation of the T600 detector was highly redundant. The control and safety systems, the detector relevant components and the ICARUS control room were connected to an uninterrupted power supply (UPS). An emergency line, connected to a manually activated diesel generator covering the base electrical power needs of the cryogenic plant (for valves, sensors, controls, electrical heaters for argon and nitrogen exhaust, nitrogen pumps, insulation vacuum pumps), was installed.

3 Commissioning

The commissioning of the ICARUS T600 cryogenic plant started at the beginning of 2010 following the same approach adopted in the successful surface test run in 2001 [14], with an extra attention to maximize safety and minimize interference with other underground activities. The procedure consisted in four main subsequent phases: (i) detector volume evacuation, (ii) cryostat cooling-

down, (iii) liquid Ar filling and GAr purification/re-circulation start-up, (iv) LAr-TPC detector commissioning and LAr purification/re-circulation start-up. The most critical phases were remotely operated and controlled from the ICARUS Control Room located on the opposite side of Hall B.

A dedicated area to unload cryogenic liquids from trucks was set-up in the Hall B in correspondence of the LNGS Truck Tunnel. Vacuum jacketed liquid nitrogen and liquid argon transfer lines were installed from the unloading station to the two storage tanks on the top of the ICARUS service structure at a distance of about 80 m.

3.1 Vacuum phase

The adopted strategy to ensure an acceptable initial LAr purity relied on the cryostat evacuation down to a residual pressure of about $10^{-4} \div 10^{-5}$ mbar to perform an appropriate out-gassing of all the internal walls and detector materials and to remove air pockets in the inner detector structures.

To this purpose, each T600 module was equipped with four identical remotely controlled pumping groups, mounted on four UHV-CF200 flanges on the T600 insulation top. Each pumping system consisted of a 24 m³/h primary Varian⁸ Dry Scroll DS600 pump, a 1000 l/s Varian Turbo-V 1001 Navigator pump and three electro-pneumatic gate valves (two on UHV-CF200 flanges, one on UHV-CF35 flange), which allowed intercepting the pumping group, isolate the inner volumes and start vacuum phase with only primary pumps. A safety valve was mounted in parallel to each dry scroll pump to prevent air return in case of power failure.

Before evacuation, the tightness of both T600 modules was tested to a moderate internal over and under-pressure⁹ in order to find and repair major leaks. The commissioning procedure continued with the vacuum pumping of all the volumes to be filled with argon both in liquid and gaseous phases (the main volumes, the purifiers, the argon transfer lines and the re-circulation units) to remove air and other pollutants. In order to limit vacuum load only to the external skin of the cold vessels panels, the aluminum honeycomb structures of the cold vessels walls were evacuated by means of rotary vane pumps and their pressure was continuously monitored.

The start of the evacuation procedure of the two modules was performed in sequence. In both cases the effective time to reach 0.2 mbar was approximately 30 hours. The turbo-molecular pumps were then switched on to proceed with the high vacuum phase. For both modules a systematic search and repair of leaks resulted in a sudden improvement of vacuum level. Figure 7 shows the pressure evolution in the two modules during the pumping phase as a function of the effective pumping time.

During the whole vacuum phase a continuous monitoring of the mechanical deformations of the inner walls was carried out by position meters. As expected from simulations and from the T600 surface test run [14], the walls deformation increased linearly with decreasing pressure and reached a maximum of about 35 mm at the center of the longest vertical walls in both modules.

The target pressure of 10^{-4} mbar was reached in less than three weeks in both modules. In the following period, before the scheduled cooling phase, the detector was kept under vacuum allowing performing search and repair of residual leaks. The final equilibrium pressure was $4.5 \cdot 10^{-5}$ mbar ($3.8 \cdot 10^{-5}$ mbar) for the West (East) module. These values correspond to a global leak rate of about

⁸www.varianinc.com.

⁹Ambient pressure in the tunnel is about 900 mbar as it is located at the height of about 1000 m above the sea level.

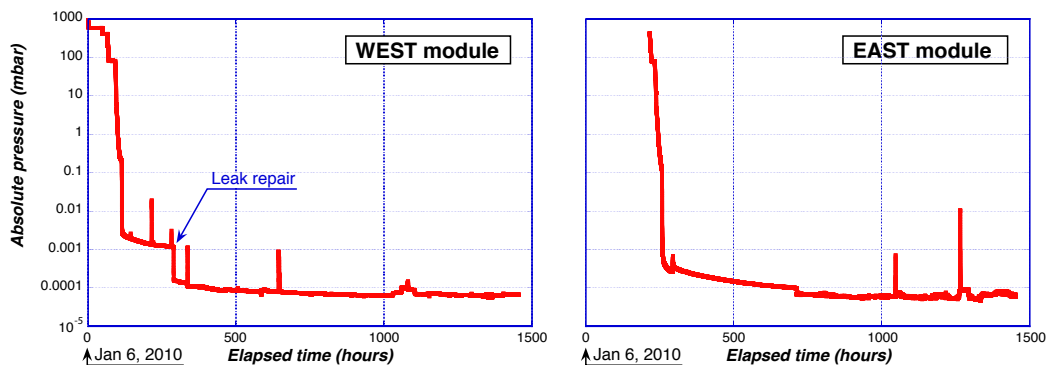


Figure 7. Pressure on the West (left) and East (right) modules as a function of the pumping time. The spikes in the plot are due to interventions devoted to leak repair. The large step at about 300 h in the West module is due to the repair of a major leak. Peaks are due to the stop of one of the four turbo-molecular pumps.

$6 \cdot 10^{-2}$ mbar l/s ($4 \cdot 10^{-2}$ mbar l/s), dominated by internal outgassing as verified by measuring the residual gas composition with mass spectrometers installed on two of the top flanges. The measurements showed a 1 ÷ 10 relative content of air to water, showing that outgassing was the dominant source of the residual gas which was expected to freeze on the internal surfaces during the cooling-down phase; contributions from other components were negligible.

3.2 Cooling phase

The Stirling plant was commissioned in 2009 and it had been successfully operating for one year when the cooling phase started. During this period, a series of tests was performed, simulating different working situations, transient phases and cold power requests demonstrating the correct behavior of the system in agreement with specifications. Failure tests were also successfully performed, including lack of water cooling, power-cuts, liquid nitrogen transfer pump stop.

Immediately after the vacuum pumping stop the two T600 modules were loaded with ultra-pure gas argon (Ar N60: < 0.5 ppm H₂O, < 0.1 ppm O₂, < 0.3 ppm N₂) at 100 mbar overpressure, to minimize back-diffusion of air from residual leaks. Then LN₂ circulation was started inside the cooling screens using nitrogen from the 30 m³ storage tank. Both forced and gravity driven circulations were successfully tested and operated. A constant overpressure of 100 mbar was maintained by means of continuous injection of purified gas argon in both modules. Cryostat internal pressure, cryostat wall displacement, temperature gradients on the wire chambers, insulation external temperatures and displacement were monitored.

During the cooling phase, all cryocoolers were fully active and able to handle most of the nitrogen evaporation, which was partially exceeding the re-condensation power only during the beginning of the cooling of the 100 ton mass of the metallic containers. The residual nitrogen vapor was warmed-up through the 50 kW electrical heater and safely evacuated from Hall B via the ventilation system. The cooling phase lasted about eight days, reaching 90 K at an average rate of about -1 K/h. The cooling was slowed-down when required to keep the internal temperature gradients on the wire chambers within specifications (50 K). Figure 8 shows the temperature trend on the wire chambers structures of the West and East modules; the wiggles on the cooling trends are

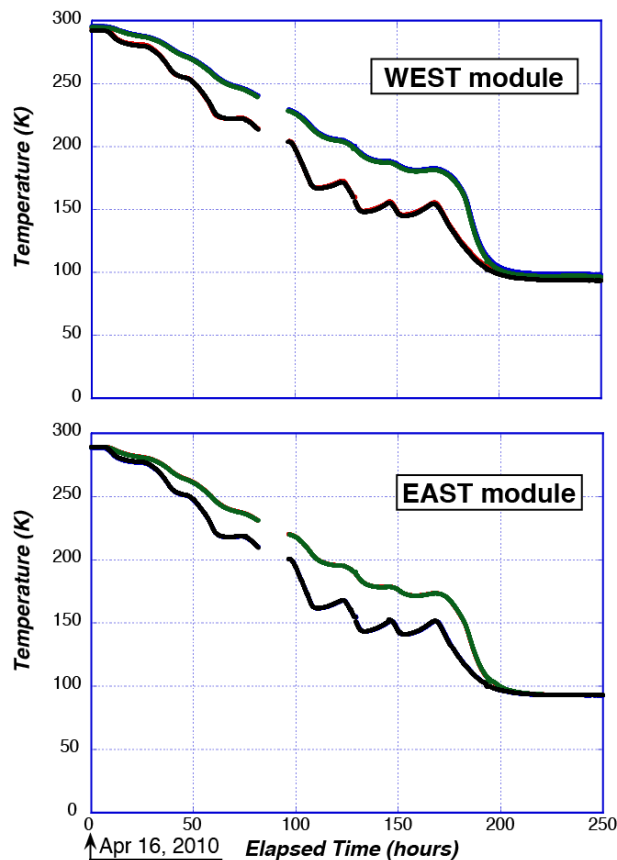


Figure 8. Internal temperature trend on the wire chambers structures in the West (top) and East (bottom) modules as a function of time along the whole cooling phase. The values of two temperature probes (out of 15) for each wires chamber are shown, one on the top and one at the bottom of the structure.

due to the stops of the liquid nitrogen circulation that were necessary to keep the thermal gradients within specifications. The total LN₂ consumption was only 55,800 l, to be compared with an estimate of 200,000 l required in case of full open loop.

After the conclusion of the cooling phase, when the stabilization of the system was achieved and with nitrogen re-condensation system off, the power consumption (insulation losses, plus feet, pipes, cables, chimneys heat input) was determined to be 24 kW in total, well within the capability of the re-liquefaction system with all the cryogenic plant activated. The specific contribution to the heat losses of the thermal insulation was estimated to be ~ 20 kW, as derived from the temperature differences with respect to ambient air measured on the outer skin of the insulation panels (see figure 9), a value exceeding the design one.¹⁰

3.3 LAr filling phase

To ensure filling without interruptions, one of the 30 m³ tanks was used as LAr storage buffer, continuously feeding the purification cartridges of re-circulation systems of the two modules.

¹⁰Only the insulation bottom panel resulted within specifications with an internal working pressure of $\sim 10^{-4}$ mbar.

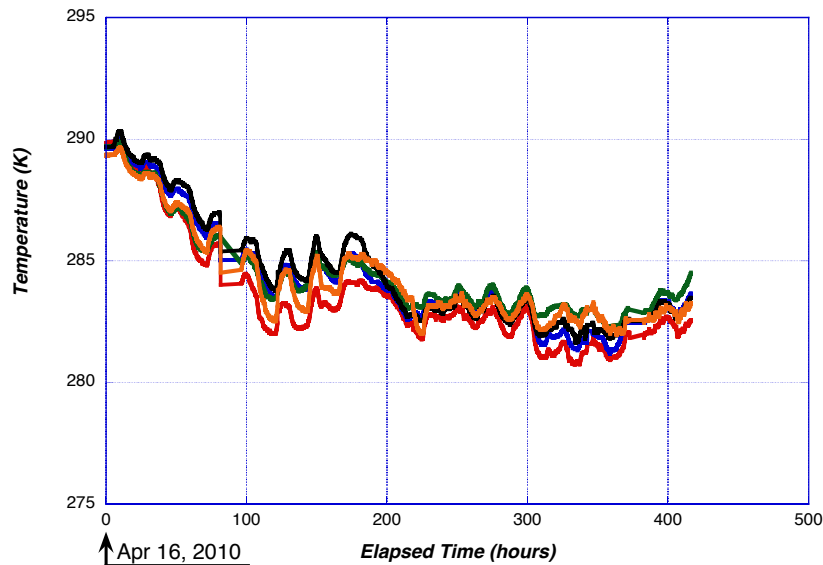


Figure 9. Temperature trend of Pt1000 probes located on the outer skin of the insulation vessel: south (red), West (blue and green), East (black and orange). Temperature values stabilization were $282\text{ K} \div 284\text{ K}$ while the difference with respect to ambient value was about -7 K .

A dedicated cryocooler (Stirling Cryogenics BV 1-cylinder SPC-1 500 with a nominal cold power of 1 kW at 77 K) was installed on the liquid argon tank only for the commissioning phase with the aim of stabilizing the argon pressure by means of re-condensation.

Each liquid argon delivery (13 m^3), certified to be within purity specifications ($\text{H}_2\text{O} \leq 1\text{ ppm}$, $\text{O}_2 \leq 0.5\text{ ppm}$, $\text{N}_2 \leq 3\text{ ppm}$), was downloaded into the LAr 30 m^3 vessel.

An additional buffer tank (1.3 m^3) was installed at the unloading station to keep the transfer line filled with liquid Argon, avoiding pollution between LAr deliveries.

A filter composed by a standard OxisorbTM/HydrosorbTM cartridge with high purification capability was put at the outlet of the 30 m^3 vessel, to avoid early saturation of the T600 main purification cartridges. The liquid argon quality was monitored on-line at the 30 m^3 storage inlet and downstream this filter by means of a gas chromatograph. On average, a typical contamination of 30 ppb in oxygen and 100 ppb in nitrogen¹¹ after the additional filter was measured.

To minimize argon pollution due to outgassing from surfaces, T600 filling was performed in the shortest possible time, while avoiding to reach the opening pressure of the magnetic safety disks. Before starting the filling phase, all transfer lines and storage vessels were accurately purged with high purity gas argon, until the residual oxygen and water content was lower than 1 ppm.

In order to intercept residual outgassing impurities, the four GAR re-circulation/purification units were put into operation at the beginning of the filling, at a rate slightly exceeding the nominal value of $25\text{ Nm}^3/\text{hour}$ per unit. To guarantee an internal overpressure, the cryostat filling was started with ultra-pure Ar gas followed by injection of the first 10,000 liters of liquid argon in West module. A similar procedure was followed for the East cryostat.

¹¹Initial nitrogen content in LAr was not removed by means of the ICARUS purification system. Even if nitrogen is not electro-negative, it has to be maintained as low as possible as it affects the scintillation light production, that is fundamental for internal trigger and timing purposes as explained in the following.

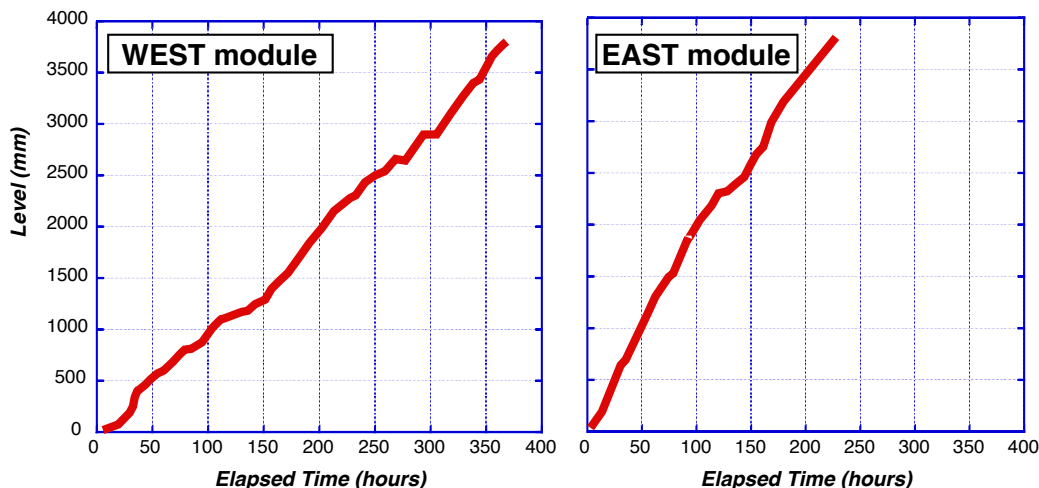


Figure 10. Liquid argon level during filling inside West (left) and East (right) modules.

Few days after, as required to fully thermalize the inner detector structures, the continuous liquid argon filling in both modules started with an overall rate of about $2 \text{ m}^3/\text{h}$. The whole filling lasted about two weeks and was carried out without the need of opening the cryostat exhaust valves. The final level of liquid argon was precisely set at $3825 \pm 5 \text{ mm}$ from the cold vessels floor by means of an arrays of discrete level meters to ensure a safe coverage of the high voltage region of the TPC field cage. The total amount of downloaded liquid argon was 610,511 liters (47 deliveries). In figure 10 the liquid argon level trend during filling is shown for both modules, as monitored by the continuous level meters.

3.4 Detector commissioning and LAr re-circulation and purification start-up

After the completion of the cryogenic plant commissioning, the T600 detector steady state working conditions were reached in few days. Soon after, the TPC in the West module was activated by turning on the high voltage biasing system (-75 kV at the cathode), the data acquisition and PMT trigger system: the first ionization track was immediately recorded and visualized [1].

As already mentioned, the detector cooling and filling procedures did not produce any significant effect on the internal detector structures, the TPC wires and the PMTs. The initial electronic noise level was in agreement with expectations, without detectable microphonic effect due to the cryogenic plant operation.

On May 28th 2010 the first CNGS neutrino interaction was recorded (figure 11). With uniquely the gaseous re-circulation systems active, the initial electron lifetime τ_{ele} , measured with cosmic muon tracks, was found to be uniform in the whole sensitive volume and to exceed $600 \mu\text{s}$, corresponding to a liquid argon residual contamination of about 0.5 ppb of O_2 equivalent. Soon after, the East module was activated showing very similar initial performance.

The liquid re-circulation systems of both modules were also turned on, leading to a steady increase of the LAr purity.

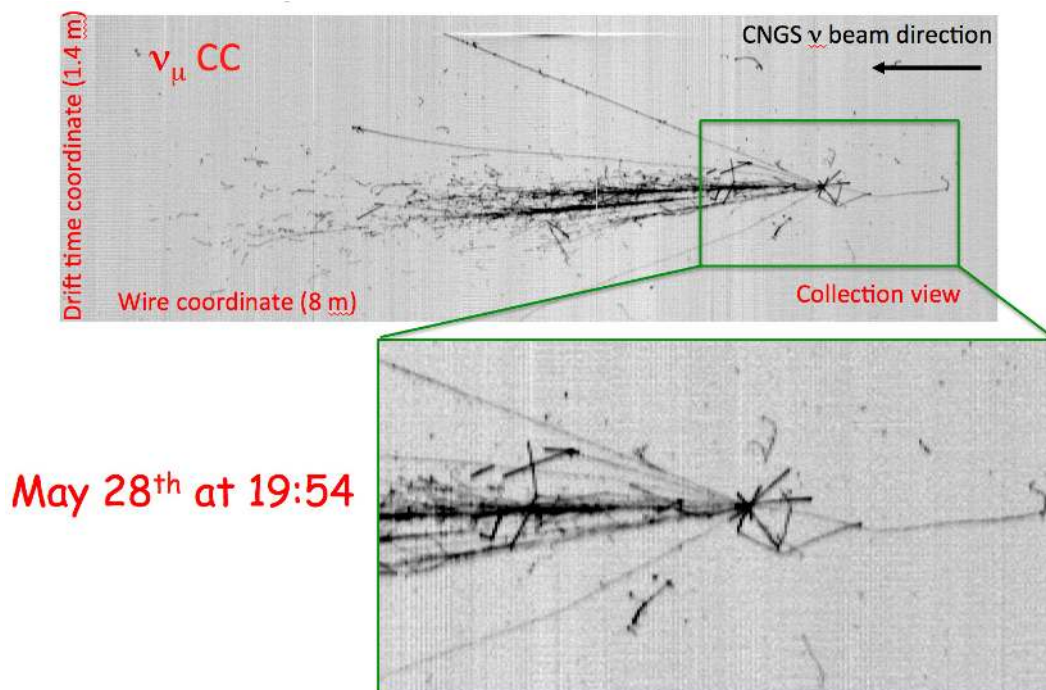


Figure 11. First CNGS neutrino interaction observed in the ICARUS T600 detector.

4 Cryogenic plant operation and performance

In the first few months of T600 operation, the whole cryogenic plant was tested, all the settings were fine-tuned and the related parameters were then stabilized. A complete set of tests on possible failures of the apparatus and emergency events were satisfactorily carried out with the automatic intervention of the dedicated backup systems:

- stop of LN₂ circulation pumps, replaced by redundancy or gravity driven operation;
- complete lack of electrical power, replaced by UPS and/or emergency diesel generator;
- lack of compressed air, replaced by operation with nitrogen gas bottles supply;
- failure of the main ICARUS PLC control system, recovered with automatic activation of redundancies;
- cold gas exhaust at the vent to check electrical heater functionality, temperature and oxygen trend at the exit.

Further redundancy and safety systems were afterwards implemented including a gravity driven LN₂/GAr heat exchanger to re-condense the GAr phase, an emergency power line, a fully pneumatic control system for valves operation to specifically handle the emergency situations of total lack of power in the underground Laboratory.

With all the implemented upgrades and the high intrinsic redundancy, the cryogenic plant was operated safely and reliably during the whole period of steady state T600 run even in case

of severe emergency situations and without stopping the data taking. The control and supervision systems demonstrated to be extremely efficient allowing adopting a smooth surveillance strategy based on an on-call group of experts intervening underground in case of need. As a result, the few recorded emergency situations, all to be ascribed to external power cuts, were rapidly and successfully handled.

Major attention was dedicated to study the reliability and verify proper redundancy of the involved dynamic components, such as cryocoolers and pumps, as they typically represent the most critical part of a working plant.

The nitrogen re-liquefaction system demonstrated to cover the maximum T600 cold power request with flexibility and margin. The system design redundancy allowed performing periodic maintenance to substitute worn components (in the 3,000 ÷ 12,000 hour range, depending on the component) without affecting the refrigeration request. During normal operation the average number of active cryo-coolers was found to be ~ 9 (figure 12).

Due to the cryogenic system complexity, the wear of consumable components and some residual pollution in the re-generators, the cooling system tended to lose efficiency during operation. With maintenance interventions more frequent than initially planned a stable average number of active Stirling units around nine was achieved. Therefore the average cold power delivery was found to balance the insulation losses measured after the plant commissioning (cfr. section 3.2) and the additional 6 ÷ 8 kW heat load from the cryogenic equipment (mainly GAr and LAr recirculation systems switched on for detector operation).

The observed stability of the cold power request demonstrated that no aging effects or degradations of the thermal insulation performance occurred over the whole three years operation.

The liquid nitrogen pumps (Barber Nichols Inc. with external motor) showed an extremely high reliability and stability without interruptions over more than 10000 working hours.

The LAr re-circulation system operation was found to be very effective in increasing the LAr purity which was continuously monitored by measuring the electron lifetime in LAr by the charge attenuation along ionizing cosmic muon tracks crossing the full drift volume. About 100 muon tracks were sufficient to measure day-by-day the electron charge attenuation within few percent.

The evolution of the residual impurity concentration was roughly described with a simple model [1] including the time needed to re-circulate a full detector volume, a constant pollution rate due to external leaks/outgassing in gas phase and the initial contribution of internal residual outgassing which was assumed to vanish with time.¹² Uniform distribution of the impurities throughout the detector volume was also considered, as experimentally supported by the lifetime measurement with muon tracks in different regions of the TPCs [29]. As a result a full volume re-circulation time of $\sim 5 \div 6$ days, in agreement with the nominal pump speed, and an extremely low leak rate ($< \text{few ppt/day O}_2$ equivalent) were found in both modules.

The ACD AC-32 immersed pumps resulted to be less reliable than expected due to excessive bearing case damages that caused frequent system faults with consequent LAr purity drop. A precise and fast intervention procedure was adopted for the LAr pump substitution with a spare one. On average the time interval between two consecutive faults was about 2,000 h.

¹²This model can be applied to short periods including few pump maintenance stops, because it is known that the effective pump speed and the impurity level at each re-circulation pump restart vary as much as 30% due to the maintenance intervention procedure as it can be inferred from figure 13.

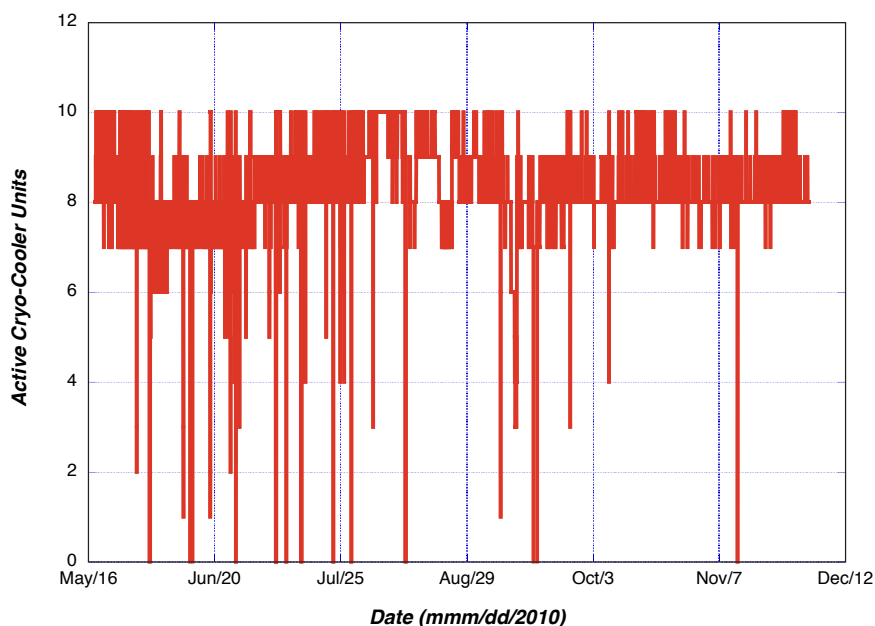


Figure 12. Number of active cryo-coolers during the first months of the T600 operation. Some stops of the cooling system are present, due to power cuts or to failure tests.

In spite of the LAr re-circulation stops, the impurity concentration was maintained below 0.1 ppb all over the detector run (see figure 13). Similar purity trend were observed in both the T600 modules. Electron lifetime values of the order of $7 \div 8$ ms were reached in both modules, corresponding to an impurity content of few tens of ppt that implies a maximum attenuation of free electrons of $\sim 12\%$.

In order to improve the reliability of the LAr re-circulation system a detailed study was performed comparing the different characteristics and reliability between the ACD immersed pumps used in the LAr circuits and the Barber Nichols external motor ones present in the LN_2 transfer lines. This resulted in a significant upgrade of the liquid argon re-circulation system achieved in the last few months of detector operation [30]. One of the ACD AC-32 pumps was substituted with a new Barber Nichols BNHEP-23-000 model similar to the other Barber Nichols pumps used on the liquid nitrogen circulation that showed much longer lifetime between ordinary maintenance cycles. The new pump, characterized by magnetic coupling and vacuum housing, was installed inside a new dedicated vacuum insulated cryostat. A LAr/ LN_2 heat exchanger was added up-stream of the pump aspiration to under-cool liquid argon and to ensure mono-phase liquid state. A Venturi flow-meter was inserted down-stream of the pump output, profiting of the mono-phase argon to measure the flux. After the new pump was switched on, the electron lifetime started increasing at a rate faster than before. At the end of the ICARUS data taking an electron lifetime exceeding 15 ms still rising was measured corresponding to 20 parts per trillion of O_2 -equivalent contamination and an attenuation length of 25 meters, a milestone for any future project involving liquid argon TPC [29]. These results demonstrated the effectiveness of the single phase LAr-TPC detectors paving the way to the construction of huge detectors with longer drift distances. With the achieved purity level only 23% of the signal attenuation is expected at 5 m from the wire planes.

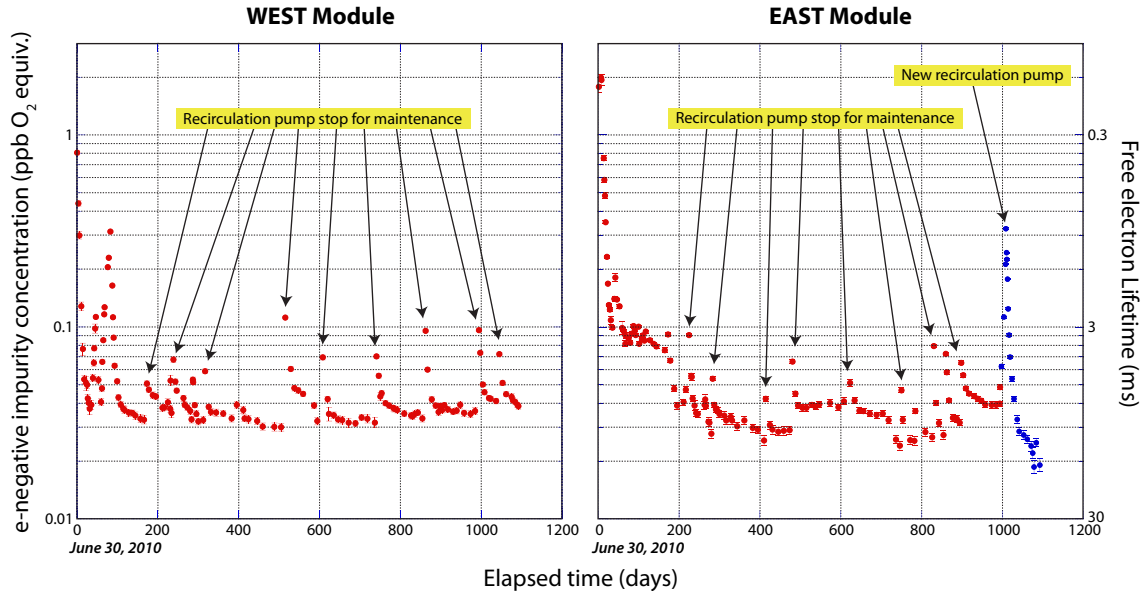


Figure 13. Evolution of the concentration of electronegative impurities concentration in the West (left) and East (right) modules as a function of the elapsed time for more than two years of operation of the T600 detector. The corresponding free electron lifetime is shown on the right axis.

The oxygen contamination contents inferred by the electron lifetime measurements all over the T600 detector run were perfectly compatible with the specifications for untouched scintillation light production and transport¹³ [31]. Together with oxygen, also the nitrogen concentration had to be continuously monitored as it was demonstrated that concentrations of few ppm analyzed of N_2 strongly quench scintillation light [32] and it couldn't be removed by the ICARUS T600 filtering system. As a consequence a custom set-up based on a commercial mass spectrometer (Pfeiffer QMG 220) was specifically developed to measure nitrogen contamination in Ar. A sample of the T600 gas phase was periodically analyzed and N_2 concentration was always found below the 1 ppm sensitivity of the instrument according to the evidence from the PMT signals.

Beside LAr purity, other cryogenic parameters affecting the LAr-TPC performance were accurately monitored along the whole detector operation. In particular, the internal temperature, directly connected to the electron drift velocity, was found stable and uniform to better than 0.25 K (figure 14). This was confirmed by the observed stability of the internal LAr absolute pressure (figure 15) in spite of the previously mentioned emergency situations.

¹³ O_2 contamination in LAr leads to the attenuation of both the free electron charge (via attachment process) and the scintillation light (via quenching and absorption mechanisms). The request on O_2 concentration to avoid scintillation light reduction is much less stringent than that for electron attachment (effects are visible for concentrations above 0.5 ppm).

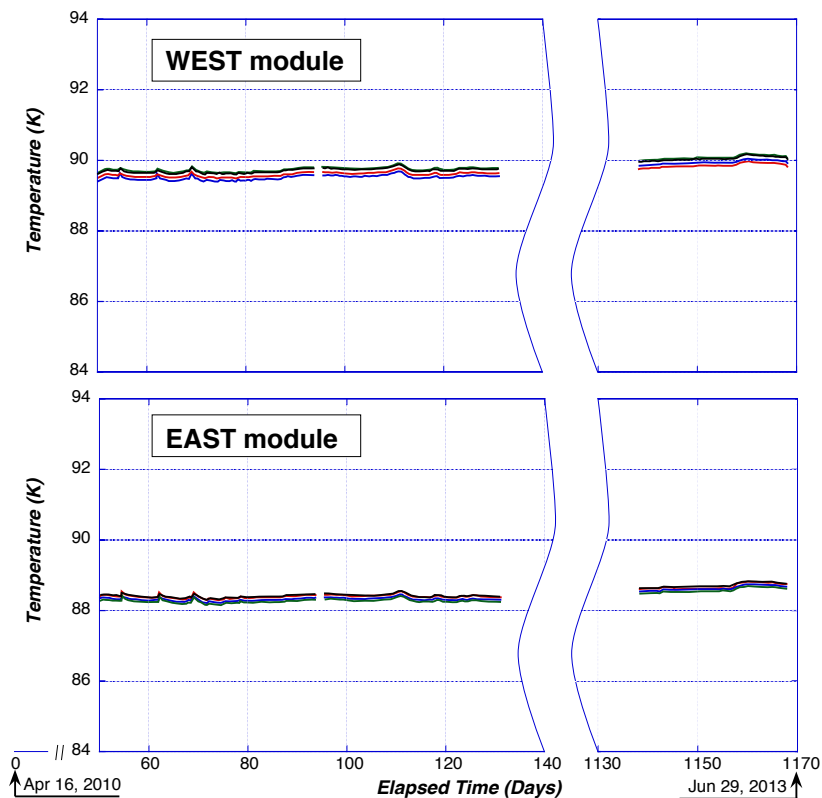


Figure 14. Trend of the internal temperatures measured in several locations along the vertical direction in the two modules recorded in two periods of the detector live time, one at the beginning of the run, in 2010, and the second in 2013, close to the end of the run.

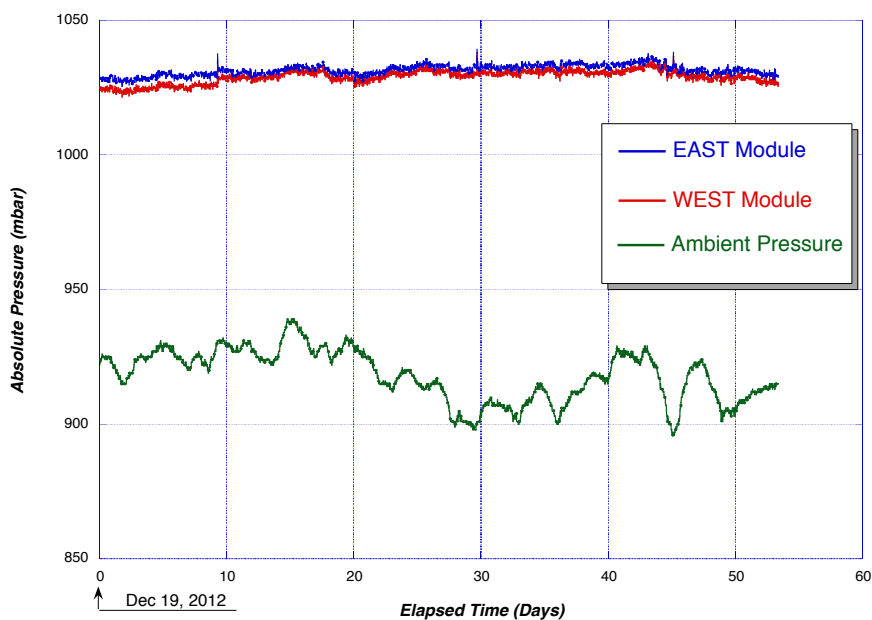


Figure 15. Absolute internal pressure in the two modules during a period of about two months between the end of 2012 and the beginning of 2013. The internal pressure was kept uniform and stable within ≈ 10 mbar.

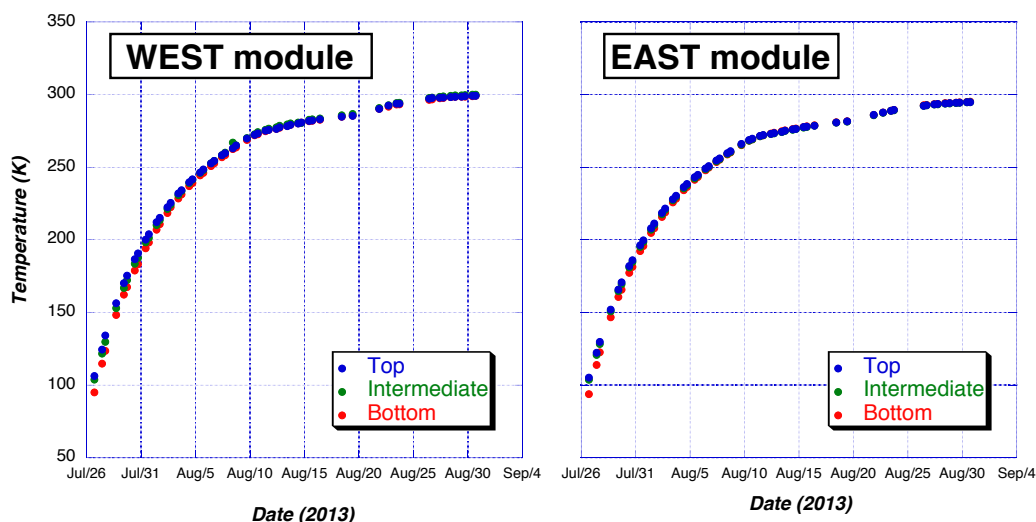


Figure 16. Temperature trends on the wire-chamber structure all over the T600 warm-up phase.

5 Decommissioning

The preparation for the T600 decommissioning started during the last months of detector operation. In particular an emptying skid was installed to host an immersed LAr pump ADC AC-32, together with an intermediate buffer to speed up the emptying process. The decommissioning process started on June 27th 2013 proceeding along the following phases:

1. The cryostat emptying phase lasted less than one month and was operated in a safe and smooth way in parallel on the two modules. To speed up the process, LAr was transferred at 7,000 l/h rate into an intermediate vessel (20,000 l), allowing the decoupling of the emptying procedure from the truck uploading. About 740 LAr tons over a total of 760 were recovered for a total number of 33 trucks (1-2 trucks/day).
2. The successive cryostat warming-up started on July 25th and took about one month proceeding with the help of a heating system to speed up the process by circulating warm nitrogen gas inside T600 cooling screens while keeping the thermal gradients within the $\Delta T < 50$ K specification to prevent thermal shock on wire chambers (figure 16).
3. The T600 detector dismantling started in September 2013 and lasted about 15 months. It was finalized to the cryostat opening to extract the TPC detectors as a whole including the light detection system, cabling and ancillary equipment, and place them into dedicated boxes specifically designed for the transport to CERN. The cryogenic plant, DAQ and trigger electronic systems were recuperated and separately sent to CERN.

6 Conclusions

The ICARUS T600 LAr-TPC, installed at LNGS, is the biggest liquid argon detector ever realized and represents so far the state of the art of the liquid argon TPC technology. Industry partnership was crucial to perform the scaling-up of the technology from the laboratory prototypal scale to the kton mass scale.

The commissioning at LNGS was successfully and safely performed during the first half of 2010. The detector smoothly reached optimal working conditions and took cosmic and CNGS neutrino beam data with extremely high liquid argon purity and high detector live-time, performing even beyond expectations. The obtained results demonstrated, as reported in several published papers, the effectiveness of the single phase LAr-TPC detectors paving the way to the construction of huge detectors with longer drift distances.

The three years safe and stable operation in the severe underground environment conditions was an important achievement for LAr-TPC technique demonstrating the technology is mature and scalable to several kton mass as required by future projects. Lessons learned from the plant operation, accidental events and plant improvements will be useful for the next developments.

Acknowledgments

The ICARUS Collaboration acknowledges the fundamental support of INFN and, in particular, of the LNGS Laboratory, all the staff and its Directors, to the construction and operation of the experiment. Moreover the authors thank LNGS Safety and Prevention Service, the Research and Technical Divisions, and in particular the Experiment Support Service, the LNGS cryogenic group and the Exercise and Maintenance Service for their contribution to the commissioning and operation of the T600 apparatus. The collaboration recognizes the fundamental involvement of the industrial companies Air Liquide, Stirling Cryogenics BV and Luca Scarcia, which contributed in the realization, operation and maintenance of the cryogenic plant. A special thank to Marco Brugnolli, Arnaldo Di Cesare and Donatello Ciccotti. The authors warmly thank the Electronics Service of INFN Pavia, in particular M.C. Prata, for the design and realization of the slow control electronics and of the vacuum system remote controls. The Polish groups acknowledge the support of the National Science Center, Harmonia (2012/04/M/ST2/00775) and Preludium (2011/03/N/ST2/01971) funding schemes.

References

- [1] C. Rubbia et al., *Underground operation of the ICARUS T600 LAr-TPC: first results*, 2011 *JINST* **6** P07011 [[arXiv:1106.0975](#)].
- [2] C. Rubbia, *The liquid-argon time projection chamber: a new concept for neutrino detector*, CERN-EP/77-08 (1977).
- [3] M. Antonello et al., *Precise 3D track reconstruction algorithm for the ICARUS T600 liquid argon time projection chamber detector*, *Adv. High Energy Phys.* **2013** (2013) 260820 [[arXiv:1210.5089](#)].
- [4] ICARUS collaboration, M. Antonello et al., *Search for anomalies in the ν_e appearance from a ν_μ beam*, *Eur. Phys. J. C* **73** (2013) 2599 [[arXiv:1307.4699](#)].
- [5] M. Antonello et al., *Experimental search for the “LSND anomaly” with the ICARUS detector in the CNGS neutrino beam*, *Eur. Phys. J. C* **73** (2013) 2345 [[arXiv:1209.0122](#)].
- [6] M. Antonello et al., *ICARUS at FNAL*, [arXiv:1312.7252](#);
LAR1-ND, ICARUS-WA104 and MICROBoONE collaborations, M. Antonello et al., *A Proposal for a Three Detector Short-Baseline Neutrino Oscillation Program in the Fermilab Booster Neutrino Beam*, [arXiv:1503.01520](#).

- [7] LSND collaboration, A. Aguilar-Arevalo et al., *Evidence for neutrino oscillations from the observation of anti-neutrino(electron) appearance in a anti-neutrino(muon) beam*, *Phys. Rev. D* **64** (2001) 112007 [[hep-ex/0104049](#)].
- [8] MINIBooNE collaboration, A.A. Aguilar-Arevalo et al., *Improved Search for $\bar{\nu}_\mu \rightarrow \bar{\nu}_e$ Oscillations in the MiniBooNE Experiment*, *Phys. Rev. Lett.* **110** (2013) 161801 [[arXiv:1207.4809](#)].
- [9] Long Baseline Neutrino Experiment (LBNE) Project, *Conceptual Design Report*, <http://lbne2-docdb.fnal.gov/cgi-bin/ShowDocument?docid=5235&asof=2112-11-06>; LBNE collaboration, C. Adams et al., *The Long-Baseline Neutrino Experiment: Exploring Fundamental Symmetries of the Universe*, [arXiv:1307.7335](#).
- [10] D. Angeli et al., *Towards a new Liquid Argon Imaging Chamber for the MODULAR project*, 2009 *JINST* **4** P02003;
B. Baibussinov et al., *A New, very massive modular Liquid Argon Imaging Chamber to detect low energy off-axis neutrinos from the CNGS beam: Project MODULAR*, *Astropart. Phys.* **29** (2008) 174 [[arXiv:0704.1422](#)].
- [11] A. Rubbia, *Underground Neutrino Detectors for Particle and Astroparticle Science: The Giant Liquid Argon Charge Imaging Experiment (GLACIER)*, *J. Phys. Conf. Ser.* **171** (2009) 012020 [[arXiv:0908.1286](#)].
- [12] A. Antonello et al., *Search for anomalies in the neutrino sector with muon spectrometers and large LArTPC imaging detectors at CERN*, [arXiv:1208.0862](#).
- [13] MICROBooNE collaboration, G. Karagiorgi, *MicroBooNE: Searching for new physics in the neutrino sector with a 100-ton-scale liquid argon TPC*, *J. Phys. Conf. Ser.* **375** (2012) 042067.
- [14] ICARUS collaboration, S. Amerio et al., *Design, construction and tests of the ICARUS T600 detector*, *Nucl. Instrum. Meth. A* **527** (2004) 329.
- [15] P. Benetti et al., *First results from a Dark Matter search with liquid Argon at 87 K in the Gran Sasso Underground Laboratory*, *Astropart. Phys.* **28** (2008) 495 [[astro-ph/0701286](#)].
- [16] ICARUS collaboration, M. Antonello et al., *The trigger system of the ICARUS experiment for the CNGS beam*, 2014 *JINST* **9** P08003 [[arXiv:1405.7591](#)].
- [17] M. Antonello et al., *Precision measurement of the neutrino velocity with the ICARUS detector in the CNGS beam*, *JHEP* **11** (2012) 049 [[arXiv:1208.2629](#)].
- [18] ICARUS collaboration, M. Antonello et al., *Measurement of the neutrino velocity with the ICARUS detector at the CNGS beam*, *Phys. Lett.* **B 713** (2012) 17 [[arXiv:1203.3433](#)].
- [19] P. Benetti et al., *A 3-ton liquid argon time projection chamber*, *Nucl. Instrum. Meth. A* **332** (1993) 395.
- [20] P. Cennini et al., *Performance of a 3-ton liquid argon time projection chamber*, *Nucl. Instrum. Meth. A* **345** (1994) 230.
- [21] F. Arneodo et al., *Performance of the 10 m³ ICARUS liquid argon prototype*, *Nucl. Instrum. Meth. A* **498** (2003) 292.
- [22] C. Vignoli, *ICARUS: an innovative large LAr detector for neutrino physics*, *Adv. Cryog. Eng.* **51** (2006) 1643.
- [23] ICARUS collaboration, A. Ankowski et al., *Energy reconstruction of electromagnetic showers from pi0 decays with the ICARUS T600 Liquid Argon TPC*, *Acta Phys. Polon.* **B 41** (2010) 103 [[arXiv:0812.2373](#)].

- [24] ICARUS collaboration, A. Ankowski et al., *Measurement of through-going particle momentum by means of multiple scattering with the ICARUS T600 TPC*, *Eur. Phys. J. C* **48** (2006) 667 [[hep-ex/0606006](#)].
- [25] ICARUS collaboration, S. Amoruso et al., *Study of electron recombination in liquid argon with the ICARUS TPC*, *Nucl. Instrum. Meth. A* **523** (2004) 275.
- [26] ICARUS collaboration, S. Amoruso et al., *Measurement of the μ decay spectrum with the ICARUS liquid argon TPC*, *Eur. Phys. J. C* **33** (2004) 233 [[hep-ex/0311040](#)].
- [27] S. Amoruso et al., *Analysis of the liquid argon purity in the ICARUS T600 TPC*, *Nucl. Instrum. Meth. A* **516** (2004) 68.
- [28] F. Arneodo et al., *Observation of long ionizing tracks with the ICARUS T600 first half-module*, *Nucl. Instrum. Meth. A* **508** (2003) 287 [Erratum *ibid.* **A 516** (2004) 610].
- [29] M. Antonello et al., *Experimental observation of an extremely high electron lifetime with the ICARUS-T600 LAr-TPC*, *2014 JINST* **9** P12006 [[arXiv:1409.5592](#)].
- [30] ICARUS collaboration, C. Vignoli, *The ICARUS T600 Liquid Argon Purification System*, *Phys. Procedia* **67** (2015) 796.
- [31] WARF collaboration, R. Acciarri et al., *Oxygen contamination in liquid Argon: Combined effects on ionization electron charge and scintillation light*, *2010 JINST* **5** P05003 [[arXiv:0804.1222](#)].
- [32] WARF collaboration, R. Acciarri et al., *Effects of Nitrogen contamination in liquid Argon*, *2010 JINST* **5** P06003 [[arXiv:0804.1217](#)].