

Plasma Surface Modification of Biomedical Polymers: Influence on Cell-Material Interaction

Tinneke Jacobs · Rino Morent · Nathalie De Geyter · Peter Dubruel · Christophe Leys

Received: 7 February 2012 / Accepted: 21 June 2012 / Published online: 1 July 2012
© Springer Science+Business Media, LLC 2012

Abstract Polymers are commonly used in industry because of their excellent bulk properties, such as strength and good resistance to chemicals. Their surface properties are for most application inadequate due to their low surface energy. A surface modification is often needed, and plasma surface modification is used with success the past decades. In the past few years, also plasma surface modification for biomedical polymers has been investigated. For biomedical polymers, the surface properties need to be altered to promote a good cell adhesion, growth and proliferation and to make them suitable for implants and tissue engineering scaffolds. This review gives an overview of the use of plasma surface modification of biomedical polymers and the influence on cell-material interactions. First, an introduction on cell-material interaction and on antibacterial and antifouling surfaces will be given. Also, different plasma modifying techniques used for polymer surface modification will be discussed. Then, an overview of literature on plasma surface modification of biopolymers and the resulting influence on cell-material interaction will be given. After an overview of plasma treatment for improved cell-material interaction, plasma polymerization and plasma grafting techniques will be discussed. Some more specialized applications will be also presented: the treatment of 3D scaffolds for tissue engineering and the spatial control of cell adhesion. Antibacterial and antifouling properties, obtained by plasma techniques, will be discussed. An overview of research dealing with antibacterial surfaces created by plasma techniques will be given, antifouling surfaces will be discussed, and how blood compatibility can be improved by preventing protein adhesion.

Keywords Plasma · Biomedical polymer · Surface modification · Cell-material interaction

T. Jacobs (✉) · R. Morent · N. De Geyter · C. Leys
Research Unit Plasma Technology (RUPT), Department Of Applied Physics, Faculty of Engineering,
Ghent University, Sint-Pietersnieuwstraat 41 - B4, 9000 Ghent, Belgium
e-mail: tinneke.jacobs@ugent.be

P. Dubruel
Polymer Chemistry and Biomaterials Group, Department of Organic Chemistry, Faculty of Sciences,
Ghent University, Krijgslaan 281 S4, 9000 Ghent, Belgium

Introduction

In the past decades, modern medicine has been challenged with complex problems, which have led to technological advancements in the area of healthcare. However, in the domain of tissue engineering, many complex problems still remain. It is a multidisciplinary field combining principles of biology, medicine and engineering, that aims at replacing damaged, injured or missing organs and tissue with a functional artificial substitute [1, 2]. This substitute can be a combination of both a scaffold and cells, an acellular scaffold or cells only [3]. The complexity of the problems arising when replacing tissue, set very high and diverse demands on the used materials. Biocompatibility, biodegradability, providing strength and structure if needed, enabling cell attachment, proliferation and sometimes even differentiation are just some of the possible necessities. In some other cases including, catheters and stents, prevention of cell attachment and adsorption of proteins is required. Moreover, no inflammatory responses, formation of unusual tissues or other deleterious reactions should occur. Most of the demands and problems involve the reaction to and interaction with the surrounding tissue of the implanted material once it is implanted in the body. In this respect, the surface of the material plays a key role [4]. The final purpose of the implant determines the required properties and thus also the optimal surface characteristics (composition and topography).

It is very difficult to find a material that meets all the requirements. One strategy is to use composite materials that combine the properties of its components. Another way is to use a material that has the required bulk properties (biodegradability, strength, ...) and to perform a surface treatment to modify the surface characteristics. Biomedical polymers (see Fig. 1), such as polylactic acid (PLA), poly- ϵ -caprolactone (PCL), poly(lactic acid-co-glycolic acid) (PLGA) and poly(hydroxybutyrate), are materials with good bulk properties for biomedical applications [5]. They are biocompatible, in some cases also biodegradable, and have good mechanical and structural properties. However, their surface properties are unsuitable to attract cells and a surface treatment is often required. In the past decades, surface treatment of polymers with non-thermal plasmas has been extensively studied [6], and it has become evident that also for biomedical polymers this is a promising approach [7, 8]. Plasma modification of biomedical polymers gives the opportunity to change the surface characteristics of polymeric implants to achieve a better biocompatibility without altering the bulk properties. Due to the versatility of the technology, it can be useful in many different applications [9].

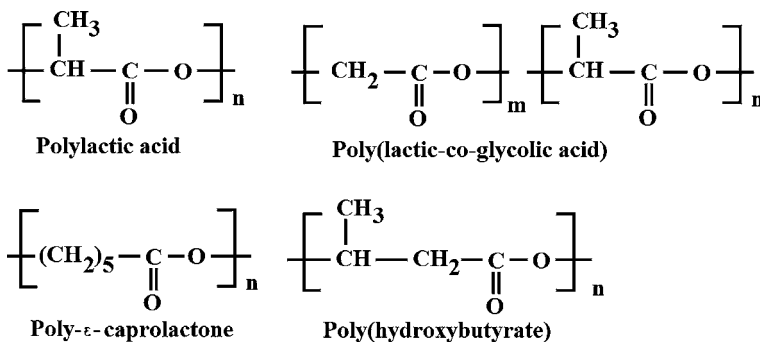


Fig. 1 Chemical structures of common biomedical polymers

In the next paragraph, the interactions between a material (implant) and cells (surrounding tissues) will be described. After that, the importance of antibacterial and antifouling properties of a surface in specific applications will be explained. Then, different plasma modifying techniques that can be used to enhance biocompatibility of biomedical polymers will be discussed. In the second section, an overview of literature on plasma surface modification of biomedical polymers and the resulting influence on cell-material interaction will be given. After an overview of plasma treatment for improved cell-material interaction, plasma polymerization and plasma grafting techniques will be discussed. Finally, some more specialized applications will be presented: the treatment of 3D scaffolds for tissue engineering and the spatial control of cell adhesion. In the third section, antibacterial and antifouling properties, obtained by plasma techniques, will be discussed. First, an overview of research dealing with antibacterial surfaces created by plasma techniques will be given. Afterwards, antifouling surfaces will be discussed, and how blood compatibility can be improved by preventing protein adhesion. At last, general conclusions and an outlook will be given.

Cell-Material Interactions

As mentioned above, the interaction of the biomedical material with the surrounding tissue is a key factor in the final success of the implant. The response of a cell in contact with the surface and the adhesion of cells to the material play an important role in the biocompatibility of the implant. It is thus important to understand how cells interact with their environment.

Cells sense their surroundings through so-called protrusions. These are micrometer sized sheet-like structures composed of an actin filament mesh. At the extremes, smaller hair-like protrusions, called ‘filopodia’, composed of long, thin actin filament bundles, ‘sense’ the extracellular matrix (ECM), and the materials surface [10]. For example, when the filopodia find a suitable binding site for adherence, a feedback signal within the cell allows for so-called integrin receptors to bind to that specific binding site.

Receptors are located on the outer wall of the cells and are responsible for the intracellular interaction and communication. When these receptors bind specifically with a ligand, a receptor response occurs, starting a cascade of events within the cell, leading to an appropriate trigger response.

One very important class of cell receptors called ‘integrins’ bind selectively to binding sites such as arginine-glycine-aspartic acid (RGD) tripeptide found in cell adhesive proteins such as laminin, fibronectin and vitronectin [11, 12]. When the filopodia find such a binding site, a feedback signal allows for the integrin receptor to bind to that site and allows more integrin receptors to be localized in that region of the cell. This leads to the adhesion of the cell to that region.

Integrins also function as signal transducers, activating various intracellular signaling pathways when activated upon ECM binding. The signals the cell receives through the integrin can be related to cell growth, proliferation (division) and differentiation.

When a material is placed inside a biological environment, a water shell is created around the material within nanoseconds. In the next seconds to hours, the surface becomes covered with a layer of adsorbed proteins, such as fibronectin and vitronectin, initially present in the ECM. In the third stage, the cells of the surrounding tissue reach the material, interacting through the adsorbed protein covering. This stage occurs from as fast as minutes to days after the implantation, and adhesion, migration and differentiation of cells takes place. It is influenced by biological molecules, the biophysical environment and

surface properties. The fourth stage, the useful life of the implant, is the continuing development of the early implant stages [3, 10]. The duration of this stage can vary from days to several decades.

Antibacterial and Antifouling Properties

Besides the cell-material interaction, also the antibacterial properties play an important role in medical implants. When an acellular scaffold is implanted, both cells and bacteria compete to adhere and grow onto the surface. When the situation is in favor of the bacteria, the attached and growing bacterial colonies soon produce an extracellular polysaccharide matrix [13]. This protects the bacteria against antibiotics and the body's defense system and allows the bacteria to form a biofilm. Studies of biofilms have shown differentiated and structured groups of cells with community properties [14]. Antibiotics are thus much less efficient in destroying the bacterial biofilms than circulating bacteria. This biofilm leads in most cases to further infections and inflammations, which can result in the (partial) removal of the infected implant.

For the correct functioning of an implant, it is thus critical that the attachment of bacteria is prevented. This can be achieved by making the surface of the implant antibacterial. One way is to deposit a coating on the implant surface that offers resistance to bacterial colonization. There exist some antibacterial polymers, that kill bacteria or prevent them from attaching, which can be used for such a coating [15]. Antibacterial properties can also be achieved by the release of low molecular weight antibiotics from the biomedical device, by loading these antibiotics into polymers or polymer composite films [16]. Another possible approach is grafting a layer of antibiotic molecules that prohibits the adhesion of bacteria to the surface. However, it should be kept in mind that the antibacterial properties of the surface should not compromise the attachment of cells of the surrounding tissue.

Besides antibacterial properties, sometimes antifouling properties are needed, where the adhesion of certain cells, proteins, platelets, or any other biological entities are prevented. For example for blood contacting materials, the prevention of thromboembolism formation is a key requirement. For contact lenses, wound healing materials, catheters and biosensors, it is important to avoid unspecific protein adsorption. Moreover, the formation of an adsorbed protein layer can provide a conditioning layer for microbial colonization and biofilm formation [17]. Further application can be found in marine equipments, like ship hulls, where antifouling surfaces can be used to prevent biofouling by sea microorganisms, diatoms and algae [18]. Antifouling surfaces can be obtained by coating the surface with heparin, which is often used for blood contacting materials to prevent the adhesion of blood proteins [19]. The grafting of polyethylene glycol (PEG) or polyethylene oxide (PEO) (possessing the same chemical structure but only differing in molecular weight) onto surfaces has shown to have excellent protein resistance properties. Coatings containing polysaccharides, fluorinated coatings, polydimethyl-siloxane (PDMS) elastomers, zwitterionic polymers, are some of the other possibilities [20].

Different Plasma Modifying Strategies

Given the many different biomedical devices and implants, as well as the different cells, tissues, bacteria, and proteins that are involved, there is no universal solution to all problems, and the cell adhesion, antibacterial and antifouling properties have to be tailored to each specific need. As stated above, a common strategy is to use a material with the

suitable bulk characteristics and to modify the surface properties to meet the requirements. Biomedical polymers are excellent candidates for such an approach [5]. This has led to a variety of polymer surface modification strategies, of which plasma surface modification will be the focus of this review paper. Plasma surface modification is a very suitable and versatile technique that does not change the bulk properties, it can be used to uniformly treat complex shaped surfaces and it is a solvent-free technology [8, 21, 22].

Plasma is often referred to as the fourth state of matter. It is a mixture of charged and neutral particles, such as atoms, molecules, ions, electrons, radicals, photons, etc. There are two main categories, thermal and non-thermal plasmas [23]. Thermal plasmas cannot be used for the surface treatment of polymers because of their high gas temperature. Non-thermal plasmas however, have a much lower gas temperature but relatively high electron temperature. They do not cause any thermal damage to the surface of heat sensitive materials, although the reactive species in a non-thermal plasma can cause chemical and physical modifications to the surface [24].

Since a plasma contains diverse active species, different interactions of the plasma with the surface can occur. As a result, different plasma modifying techniques can be distinguished, which will be discussed below. In Fig. 2, a schematic representation is shown of

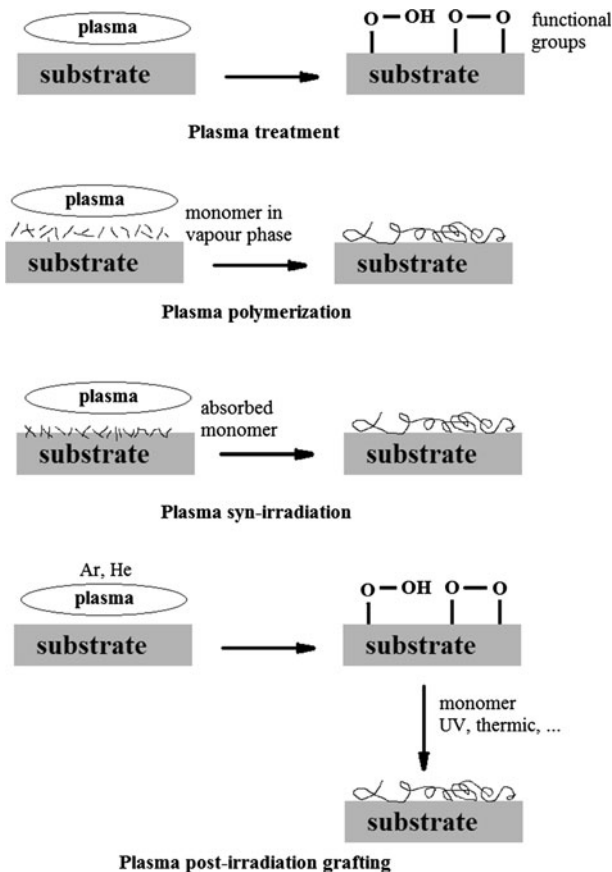


Fig. 2 Schematic representation of the different plasma modifying strategies

the different technologies. In the next section, it will be shown how each of these techniques can be used to influence the cell-material interaction.

During exposure, different chemical functional groups can be implanted at the surface [25]. This is often referred to as plasma treatment. In this case, the plasma is generated in oxygen or nitrogen containing gases or inert gases. The incorporated groups change the surface properties, mainly the surface wettability and thus the surface energy, but also the surface roughness [26]. The plasma-treated surfaces can be used to immobilize biologically active ligands. One major and important drawback of plasma treatment is the durability of the treatment effect. The surface undergoes a hydrophobic recovery after treatment and part of the generated effect is lost [27, 28].

Plasma polymerization is a deposition technique where a gaseous or liquid monomer is introduced in the plasma discharge and converted into reactive fragments [29–32]. These can react with the surface to form a so-called plasma polymer coating, that has unique physical and chemical properties. These coatings are pinhole-free, highly cross-linked and are therefore insoluble, thermally stable, chemically inert and mechanically tough. Often these films are highly coherent and adherent to a variety of substrates including conventional polymer, glass and metal surfaces [33].

Rather than introducing a monomer in the plasma itself, the monomer can also be first adsorbed to the substrate, which is then subjected to a plasma. The plasma will create surface radicals in the monomer layer and the substrate surface, resulting in a cross-linked polymer top-layer. This process is called plasma syn-irradiation [8].

When depositing a plasma polymer in a plasma polymerization or plasma syn-irradiation process, the monomer is directly exposed to the plasma. However, it is also possible to firstly activate and functionalize the surface with a plasma treatment. The induced functionalities can subsequently be employed for the initiation of a polymerization reaction, by bringing the surface in contact with monomers in the gas or liquid phase [34]. Since the monomer is not subjected to the plasma, the grafted polymer will have the same composition as polymers obtained by conventional polymerization processes. This two step technique is called plasma post-irradiation grafting.

For the different plasma surface modification techniques discussed above, a wide variety of plasma sources is available. Radio frequency (RF) discharges, glow discharge plasmas, dielectric barrier discharges (DBDs), microwave plasmas, etc. are some of the possibilities. Reviews on these different discharges are available elsewhere [35, 36] and will therefore not be discussed here.

Besides the various plasma modifying strategies, also non-plasma based approaches are available to introduce chemical functional groups or to immobilize proteins and other bioactive molecules at a biomaterial's surface. Several of these strategies will be briefly discussed here, with special attention to the advantages and disadvantages compared to plasma modification. Wet-chemical methods, such as aminolysis and hydrolysis, involves the reaction between a surface and a chemical compound in a solution [37, 38]. In this way, hydroxyl, carboxyl and amino groups are created at the surface. These methods have shown to increase hydrophilicity and improve cell attachment [39, 40]. However, they are non-specific and not reproducible, cause degradation and irregular etching and produce chemical waste.

Ozone treatment, in combination with UV irradiation, UV treatment, photografting and gamma radiation are also used to introduce chemical groups [41–48]. These have all been used for the grafting of monomers and graft polymerization [49–52]. Also ozone treatment, UV-treatment and gamma radiation are techniques that cause degradation and are often non permanent and nonspecific.

Although the aforementioned techniques have proven to be valuable, plasma surface modification has several advantages that make this technology an excellent candidate for polymeric materials treatment. Firstly, it does not require hazardous solvents. It does not affect bulk properties or cause degradation. Moreover, it can be utilized to uniformly treat complex shaped structures. The deposition of coatings and the immobilization of bioactive molecules is also possible with plasma based techniques. It is thus clear that plasma modification of biomedical polymers has great potential, and will therefore be the focus of this review paper.

Improved Cell Adhesion and Proliferation by Plasma Surface Modification

In this section, an overview of literature on plasma surface modification of biomedical polymers and the resulting influence on cell-material interactions will be given. It is important to note that although cell attachment in many cases is a advantage and even a requirement, many applications require prevention of adhesion of any kind. These antibacterial and anti-fouling surfaces will be discussed in section “[Antibacterial and Anti-fouling Surfaces by Plasma Surface Treatment](#)”.

First, an overview of literature on plasma treatment of biomedical polymers for improved cell-material interaction will be given. Subsequently, plasma polymerization and plasma grafting techniques will be discussed. Finally, some more specialized applications will be presented including the treatment of 3D scaffolds for tissue engineering and the spatial control of cell adhesion. In Tables 1, 2 and 3 a schematic overview of the various cited works can be found.

Plasma Surface Treatment

As already mentioned, plasma treatment of a polymer surface results in the introduction of different chemical groups onto the surface [53–55], thereby changing the surface properties. In this part, the focus will be on how these functional groups are able to change and improve the cell-material interactions. There is a lot of literature available on plasma surface treatment of a wide variety of biomedical polymers. However only studies which deal with cell-surface interaction will be discussed here.

Cell adhesion on plasma-treated PLA surfaces has been widely investigated [56–63]. Different plasma gases have been used, and different cells have been cultivated on the modified surfaces, mostly with satisfying results. Khorasani et al. [56] modified PLLA films with an RF plasma in oxygen at low pressure. After plasma treatment, the hydrophilicity was greatly increased. The contact angle dropped from about 85° for untreated PLLA films, to approximately 10° after oxygen plasma treatment. Attenuated total reflectance Fourier transform infrared spectroscopy (ATR-FTIR) studies confirmed the presence of oxygen containing functional groups (acidic, carboxylic, hydroxyl and carbonyl groups) at the surface of the treated films. Cell culture tests using nerve tissue B65 cells revealed a better cell attachment and growth on the treated PLLA samples. The cells were observed to be in a webbing and flattening state (active adhesion or activation state). The authors attributed this behavior to a combined effect of the surface chemistry and—wettability. In another study [57], researchers used a CO₂ plasma to modify PLA samples. The contact angle was decreased to 45°, and more oxygen containing functional groups were found on the surface of treated samples. Using atomic force microscopy (AFM), it was shown that after treatment, the surface is rougher and micro-spherulites appear. For

Table 1 Representative overview of plasma treatment of polymers and influence on cell-material interactions

| Substrate | Plasma | Cell type | Observations | References |
|--------------|-------------------------------------|---|--|------------|
| PLA | O ₂ | Nerve tissue B65 | Flattened cells | [40] |
| PLA | CO ₂ | Glial B65 | Flattened cells | [41] |
| PLA | CO ₂ | L929 fibroblasts | No difference | [41] |
| PLA | Air | Osteoblast MC3T3-E1 | Improved proliferation and adhesion | [42, 43] |
| PLA | Ammonia | HUVEC | Increased cell density | [44] |
| PLA | Ammonia | 3T3 fibroblasts | Spindle shaped cells | [45] |
| PLA | Ammonia | 3T3 fibroblasts | Better adhesion under shear stress | [47] |
| PLA | Sulphur dioxide | Rat osteoblasts | Decreased cell adhesion | [46] |
| PCL | O ₂ | 7F2 osteoblasts | Increased proliferation, confluent cell layer | [48] |
| PCL | Air | HPEC | Improved proliferation and adhesion | [49] |
| PCL | Ar and mixtures | HPEC | Increased cell attachment | [50] |
| PLGA | O ₂ | Nerve tissue B65 | Flattened cells | [40] |
| PLGA | O ₂ | 3T3 fibroblasts | Improved attachment | [51] |
| PLGA | O ₂ | 3T3 fibroblasts | Improved adhesion under shear stress | [52] |
| PLGA | Air | Hepatoma HEP G2, osteoblast MG 63, CPAE, 3T3 fibroblasts | Spreaded and flattened cells | [53] |
| PLGA | Ammonia | 3T3 fibroblasts | Improved attachment and more spreading of cells | [54] |
| PHBV | O ₂ | Dog bone marrow stromal cells | Improved attachment and proliferation | [55] |
| PHBV | O ₂ | Human retinal pigment epithelium | Improved attachment and proliferation | [56] |
| PHBV | O ₂ , Ar, N ₂ | HaCaT | Better attachment, flattened cells | [57] |
| PHB | Ammonia/ water vapour | HUVEC | Flat confluent monolayer/formation of capillary-like networks | [58] |
| PHBHHx | Ammonia | HUVEC, SMC | Evenly distributed and spread (HUVEC), no difference (SMC) | [59] |
| PEGT/ PBT | Ar | Chondrocytes | Increased cell number and pseudopodia formation, reduced re-differentiation capacity | [60] |

The table presents a comprehensive overview of the substrates, the plasma type, cell type, results on modified cell-material interactions

cell culture tests, two cell types were used: glial B65 cells and L929 fibroblasts. The results for the B65 cells were comparable to the study of Khorasani et al. [56]. For the L929 cells however, no significant difference in cell adhesion and growth was observed. The authors reaffirmed conclusions by other groups in the field using other materials that cell-polymer interactions depend on both surface wettability, and—morphology.

Table 2 Representative overview of plasma polymerization and grafting of polymers and influence on cell-material interactions

| Substrate | Grafted monomer/ molecule | Cell type | Observations | References |
|--------------------------------------|------------------------------|------------------------------------|---|------------|
| PCL | Collagen | SMC | Increased cell number, spindle-like morphology | [61] |
| PCL | Collagen | HDF, human myoblasts | Flattened cells with spindle morphology | [62] |
| PCL | Collagen | HUVEC | Higher proliferation rate, elongated and flattened cells | [63] |
| PHB/PHV | Insulin | Fibroblast | Improved proliferation, fully spread cells | [64] |
| PTFE | RGDC peptide | HUVEC | Improved attachment level | [65] |
| Acrylic acid thin film on Ti surface | RGD peptide | MC3T3-E1 | Improved differentiation | [66] |
| PLLA | Gelatin | HUVEC | Enhanced cell adhesion, spreading and proliferation | [67] |
| PCL fibres | Collagen | HDF | Confluent layer of long spindle shaped cells, protrusions between cell and collagen-coated fibres | [68] |
| PLGA | Collagen | 3T3 fibroblasts | Improved attachment, spreading and viability | [69] |
| PLA | Collagen | 3T3 fibroblasts | Increased cell number and improved attachment | [70] |
| PLA-co-PCL fibres | Collagen | Endothelial cells | Improved attachment, spreading and viability | [71] |
| PLA | Chitosan | L929 fibroblast and L02 hepatocyte | Poor adhesion and spreading, proliferation rate comparable to cells cultured on glass plate | [73] |
| Substrate | Polymerized monomer | Cell type | Observations | Reference |
| PLA | Allylamine | Euglypha, vorticella | Dence adhered biofilm | [74] |
| PLLA, PCL | Allylamine with PEG | Hepatocyte | Improved attachment | [75] |
| Silicone | Allylamine | Fibroblasts | Improved adhesion and proliferation, elongated triangular cell morphology | [76] |
| PGA, PLA, PLGA | Acrylic acid | Fibroblasts | Improved adhesion and spreading, increased cell number | [77] |
| PS | Isopropyl alcohol | Fibroblasts | Improved adherence, flatter cell morphology and increased cell density | [78] |

The table present a comprehensive overview of the substrates, the modification type, results on modified cell-material interactions

Table 3 Representative overview of plasma modification of 3D scaffolds and spatial control of cell attachment, together with the influence on cell-material interactions

| Scaffold | Modification | Cell type | Observations | References |
|------------------------|--|------------------------------|--|------------|
| <i>3D scaffolds</i> | | | | |
| PLA | Ammonia plasma | 3T3 fibroblasts | Improved cell attachment | [81] |
| PLA | Deposition of allylamine | 3T3 fibroblasts | Cell grow and attach inside the scaffold | [82] |
| PLA | Polymerized acylic acid | Chondrocytes | Improved attachment and proliferation | [83] |
| PLA | O ₂ plasma | Embryonic palatal mesenchyme | Better adherence, spindle-shaped cells with filopodia, cells inside the scaffold | [84] |
| PLA | O ₂ plasma | CHO | Increased attachment, no improved proliferation | [85] |
| PLA | RGDS immobilization | Osteoblast-like cells | Higher cell censities, bone-like tissues | [86] |
| PLLA | Gelatin anchoring | Chondrocytes | Better proliferation and ECM production, tissue-like cell constructs | [87] |
| PCL | Air plasma | Schwann cells | Improved proliferation | [88] |
| PCL | O ₂ plasma + fibronectin adsorption | 7F2 osteoblasts | Increased attachment and proliferation | [89] |
| PHBV | O ₂ plasma | Osteoblast | Adhesion and spreading inside scaffold | [90, 91] |
| Substrate | Modification | Cell type | Observations | References |
| <i>Spatial control</i> | | | | |
| PE | Air plasma | Pheochromocytoma PC-12 | Maximum adhesion at WCA 55°, typical neuronal morphology | [95] |
| PE | Air plasma | 3T3 fibroblasts | Maximum adhesion at WCA 55°, protruding fillopodia, flattened morphology | [96] |
| PE | Air plasma | CHO, endothelial cells | Maximum adhesion at WCA 55°, protruding fillopodia, flattened morphology | [97] |
| Glass | Polymerized hexane and allylamine | 3T3 fibroblasts | High cell density on allylamine side, low density on hexane side | [98] |
| Glass | Polymerized oxadiene and acrylic acid | Mouse embryonic stem cells | Cells attached better to hydrophilic region, improved differentiation, flat mololayered colonies | [99] |
| PS | Polymerized isopropyl alcohol | Fibroblasts | Cells attached preferentially to treated zones | [100] |

Table 3 continued

| Substrate | Modification | Cell type | Observations | References |
|------------|--|---------------------------------|--|------------|
| PS | Polymerized acetone | Fibroblasts | Cells attached preferentially to treated zones | [101] |
| PS | Polymerized n-hexane | CHO | Cells grow preferentially to untreated zones, aligned and elongated cells | [102] |
| PS | Deposition of PEO | Fibroblast | Alignment of cells along predefined directions | [103] |
| FEP | Polymerized acetaldehyde and deposition of PEO | Epithelial cells | Inhibition of cell growth on PEO coated regions, enhanced cell growth on acetaldehyde coated regions | [104] |
| Petri dish | Ar and acetylene plasma | Mammalian cervical cancer cells | Increased cell density, elongated cells | [105] |

The table presents a comprehensive overview of the substrates, the modification type, results on modified cell-material interactions

Nakagawa et al. [58] and Teraoka et al. [59] modified PLA surfaces with an atmospheric air plasma jet. After plasma treatment, the contact angle decreased from 80° to approximately 40°. X-ray photoelectron spectroscopy (XPS) indicated that oxygen-containing groups such as C–O, C=O and O–C=O were incorporated. Cell culture tests with mouse osteoblast-like MC3T3-E1 cells showed that both cell adhesion as well as cell proliferation could be improved with a plasma treatment.

Some authors have used ammonia plasma to modify PLA [60–63]. In a study by Chu et al. [60], the surface of PLA displayed a better proliferation of human umbilical vein endothelial cells (HUVEC) and rabbit microvascular endothelial cell (RbMVEC cells) after ammonia plasma treatment. After 7 days, an increased surface coverage by both animal and human cells was observed (see Fig. 3). The cell density increased from 4.8×10^2 HUVEC/cm² for untreated PLA to 8.11×10^4 HUVEC/cm² for plasma modified PLA; similar results hold for the RbMVEC. The authors state that ammonia plasma treatment leads to the incorporation of amine and amide groups on the substrate materials, of which the amines specifically interact with the cells through ionic bonding with acidic groups of N-acetylneuraminic acid on the surface of the cell membrane. According to the authors, also a more hydrophilic surface can contribute to a better attachment of cell binding proteins. In the study of Chu et al., no results are available on the type and amount of incorporated groups nor on the change in wettability of the samples after plasma treatment. Jian Yang et al. [61], Gugala et al. [62] and Wan et al. [63] also used ammonia plasmas to modify the surface of PLA, and observed an improved cell attachment of mouse 3T3 fibroblasts and rat osteoblasts. The fibroblasts appeared spindle shape, were evenly distributed and very well stretched [61]. From chemical analyses performed, it was found that both nitrogen and oxygen containing functionalities were incorporated, leading to an increased wettability, and thus a better cell attachment [61]. Wan et al. [63] clearly showed that the attachment of cells was better on treated samples, by placing the samples under shear stress conditions: on treated samples, more cells stayed attached.

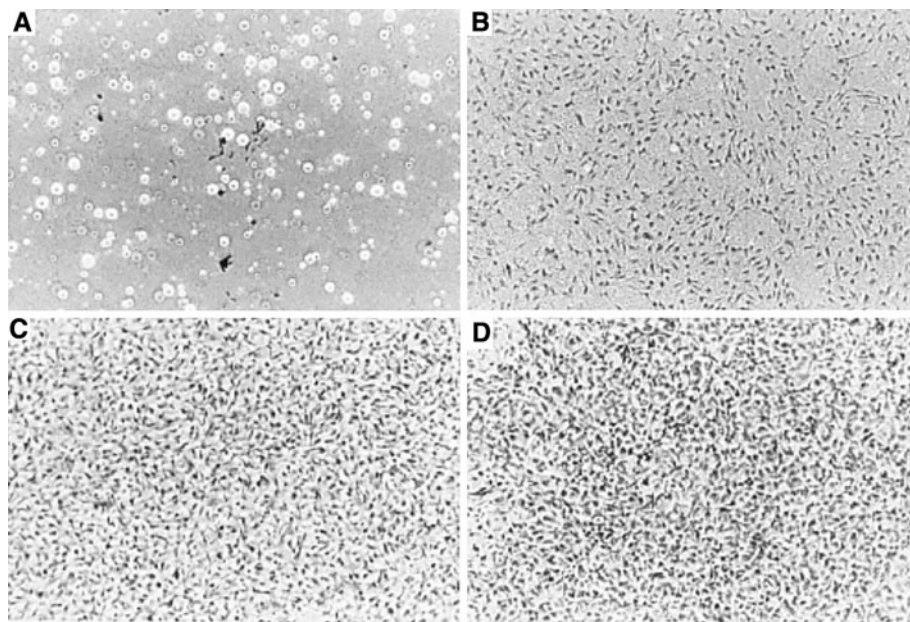


Fig. 3 Photomicrographs of HUVEC grown on various PLLA substrates. HUVEC were plated on various PLLA substrates at a density of 2.5×10^4 cells/cm². After 7 days, samples were fixed with 4 % glutaraldehyde and stained with 0.1 % toluidine blue. **a** Control PLLA; **b** Fn-coated control PLLA; **c** modified PLLA; **d** Fn-coated modified PLLA ($\times 100$) [167]

Besides ammonia plasma treatment, also sulfur dioxide plasma treatment of PLA has been investigated in [62]. The authors found that cell attachment was decreased and conclude that this is due to the—SH groups present at the surface which make it resistant to nonspecific adsorption of proteins. This, in turn, diminishes the attachment and proliferation of cells. These results indicate that the plasma gas can have a great influence on the cell attachment.

Besides PLA, also PCL and PLGA are commonly studied with respect to plasma treatment to improve cell-material interactions. By using an atmospheric pressure DBD oxygen plasma, Yildirim et al. [64] were able to decrease the water contact angle of PCL samples from about 80° to about 35° and to increase the surface roughness. The cell proliferation rate of mouse 7F2 osteoblasts on plasma-treated samples increased 90 % in comparison with untreated samples. A confluent cell layer was observed on plasma-treated samples, in contrast to untreated surfaces where cells were hardly spread out.

Lee et al. also used an atmospheric pressure DBD operating in air to modify PCL films [65]. Similarly, they found an increased surface wettability and an increased surface roughness. By FT-IR spectroscopy and XPS, a higher amount of oxygen containing hydrophilic groups (C—O, COOH, C=O and OH) could be detected on the plasma-treated films. The cell attachment and proliferation of human prostate epithelial cells (HPECs) was found to be ten times better on plasma-treated PCL films compared to untreated film. The authors suggest that the proteins of the cell membrane, which contain hydrophilic amino acids, possess a better affinity towards the hydrophilic surface of the plasma-treated films.

In another study [66], the same authors used different gas mixtures for plasma treatment and determined the effect on surface wettability, - morphology, - chemistry and cell

attachment. When Ar + H₂ was used as a discharge gas, the contact angle was found to increase after treatment, while the surface became smoother. Opposite results were found for Ar + N₂, Ar and Ar + O₂. For the Ar + H₂ treated samples, more CH₂ and CH₃ functional groups and less oxygen containing groups were detected at the surface compared to the untreated samples whereas for the Ar + N₂, Ar and Ar + O₂ treated samples, more C=O, COO and NH- groups were detected. To determine the influence of each gas plasma treatment on cell material interactions, the authors studied the cell attachment and proliferation of HPECs on the various samples. After 12 h of culture, cell attachment increased from 32 % on the pristine films to 76 % for the Ar + O₂ plasma-treated film. Also for Ar and Ar + N₂, the cell attachment increased, however for Ar + H₂, cell attachment decreased to less than 20 %. Moreover, the number of cells after 7 days of culture decreased for Ar + H₂ treated samples to 1×10^5 cells/ml compared to 2.75×10^5 cells/ml for untreated samples. For Ar + O₂ treated samples, this number was increased to 1.82×10^6 cells/ml. This clearly indicates the better cell proliferation on Ar + O₂ plasma-treated films. The authors concluded that the incorporated hydrophilic groups play an important role in enhancing the cell-material adhesion strength. The main reason is that the protein of the cell membrane, hydrophilic amino acids, is present in the outer region of the membrane. The increased affinity between the protein and the PCL surface, caused by the hydrophilic properties of the Ar + N₂, Ar and Ar + O₂ plasma-treated surface, improves the extent of cell attachment.

In [56], Khorasani et al. plasma-treated besides PLA also poly(lactic-co-glycolic acid) (PLGA) with an RF plasma in oxygen at low pressure. The cell adhesion improved, however to a lower extent than for the PLA films. Similar to Khorasani et al. [56], Hasirci et al. used an RF oxygen plasma to modify the surface of PLGA films [67]. In addition, Wan et al. have used an oxygen plasma to treat PLGA films [68]. Both research groups found an increased concentration of oxygen containing groups (C–O, COOH, C=O, C–O–C=O), leading to an improved hydrophilicity, and an increased surface roughness. It was also observed that 3T3 mouse fibroblasts could attach better to plasma-treated PLGA [67]. On the untreated films, the cells were observed as aggregates most probably due to a weak spreading of the initially added drop of cell suspension on the hydrophobic surface. In contrast on the treated films, the borders of the attaching cells could be easily seen. Wan et al. studied the cell detachment of mouse 3T3 fibroblasts from the samples under shear stress. For untreated samples, cell detachment rates were higher than for the plasma-treated samples. After 60 min of applied shear stress, 90 % of the cells were still attached to the surface of the plasma treated samples. For untreated samples however, the cells detached completely within 10 min, clearly indicating the improved cell adhesion after plasma treatment.

In another study, PLGA films were subjected to different physicochemical modification techniques, including air plasma and corona discharge treatment, before different cell types (hepatoma (Hep G2), osteoblast (MG 63), bovine aortic endothelial cells (CPAE), fibroblast (NIH/3T3)) were cultured on the surfaces obtained [69]. After plasma treatment, the water contact angle decreased from 73° to 52°, and the O1 s/C1 s ratio increased from 0.46 to 0.65. The cells adhered better on the surface-modified PLGA samples regardless of the cell type. Moreover, the cell morphology was different on the treated PLGA than on the pristine PLGA: the cells had protruded filopodia and lamelliopodia that spread out and flattened more (see Fig. 4). After 2 days of culturing, the cells were almost flattened on the plasma-treated samples, whereas the untreated samples still showed round cell morphology, indicating poor cell attachment.

Besides air and oxygen, also the effect of ammonia plasma treatment on PLGA has been investigated [70]. Electrospun PLGA nanofiber matrices were treated with an ammonia glow discharge plasma. The contact angle of untreated nanofibers was approximately 140°,

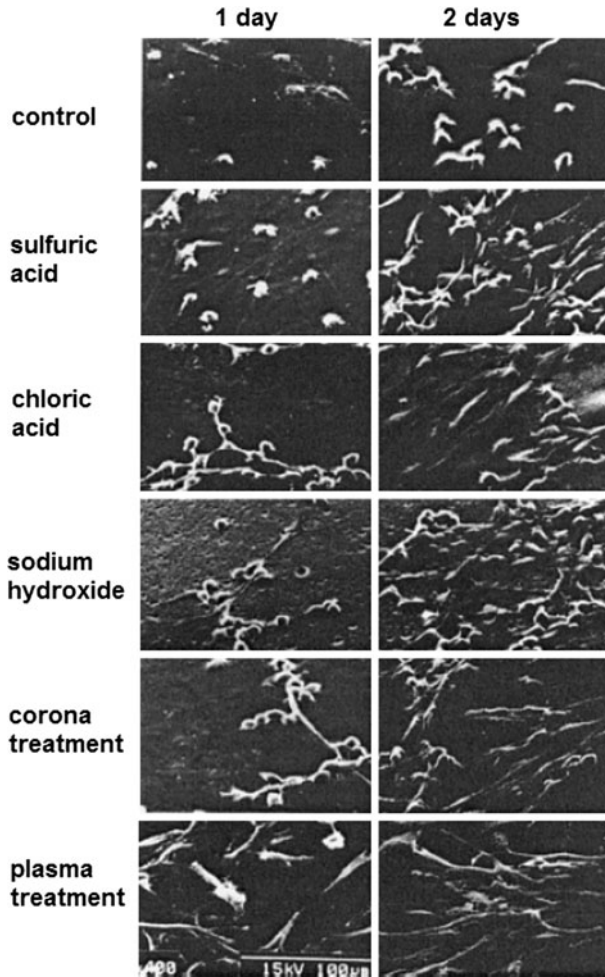


Fig. 4 SEM microphotographs of fibroblast cells attached to physicochemically treated PLGA surfaces after 1 and 2 days of culturing (original magnification: $\times 400$) [69]

while after plasma treatment of 30 s, 60 s and 180 s, the contact angle decreased to 53° , 51° and 47° , respectively. However, only a small nitrogen content of 1, 2 and 3 % was detected after plasma treatment of 30, 60 and 180 s, respectively. Mouse 3T3 fibroblasts, seeded on the plasma-treated PLGA samples, could adhere better and spread out more thus occupying a larger surface area than cells on non-treated matrices. However, for matrices treated longer than 60 s, the cell attachment and viability decreased. This finding indicated that an optimum concentration of N-containing functional groups such as amines might be essential for cellular adhesion and spreading, as hydrophilicity of plasma-treated nanofiber matrices used in this study was almost constant.

Some studies reported on the cell attachment after plasma treatment of the a 3-hydroxybutyrate-3-hydroxyvalerate (PHBV) copolymer [71–73]. PHBV surfaces were treated with an RF plasma operating in oxygen [71, 72]. Both studies showed an increased

hydrophilicity caused by a higher oxygen content at the surface after treatment. Both dog bone marrow stromal cells [71] and human retinal pigment epithelium D407 cells [72] could attach and proliferate better on treated surfaces. More recently, RF plasma treatment of PHBV in oxygen, nitrogen and argon was studied by Garrido et al. [73]. After plasma treatment, the surface became more hydrophilic, indicated by the lower water contact angle. The water contact angle decreased from 73° for untreated samples, to approximately 55° after 20 s of treatment, independent of the discharge gas. Only for oxygen plasma treatment, a longer treatment time led to an even lower contact angle value of about 49°. It was also observed that the chemical composition of the surface after treatment depended on the applied gas: oxygen plasma led to the incorporation of C–O, nitrogen led to the incorporation of C=N and C≡O groups. For argon plasma, more C=C bonds were detected. Non-transformed, immortal human keratinocytes (HaCaT) were seeded on the surface of PHBV films. The results showed that cells attached better to oxygen and argon treated samples than to nitrogen treated samples, which still showed better results than the untreated film. The attached cells had a flattened appearance. Surprisingly, the best cell adhesion was found on samples treated for 10 s, while samples treated for 90 s showed a much lower cell adhesion. The authors suggest that after the initial decrease of hydrophobicity, the chemical functionality of the surface plays an important role, more specifically the presence of unsaturated bonds after treatment.

Pompe et al. used an ammonia and a water vapour plasma to modify the surface of poly(hydroxybutyrate) (PHB) films to influence cell adhesion [74]. XPS analysis showed that oxygen was built in for water vapour plasma treatment and nitrogen for ammonia plasma treatment. The cell culture tests with HUVECs showed that on NH₃ plasma-treated films, the cells exhibited a flat monolayer morphology, while on H₂O plasma-treated surfaces the formation of capillary-like networks was observed with an elongated and branched pattern of the cells assemblies (see Fig. 5).

Qu et al. treated copolymers of 3-hydroxybutyrate and 3-hydroxyhexanoate (PHBHHx) with an ammonia plasma [75]. The contact angle decreased from 82° to 68°, and oxygen (C–O, C=O) and nitrogen (C–N) groups were incorporated on the surface. Both HUVECs and rabbit aorta smooth muscle cells (SMCs) were used for cell culture tests. The HUVECs grew well on the plasma treated PHBHHx film, however, there was no significant difference in cell proliferation between treated and untreated films when SMCs were seeded on the films. The HUVECs were evenly distributed and spread on treated films in contrast to the untreated films. The SMCs, on the other hand, were flat and well spread on both untreated as well as treated samples. This might indicate that the effects of surface properties on SMCs are not as pronounced as on HUVECs.

The polymer blend poly(ethylene glycol)-terephthalate-poly(butylene terephthalate) (PEGT/PBT) has also been treated with an RF plasma operating in argon [76]. Expanded human nasal chondrocytes were seeded on untreated and plasma treated PEGT/PBT films. The plasma treatment led to an increased cell number. Also, the cells exhibited a spread morphology and pseudopodia formation. However, the re-differentiation capacity of chondrocytes was markedly reduced. The authors therefore concluded that for clinical cartilage tissue engineering strategies relying on post-expansion re-differentiation of expanded human chondrocytes, gas plasma treatment may not be a suitable surface modification technique.

From this overview, it is clear that the plasma surface modification of biomedical polymers can have a significant influence on the cell-material interaction. However, the basic understanding of the mechanisms of cell adhesion are still not well understood. To be able to explain and comprehend how cells interact with the (modified) material is crucial to

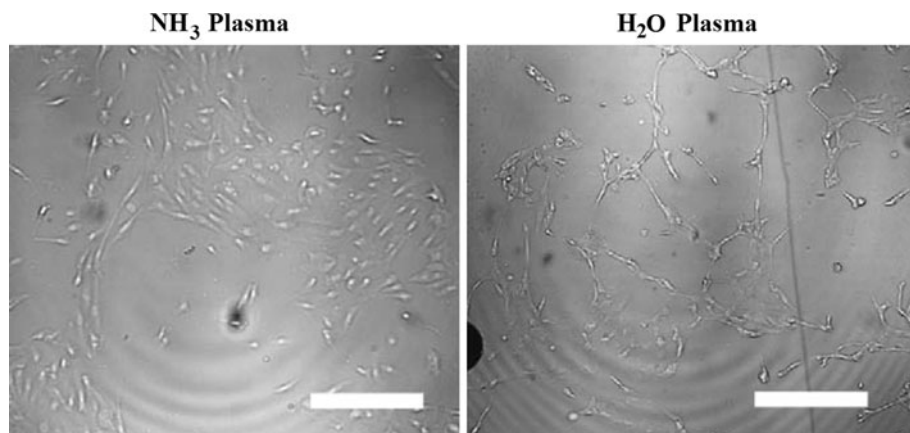


Fig. 5 Endothelial cell morphology after 5 days of cell culture on P(3HB) samples visualised by differential interface contrast demonstrating a dense packing and flat morphology on NH_3 plasma-treated samples (and on untreated samples, not shown) and frequent occurrence of capillary-like network formation on H_2O plasma-treated samples (scale bar: 250 μm) [168]

adapt the modification process to the best possible standards. Some studies, like [60] from Chu et al. and [65, 66] from Lee et al., discuss some cell-material interaction mechanisms, but further research on this matter is required. In [70, 73], the role of the implanted chemical groups on the cell attachment is discussed. Some authors also discuss the influence of plasma surface treatment on surface roughness and consequences for cell adhesion [64, 65, 67, 68]. In [77], it is proven that the surface roughness has a considerable influence on cell attachment. However, as Yildirim points out in [64], a detailed understanding of the interrelationship between particular surface properties, such as chemical composition or roughness, and cell attachment needs further research.


Most studies focus on cell numbers, shape and morphology, since they are rather easy to evaluate. They are important parameters to consider, but also cell re-differentiation, see for example the paper of Woodfield et al. [67], is for some applications also important. The intended application will not only determine which of these factors are important to take into consideration, but will also impose the needed surface properties. Most of these applications are very specific, so that probably tailor-made solutions will be necessary.

Plasma Polymerization and Grafting

Plasmas can not only be used for the introduction of chemical groups, it is also suitable for the covalent immobilization or grafting of bioactive molecules and for polymerization of different monomers. When cells reach the modified surface, they sense the grafted molecules and will interact with them rather than with the underlying surface. The main advantage of this approach is that the applied surface modification strategies are less or not affected by ageing.

The covalent immobilization of collagen on PCL surfaces by a post-irradiation technique and the influence on cell adhesion and proliferation has been widely investigated [78–81]. A schematic representation of this process is given in Fig. 6. A plasma treatment is used as a pre-treatment step, before acrylic acid is grafted onto the surface by UV-induced grafting. The carboxylic acids groups introduced were activated by exposure to a

Fig. 6 Schematic representation of the immobilization of collagen on PCL films

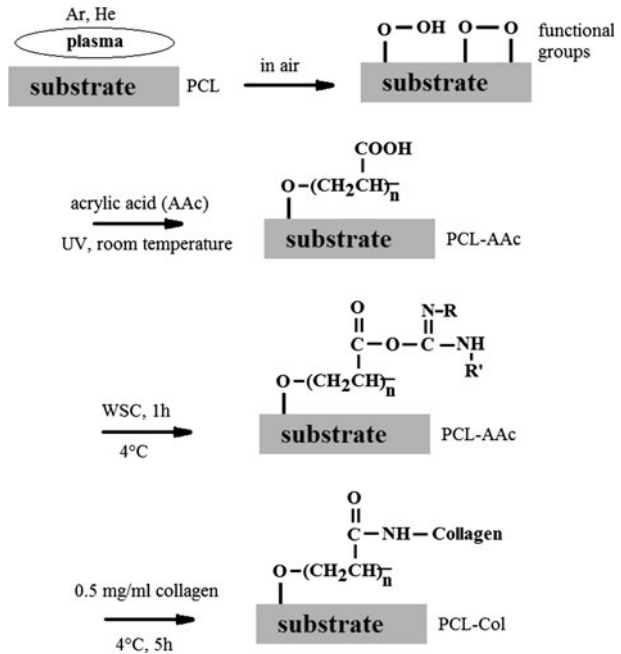

water-soluble carbodiimide followed by collagen enabling the biopolymer immobilization onto the surfaces.

Chong et al. seeded the collagen-modified PCL films with human coronary artery smooth muscle cells and found an increased cell number on the modified films and observed that the cells spread out more to adopt spindle-like morphologies compared to the untreated films [78]. They found no degradation in mechanical properties due to the surface modification. Human dermal fibroblasts (HDFs) and human myoblasts also elongated and flattened to a spindle morphology, indicating an improved attachment to the surface, and proliferated better covering the entire surface of PCL collagen immobilized films after 8 days of incubation [79]. Similar results were found by Foo et al. for HUVECs [80].

Besides the covalent immobilization of collagen, the immobilization or grafting of other biomolecules like insulin, chitosan, gelatin, Arg-Gly-Asp (RGD) or Arg-Gly-Asp-Cys (RGDC) has been pursued leading to a better cell-material interaction [81–84]. Insulin functionalization of PHBV lead to an increased cell proliferation of human fibroblast cells and full cell spreading on the surface [81]. By using a spacer arm bNH₂PEG (O,O'-bis-(2-aminopropyl)-polyethylene glycol 500), the RGDC peptide could be immobilized on the surface of acrylic acid grafted poly(tetrafluoroethylene) (PTFE) [82]. The attachment level of HUVECs was observed to be four times higher for the modified polymer than for the non-modified one. However, the authors could not confirm whether this trend was related to a specific cellular recognition mechanism or to the increase of wettability of the modified sample. The RGD peptide immobilization on an acrylic acid (AA) thin film layer on Ti surfaces has an effect on osteoblastic differentiation of MC3T3-E1 cells and has a potential use in osteo-conductive bone implants [83]. Gelatin immobilization was found to enhance cell adhesion, spreading and focal adhesion formation and proliferation of HUVECs on PLLA surfaces, as shown in Fig. 7 [84].

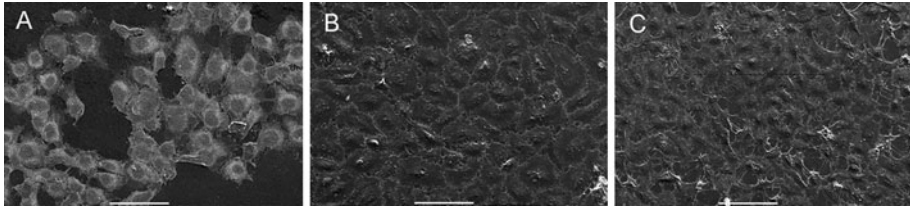


Fig. 7 Cell morphology observed on **a** PLLA, **b** PLLA-gAA-gelatin, and **c** PLLA-gAA-chitosan by SEM at day 7. Complete endothelialisation was observed on both modified PLLA substrates, but not on PLLA substrate. Scale = 100 μ m [169]

Duan et al. used a post-irradiation technique for collagen immobilization on PCL nanofibrous mats [85]. The pristine PCL nanofibers were smooth and beadless, while the surface of collagen-coated fibers became rough and thick due to the coating layer and possessed an increased wettability. The proliferation of primary HDFs was increased and a confluent layer of long, bipolar, spindle-shaped layer was formed. Also, a number of discrete filopodia-like protrusions between the cells and collagen-coated fibers were observed, indicating good interaction between the cells and the scaffold. The cells were found to migrate through the pores of nanofibers, which was not observed for the pristine fibers.

Besides the covalent immobilization, some authors have been immersing plasma pre-treated biomedical polymers into protein containing solutions leading to non-covalent linking of proteins to the surface. Although these proteins can be easily removed, they also lead to a better cell attachment and proliferation onto the modified surface [86–89]. The anchorage of collagen on PLGA leads to a better cell attachment, spreading and viability of mouse NIH 3T3 fibroblasts [86]. On PLA, the anchorage of collagen could lead to an increased cell number and a better attachment of 3T3 fibroblasts [87]. He et al. used a nanofiber mesh out of the co-polymer poly(L-lactide acid)-co-poly(ϵ -caprolactone). Upon collagen coating, the cell spreading, viability and attachment of human coronary artery endothelial cells onto the mesh was enhanced [88].

In a study by Ding et al., the plasma syn-irradiation technique was used to immobilize chitosan onto PLA films [90]. The two cell types they used for cell culture tests (L929 mouse fibroblasts and L02 human hepatocytes) showed a poor cell adhesion and hardly spread, but they proliferated at the same speed as cells cultured on glass.

The plasma polymerization technique has also been investigated by many authors [91–95]. It can be used to coat the substrate rather than covalently bind species. Guerrouani et al. plasma polymerized allylamine onto PLA surfaces [91]. Microorganisms such as euglypha and vorticella formed a dense biofilm. Carlisle et al. used PLLA and PCL plasma polymerized with allylamine to link cell adhesion peptides polyethylene glycol (PEG) to the polyester surface [92]. These surfaces were found to significantly increase hepatocyte cell adhesion from 31 to 53 % on PCL surfaces and from 42 to 76 % on PLLA. Allylamine can also be plasma polymerized on a silicone elastomer to improve the biocompatibility [93]. Cell culture tests with human skin fibroblasts showed that the cells attached and proliferate better onto the modified elastomer. The cell shape changed from round shape to an elongated triangular morphology.

Besides allylamine, acrylic acid can also be plasma polymerized on biocompatible polymers to improve cell material interaction. When acrylic acid is deposited onto polyglycolic acid (PGA), PLA or PLGA, the adhesion and spreading of fibroblasts was enhanced [94]. Also the total cell number increased. Mitchell et al. used an isopropyl

alcohol (IPA) plasma to modify polystyrene surfaces [95]. Fibroblasts adhered and proliferated to a higher extent on the modified samples. The cells showed a flatter morphology and cell densities increased tenfold upon incubation for 72 h.

For plasma grafting and plasma polymerization, the same conclusions about the importance of knowledge of cell-material interaction can be made than for the previous chapter about plasma treatment. The main difference with plasma grafting or plasma polymerization is that the cell-material interaction can be mimicked to comply with the normal in vivo cellular recognition mechanisms. By grafting the appropriate bioactive molecules, the cells will ‘sense’ these molecules as a biological environment and not the foreign surface. As a result, the normal cell responses for adhesion can be triggered. An important factor is the graft density, which also depends on the size of the biologically active molecules which are immobilized [96, 97]. Often, achieving a higher graft density is not always necessary or even beneficial to achieve a better cell-material interaction [98]. This indicates that the graft density should be carefully monitored and optimized.

Use of Plasma Modification Techniques for Specialized Purposes

3D Scaffolds for Tissue Engineering

The development of 3D porous scaffolds is crucial for the final success of tissue engineering approaches. Since cells without their native ECM do not enable three dimensional tissue growth, administering cells alone is not adequate in large size defects [2]. The design of an artificial ECM to induce tissue regeneration by allowing cells to adhere and proliferate is thus essential [99]. Cells seeded on the scaffolds and from the native surrounding penetrate the porous scaffold, adhere and start to proliferate. During these processes, natural ECM is being synthesized. It is desirable to have scaffolds that produce a minimal immunogenic reaction, since this leads to failure of the implant. Hence, adhesion of cells on the scaffolds and the overall biocompatibility of the implant are key issues [100]. Moreover, in some cases the ingrowth of blood vessels should also be promoted, as cells need sufficient nutrients to grow and proliferate and the possibility to drain waste products [100]. The modification of 3D scaffolds is more complicated than for 2D surfaces, such as films. For a proper functioning of the implant, a homogeneous scaffold modification is essential since cells need to adhere and proliferate at all scaffold parts. Similar to the treatment of 2D surfaces, many authors have studied the plasma modification of 3D structures and their influence on cell adhesion.

In this respect, PLA has been widely studied [101–106]. Fibroblasts were grown on PLA scaffolds modified by ammonia plasma [101] and by allylamine grafting [102]. In both studies, an improved cell attachment was observed. By the depositing allylamine onto the porous PLA scaffold, cells homogeneously populated the scaffolds after only 24 h of cell culture [102] (see Fig. 8). This was not observed after the grafting procedure. According to the authors, this was due to the lower nitrogen content on the surface. Also the graft polymerization of acrylic acid lead to a better chondrocyte adhesion and proliferation on 3D PLA scaffolds [103]. Chim et al. used a pure oxygen glow plasma treatment, and found that human embryonic palatal mesenchyme cells adhered better to treated scaffolds: the cells adopted a spindle-shape morphology with filopodia aiding attachment [104]. Confocal laser micrographs revealed an increased cell density throughout the scaffold. Cell aggregates were observed, with confluent cell sheets by day 10. Oxygen plasma treatment also had a positive effect on the cell attachment of Chinese hamster ovary (CHO) cells on PLA membranes [105]. Not only was the percentage of adherent cells

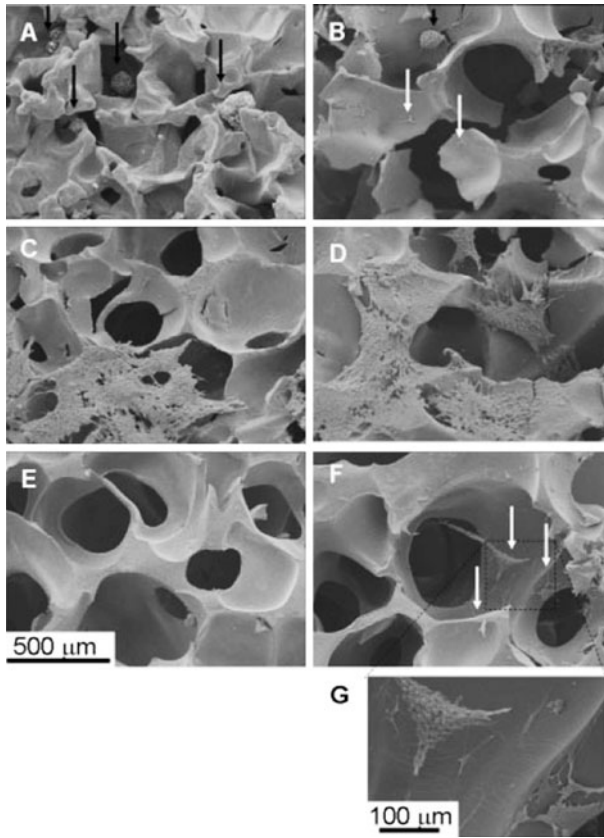


Fig. 8 SEM images of murine 3T3 fibroblasts cultured for 24 h on **a** unmodified P_DL_A; **b** allylamine-grafted P_DL_A, and **c** 3 W and **d** 20 W plasma-polymerized allylamine-deposited surfaces. Images **a–d** are from the outer surfaces of the scaffold, while **e**, **f** are representative of the unmodified/grafted (**e**) and plasma-polymerized 3W(**f**) inner surfaces. All images are the same magnification. Images (**e**, **f**) were taken from approximately the middle of the diameter of the sample. In all images, the *white arrows* denote cells that have assumed characteristic fibroblast morphology, while the *black arrows* denote cells that have not. **g** Higher-magnification image of **f** showing cells adhering to the modified P_DL_A surface [102]

greatly increased by plasma treatment, also the cells spread out resulting in sheet like formation. However, cell proliferation was not improved by plasma treatment. Ho et al. used the immobilization of RGDS (Arg-Gly-Asp-Ser) peptides to promote the cell growth of rat osteosarcoma osteoblast-like cells on porous PLA scaffolds [106]. Cell attachment was promoted, resulting in higher cell densities while the cells were found to form bone-like tissues, indicated by the deposition of calcium salts. The authors were able to uniformly immobilize the RGDS inside the scaffold, however they did not investigate whether cells were able to attach and grow inside the scaffold. The anchoring of gelatine by oxygen plasma pretreatment on PLLA nanofibers led to a better cell proliferation of chondrocytes and ECM production [106]. Moreover, the seeded cells grew into tissue-like constructs.

Some authors reported on plasma modification of PCL and PHBV scaffolds. Air plasma treatment of porous nanofibrous PCL scaffolds led to a better cell proliferation [108], and a combined oxygen plasma modification followed by fibronectin adsorption has shown to increase cell attachment and proliferation of 7F2 mouse osteoblasts [109]. The influence of

oxygen plasma treatment on PHBV foams was studied by Köse et al. [110, 111]. They showed that adhesion and spreading of osteoblasts inside the foams structure could be improved, and interconnections between cells were observed indicating that PHBV matrices could have a potential in bone tissue engineering.

Spatial Control of Cell Adhesion

Instead of a uniform surface modification, several authors investigate the creation of so called gradient or patterned surfaces on biodegradable polyesters by plasma modification techniques. On a gradient surface, the chemical composition (or another surface characteristic such as roughness, wettability, etc.) gradually varies along one dimension. Such a surface is of great interest for studies on the interactions between biological species and surfaces, as the dependence of the surface property on this interaction can be examined in a single experiment on one surface [112]. It is a simple and fast method for investigating optimal surface conditions for cellular responses such as attachment and growth. In this subsection, we will focus on the interaction of cells with these gradient surfaces, information on preparation of such surfaces can be found in other excellent reviews in the field [112, 113].

On a patterned surface, the chemical composition is different from one region of the surface to another, thus creating a pattern. Depending on the chemical composition, the cell adhesion will be either promoted or reduced. In this way, the cells are ‘guided’ to grow in a specific pattern on the surface. One can correctly align and position cells by providing the proper (chemical) cues, which offers numerous possibilities for tissue engineering [114].

Lee et al. [115], Choe et al. [116] and Lee et al. [117] used an air corona discharge treatment from a knife-type electrode whose power gradually increases along the sample length to create a wettability gradient on polyethylene (PE). The water contact angle of the PE surface was shown to gradually decrease along the sample length from 93° to 43°. When 3T3 fibroblasts were seeded on the surface of such samples (see Fig. 9) they found that the cells grew significantly more on the positions with moderate hydrophilicity (i.e. water contact angle about 55°). In addition, on this position more cells with protruding filopodia and lamellipodia and with flattened morphology were observed [116]. Also CHO cells and bovine pulmonary artery endothelial cells were found to adhere better to regions of moderate hydrophilicity and similar observations regarding cell shape were found [117]. Rat pheochromocytoma PC-12 cells appeared to have maximum adhesion to the gradient surface where the water contact angle was about 55° [115]. As the surface wettability increased along the sample length, the adhered cells were induced to differentiate into cells with typical neuronal morphology. The maximum number of neurites of the PC-12 cells on the PE surfaces appeared at the position with a contact angle of 55°. Higher hydrophilic position showed no further increase of neurites.

Zelzer et al. [118] and Wells et al. [119] used a plasma polymerization technique of hexane combined with allylamine and octadiene with acrylic acid respectively to produce gradient surfaces. On the hexane (hydrophobic) side of the sample, 3T3 fibroblast were hardly adhering, while on the allylamine (hydrophilic) side, the cell density was high [118]. Also, a gradually varying cell density was observed along the gradient surface from one side to the other. Also plasma polymerization of octadiene combined with acrylic acid lead to a wettability gradient caused by a gradient in acid (COOH) functionalities [119]. Mouse embryonic stem cells were found to adhere better on the hydrophilic side of the gradient. On these regions, the cells appear to form flat monolayered colonies where many cells are differentiated.

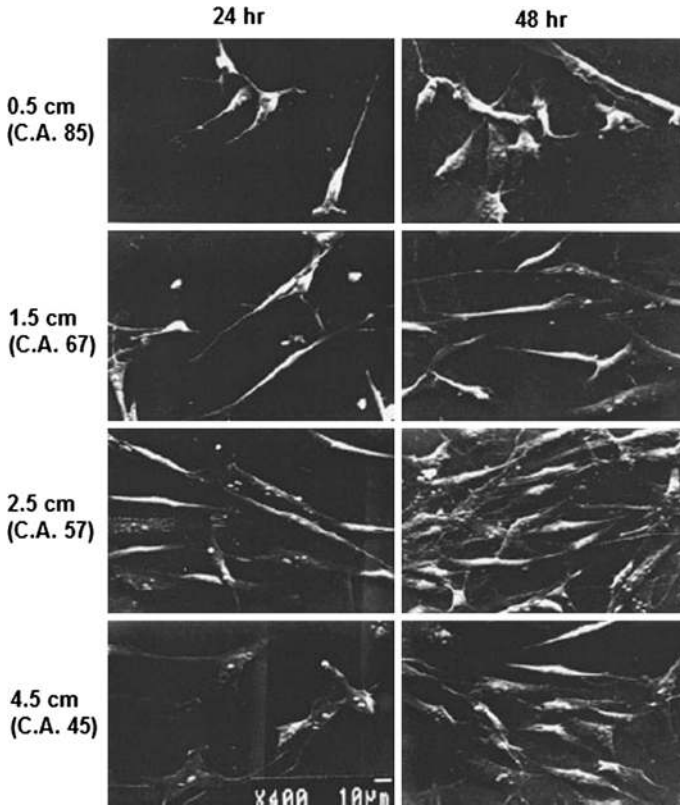


Fig. 9 SEM pictures of the fibroblast cells adhered on wettability gradient PE surfaces after 24 and 48 h of culture (original magnification: $\times 400$). CA: water contact angle (degrees) [116]

Several authors also studied the creation of patterned surfaces on polystyrene (PS) by combining plasma polymerization with a simple masking technique [120–123]. By placing a transmission electron microscope (TEM) grid on the surface during plasma exposure, a patterned surface could be created. Human fibroblast cells grown on such a patterned surface created with isopropyl alcohol plasma [120] or acetone plasma [121] preferentially attach to the unmasked, hydrophilic, treated zones. After longer incubation times, when the treated areas have become nearly confluent, cells also begin to spread onto the untreated areas. HCO cells were found to preferentially grow on the untreated areas of a patterned surface created with n-hexane plasma polymerization [122]. The cells were also found to spread preferentially in the direction of the untreated surface, resulting in aligned and elongated cells. Sardella et al. deposited patterned PEO-like coatings, and found that fibroblast cells would not adhere to PEO regions deposited at low power, and they could thus create a cell pattern onto the PS surface and induce the alignment of cells along predefined directions [123].

Thissen et al. used a similar technique to deposit a patterned surface of acetaldehyde plasma polymer adhesive regions and PEO non-adhesive regions onto perfluorinated poly(ethylene-co-propylene) (FEP) to precisely control the outgrowth of bovine corneal epithelial tissue on the surface [124].

By using an atmospheric pressure plasma jet operating in argon and acetylene, a patterned polymer film could be deposited onto a petri dish surface [125]. After 4 h of inoculation, mammalian cervical cancer cells showed cell alignment on the edge of the organic film, and these cells were more elongated. On the plasma polymer film, the cell density increased twofold over the next 48 h.

By combining the spatial control of cell adhesion with 3D scaffolds, the basis of tissue engineering can be developed. In this respect, the results obtained by Chim et al. [104], Yamaguchi et al. [105], Chen et al. [107] and Wells et al. [119] concerning the observation of so-called cell sheets or cell layers and tissue like constructs is very promising. Moreover, the differentiation of cells was also detected by Wells et al. [119]. This shows that the cells exhibit abilities to form tissues on the modified biomedical polymers.

Antibacterial and Antifouling Surfaces by Plasma Surface Treatment

In this last part, antibacterial and antifouling surfaces, obtained by plasma techniques, will be discussed. Antibacterial refers to the prevention of bacterial adhesion, whereas antifouling refers more generally to the prevention of attachment large molecules, microorganisms and cells. As mentioned before, the prevention of bacterial and protein adhesion is needed in many applications, such as medical implants, intraocular lenses, catheters and blood contacting materials [8, 9]. When an implant is placed into the body, both cells of the surrounding tissue as well as bacteria present compete to attach to the surface. This process is called the ‘race for the surface’ [126]. If the tissue cells win the race, the surface of the implant is covered by tissue. But if the race is won by bacteria, the surface will be covered by a biofilm and an inflammatory reaction may be the consequence and removal of the implant may be necessary [127, 128]. Excellent reviews on the mechanisms of bacterial adhesion can be found in [126, 129, 130].

For blood contacting materials, like heart-valve or vascular prosthetics, the adhesion of platelets and fibrinogen should be prevented, since this can lead to the formation of a thrombus (blood clot).

First, an overview of research dealing with antibacterial surfaces created by plasma techniques will be given. Afterwards, antifouling surfaces will be discussed, and how blood compatibility can be improved by preventing protein adhesion.

Antibacterial Surfaces


Several groups have studied plasma created antibacterial surfaces of medical grade PVC to be applied as endotracheal tubes [131–136]. An oxygen glow discharge has been used to modify small coupons of PVC to prevent the adhesion of several *Pseudomonas aeruginosa* strains [131, 132]. The treatment made the surface more hydrophilic, and a 57–70 % reduction in bacterial adhesion was observed. This reduction is believed to be attributed to the incorporation of oxygenated functional groups. The authors stated however that it is unlikely that the effect will be sufficient to delay or prevent biofilm formation. Therefore, the same authors also combined the oxygen glow discharge with an NaOH/AgNO₃ incubation for the treatment of PVC [133]. Using this technique, they found a complete reduction in bacterial adhesion, and the biofilm formation could be reduced. According to the authors, the silver content is essential to provide anti-bacterial properties to the surfaces.

Asadinezhad et al. used plasma co-polymerization of acrylic acid followed by irgasan [134] and benzalkonium chloride, bronopol or chlorhexidine coating [135] to modify PVC surfaces (see Fig. 10). The irgasan coating was capable of inhibiting bacterial growth of *S. aureus* and *E. coli* bacteria; however, it was unable to hamper bacterial adherence and biofilm formation after 24 h culture [134]. Benzalkonium chloride and bronopol coatings were able to reduce the *E. coli* adhesion (85 % resp. 75 %), but no reduction was observed in adhesion of *S. aureus* for both coatings [135]. The chlorhexidine was found to be effective against both bacteria: a reduction of 50–60 % in the adhesion was observed [135].

Oxygen plasma pretreatment, followed by triclosan or bronopol coating and a argon plasma ion bombardment has also proven to give antibacterial properties to PVC surfaces [136]. Triclosan was able to reduce the number of active *S. aureus* and *E. coli* bacteria with 82.2 % resp. 79.5 % compared to the untreated PVC. For bronopol, the reduction was 98 % resp. 77.3 %.

The combination of a plasma treatment followed by a deposition, coating or grafting of a polymer or other molecule, is a rather common technique. The grafting of poly(ethylene glycol) (PEG) has proven to effectively reduce the adherence of *S. aureus* bacteria, as shown in Fig. 11 [137]. When this PEG layer was end group functionalized with RGD-peptide, fibroblast and osteoblast attachment was enhanced, while bacterial adhesion was still greatly reduced. The plasma pretreatment of poly(methyl methacrylate) (PMMA) followed by a TiO₂ coating gives the PMMA surface bactericidal properties caused by TiO₂ photocatalysis [138], while the grafting of N-vinyl-2-pyrrolidone onto plasma treated nonwoven polyethylene terephthalate PET restrained *S. aureus* bacteria from growing onto the nonwoven [139]. Another example of this technique is the coating of PS with polysaccharides alginic acid and hyaluronic acid, which leads to an adhesion reduction of *S. epidermidis* and *E. coli* bacteria [140].

Fig. 10 Chemical structure of irgasan, bronopol, chlorhexidine and benzalkonium chloride

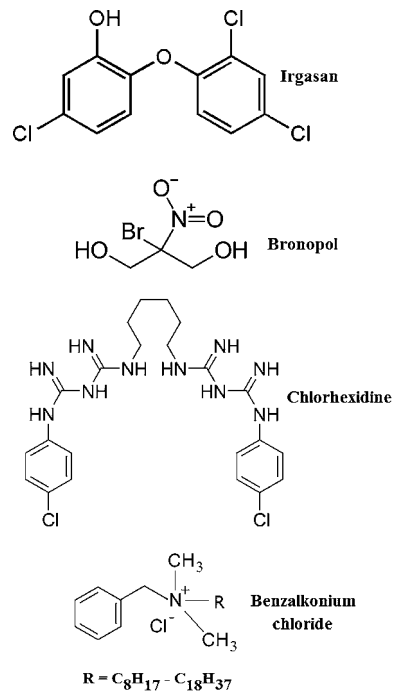

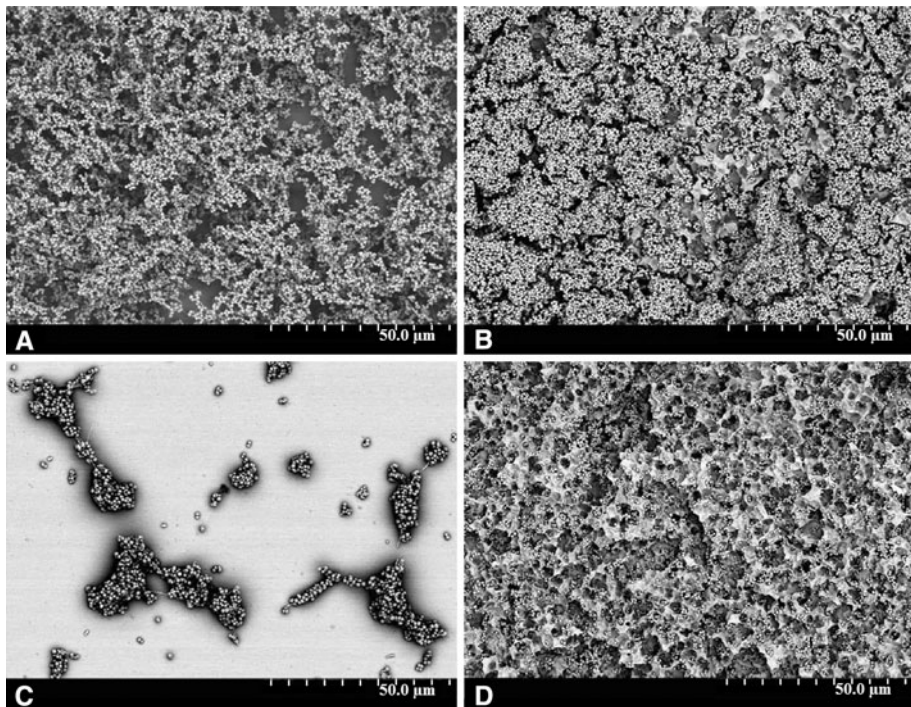


Fig. 11 BSE images of *S. aureus* cultured on the different surfaces for 4 h at 37 °C: **a** Ti (smooth), **b** Ti (rough), **c** Ti (smooth)-PEG, and **d** Ti (rough)-PEG. A confluent layer of *S. aureus* is observed on the Ti (smooth) and Ti (rough) surfaces. Less bacteria are seen on the Ti (smooth)-PEG surface, whilst bacteria are seen clumping in the acid-etched crevices of the Ti (rough)-PEG surface [170]

Some authors also used a single plasma treatment step to achieve anti-bacterial properties. Cordeiro et al. [141] used a low pressure CF_4 plasma to make the surface of PDMS coatings less prone to marine bacterial attachment while Katsikogianni et al. [142] used He and He/O_2 plasmas to treat PET films leading to a reduction in the adhesion of *S. epidermidis* compared to untreated PET, even 58 days after plasma treatment.

Antifouling Surfaces and Improving Blood Compatibility

Like antibacterial surfaces, antifouling surfaces can easily be created by plasma techniques. Both a single plasma step, as a plasma pretreatment followed by a polymerization, grafting or coating step have been used. Some authors have studied the grafting of PEG onto surfaces to generate antifouling characteristics. The grafting of PEG onto PET reduces the adhesion of macrophage-like human leukocytes [143], while polyethylene glycol acrylate grafting onto PP has shown to reduce the fibrinogen adsorption with almost 85 % [144]. The grafting of PEG onto allylamine plasma polymerized on silicon wafers prevented the adsorption of horseradish peroxidase enzyme and collagen [145], while grafted onto plasma modified poly(dimethylsiloxane) (PDMS) it can prevent the avidin protein adsorption [146].

For membranes used for separation processes, including biological, pharmaceutical and sterilization filtration, antifouling properties are most important [147]. The immobilization of PEG onto poly(vinylidene fluoride) membranes leads to a significant reduction in

γ -globulins adsorption [148]. However, a decrease in water flux with increasing surface concentration of the grafted PEG polymer was observed. Kang et al. coated PP membranes with allylamine and acrylic acid [149]. Even though the plasma-treated membranes had smaller micropore sizes than the untreated membrane, they had a greater flux due to their higher hydrophilicity, as shown in Fig. 12. Plasma treatment with acrylic acid reduced the fouling with bovine serum albumin (BSA) to less than half. Deposition of acrylic acid followed by the grafting of amino-PEG onto PP membranes also leads to a reduced protein adsorption [150]. Kull et al. used nitrogen-based plasmas to modify polyethersulfone membranes [151]. After plasma treatment, the water flux through the membranes was increased and the protein fouling was reduced by 51–73 %.

The group of Timmons has developed antifouling coatings of ethylene oxide (EO) by pulsed plasma polymerization [152, 153]. They found that ultra short chain length PEO modified surfaces are biologically non-fouling. Baydal et al. has done research on bactericidal and antifouling surfaces [154–156], some of the developed coatings are being commercially used.

For blood contacting materials, non-fouling properties and minimal interaction with the biological environment are necessary to achieve a good hemocompatibility and decrease the possibility of thrombosis. In [157], an overview is given of various plasmachemical processes of fluoropolymer (like polytetrafluoroethylene (PTFE)) modification for improved hemocompatible materials. PTFE is used in ophthalmology, endoscopy, ortho-cathepedics and in cardiac surgery. For synthetic vessels, drainage tubes, vascular prostheses and other catheters, a good hemocompatibility is crucial. Plasma treatment with O_2 , Ar, N_2 and NH_3 of PTFE could significantly reduce platelet adhesion, while for Ar and N_2 plasmas can even reduce the platelet activation (spreading) [158]. A combination of plasma polymerization of acetylene to deposit diamond-like carbon (DLC), followed by an ammonia plasma treatment, and deposition of heparin could increase the blood coagulation time by a factor of 10 [159] (see Fig. 13). The amount of immobilized heparin on the surface was clearly correlated to the coagulation time.

Some authors have studied the improvement of hemocompatibility of PET by plasma modification [160–162]. Both helium plasma [160] and acetylene plasma treatment [161]

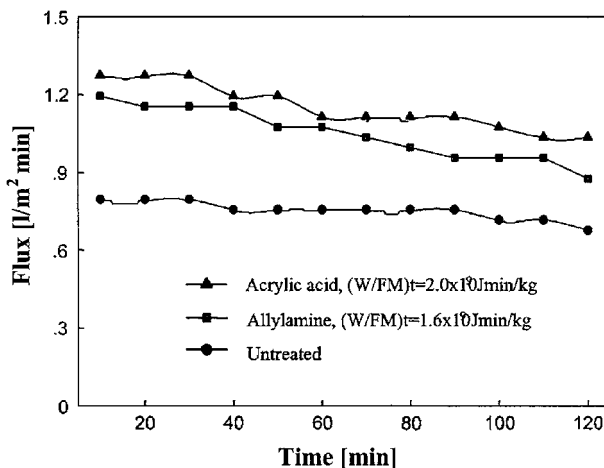


Fig. 12 Comparison of pure water fluxes through the membranes before and after the plasma treatment at 5 W and 5.332 Pa for 10 min [149]

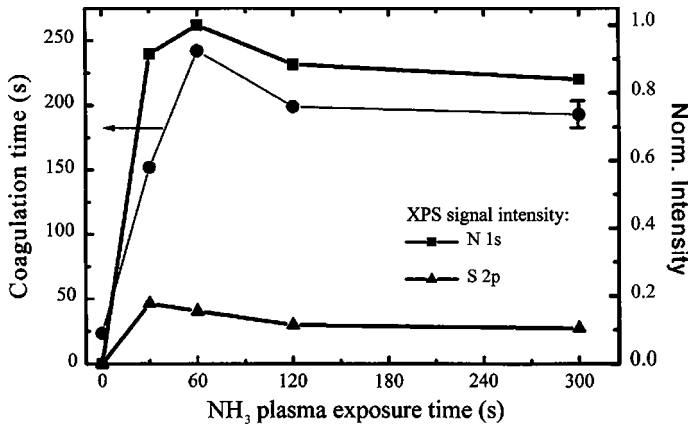


Fig. 13 Comparison between the normalized XPS signal intensities (S 2p and N 1s) and thrombin time until blood coagulation in dependence on the exposure time in an ammonia plasma beam for heparinised DLC films on PTFE vascular grafts. The data are connected by lines to guide the eye. Note the correspondence between heparin coverage and antithrombogenic activity [159]

increased the clotting time and decreased platelets adhesion and activation. Plasma polymerization of PEG also leads to a surface which is less thrombogenic due to a reduced adhesion and aggregation of platelets [162]. Ar plasma treatment and subsequent graft polymerization of glycidyl methacrylate onto polyethylene (PE) films followed by immobilization of heparin decreased the amount of adhered platelets [163], while the preirradiation grafting technique of epoxypropyl methacrylate on PP followed by heparin immobilization reduced the amount of thrombi formed on the surface [164]. Also nitrogen RF plasma treatment of polyetherurethane (PEU) could reduce clotting time [165], whereas the surface of poly(dimethyl siloxane) activated with argon plasma and grafted with poly(ethylene glycol) methyl methacrylate showed no improved blood compatibility [166].

Conclusions

During the last decades, the more demanding needs of the growing and ageing population have stated more challenging requirements to health care. Especially in the field of tissue engineering: more people than ever need an implant or an organ transplantation. To be able to supply the growing demands, extensive efforts have been made to lead the emerging interdisciplinary field of tissue engineering to a promising, fast developing, yet challenging research topic. A better understanding of cell biology, biomaterial science and cell-material interaction, have led to some hopeful advances. In this context the surface modification of biocompatible polymers is of interest for many research groups. The last decade extensive efforts have been made to optimize the surface properties of biocompatible polymers to make them suitable candidates for implants and for tissue engineering scaffolds. To be able to develop environmentally friendly technologies and to avoid the use of toxic chemicals which might cause problems towards cell viability, plasma surface modification is becoming more and more prominent. Plasma surface modification of traditional polymers has proven its possibilities, and modification of biocompatible polymers is showing promising results. However, tissue engineering remains an interdisciplinary field, and still

some crucial information on and a good understanding of cell-polymer interaction is missing. As we gain more insight into this fundamental phenomena, researchers will be able to fine-tune the surface modification to the specific needs of cell adhesion, proliferation and differentiation.

We hope this review has given a comprehensive literature overview of plasma surface modification of biocompatible polymers to change the cell-material interactions. Traditional plasma treatment is most commonly used, however other plasma technologies, like plasma polymerization and plasma grafting, are emerging. These technologies all have shown to improve the cell-material interaction of various biomedical polymers. Besides better cell adhesion and growth on the surface of an implant or scaffold, also the prevention of bacterial adhesion is crucial. Although less investigated, the use of plasma modification to prohibit bacteria to adhere onto polymer surfaces has proven to be valuable. The challenge lies in being able to prevent bacterial adhesion without compromising the cell attachment. Also non-fouling surfaces to prevent blood clot formation, are an important aspect, for example for heart valves. Due to the various possible applications of biomedical polymers, with even more divers requirements, it is evident that different specialized plasma modifying procedures and technologies will have to be developed to meet the various needs. Two of these specialized procedures are the treatment of 3D structures and the spatial control of cell adhesion. Together, these can be used to create and design new, complete artificially grown organs. If different cells types can be grown on different locations of 3D structures, one should be able to create tissue engineered products and even organs like kidneys, livers and hearts. To achieve this ambitious goal, still many research has to be done, and interdisciplinary collaborations should be undertaken. The development and (plasma) treatment of porous structures, the first steps in this process, are still the subject of many studies. It is expected that this research topic will become more and more important in the near future.

References

1. Tabata Y (2001) Recent progress in tissue engineering. *Drug Discov Today* 6:483–487
2. Vasita R, Shanmugam K, Katti D (2008) Improved biomaterials for tissue engineering applications: surface Modification of Polymers. *Curr Top Med Chem* 8:341–353
3. Jiao YP, Cui FZ (2007) Surface modification of polyester biomaterials of tissue engineering. *Biomed Mater* 2:R24–R37
4. Oehr C (2003) Plasma surface modification of polymers for biomedical use. *Nucl Instrum Methods B* 208:40–47
5. Ikada Y, Tsuji H (2000) Biodegradable polyesters for medical and ecological applications. *Macromol Rapid Comm* 21:117–132
6. Chan CM, Ko TM, Hiraoka H (1996) Polymer surface modification by plasmas and photons. *Surf Sci Rep* 24:3–54
7. Morent R, De Geyter N, Desmet T, Dubruel P, Leys C (2011) Plasma surface modification of biodegradable polymers: a review. *Plasma Process Polym* 8:171–190
8. Desmet T, Morent R, De Geyter N, Leys C, Schacht E, Dubruel P (2009) Nonthermal plasma technology as a versatile strategy for polymeric biomaterials surface modification: a review. *Bio-macromolecules* 10:2351–2378
9. Chu PK, Chen JY, Wang LP, Huang N (2002) Plasma-surface modification of biomaterials. *Mater Sci Eng* 36:143–206
10. Roach P, Eglin D, Rohde K, Perry CC (2007) Modern biomaterials: a review—bulk properties and implications of surface modifications. *J Mater Sci Mater Med* 18:1263–1277
11. Keselowsky BG, Collard DM, Garcia AJ (2005) Intergin binding specificity regulates biomaterial surface chemistry effects on cell differentiation. *Proc Natl Acad Sci USA* 102:5953–5957

12. Lutolf MP, Hubbell JA (2005) Synthetic biomaterials as instructive extracellular microenvironments for morphogenesis in tissue engineering. *Nat Biotechnol* 23:47–55
13. Vasilev K, Cook J, Griesser HJ (2009) Antibacterial surfaces for biomedical devices. *Expert Rev Med Devic* 6:553–567
14. Costerton JW, Steward PS, Greenberg EP (1999) Bacterial Biofilms a common Cause of Persistent Infections. *Science* 284:1318–1322
15. Martin TP, Kooi SE, Chang SH, Sedrans KL, Gleason KK (2007) Initiated chemical vapor deposition of antimicrobial polymer coatings. *Biomaterials* 26:909–915
16. Hetrick EM, Schoenfisch MH (2006) Reducing implant-related infections: active release strategies. *Chem Soc Rev* 35:780–789
17. Banerjee I, Pangole RC, Kane RS (2003) Antifouling coatings: recent developments in design of surfaces that prevent fouling by proteins, bacteria, and marine organisms. *Advan Mater* 32:690–718
18. Chambers LD, Stokes KR, Walsh FC, Wood RJK (2006) Modern approaches to marine antifouling coatings. *Surf Coat Technol* 201:3642–3652
19. Amiji M, Park K (1993) Surface modification of polymeric biomaterials with poly(ethylene oxide), albumin and heparin. *J Biomat Sci Polym E* 4:217–234
20. Krishnan S, Weinman CJ, Ober CK (2008) Advances in polymers for anti-biofouling surfaces. *J Mater Chem* 18:3405–3413
21. Ho MH, Hou LT, Tu CY, Hsieh HJ, Lai JY, Chen WJ, Wang DM (2006) Promotion of cell affinity of porous PLLA scaffold by immobilization of RGD peptides via plasma treatment. *Macromol Biosci* 6:90–98
22. Shen H, Hu XX, Yang F, Bel JZ, Wang SG (2007) Combining oxygen plasma treatment with anchorage of cationized gelatin for enhancing cell affinity of poly (lactide-co-glycolide). *Biomaterials* 28:4219–4230
23. Bogaerts A, Neyts E, Gijbels R, van der Mullen J (2002) Gas discharge plasmas and their applications. *Spectrochim Acta B* 57:609–658
24. Zenkiewicz M, Rytlewski P, Malinowski R (2011) Low-temperature plasma modification of polymers—methods and equipment. *Polimery* 56:185–195
25. De Geyter N, Morent R, Leys C, Gengembre L, Payen E (2007) Treatment of polymer films with a dielectric barrier discharge in air, helium and argon at medium pressure. *Surf Coat Technol* 201:7066–7075
26. Cui NY, Brown NMD (2002) Modification of the surface properties of a polypropylene (PP) film using an air dielectric barrier discharge plasma. *Appl Surf Sci* 189:31–38
27. Morent R, De Geyter N, Leys C, Genbembre L, Payen E (2007) Study of the ageing behavior of polymer films treated with a dielectric barrier discharge in air, helium and argon at medium pressure. *Surf Coat Technol* 201:7847–7854
28. De Geyter N, Morent R, Leys C (2008) Influence of ambient conditions on the ageing behavior of plasma-treated PET surfaces. *Nucl Instrum Meth B* 226:3086–3090
29. Morent R, De Geyter N, Van Vlierberghe S, Beaurain A, Dubruel P, Payen E (2011) Influence of operating parameters on plasma polymerization of acrylic acid in a mesh-to-plate dielectric barrier discharge. *Prog Org Coat* 70:336–341
30. De Geyter N, Morent R, Van Vlierberghe S, Frere-Trentesaux M, Dubruel P, Payen E (2011) Effect of electrode geometry on the uniformity of plasma-polymerized methyl methacrylate coatings. *Prog Org Coat* 70:293–299
31. Morent R, De Geyter N, Van Vlierberghe S, Dubruel P, Leys C, Gengembre L, Schacht E, Payen E (2009) Deposition of HMDSO-based coatings on PET substrates using an atmospheric pressure dielectric barrier discharge. *Prog Org Coat* 64:304–310
32. Morent R, De Geyter N, Van Vlierberghe S, Vanderleyden E, Dubruel P, Leys C, Schacht E (2009) Deposition of polyacrylic acid films by means of an atmospheric pressure dielectric barrier discharge. *Plasma Chem Plasma Process* 29:103–117
33. Arefi F, Andere V, Montazer-Rahmati P, Amouroux J (1992) Plasma polymerization and surface treatment of polymers. *Pure Appl Chem* 64:715–723
34. Vasilets VN, Hermel G, Konig U, Werner C, Muller M, Simon F, Grundke K, Ikada Y, Jacobasch JH (1997) Microwave CO₂ plasma-initiated vapour phase graft polymerization of acrylic acid onto polyterafuoroethylene for immobilization of human thrombomodulin. *Biomaterials* 18:1139–1145
35. Conrads H, Schmidt M (2004) Plasma generation and plasma sources. *Plasma Soures Sci Technol* 9:441–454
36. Tendero C, Tixier C, Tristant P, Desmaison J, Leprince P (2008) Atmospheric pressure plasma: a review. *Spectrochim Acta B* 61:2–30

37. Jiao YP, Cui FZ (2007) Surface modification of polyester biomaterials for tissue engineering. *Biomed Mater* 2(4):R24–R37
38. Cao Y, Liu W, Zhou G, Cui L (2007) Tissue engineering and tissue repair in immunocompetent animals: tissue construction and repair. *Handchir Mikrochir Plast Chir* 39(3):156–160
39. Chong MSK, Lee CN, Teoh SH (2007) Characterization of smooth muscle cells on poly(ϵ -caprolactone) films. *Mater Sci Eng C Biomimetic Supramol Syst* 27(2):309–312
40. Choong CSN, Hutmacher DW, Triffitt JT (2006) Co-culture of bone marrow fibroblasts and endothelial cells on modified polycaprolactone substrates for enhanced potentials in bone tissue engineering. *Tissue Eng* 12(9):2521–2531
41. Mathieson I, Bradley RH (1996) Improved adhesion to polymers by UV/ozone surface oxidation. *Int J Adhes Adhes* 16(1):29–31
42. Mathieson I, Bradley RH (1995) Effects of ultra-violet ozone oxidation on the surface-chemistry of polymer-films. *Adv Eng Mater* 99–1:185–191
43. Davidson MR, Mitchell SA, Bradley RH (2005) Surface studies of low molecular weight photolysis products from UV-ozone oxidised polystyrene. *Surf Sci* 581(2–3):169–177
44. Kato K, Uchida E, Kang ET, Uyama Y, Ikada Y (2003) Polymer surface with graft chains. *Prog Polym Sci* 28(2):209–259
45. Deng J, Wang L, Liu L, Yang W (2009) Developments and new applications of UV-induced surface graft polymerizations. *Prog Polym Sci* 34(2):156–193
46. Yang Y, Porte MC, Marmey P, El Haj AJ, Amedee J, Baquey C (2003) Covalent bonding of collagen on poly(L-lactic acid) by gamma irradiation. *Nucl Instrum Methods Phys Res Sect B Beam Interact Mater Atoms* 207(2):165–174
47. Cho EH, Lee SG, Kim JK (2005) Surface modification of UHMWPE with gamma-ray radiation for improving interfacial bonding strength with bone cement (II). *Curr Appl Phys* 5(5):475–479
48. Shojaei A, Fathi R, Sheikh N (2007) Adhesion modification of polyethylenes for metallization using radiation-induced grafting of vinyl monomers. *Surf Coat Technol* 201(16–17):7519–7529
49. Gatenholm P, Ashida T, Hoffman AS (1997) Hybrid biomaterials prepared by ozone-induced polymerization 0.1. Ozonation of microporous polypropylene. *J Polym Sci Part A Polym Chem* 35(8):1461–1467
50. Yu HY, He JM, Liu LQ, He XC, Gu JS, Wei XW (2007) Photoinduced graft polymerization to improve antifouling characteristics of an SBR. *J Membr Sci* 302(1–2):235–242
51. Goda T, Matsuno R, Konno T, Takai M, Ishihara K (2008) Photografting of 2-methacryloyloxyethyl phosphorylcholine from polydimethylsiloxane: tunable protein repellency and lubrication property. *Colloids Surf B Biointerfaces* 63(1):64–72
52. Shim JK, Na HS, Lee YM, Huh H, Nho YC (2001) Surface modification of polypropylene membranes by gamma-ray induced graft copolymerization and their solute permeation characteristics. *J Membr Sci* 190(2):215–226
53. Morent R, De Geyter N, Leys C (2008) Effects of operating parameters on plasma-induced PET surface treatment. *Nucl. Instrum. Methods B* 266:3081–3085
54. Morent R, De Geyter N, Gengembre L, Les C, Payen E, Van Vlierberghe S, Payen E (2008) Surface treatment of a polypropylene film with a nitrogen DBD at medium pressure. *Europ Phys J Appl Phys* 43:289–294
55. Siow KS, Brichter L, Kumar S, Griesser HJ (2006) Plasma methods for the generation of chemically reactive surfaces for biomolecule immobilization and cell colonization—a review. *Plasma Process Polym* 3:292–418
56. Khorasani MT, Mirzadeh H, Irani S (2008) Plasma surface modification of poly (L-lactic acid) and poly (lactic-co-glycolic acid) films for improvement of nerve cells adhesion. *Rad Phys Chem* 77:280–287
57. Khorasani MT, Mirzadeh H, Irani S (2009) Comparison of fibroblast and nerve cells response on plasma treated poly (L-lactide) surface. *J Appl Polym Sci* 112:2429–3435
58. Nakagawa M, Teroaka F, Fujimoto S, Hamada Y, Kibayashi K, Takahashi J (2006) Improvement of cell adhesion on poly (L-lactide) by atmospheric plasma treatment. *J Biomed Mater Res A* 77A:112–118
59. Teraoka F, Nakagawa M, Hara M (2006) Surface modification of poly (L-lactide) by atmospheric pressure plasma treatment and cell response. *Dent Mater J* 25:560–565
60. Chu CFL, Lu A, Liszkowski M, Siphia R (1999) Enhanced growth of animal and human endothelial cells on biodegradable polymers. *Biochim Biophys Acta* 1472:479–485
61. Yang J, Bei JZ, Wang SG (2002) Improving cell affinity of poly (D, L-lactide) film modified by anhydrous ammonia plasma treatment. *Polym Advan Technol* 13:220–226

62. Gugala Z, Gogolewski S (2006) Attachment, growth, and activity of rat osteoblasts on polylactide membranes treated with various low-temperature radiofrequency plasmas. *J Biomed Mater Res A* 76A:288–299
63. Wan Y, Yang J, Yang JL, Bei JZ, Wang SG (2003) Cell adhesion on gaseous plasma modified poly(L-lactide) surface under shear stress field. *Biomaterials* 24:3757–3764
64. Yildirim ED, Ayan H, Vasilets VN, Fridman A, Gucerli S, Sun W (2008) Effect of dielectric barrier discharge plasma on the attachment and proliferation of osteoblasts cultured over poly (ϵ -caprolactone) scaffolds. *Plasma Process Polym* 5:58–66
65. Lee HU, Jeong YS, Koh KN, Jeong SY, Kim HG, Bae JS, Cho CR (2009) Contribution of power on cell adhesion using atmospheric dielectric barrier discharge (DBD) plasma system. *Current Appl Phys* 9:219–223
66. Lee HU, Jeong YS, Jeong SY, Park SY, Bae JS, Kim HG, Cho CR (2008) Role of reactive gas in atmospheric plasma for cell attachment and proliferation on biocompatible poly ϵ -caprolactone film. *Appl Surf Sci* 254:5700–5705
67. Hasirci N, Endogan T, Vardar E, Kiziltay A, Hasirci V (2010) Effect of oxygen plasma on surface properties and biocompatibility of PLGA films. *Surf Interface Anal* 42:486–491
68. Wan Y, Qu X, Lu J, Zhu C, Zhu CF, Wan LJ, Yang JL, Bei JZ, Wang SG (2004) Characterization of surface property of poly (lactide-co-glycolide) after oxygen plasma treatment. *Biomaterials* 25:4777–4783
69. Khang G, Choe JH, Rhee JM, Lee HB (2002) Interaction of different types of cells on physico-chemically treated poly(L-lactide-co-glycolide) surfaces. *J Appl Polym Sci* 85:1253–1262
70. Park H, Lee JW, Park KE, Park WH, Lee KY (2010) Stress response of fibroblasts adherent to the surface of plasma-treated poly(lactic-co-glycolic acid) nanofiber matrices. *Colloid Surface B* 77:90–95
71. Wang YJ, Ly L, Zheng YD, Chen XF (2006) Improvement in hydrophilicity of PHBV films by plasmas treatment. *J Biomed Mater Res A* 76A:589–595
72. Tezcaner A, Bugra K, Hasirci V (2003) Retinal pigment epithelium cell culture on surface modified poly(hydroxybutyrate-co-hydroxyvalerate) thin films. *Biomaterials* 24:4573–4583
73. Garrido L, Jimenez I, Ellis G, Cano P, Garcia-Martinez JM, Lopez L, de la Pena E (2011) Characterization of surface-modified polyalkanoate films for biomedical applications. *J Appl Polym Sci* 119:3286–3296
74. Pompe T, Keller K, Mothes G, Nitschke M, Teese M (2007) Surface modification of poly(hydroxybutyrate) films to control cell-matrix adhesion. *Biomaterials* 28:28–37
75. Qu XH, Wu Q, Liang J, Qu X, Wang SG, Chen GQ (2005) Enhanced vascular-related cellular affinity on surface modified copolyesters of 3-hydroxybutyrate and 3-hydroxyhexanoate (PHBHHX). *Biomaterials* 26:6991–7001
76. Woodfield TBF, Miot S, Martin I, van Blitterswijk CA, Riesle J (2006) The regulation of expanded human nasal chondrocyte re-differentiation capacity by substrate composition and gas plasma surface modification. *Biomaterials* 27:1043–1053
77. Khan SP, Auner GG, Newas GM (2005) Influence of nanoscale surface roughness on neural cell attachment to silicon. *Nanomed Nanotechnol* 1:125–129
78. Chong MSK, Lee CN, Teoh SH (2007) Characterization of smooth muscle cells on poly(ϵ -caprolactone) films. *Mater Sci Eng* 27:309–312
79. Cheng Z, Teoh SH (2004) Surface modification of ultra thin poly(ϵ -caprolactone) films using acrylic acid and collagen. *Biomaterials* 25:1991–2001
80. Foo HL, Taniguchi A, Yu H, Okano T, Teoh SH (2007) Catalytic surface modification of roll-milled poly(ϵ -caprolactone) biaxially stretched to ultra-thin dimension. *Mater Sci Eng* 27:299–303
81. Kang I-K, Choi S-H, Shin D-S, Yoon SC (2001) Surface modification of polydihydroxyalkanoate films and their interaction with human fibroblasts. *Int J Biol Macromol* 28:205–212
82. Baquey Ch, Palumbo F, Porte-Durrieu MC, Legeay G, Tressaud A, D'Agostino R (1999) Plasma treatment of expanded PTFE offers a way to a biofunctionalization of its surface. *Nucl Instrum Meth B* 151:255–262
83. Seo HS, Ko YM, Shim JW, Lim YK, Kook J-K, Cho D-L, Kim BH (2010) Characterization of bioactive RGD peptide immobilized onto poly(acrylic acid) thin films by plasma polymerization. *Appl Surf Sci* 257:596–602
84. Xia Y, Boey F, Venkatraman SS (2010) Surface modification of poly(L-lactic acid) with biomolecules to promote endothelialisation. *Biointerphases* 5:32–40
85. Duan Y, Wang Z, Yan W, Wang S, Zhang S, Jia J (2007) Preparation of collagen-coated electrospun nanofibres by remote plasma treatment and their biological properties. *J Biomater Sci Polym Ed* 18:1153–1164

86. Shen H, Hu X, Yang F, Bei J, Wang S (2007) Combining oxygen plasma treatment with anchorage of cationized gelatine for enhancing cell affinity of poly(lactide-co-glycolide). *Biomaterials* 28:4219–4230
87. Yang J, Bei J, Wang S (2002) Enhanced cell affinity of poly(D, L-lactide) by combining plasma treatment with collagen anchorage. *Biomaterials* 23:2607–2614
88. He W, Ma ZW, Young T, Teo WE, Ramakrishna S (2005) Fabrication of collagen-coated biodegradable polymer nanofiber mesh and its potential for endothelial cells growth. *Biomaterials* 26:7606–7615
89. Lopez-Perez PM, da Silva RMP, Sousa RA, Pashkuleva I, Reis RL (2010) Plasma-induced polymerization as a tool for surface functionalization of polymer scaffolds for bone tissue engineering: an in vitro study. *Acta Biomater* 6:3704–3712
90. Ding Z, Chen J, Gao S, Chang J, Zhang J, Kang ET (2004) Immobilization of chitosan onto poly-L-lactic acid film surface by plasma graft polymerization to control the morphology of fibroblast and liver cells. *Biomaterials* 25:1059–1067
91. Guerrouani N, Baldo A, Bouffin A, Drakides C, Guimon M-F, Mas A (2007) Allylamine plasma-polymerization on PLLA surface evaluation of the biodegradation. *J Appl Polym Sci* 105:1978–1986
92. Carlisle ES, Mariappan MR, Nelson KD, Thomes BE, Timmons RB, Constantinescu A, Eberhart RC, Bankey PE (2006) Enhancing hepatocyte adhesion by pulsed plasma deposition and polyethylene glycol coupling. *Tissue Eng* 6:45–52
93. Ren TB, Weigel Th, Groth Th, Lendlein A (2008) Microwave plasma surface modification of silicone elastomer with allylamine for improvement of biocompatibility. *J Biomed Mater Res A* 86:209–219
94. Park K, Ju YM, Son JS, Ahn K-D, Han DG (2007) Surface modification of biodegradable electrospun nanofiber scaffolds and their interaction with fibroblasts. *J Biomater Sci Polym Ed* 18:369–382
95. Mitchell SA, Davidson MR, Emmison N, Bradley RH (2004) Isopropyl alcohol plasma modification of polystyrene surfaces to influence cell attachment behaviour. *Surf Sci* 561:110–120
96. Siow KS, Britcher L, Kumar S, Griesser HJ (2006) Plasma methods for the generation of chemically reactive surfaces for biomolecule immobilization and cell colonization—a review. *Plasma Proc Polym* 3:292–418
97. Li B, Ma Y, Wang S, Moran PM (2005) Influence of carboxyl group density on neuron cell attachment and differentiation behaviour: gradient-guided neurite outgrowth. *Biomaterials* 26:4956–4963
98. Li B, Ma Y, Wang S, Moran PM (2005) A technique for preparing protein gradients on polymeric surfaces: effect on PC12 pheochromocytoma cells. *Biomaterials* 26:1487–1495
99. Rosso F, Giodano A, Barbarisi M, Barbarisi A (2004) From cell-ECM interactions to tissue engineering. *J Cell Physiol* 199:174–180
100. Kim BS, Mooney DJ (1998) Development of biocompatible synthetic extracellular matrices for tissue engineering. *Trends Biotechnol* 16:224–230
101. Wan Y, Tu C, Yang J, Bei J, Wang S (2006) Influences of ammonia plasma treatment on modifying depth and degradation of poly(L-lactide) scaffolds. *Biomaterials* 27:2699–2704
102. Barry JJA, Silva MCG, Shakesheff KM, Howdle SM, Alexander MR (2005) Using plasma deposits to promote cell population of the porous interior of three-dimensional poly(D, L-lactic acid) tissue-engineering scaffolds. *Adv Funct Mater* 15:1134–1140
103. Ju YM, Park K, Son JS, Kim J-J, Rhie J-W, Han DK (2008) Beneficial effect of hydrophilized porous polymer scaffolds on tissue-engineered cartilage formation. *J Biomed Mater Res B* 85B:252–260
104. Chim H, Ong JL, Schantz J-T, Huttmacher DW, Agrawal CM (2003) Efficacy of glow discharge on gas plasma treatment as a surface modification process for three-dimensional poly(D, L-lactide) scaffolds. *J Biomed Mater Res A* 65A:327–335
105. Yamagushi M, Shinbo T, Kanamori T, Wang PC, Niwa M, Kawakami H, Nagaoka S, Hiakawa K, Kamiya M (2004) Surface modification of poly(L-lactic acid) affects initial cell attachment, cell morphology, and cell growth. *J Artif Organs* 7:187–193
106. Ho M-H, Hou L-T, Tu C-Y, Hsieh H-J, Lai J-Y, Chen W-J, Wang D-M (2006) Promotion of cell affinity of porous PLLA scaffolds by immobilization of RGD peptides via plasma treatment. *Macromol Biosci* 6:90–98
107. Chen J-P, Su C-H (2011) Surface modification of electrospun PLLA nanofibers by plasma treatment and cationized gelatine immobilization for cartilage tissue engineering. *Acta Biomater* 7:234–243
108. Prabhakaran P, Venugopal J, Chan CK, Ramakrishna S (2008) Surface modified electrospun nanofiber scaffolds for nerve tissue engineering. *Nanotechnology* 19:488102 (8 pp)
109. Yildirim ED, Besunder R, Pappas D, Allen F, Güçeri S, Sun W (2010) Accelerated differentiation of osteoblast cells on polycaprolactone scaffolds driven by a combined effect of protein coating and plasma modification. *Biofabrication* 2:014109 (12 pp)

110. Köse GT, Kenar K, Hasirci N, Hasirci V (2003) Macroporous poly(3-hydroxybutyrate-co-3-hydroxyvalerate) matrices for bone tissue engineering. *Biomaterials* 24:1949–1958
111. Köse GT, Ber S, Korkusuz F, Hasirci V (2003) Poly(3-hydroxybutyric acid-co-3-hydroxyvaleric acid) based tissue engineering matrices. *J Mater Sci Mater Med* 14:121–126
112. Kim MS, Khang G, Lee HB (2008) Gradient polymer surfaces for biomedical applications. *Prog Polym Sci* 33:138–164
113. Ruardy TG, Schakenraad JM, van der Mei HC, Busscher HJ (1997) Preparation and characterization of chemical gradient surfaces and their application for the study of cellular interaction phenomena. *Surf Sci Rep* 29:1–30
114. Wilkinson CDW, Riehle M, Wood M, Gallagher J, Curtis ASG (2002) The use of materials patterned on a nano- and micro-metric scale in cellular engineering. *Mater Sci Eng C* 19:263–269
115. Lee SJ, Khang G, Lee YM, Lee HB (2003) The effect of surface wettability on induction and growth of neuritis from the PC-12 cell on a polymer surface. *J Colloid Interf Sci* 256:228–235
116. Choe J-H, Lee SJ, Lee YM, Rhee JM, Lee HB, Khang G (2004) Proliferation rate of fibroblast cells on polyethylene surfaces with wettability gradient. *J Appl Polym Sci* 92:599–606
117. Lee JH, Khang G, Lee JW, Lee HB (1998) Interaction of different types of cells on polymer surfaces with wettability gradient. *J Colloid Interf Sci* 205:323–330
118. Zelzer M, Majani R, Bradley JW, Rose FRAJ, Davies MC, Alexander MR (2008) Investigation of cell-surface interactions using chemical gradients formed from plasma polymers. *Biomaterials* 29:172–184
119. Wells N, Baxter MA, Thurnbull JE, Murray PM, Edgar D, Parry KL, Steele DA, Short RD (2009) The geometric control of E14 and R1 mouse embryonic stem cell pluripotency by plasma polymer surface gradients. *Biomaterials* 30:1066–1070
120. Mitchell SA, Davidson MR, Emmison N, Bradley RH (2004) Isopropyl alcohol plasma modification of polystyrene surfaces to influence cell attachment behaviour. *Surf Sci* 561:110–120
121. Mitchell SA, Davidson MR, Bradley RH (2005) Improved cellular adhesion to acetone plasma modified polystyrene surfaces. *J Colloid Interf Sci* 281:122–129
122. Mitchell SA, Emmison N, Shard AG (2002) Spatial control of cell attachment using plasma micro-patterned polymers. *Surf Interf Anal* 33:742–747
123. Sardella E, Gristina R, Senesi GS, d'Agostino R, Favia P (2004) Homogeneous and micro-patterned plasma-deposited PEO-like coatings for biomedical surfaces. *Plasma Process Polym* 1:63–72
124. Thissen H, Johnson G, Hartley PG, Kingshott P, Griesser HJ (2006) Two-dimensional patterning of thin coatings for the control of tissue outgrowth. *Biomaterials* 27:35–43
125. Leduc M, Coulombe S, Leask RL (2009) Atmospheric pressure plasma jet deposition of patterned polymer films for cell culture applications. *IEEE Trans Plasma Sci* 37:927–933
126. Gristina AG (1978) Biomaterial-centered infections: microbial adhesion versus tissue intergration. *Science* 237:1588–1595
127. Subbiahdoss G, Kuijter R, Grijpma DW, van der Mei HC, Busscher HJ (2009) Microbial biofilm growth vs. tissue integration: “The race for the surface” experimentally studied. *Acta Biomater* 5:1399–1404
128. Bazaka K, Jacob MV, Crawford RJ, Ivanova EP (2011) Plasma-assisted surface modification of organic biopolymers to prevent bacterial attachment. *Acta Biomater* 7:2015–2028
129. An YH, Friedman RJ (1997) Concise review of mechanisms of bacterial adhesion to biomaterial surfaces. *J Biomed Mater Res* 43:338–348
130. Hori K, Matsumoto S (2010) Bacterial adhesion: from mechanism to control. *Biochem Eng J* 48:424–434
131. Triandafillu K, Balazs DJ, Aronsson B-O, Descouts P, Tu Quoc P, van Delden C, Mathieu HJ, Harms H (2003) Adhesion of *Pseudomonas aeruginosa* strains to untreated and oxygen-plasma treated poly(vinyl chloride) (PVC) from endotracheal intubation devices. *Biomaterials* 24:1507–1518
132. Balazs DJ, Triandafillu K, Chevolut Y, Aronsson B-O, Harms H, Descouts P, Mathieu HJ (2003) Surface modification of PVC endotracheal tubes by oxygen glow discharge to reduce bacterial adhesion. *Surf Interf Anal* 35:301–309
133. Balazs DJ, Triandafillu K, Wood P, Chevolut Y, van Delden C, Harms H, Hollenstein C, Mathieu HJ (2004) Inhibition of bacterial adhesion on PVC endotracheal tubes by RF- oxygen glow discharge, sodium hydroxide and silver nitrate treatments. *Biomaterials* 25:2139–2151
134. Asadinezhad A, Novak I, Lehocky M, Sedlarik V, Vesel A, Junkar I, Saha P, Chodak I (2010) A physicochemical approach to render antibacterial surfaces on plasma-treated medical grade PVC: irgasan coating. *Plasma Process Polym* 7:504–514
135. Asadinezhad A, Novak I, Lehocky M, Sedlarik V, Vesel A, Junkar I, Saha P, Chodak I (2010) An in vitro bacterial adhesion assessment of surface-modified medical-grade PVC. *Colloid Surface B* 77:246–256

136. Zhang W, Chu PK, Ji J, Zhang Y, Liu X, Fu RKY, Ha PCT, Yan Q (2006) Plasma surface modification of poly vinyl chloride for improvement of antibacterial properties. *Biomaterials* 27:44–51
137. Harris LG, Tosatti S, Wieland M, Textor M, Richards RG (2004) Staphylococcus aureus adhesion to titanium oxide surfaces coated with non-functionalized and peptide-functionalized poly (α -lysine)-grafted-poly(ethylene glycol) copolymers. *Biomaterials* 25:4135–4148
138. Su W, Wang S, Wang X, Fu X, Weng J (2010) Plasma pre-treatment and TiO₂ coating of PMMA for the improvement of antibacterial properties. *Surf Coat Technol* 205:465–469
139. Chen K-S, Ky Y-A, Lin H-R, Yan T-R, Sheu D-C, Chen T-M (2006) Surface grafting polymerization of N-vinyl-2-pyrrolidone onto a poly(ethylene terephthalate) nonwoven by plasma pretreatment and its antibacterial activities. *J Appl Polym Sci* 100:803–809
140. Morra M, Cassinelli C (1999) Non-fouling properties of polysaccharide-coated surfaces. *J Biomater Sci Polym Ed* 10:1107–1124
141. Cordeiro AL, Nitschke M, Janke A, Helbig R, D'Souza F, Donnelly GT, Willemsen PR, Werner C (2009) Fluorination of poly(dimethylsiloxane) surfaces by low pressure CF₄—physicochemical and antifouling properties. *Express Polym Lett* 3:70–83
142. Katsikogianni M, Amanatides E, Mataras D, Missirlis YF (2008) Staphylococcus epidermidis adhesion to He, He/O₂ plasma treated PET films and aged materials: contribution of surface free energy and shear rate. *Colloid SurfacesB* 65:257–268
143. Ademovic Z, Holst B, Kahn RA, Jorring I, Brevig T, Wei J, Hou X, Winter-Jensen B, Kingshott P (2006) The method of surface PEGylation influences leukocyte adhesion and activation. *J Mater Sci Mater Med* 17:203–211
144. Zanini S, Orlandi M, Colombo C, Grimoldi E, Riccardi C (2009) Plasma-induced graft-polymerization of polyethylene glycol acrylate on polypropylene substrates. *Eur Phys J D* 54:156–164
145. Cole MA, Thissen H, Losic D, Voelcker NH (2007) A new approach to the immobilisation of poly(ethylene oxide) for the reduction of non-specific protein adsorption on conductive substrates. *Surf Sci* 601:1716–1725
146. Geissler A, Vallat M-F, Fioux P, Thomann J-S, Frisch B, Voegel J-C, Hemmerlé J, Schaaf P, Roucoules V (2010) Multifunctional stretchable plasma polymer modified PDMS interface for mechanically responsive materials. *Plasma Process Polym* 7:64–77
147. De Bartolo L, Drioli E (1998) Membranes in artificial organs. *New Biomed Mater Basic Appl Stud* 16:167–181
148. Wang P, Tan KL, Kang ET, Neoh KG (2002) Plasma-induced immobilization of poly(ethylene glycol) onto poly(vinylidene fluoride) microporous membrane. *J Membrane Sci* 195:103–114
149. Kang MS, Chun B, Kim SS (2001) Surface modification of polypropylene membrane by low-temperature plasma treatment. *J Appl Polym Sci* 81:1555–1566
150. Zanini S, Muller M, Riccardi C, Orlandi M (2007) Polyethylene glycol graftin on polypropylene membranes for anti-fouling properties. *Plasma Chem Plasma Process* 27:446–457
151. Kull KR, Steen ML, Fisher ER (2005) Surface modification with nitrogen-containing plasmas to produce hydrophilic, low-fouling membranes. *J Membrane Sci* 246:203–215
152. Wu YJ, Timmons RB, Jen JS, Molock FE (2000) Non-fouling surfaces produced by gas phase pulsed plasma polymerization of an ultra low molecular weight ethylene oxide containing monomer. *Colloid Surface B* 18:234–248
153. Beyer D, Knoll W, Ringsdorf H, Wang J-H, Timmons RB, Sluka P (1997) Reduced protein adsorption on plastics via direct plasma deposition of triethylene glycol monoallyl ether. *J Biomed Mater Res* 36:181–189
154. Schofield WC, Badyal JP (2009) A substrate-independent approach for bactericidal surfaces. *Appl Mater Inter* 1:2763–2767
155. Wood TJ, Hurst GA, Schofield WCE, Thompson RL, Oswald G, Evans JSO, Sharples G, Pearson C, Petty MC, Badyal JPS (2012) Electroless deposition of multi-functional zinc oxide surfaces displaying photoconductive, superhydrophobic, photowetting, and antibacterial properties. *J Mater Chem* 22:3859–3867
156. Badyal JPS, Teare DOH, Schofield WC (2009) Patent application title: method for producing, and a substrate with, a surface with specific characteristics—patent office: United States of America patent and trademark office. Published patent application (USPTO)—publication date: 11/19/2009—United States patent application 20090286435
157. Sevast'yanov VI, Vasilets VN (2009) Plasmochemical modifications of fluorocarbon polymers for creation of new hemocompatible materials. *Russ J Gen Chem* 79:596–605
158. Rhodes NP, Wilson DJ, Williams RL (2007) The effect of gas plasma modification on platelet and contact phase activation processes. *Biomaterials* 28:4561–4570

159. Steffen HJ, Schmidt J, Gonzalez-Elipe A (2000) Biocompatible surfaces by immobilization of heparin on diamond-like carbon films deposited on various substrates. *Surf Interf Anal* 29:386–391
160. Topala I, Dumitrascu N, Pohoatoa V (2007) Influence of plasma treatments on the hemocompatibility of PET and PET + TiO₂ films. *Plasma Chem Plasma Process* 27:95–112
161. Want J, Chen JY, Yang P, Leng YW, Wan GJ, Sun H, Zhao AS, Huang N, Chu PK (2006) In vitro platelet adhesion and activation of polyethylene terephthalate modified by acetylene plasma immersion ion implantation and deposition. *Nucl Instrum Meth B* 242:12–14
162. Kumar DS, Fujioka M, Asano K, Shoji A, Jayakrishnan A, Yoshida Y (2007) Surface modification of poly(ethylene terephthalate) by plasma polymerization of poly(ethylene glycol). *J Mater Sci Mater Med* 18:1831–1835
163. Chen Y, Liu P (2004) Surface modification of polyethylene by plasma pre-treatment and UV-induced graft polymerization for improvement of antithrombogenicity. *J Appl Polym Sci* 93:2014–2018
164. Kwon OH, Nho YC, Chen J (2003) Surface modification of polypropylene film by radiation-induced grafting and its blood compatibility. *J Appl Polym Sci* 88:1726–1736
165. Wilson DJ, Rhodes NP, Williams RL (2003) Surface modification of a segmented polyetherurethane using a low-powered gas plasma and its influence on the activation of the coagulation system. *Biomaterials* 24:5069–5081
166. Pinto S, Alves P, Matos CM, Santos AC, Rodrigues LR, Teixeira JA, Gil MH (2010) Poly(dimethyl siloxane) surface modification by low pressure plasma to improve its characteristics towards biomedical applications. *Colloid Surface B* 81:20–26
167. Reprinted from *Biochimica et Biophysica Acta* 1472, Chu CFL, Lu A, Liszkowski M, Siphia R (2010) Enhanced growth of animal and human endothelial cells on biodegradable polymers, pp 479–485, Copyright (2010), with permission from Elsevier
168. Reprinted from *Biomaterials* 28, Pompe T, Keller K, Mothes G, Nitschke M, Teese M (2007) Surface modification of poly(hydroxybutyrate) films to control cell-matrix adhesion, pp 28–37, Copyright (2007), with permission from Elsevier
169. Reprinted from *Biointerphases* 5, Xia Y, Boey F, Venkatraman SS (2010) Surface modification of poly(L-lactic acid) with biomolecules to promote endothelialization, pp 32–40, Copyright (2010) with permission from Springer Science + Business Media B.V.
170. Reprinted from *Biomaterials* 25, Harris LG, Tosatti S, Wieland M, Textor M, Richards RG (2004) Staphylococcus aureus adhesion to titanium oxide surfaces coated with non-functionalized and peptide-functionalized poly(L-lysine)-grafted-poly(ethylene glycol) copolymers, pp 4135–4148, Copyright (2004), with permission from Elsevier