

 Open access • Proceedings Article • DOI:10.1117/12.468141

Reducing the mechanical hysteresis problem in optically addressed diaphragm pressure sensors — [Source link](#)

S. A. Sharifian, David R. Buttsworth

Institutions: University of Southern Queensland

Published on: 22 May 2002

Topics: Pressure sensor

Related papers:

- [High-Sensitivity Inductive Pressure Sensor](#)
- [Thermal hysteresis in inertial sensors](#)
- ['Electrical viscosity' of piezoresistive sensors: Novel signal processing method, assessment of manufacturing quality, and proposal of an industrial standard.](#)
- [A Novel Inverse-Magnetostrictive Force Sensor](#)
- [Estimation of the long-term stability of piezoresistive LTCC pressure sensors by means of low-frequency noise measurements](#)

Share this paper:    

View more about this paper here: <https://typeset.io/papers/reducing-the-mechanical-hysteresis-problem-in-optically-8mq4bx6wxk>



Fifth International Conference on
**Vibration Measurements
by Laser Techniques:
Advances and Applications**

Enrico Primo Tomasini
Chair/Editor

18-21 June 2002
Ancona, Italy

Organized by
A.I.V.E.L.A.—Italian Association of Laser Velocimetry
Dipartimento di Meccanica, Università degli Studi di Ancona (Italy)



Volume 4827

Fifth International Conference on
**Vibration Measurements
by Laser Techniques:
Advances and Applications**

Enrico Primo Tomasini
Chair/Editor

18-21 June 2002
Ancona, Italy

Organized by
A.I.V.E.L.A.—Italian Association of Laser Velocimetry
Dipartimento di Meccanica, Università degli Studi di
Ancona (Italy)



Participating Organizations

ACI—American Concrete Institute International • AMA—Fachverband für Sensorik e.V. (Germany) • ASJ—Acoustical Society of Japan • ATA—Associazione Tecnica dell'Automobile (Italy) • GSI—Gruppo Imprese Strumentazione Italia • IAHR—International Association for Hydraulic Research • IMEKO—International Measurement Confederation • JSAE—Society of Automotive Engineers of Japan • OSA—Optical Society of America • SAE International—Society of Automotive Engineers • SEM—Society for Experimental Mechanics • SICE—Society of Instrument and Control Engineers

Published by
SPIE—The International Society for Optical Engineering



Volume 4827

SPIE is an international technical society dedicated to advancing engineering and scientific applications of optical, photonic, imaging, electronic, and optoelectronic technologies.



The papers appearing in this book compose the proceedings of the technical conference cited on the cover and title page of this volume. They reflect the authors' opinions and are published as presented, in the interests of timely dissemination. Their inclusion in this publication does not necessarily constitute endorsement by the editors or by SPIE. Papers were selected by the conference program committee to be presented in oral or poster format, and were subject to review by volume editors or program committees.

Please use the following format to cite material from this book:

Author(s), "Title of paper," in *Fifth International Conference on Vibration Measurements by Laser Techniques: Advances and Applications*, Enrico Primo Tomasini, Editor, Proceedings of SPIE Vol. 4827, page numbers (2002).

ISSN 0277-786X
ISBN 0-8194-4594-0

Published by
SPIE—The International Society for Optical Engineering
P.O. Box 10, Bellingham, Washington 98227-0010 USA
Telephone 1 360/676-3290 (Pacific Time) • Fax 1 360/647-1445
<http://www.spie.org/>

Copyright© 2002, The Society of Photo-Optical Instrumentation Engineers.

Copying of material in this book for internal or personal use, or for the internal or personal use of specific clients, beyond the fair use provisions granted by the U.S. Copyright Law is authorized by SPIE subject to payment of copying fees. The Transactional Reporting Service base fee for this volume is \$15.00 per article (or portion thereof), which should be paid directly to the Copyright Clearance Center (CCC), 222 Rosewood Drive, Danvers, MA 01923 USA. Payment may also be made electronically through CCC Online at <http://www.directory.net/copyright/>. Other copying for republication, resale, advertising or promotion, or any form of systematic or multiple reproduction of any material in this book is prohibited except with permission in writing from the publisher. The CCC fee code is 0277-786X/02/\$15.00.

Printed in the United States of America.

Reducing the mechanical hysteresis problem in optically-addressed diaphragm pressure sensors

S.A. Sharifian and D.R. Buttsworth*

Faculty of Engineering and Surveying, University of Southern Queensland, Australia

ABSTRACT

Mechanical hysteresis problems associated with pressure sensors based on interferometric measurements of diaphragm deflection are discussed. The source and importance of each contribution to the net hysteresis is calculated and compared with experimental results. Possible methods to decrease hysteresis effects are presented. Based on these suggested methods, new sensors have been manufactured and their hysteresis evaluated. The results demonstrate that significant reductions in hysteresis can be achieved with minimum cost. Future sensor development will focus on materials selection and manufacturing methods to fully realize these improvements.

Keywords: Hysteresis, optically-addressed pressure sensor, temperature sensitivity, pressure transducer, Fabry-Perot interferometer

1. INTRODUCTION

Mechanical hysteresis exists in all materials and will therefore affect the performance of pressure sensors that utilize a diaphragm. An illustration of mechanical hysteresis can be seen in the stress-strain curves for most materials: usually the curves are not precisely aligned in the increasing and decreasing load directions. Mechanical hysteresis results from friction-like irreversibilities which are dissipated as heat. The mechanical hysteresis effects can be minimized through proper choice of material and working stress level. For example, crystalline materials yield low hysteresis errors and diaphragms made of monocrystalline silicon show minimal hysteresis effects.¹ However, other optically-addressed sensor construction issues such as: 1) price; 2) reflectivity; and 3) availability in foil or thin sheet form, could limit the use of low mechanical hysteresis materials in some cases.

The pressure sensor arrangement considered in the present work closely follows that of MacPherson et al.^{2,3} in which copper diaphragms are bonded to zirconia ferrules (part of a standard fibre optic communications connector) using an epoxy. While results obtained with these devices have been very encouraging, the issue of mechanical hysteresis has not been addressed. In the present work, attempts are made to characterise and minimize the mechanical hysteresis effects associated with optically-addressed pressure sensors constructed from zirconia ferrules with bonded aluminium and copper diaphragms.

2. INTERFEROMETER AND CALIBRATION HARDWARE

The interferometer system used in the current work is illustrated in Figs. 1 and 2, and is very similar to the system used by MacPherson et al.^{2,3} Light from a 20mW laser diode at 780nm is launched into a single mode fibre attached to a 50/50 bi-directional coupler. Light reflects off the cleaved end of the fibre, which is located about 10 μm from the diaphragm and propagates back towards the signal detector. Some of the light transmitted into the air cavity couples back into the fibre after it reflects off the diaphragm and also propagates back towards the signal detector. Deflection of the diaphragm due to changes in the external pressure alters the length of the air cavity and thus the relative phase of the two reflected signals. Changes in the relative phase of the two reflected waves are identified as changes in the intensity at the signal detector.

A tube was used for the pressure calibration of the optically-addressed sensors. The tube was approximately 2m long with an internal diameter of 27.5mm. The tube initially contained air from the laboratory environment at the local atmospheric pressure and ambient temperature. The laboratory ambient temperature was approximately 18°C, and the local atmospheric pressure was around 94kPa (Toowoomba is approximately 800m above sea level). The tube pressure was increased by adding compressed air from a regulated supply, and the subsequent decrease in pressure was achieved by venting the tube to the atmosphere. Each optically-addressed pressure sensor was mounted in a plate that was bolted

*buttswod@usq.edu.au; Faculty of Engineering and Surveying, University of Southern Queensland, Toowoomba, 4350, Australia

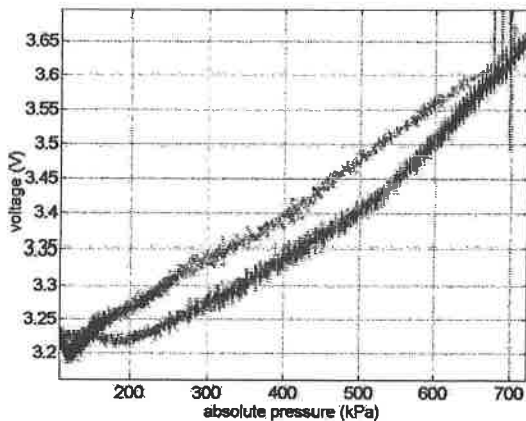


Figure 29: Calibration of a sensor made with 12.7µm thick copper (110) diaphragm after 500 pressure load cycles applied to the finished sensor

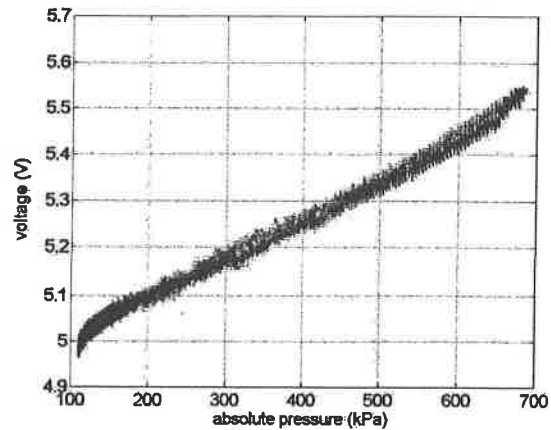


Figure 30: Calibration of the same sensor in Fig. 29 after 2000 pressure load cycles applied to the finished sensor

5. CONCLUSION

The hysteresis effects associated with fibre optically-addressed diaphragm pressure sensors have been investigated. It is demonstrated that without due attention to hysteresis issues, substantial problems are likely to be encountered. A number of techniques to reduce hysteresis effects have been proposed and investigated theoretically. Experimental results demonstrate the substantial reduction of hysteresis effects that can be achieved by: 1) tension load cycling the diaphragm material prior to bonding to the ferrule; and 2) pressure load cycling subsequent to sensor construction. Using the techniques outline in this publication, practical miniature pressure sensors with metallic diaphragms and a high measurement bandwidth can now be constructed at a low cost.

ACKNOWLEDGMENTS

The first author wishes to acknowledge financial support from an International Postgraduate Research Scholarship.

REFERENCES

1. M. Di Giovanni, *Flat and Corrugated Diaphragm Design Handbook*, Marcel Dekker, New York, 1982.
2. W.N. MacPherson, J.M. Kilpatrick, J.S. Barton, J.D.C. Jones, "Miniature fibre optic pressure sensor for turbomachinery applications," *Rev. Scientific Instr.* **70**, pp. 1868-1874, 1999.
3. W.N. MacPherson, M.J. Gander, J.S. Barton, J.D.C. Jones, C.L. Owen, A.J. Watson, R.M. Allen, "Blast pressure measurement with a high bandwidth fibre optic pressure sensor," *Meas. Sci. Technology* **11**, pp. 95-102, 2000.
4. *Structural adhesives directory and databook*, Chapman-Hall, London, 1996.
5. J.P. Holman, *Heat Transfer*, 6th edition, McGraw-Hill, Singapore, 1986.