

# Sensors in Assisted Living

*A survey of signal and image processing methods*

Our society will face a notable demographic shift in the near future. According to a United Nations report, the ratio of the elderly population (aged 60 years or older) to the overall population increased from 9.2% in 1990 to 11.7% in 2013 and is expected to reach 21.1% by 2050 [1]. According to the same report, 40% of older people live independently in their own homes. This ratio is about 75% in the developed countries. These facts will result in many societal challenges as well as changes in the health-care system,

such as an increase in diseases and health-care costs, a shortage of caregivers, and a rise in the number of individuals unable to live independently [2].

Thus, it is imperative to develop ambient intelligence-based assisted living (AL) tools that help elderly people live independently in their homes. The recent developments in sensor technology and decreasing sensor costs have made the deployment of various sensors in various combinations viable, including static setups as well as wearable sensors. This article presents a survey that concentrates on the signal processing methods employed with different types of sensors. The types of sensors covered are pyro-electric infrared (PIR) and vibration sensors, accelerometers, cameras, depth sensors, and microphones.

## Introduction

AL systems basically aim to provide more safety and autonomy and improve wellness and health conditions of older people while allowing them to live independently, as well as relieving the workload of caregivers and health providers.

A fundamental component of the AL systems is the use of different types of sensors to monitor the activities of the residents. These sensors can be broadly categorized into two groups: 1) static sensors at fixed locations, e.g., PIR sensors, vibration sensors, pressure sensors, cameras, and microphones, and 2) mobile and wearable sensors, e.g., accelerometers, thermal sensors, and pulse oximeters. There are several choices of specific sensors or sensor combinations—currently there are many AL

IMAGE LICENSED BY ANGRAM PUBLISHING  
WOMAN—© ISTOCKPHOTO.COM/SIMUWANSEN



systems implementing various tasks, such as fall detection [3]–[5], mobile emergency response [6], video surveillance [7], automation [8], monitoring activities of daily living [9], and respiratory monitoring [10]. Falls among the elderly are a major concern for both families and medical professionals. Falls are considered to be the eighth leading cause of death in the United States [11] and fall injuries can result in serious complications [12], [13]. Autonomous fall detection systems for AL can reduce the severity of falls by informing other people to deliver help and reduce the amount of time people remain on the floor. These systems can increase safety and independence of the elderly.

To truly assist elderly people, an AL system should satisfy some basic requirements [14]:

- *Low-cost*: Almost 90% of the older adults prefer to stay in the comfort of their own homes. Therefore, an AL system should be affordable by the average elderly person or couple.
- *High accuracy*: Since the aim is to enhance the wellness and the life quality of elderly people, a tolerable error rate should be achieved.
- *User acceptance*: The AL systems should be compatible with the ordinary activities of people so that they can interact with the system easily, i.e., by speaking naturally, using simple gestures, etc. Also, users do not find wearable systems or those that need to be carried practical. Thus, contact-free and remotely controllable systems are desired.
- *Privacy*: The AL systems should be non-visual and share minimal private data with the monitoring call center regarding the daily living activities of individuals.

Despite the presence of surveys [2], [15], [16] and proliferation of different types of sensors in the AL field, a comprehensive study concentrating on the utilized sensor signal processing methods is not available. This article aims to provide an overview of most recent research trends in the AL field by focusing on PIR sensors, vibration sensors, accelerometers, cameras, depth sensors, and microphones and the related signal processing methods, which together meet most of the aforementioned requirements. Ambient information monitoring sensors are used in home safety [17]–[19], home automation [8], [20]–[23], activity monitoring [14], [24]–[27], fall detection [28]–[34], localization and tracking [35]–[37], and monitoring the health status indicators of elderly and chronically diseased people outside hospitals [38]–[44].

## Human activity recognition using various sensor modalities

The most important signal processing problem in AL systems is the recognition of human activity from signals generated by various sensors including vibration sensors, PIR sensors, and wearable accelerometers. Obviously, each sensor generates different kinds of time-series data. Therefore, signal-processing

and machine-learning algorithms tailored for each specific sensor need to be developed.

### PIR sensor signal processing


PIR sensors are low-cost devices designed to detect the presence of moving bodies from stationary objects. They are easy to use and can even work in the dark, unlike ordinary vision-based systems, because they image infrared light. A PIR sensor functions by measuring the difference in infrared radiation between the two pyro-electric elements inside of it. This difference occurs due to the motion of bodies in the viewing range of the sensor. When the two pyro-electric elements are subject to the same infrared radiation level, they generate a zero-output signal by canceling each other out. Therefore, the analog circuitry of a PIR sensor can reject false detections very accurately.

PIR sensors are widely used in the context of AL. In [38], eight PIR sensors are installed in the ceiling of hospital rooms to assess the daily activities of elderly patients. The activities are classified in 24 different categories by checking the number of sensors activated and recording the time interval for which they remain activated. Barger et al. [24] introduce a system of distributed PIR sensors to monitor a person's in-home activity. The activity level of the person is defined as the number of sensor firings in a room per time spent in the room. Mixture models are applied to the sensor data in the training set to develop a probabilistic


model of event types. These models are then used to identify the type of event associated with each observation in the test set. In [27], a PIR sensor installed in a corner of a living room is employed to detect the abnormalities in daily activities of an elderly person. The PIR sensor sends the value “1” to the controller if there are activities from the person and the value “0” otherwise. Hidden Markov models (MMs), forward algorithms, and Viterbi algorithms are used to analyze the obtained data sequence. If a certain deviation from the constituted models is detected, the caregiver receives an alert. In [26] a wireless sensor network including PIR, chair, bed, toilet, and couch sensors is suggested to determine the wellness of the elderly. Time-stamped sensor activities are recorded and fed to predefined wellness functions.

In [25], PIR and contact sensors are used to assess neurologic function in cognitively impaired elders. The contact sensor is responsible for tracking the presence or the absence of the resident and recording the time spent in the home and out of the home. PIR sensors are utilized for the estimation of walking speed and daily activity. The walking speed of the resident is estimated from the time of PIR sensor firings that are placed sequentially along a hall. The amount of daily activity is decided based on the number of sensor firings per minute when the subject is in the home.


**The most important signal processing problem in AL systems is the recognition of human activity from signals generated by various sensors including vibration sensors, PIR sensors, and wearable accelerometers.**

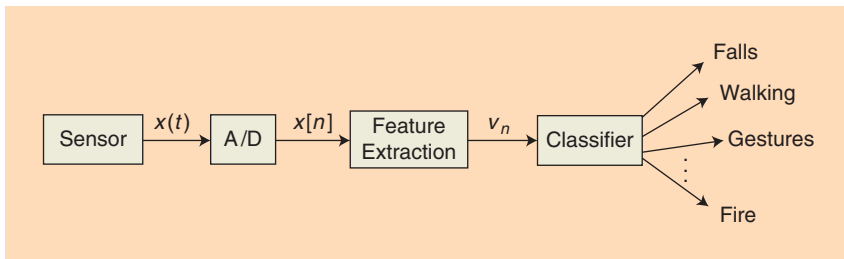

**FIGURE 1.** A block diagram of an intelligent PIR sensor signal processing system.

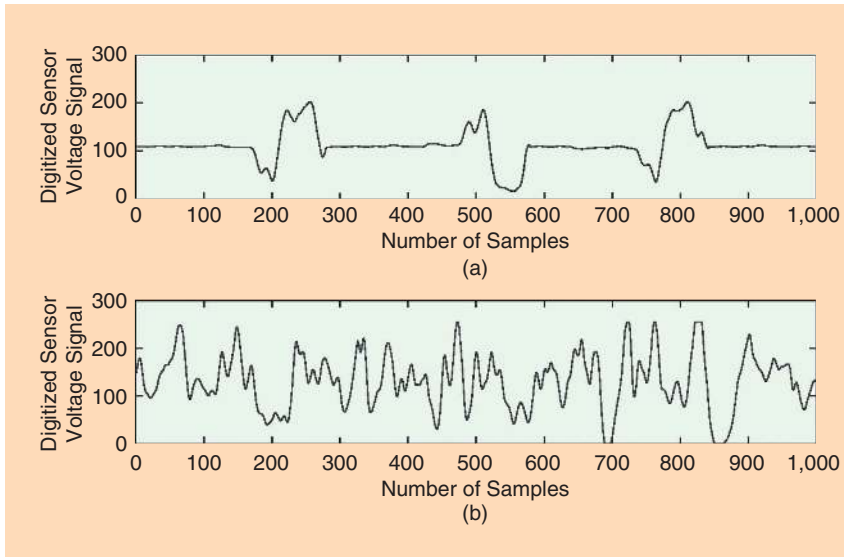

**FIGURE 2.** A PIR sensor raw output signal recorded at a distance of 5 m (a) for a person walking and (b) for a flame of an uncontrolled fire.

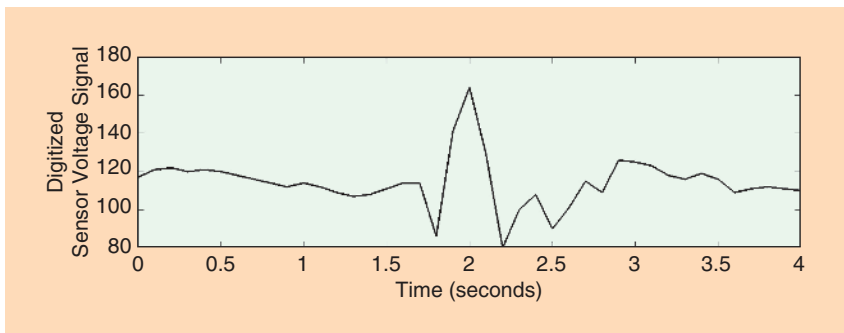

**FIGURE 3.** A time-domain PIR sensor signal record due to a person falling.

In [35], a system to actively assist in the resident's life such as housework, rest, sleep, etc. is described. The system is formed by an array of PIR sensors and locates a resident with a reasonable accuracy by combining the overlapping detection areas of adjacent sensors. In [17], an intruder detection system based on PIR sensors is developed. Mrazovac et al. [8] use a microphone array and a three-dimensional (3-D) camera in addition to PIR sensors for home automation, i.e., to detect the presence of and localize the users for smart audio/video playback control.

The aforementioned studies all use the binary outputs produced by the analog PIR motion detector circuits. However, it is possible to capture a continuous-time analog signal corresponding to the amplitude of the voltage signal of the PIR sensor that represents the transient behavior of the sensor circuit. By processing these analog signals, more complicated tasks, as opposed to just the on/off type operations, can be accomplished. The block diagram of an intelligent PIR sensor signal processing system is shown in Figure 1. The original output of the sensor signal  $x(t)$  is first digitized using an analog-to-digital converter. Feature vectors  $v_n$  are then extracted from the digitized signal  $x[n]$ . It is possible to extract a feature vector for each signal sample. However, it is computationally more efficient to extract a feature vector for a frame of data, as in speech processing systems. Finally, these feature vectors are fed to a classifier to detect the events of interest such as walking, falls, uncontrolled fires etc. The classifier is usually trained using past and/or simulated data.

A PIR sensor-based system for human activity detection is described in [19], [33], and [45]. The system is capable of detecting accidental falls and the flames of a fire. Instead of the binary signal produced by the comparator structure in the PIR sensor circuit, an analog output signal is captured and transferred to a digital signal processor for further processing. As shown in Figure 2(a), a walking event is almost periodic when the person walks across the viewing range of the sensor. On the other hand, a person falling produces a clearly distinct signature as shown in Figure 3, and uncontrolled flames lead to a signal with high-frequency content. Since flames of an uncontrolled fire flicker up to a frequency of 13 Hz, a sampling frequency of 50 Hz, which is well above

the Nyquist rate, is chosen. The goal is to recognize falls, uncontrolled fire events, and a person's daily activities. In practice, PIR signals are not as clearly distinguishable as the ones shown in Figures 2 and 3. For example, the person may walk toward the sensor and the periodic behavior is no longer clearly visible.

Wavelet transform is used for feature extraction from the PIR sensor signal. In the training stage, wavelet coefficients corresponding to each event class signals are computed and concatenated. Three, three-state MMs are designed to recognize the three classes. The characteristics of the

transitions between the three states of the MMs are different for each event class. The wavelet coefficient sequence corresponding to the current time window of two seconds is fed to the three MMs, and the MM producing the highest frequency determines the activity within the window. Uncontrolled flames are very accurately detected, since the sensor signal for a flickering flame exhibit high frequency activity that no person can produce by moving his or her body as shown in Figure 2(b).

It is not possible to distinguish a fall from sitting on the floor or a couch using only a single PIR sensor. In [33] and [45], multisensor systems are developed for fall detection. Sound, PIR, and vibration sensors are placed in a home. MMs are used as classifiers in these multisensor systems. They are trained for regular activities and falls of an elderly person using PIR, sound, and vibration sensor signals. Vibration and sound sensor data processing will be described in the next two sections. Decision results of MMs are fused by using a logical “and” operator to reach a final decision.

In [21], a remote control system is developed based on a PIR sensor array and a camera for home automation. The system recognizes hand gestures. The camera is responsible to detect the hands of the user. Once a hand is detected, simple hand gestures such as left-to-right, right-to-left, and clockwise and counterclockwise hand movements are recognized by the PIR sensor signal analysis to remotely interact with an electrical device. The system includes three PIR sensors, each of which is located at a corner of a triangle. Signals received from each PIR sensor are transformed into wavelet domain and then concatenated according to a predefined order. In this case, the distinctive property of the resulting wavelet features for different hand gestures is not the oscillation characteristics, but the order of the appearances of the peaks in the wavelet sequence. Therefore, the winner-take-all (WTA) hashing, which is an ordinal measure, is used for further feature extraction and classification instead of MMs. Wavelet sequences are converted to binary codes using the WTA hash method, and Jaccard distances are calculated between the trained and test binary codes. The model yielding the smallest distance is determined as the class of the current test signal. The system described in [21] produces higher recognition results than the system in [22], which uses only the binary outputs of the analog PIR sensor circuitry for the same task.

In [41], a method for the detection of breathing movement using PIR sensors is proposed. PIR sensors are placed near a person’s bed. Sensor signals, corresponding to body movements due to breathing activity, are recorded. Short-time Fourier analysis of the PIR sensors’ signals is carried out. The recorded signals are divided into windows, and the existence of sleep apnea within each window is detected by analyzing the spectrum. If there are no peaks in a window, that is an indicator of a sleep apnea. It may also be possible to measure the respiratory rate of a person who is sleeping using PIR sensor signals.

## Vibration and acoustic sensor signal processing

Accelerometers designed to measure vibration are either based on the piezoelectric effect or electromechanical energy conversion. They are transducers for measuring the dynamic acceleration of a physical device. All of the commercially available wearable fall detection systems are based on accelerometers. They convert vibrations into electrical signals depending on the intensity of the vibration waves in the axis of the vibration sensor. Vibration sensors can be categorized into two groups based on the number of their axes: one-axis and three-axes sensor types.

As mentioned previously, vibration sensors can be wearable or they can be installed on intelligent homes with the aim of sensing the vibrations on the floor. In this section, we first review the stationary systems.

Regular daily activities, such as walking, running, sitting on a chair, or objects falling on the floor cause measurable vibrations on the floor. Human falls also cause vibrations, which are transmitted through the floor. Therefore, a vibration sensor installed in each room of a house or an apartment can pick up the vibrations on the floor, and it may be possible

to detect a human’s fall by continuously analyzing the sensor signal. In Figure 4, a ten-second-long vibration sensor signal generated by a person walking is shown. It is clearly different from the human fall signal shown in Figure 5. This signal was recorded on a concrete floor and the fall took place 3 m away from the sensor. Human falls usually take about two seconds and create strong vibration signals because a typical human is more than 100 lb heavier than most of the objects that can


fall on the floor in a house. Machine-learning techniques can be used to classify the vibration signals.

In [33], a multisensor AL system consisting of PIR sensors and vibration sensors is developed. Vibration sensor signals are sampled with a rate of 500 Hz. As shown in Figure 5, there is very little signal energy above 125 Hz on a concrete floor. Since vibrations and acoustic and sound waves are related to each other, it is natural to use the feature extraction techniques utilized in speech processing to analyze the vibration signals. Various wavelet and frequency domain feature extraction schemes are employed every two seconds to extract feature vectors from the signals. Wavelet and different frequency analysis methods are studied and compared to each other. Discrete Fourier transform (DFT) subband energy values, MFCCs, discrete wavelet transform (DWT), and dual-tree complex wavelet transform (DT-CWT)-based feature extraction methods are studied for feature extraction [33]. These feature vectors are classified using a support vector machine (SVM) for fall detection. They can also be used to estimate a person’s daily activity and can provide feedback to him or her.


In [33], the data set contains 2,048-sample-long signals corresponding to 100 falls, 1,419 walking/running incidents, 30 sitting cases on the floor, 30 slammed door cases, and 65 cases of

**Even though several user-activated commercial devices are available for fall detection, they have limited benefits, especially in situations where the user loses consciousness.**



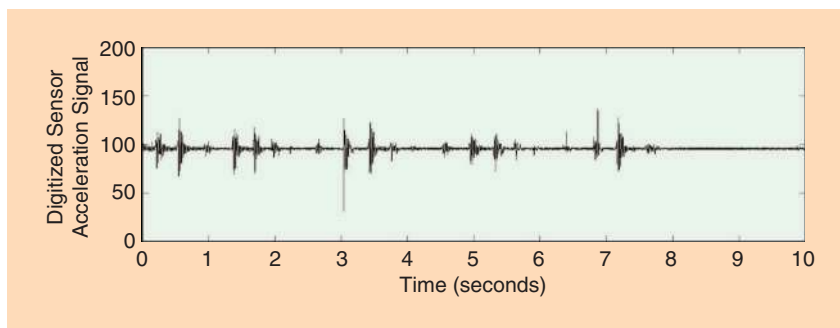

**FIGURE 4.** A ten-second-long vibration sensor signal generated by a person walking.

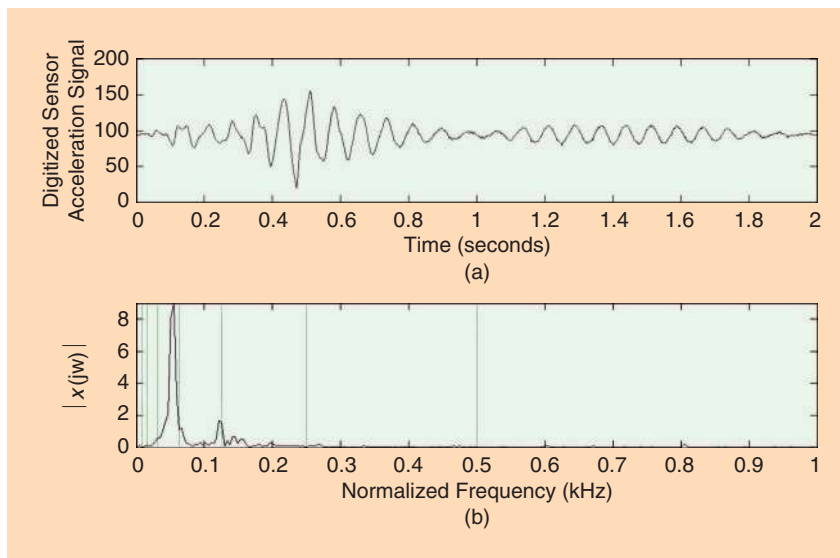

**FIGURE 5.** (a) A two-second-long human fall record. (b) The Fourier transform magnitude. The Fourier transform domain is divided into eight nonuniform bands, and subband energy values are used as a feature set representing the time-domain vibration signal together with wavelet coefficients and Mel-frequency cepstral coefficients (MFCCs).

fallen items. Eight MFCCs, eight DFT coefficients, eight wavelet coefficients, and eight CWT coefficients are extracted for each record. About 40% of falling and walking/running records are used for training the SVM classifier. About one-third of sitting, slammed door, and fallen object records are also used for training. Remaining records are used as the test data set. The data set is available to the public. Best recognition results are obtained when complex wavelet transform based features and modified mel-frequency cepstrum coefficients are used. When combined with PIR sensors the multisensor AL system becomes very reliable. The AL system has the capability to place a phone call to a call center whenever a fall is detected.


In [46], acoustic sensors are used instead of vibration sensors for fall detection. The acoustic sensor is placed like a stethoscope on the floor. In a practical system, it is desirable to

have a single vibration sensor unit installed on each floor of a house; however, there are some challenges. This unit has to be robust against variations on the type of the floor and the weight of the person as well as the distance between the sensor and the fall. The distance problem can be solved by installing two or more sensors, but this increases the cost. To cover all possibilities, extensive studies have to be implemented. In addition, the overall multisensor system described in [62] turns out to be a little bit too costly for a typical house and the network infrastructure. We hope that the Internet of Things (IoT) will be widespread in the near future, which will make the entire system feasible.

**AL systems may provide safety and autonomy for elderly people while allowing them to live independently, as well as relieve the workload of caregivers and health providers.**

#### *Wearable accelerometer sensor signal processing*

Even though several user-activated commercial devices are available for fall detection, they have limited benefits, especially

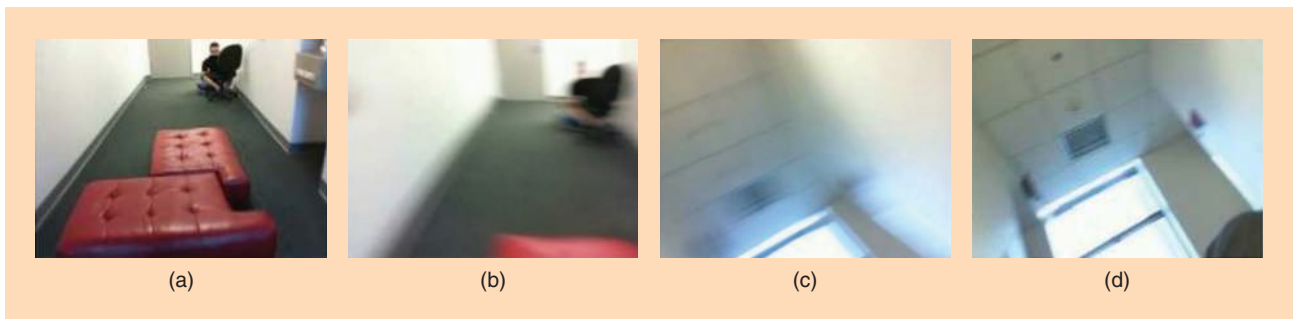

**FIGURE 6.** Example frames captured during a fall from a standing position.

in situations where the user loses consciousness. As previously mentioned, all commercially available autonomous fall detection systems are based on wearable accelerometers. Such systems can also provide information about an individual's functional ability and lifestyle. Wearable devices also use tilt sensors to automatically detect a fall event. One drawback is that the individual has to wear the device continuously day and night. On the other hand, monitoring is not limited to confined areas, where the static sensors are installed, and can be extended wherever the subject may travel.

Dai et al. [47] developed a fall detection system using the accelerometers of a mobile phone. The app is capable of detecting falls when the phone is placed in a shirt pocket, on a belt, or in a pants pocket. When the average magnitude of the 3-D acceleration vector and the average value of the vertical acceleration in a short-time window exceed predefined thresholds a fall is reported. In [48] and [49], adaptive thresholds are developed. In [48], the threshold is determined using the body mass index of the user. Currently, mobile phone apps are not widely used by elderly people. In addition, methods based on using thresholds cannot be as reliable as systems that use machine-learning techniques, since threshold-based methods are more prone to producing frequent false alarms.

In [50], artificial neural networks (ANNs) are used for human-activity recognition. A single triaxial accelerometer is attached to the subject's chest. Acceleration signals are modeled using autoregressive (AR) modeling. AR model coefficients along with the signal-magnitude area and the tilt angle form an augmented feature vector. The resulting feature vector is further processed by the linear-discriminant analysis and ANNs to recognize various human activities.

### *Camera sensor-based methods*

In recent years, one of the key aspects of elderly care has been intensive activity monitoring, and it is very important that any such activity monitoring be also autonomous. An ideal autonomous activity monitoring system should be able to classify activities into critical events, such as falling, and noncritical events, such as sitting and lying down. While fast and precise detection of falls is critical in providing immediate medical attention, other noncritical activities like walking, sitting, and lying down can provide valuable information in the study of chronic diseases and functional ability monitoring [51], [52] and

for early diagnosis of potential health problems. Furthermore, the system should be able to smartly expend its resources for providing quick and accurate real-time response to critical events versus performing computationally intensive operations for noncritical events.

There has been a lot of work on activity monitoring by vision-based sensors [28], [53]–[61]. However, in all of these methods, cameras are static at fixed locations watching the subjects, thus introducing the issue of confining the monitoring environment to the region where the cameras are installed. The images acquired from the cameras are usually offloaded to a dedicated central processor. Also, 3-D model-based techniques require initializations and are not always robust. Another major practical issue is that the subjects who are being monitored often raise privacy concerns [54], as they feel they are being watched all the time.

In contrast to static camera-based methods, Ozcan et al. [5] take a different approach, introducing an autonomous fall detection and activity classification system by using wearable embedded smart cameras. Since the camera is worn by the subject, the monitoring is not limited to confined areas and extends to wherever the subject may travel, as opposed to static sensors installed in certain rooms. In addition, since the images captured will not be of the subject, as opposed to static cameras watching the subject, privacy issues for the subjects is alleviated. Moreover, captured images are processed locally on the device, and they are not saved or transmitted anywhere. Only when a fall occurs can an appropriate message be wirelessly sent to emergency response personnel, optionally including an image from the subject's camera. This image of the surroundings can be helpful in locating the subject. Also, the captured images carry an abundance of information about the surroundings that other types of sensors cannot provide. A recent study about privacy behaviors of lifeloggers using wearable cameras discusses privacy of bystanders and ways to mitigate concerns [62]. It is also expected that wearable cameras will be employed more to understand lifestyle behaviors for health purposes [63].

The proposed approach [5] is based on the oriented image gradients. Different from the original histograms of oriented gradients (HOG), separate histograms for gradient strength and gradient orientations are constructed, and the correlation between them is found. The gradient orientation range is between 0–180°, and it is equally divided into nine bins. The



**FIGURE 7.** An Android smartphone attached to the waist.

gradient strength histogram contains 18 bins. Moreover, instead of using a constant number of cells in a block, the cells that do not contain significant edge information are adaptively and autonomously determined and excluded from the descriptor in this proposed modified HOG algorithm. In [5], it is shown that the proposed method is more robust compared to using fixed number of cells in detecting falls. In addition to detecting falls, the proposed algorithm provides the ability to classify events of sitting and lying down using optical flow. The method is composed of two stages. The first stage involves detection of an event. An event can be one of the following: falling, sitting, or lying down. Once an event is detected, the next stage is the classification of this event. An example set of captured frames for falling from standing up position is presented in Figure 6.

As reported in [5], the fall detection part of the algorithm was implemented on the CITRIC embedded camera platform [64], which is a small, stand-alone, battery-operated unit. It features a 624-MHz fixed-point microprocessor, 64 MB synchronous dynamic random access memory, and 16 MB NOR FLASH memory. The wireless transmission of data is performed by a Crossbow TelosB mote. The images are processed locally onboard, and then dropped, thus, they are not transferred anywhere. For the falls starting from a standing position, an average detection rate of 87.84% has been achieved with prerecorded videos. With the embedded camera implementation, the fall detection rate is 86.66%. Moreover, the correct classification rates for the events of sitting and lying down are 86.8% and 82.7%, respectively.

More recently, we have implemented the fall detection part of this algorithm on a Samsung Galaxy S4 phone with Android OS and performed experiments with ten subjects carrying this phone. The experimental setup can be seen in Figure 7. We have also implemented a method to fuse two sensor modalities: the accelerometer and camera data. The average sensitivity rates for fall detection are 65.66%, 74.33%, and 91%, when we use only accelerometer data, only camera data, and camera data together with accelerometer data, respectively.

**Vibration sensors can be categorized into two groups based on the number of their axes: one-axis and three-axis sensor types.**

Zhan et al. [65] propose an activity recognition method that uses a front-facing camera embedded in a user's eyeglasses. Optical flow is used as the feature extraction method. Three classification approaches—k-nearest neighbor, logitBoost, and SVM—are employed. Further smoothing with hidden MMs provide an accuracy of 68.5–82.1% for a four-class classification problem, including drinking, walking, going upstairs, and going downstairs, on recorded videos.

Moghimani et al. [66] use an RGB-D camera mounted on a helmet to detect the users' activities. They use compact and global image descriptors, including GIST, and a skin segmentation-based histogram descriptor. For activity classification, learning-based methods such as bag of scale invariant feature transform words, convolutional neural networks, and SVMs were explored.

Ishimaru et al. [67] propose an activity recognition method using eye blink frequency and head motion patterns acquired from Google glass. An infrared proximity sensor is used for blink detection. The average variance of a 3-D-accelerometer is calculated to construct the head motion model. In the classification framework, four features (variance value of accelerometer, mean value of blink frequency, and the x-center and y-center of mass value of the blink frequency histogram) have been used to classify five different activities (watching, reading, solving, sawing, and talking) on eight participants with overall accuracy of 82%.

## Conclusions

AL systems may provide safety and autonomy for elderly people while allowing them to live independently as well as relieve the workload of caregivers and health providers. However, to find widespread use, these systems should be robust and reliable. Current commercially available autonomous systems, which are not user activated, employ simple threshold-based algorithms for sensor data processing. As a result, they are prone to producing too many false alarms. Advanced signal processing techniques have to be developed to take full advantage of the recent developments in sensor technologies and provide robustness against variations in real-life conditions and the environment. Moreover, fusing multiple sensor modalities provides promising results with higher accuracy. Computational problems can be solved with the help of the IoT, which refers to wireless systems connecting industrial, medical, automotive, and consumer devices to the Internet. The IoT will allow objects and people to be sensed over existing Internet infrastructure. Vibration and PIR sensors, acoustic sensors and microphones, and cameras can be connected to form a network for an intelligent home designed for elderly people. The data and decision results that the sensors produce can be processed and fused over a cloud or a fog. We expect that the IoT will lead to remote health monitoring and emergency notification AL systems that will operate autonomously, without requiring user intervention.

## Acknowledgement

This work has been funded in part by the National Science Foundation (NSF) under CAREER grant CNS-1206291 and NSF grant CNS-1302559.

## Authors

**Fatih Erden** (fatih.erden@atilim.edu.tr) received his B.S. and M.S. degrees in electrical and electronics engineering with high honors from Bilkent University, Ankara, Turkey, in 2007 and 2009, respectively, and his Ph.D. degree in electrical and electronics engineering from Hacettepe University, Ankara, Turkey, in 2015. He is currently a faculty member of the Department of Electrical and Electronics Engineering at Atilim University, Ankara, Turkey. His research interests include sensor signal processing, infrared sensors, sensor fusion, multimodal surveillance systems, and pattern recognition. He received the Best Paper Award in the Fourth International Conference on Progress in Cultural Heritage Preservation organized by UNESCO and Cyprus Presidency of the European Union.

**Senem Velipasalar** (svelipas@syr.edu) received her B.S. degree in electrical and electronic engineering with high honors from Bogazici University, Istanbul, Turkey, in 1999; her M.S. degree in electrical sciences and computer engineering from Brown University, Providence, Rhode Island, in 2001; and her M.A. and Ph.D. degrees in electrical engineering from Princeton University, New Jersey, in 2004 and 2007, respectively. She is currently an associate professor in the Department of Electrical Engineering and Computer Science at Syracuse University, New York. Her research has focused on mobile camera applications, wireless embedded smart cameras, and multicamera tracking and surveillance systems. She received a Faculty Early Career Development Award from the National Science Foundation in 2011. She is the recipient of the Excellence in Graduate Education Faculty Recognition Award. She is a Senior Member of the IEEE.

**Ali Ziya Alkar** (alkar@hacettepe.edu.tr) received his M.S. and Ph.D. degrees in electrical and computer engineering from the University of Colorado at Boulder, in 1991 and 1995, respectively. He is currently an associate professor in the Department of Electrical and Electronics Engineering at Hacettepe University, Ankara, Turkey. He has worked as a consultant at several companies and has supervised several government and internationally funded projects. His research interests include image processing, networking, and video analytics in embedded systems. His awards include the Best Thesis Award from the Technology Development Foundation of Turkey and the Ihsan Dogramaci High Success Award. He is a Member of the IEEE.

**A. Enis Cetin** (cetin@bilkent.edu.tr) studied electrical engineering at Middle East Technical University, Ankara, Turkey. He received his M.S. and Ph.D. degrees from the University of Pennsylvania. Currently, he is a full professor at Bilkent University, Ankara, Turkey. He was previously an assistant professor at the University of Toronto, Canada. He is the editor-in-chief of *Signal, Image, and Video Processing* (Springer), and a member of the editorial boards of *IEEE Transactions on*

*Circuits and Systems for Video Technology* and *IEEE Signal Processing Magazine*. He holds four U.S. patents and is a Fellow of the IEEE.

## References

- [1] "World Population Ageing 2013," United Nations Department of Economic and Social Affairs, Population Division, Report ST/ESA/SER.A/348, 2013.
- [2] P. Rashidi and A. Mihailidis, "A survey on ambient-assisted living tools for older adults," *IEEE J. Biomed. Health Inform.*, vol. 17, no. 3, pp. 579–590, May 2013.
- [3] F. Ahmad, B. Jokanovic, M. G. Amin, and Y. D. Zhang, "Multi-window time-frequency signature reconstruction from undersampled continuous-wave radar measurements for fall detection," *IET Radar Sonar Navig.*, vol. 9, no. 2, pp. 173–183, Feb. 2015.
- [4] M. Popescu, Y. Li, M. Skubic, and M. Rantz, "An acoustic fall detector system that uses sound height information to reduce the false alarm rate," in *Proc. Annu. Int. Conf. IEEE Engineering in Medicine and Biology Society*, 2008, pp. 4628–4631.
- [5] K. Ozcan, A. K. Mahabalagiri, M. Casares, and S. Velipasalar, "Automatic fall detection and activity classification by a wearable embedded smart camera," *IEEE J. Emerg. Sel. Top. Circuits Syst.*, vol. 3, no. 2, pp. 125–136, 2013.
- [6] B. Silva, J. Rodrigues, T. Simoes, S. Sendra, and J. Lloret, "An ambient assisted living framework for mobile environments," in *Proc. IEEE-EMBS Int. Conf. Biomedical Health Informatics (BHI)*, 2014, pp. 448–451.
- [7] Z. Zhou, X. Chen, Y. C. Chung, Z. He, T. X. Man, and J. M. Keller, "Activity analysis, summarization, and visualization for indoor human activity monitoring," *IEEE Trans. Circuits Syst. Video Technol.*, vol. 18, no. 11, pp. 1489–1498, Nov. 2008.
- [8] B. Mrazovac, M. Z. Bjelica, I. Papp, and N. Teslic, "Smart audio/video playback control based on presence detection and user localization in home environment," in *Proc. 2nd Eastern European Regional Conf. Engineering Computer Based Systems*, 2011, pp. 44–53.
- [9] A. K. Bourke, S. Prescher, F. Koehler, V. Cionca, C. Tavares, S. Gomis, V. Garcia, and J. Nelson, "Embedded fall and activity monitoring for a wearable ambient assisted living solution for older adults," in *Proc. Annu. Int. Conf. IEEE Engineering in Medicine and Biology Society*, 2012, pp. 248–251.
- [10] M. Uenoyama, T. Matsui, K. Yamada, S. Suzuki, B. Takase, S. Suzuki, M. Ishihara, and M. Kawaki, "Non-contact respiratory monitoring system using a ceiling-attached microwave antenna," *Med. Biol. Eng. Comput.*, vol. 44, no. 9, pp. 835–840, 2006.
- [11] M. Heron, "Deaths: Leading causes for 2007," *Nat. Vital Stat. Rep.*, vol. 59, no. 8, pp. 1–95, 2011.
- [12] J. Sheller, D. Zapala, and L. Lundy, "Fall risk, vestibular schwannoma, and anticoagulation therapy," *J. Am. Acad. Audiol.*, vol. 19, no. 3, pp. 237–245, 2008.
- [13] R. C. O. Voshhaar, S. Banerjee, M. Horan, R. Baldwin, N. Pendleton, R. Proctor, N. Tarrier, Y. Woodward et al., "Predictors of incident depression after hip fracture surgery," *Am. J. Geriatr. Psychiatry*, vol. 15, no. 9, pp. 807–814, 2007.
- [14] S. Chernbumroong, S. Cang, A. Atkins, and H. Yu, "Elderly activities recognition and classification for applications in assisted living," *Expert Syst. Appl.*, vol. 40, no. 5, pp. 1662–1674, 2013.
- [15] F. Cardinaux, D. Bhowmik, C. Abhayaretne, and S. Mark, "Video based technology for ambient assisted living: A review of the literature," *J. Ambient Intell. Smart Environ.*, vol. 3, no. 3, pp. 253–269, 2011.
- [16] A. A. A. Chaaraoui, P. Climent-Perez, F. Florez-Revuelta, P. Climent-Pérez, and F. Flórez-Revuelta, "A review on vision techniques applied to human behaviour analysis for ambient-assisted living," *Expert Syst. Appl.*, vol. 39, no. 12, pp. 10873–10888, 2012.
- [17] M. Moghavvemi and L. C. S. L. C. Seng, "Pyroelectric infrared sensor for intruder detection," in *Proc. IEEE Region 10 Conf. TENCN*, 2004, vol. D., pp. 656–659.
- [18] F. Erden, E. B. Soyer, B. U. Toreyin, A. E. Çetin, and A. C. Enis, "VOC gas leak detection using pyro-electric infrared sensors," in *Proc. IEEE Int. Conf. Acoustics, Speech and Signal Processing (ICASSP)*, 2010, pp. 1682–1685.
- [19] F. Erden, B. U. Toreyin, E. B. Soyer, I. Inac, O. Gunay, K. Kose, and A. E. Cetin, "Wavelet based flickering flame detector using differential PIR sensors," *Fire Saf. J.*, vol. 53, pp. 13–18, Oct. 2012.
- [20] M. A. Sehili, D. Istrate, B. Dorizzi, and J. Boudy, "Daily sound recognition using a combination of GMM and SVM for home automation," in *Proc. European Signal Processing Conf. (EUSIPCO)*, 2012, pp. 1673–1677.
- [21] F. Erden and A. E. Cetin, "Hand gesture based remote control system using infrared sensors and a camera," *IEEE Trans. Consum. Electron.*, vol. 60, no. 4, pp. 675–680, Nov. 2014.
- [22] P. Wojtczuk, A. Armitage, T. Binnie, and T. Chamberlain, "PIR sensor array for hand motion recognition," in *Proc. SENSORDEVICES 2011: The 2nd Int. Conf. Sensor Device Technologies and Applications*, pp. 99–102.



- [23] M. Vacher, D. Istrate, F. Portet, T. Joubert, T. Chevalier, S. Smidtas, B. Meillon, B. Lecouteux et al., "The SWEET-HOME project: Audio technology in smart homes to improve well-being and reliance," in *Proc. Annu. Int. Conf. IEEE Engineering in Medicine and Biology Society*, 2011, pp. 5291–5294.
- [24] T. S. Barger, D. E. Brown, and M. Alwan, "Health-status monitoring through analysis of behavioral patterns," *IEEE Trans. Syst. Man Cybern. Part A Syst. Hum.*, vol. 35, no. 1, pp. 22–27, Jan. 2005.
- [25] T. L. Hayes, F. Abendroth, A. Adami, M. Pavel, T. A. Zitzelberger, and J. A. Kaye, "Unobtrusive assessment of activity patterns associated with mild cognitive impairment," *Alzheimers Dement.*, vol. 4, no. 6, pp. 395–405, Nov. 2008.
- [26] N. K. Suryadevara and S. C. Mukhopadhyay, "Determining wellness through an ambient assisted living environment," *IEEE Intell. Syst.*, vol. 29, no. 3, pp. 30–37, 2014.
- [27] G. Yin and D. Bruckner, "Daily activity learning from motion detector data for ambient assisted living," in *Proc. 3rd Int. Conf. Human System Interaction*, 2010, pp. 89–94.
- [28] A. N. Belbachir, S. Schraml, and A. Nowakowska, "Event-driven stereo vision for fall detection," in *Proc. IEEE Computer Society Conf. Computer Vision Pattern Recognition Workshops*, 2011, pp. 78–83.
- [29] R. Cucchiara, A. Prati, and R. Vezzani, "A multi-camera vision system for fall detection and alarm generation," *Expert Syst.*, vol. 24, no. 5, pp. 334–345, 2007.
- [30] L. Palmerini, F. Bagalà, A. Zanetti, J. Klenk, C. Becker, and A. Cappello, "A wavelet-based approach to fall detection," *Sensors*, vol. 15, no. 5, pp. 11575–11586, 2015.
- [31] M. Van Wieringen and J. Eklund, "Real-time signal processing of accelerometer data for wearable medical patient monitoring devices," in *Proc. Annu. Int. Conf. IEEE Engineering in Medicine and Biology Society*, 2008, pp. 2397–2400.
- [32] J. J. Villacorta, M. I. Jiménez, L. del Val, and A. Izquierdo, "A configurable sensor network applied to ambient assisted living," *Sensors*, vol. 11, no. 11, pp. 10724–10737, 2011.
- [33] A. Yazar, F. Keskin, B. U. Töreyn, and A. E. Çetin, "Fall detection using single-tree complex wavelet transform," *Pattern Recognit. Lett.*, vol. 34, no. 15, pp. 1945–1952, 2013.
- [34] B. U. Töreyn, Y. Dedeoglu, and A. E. Cetin, "HMM based falling person detection using both audio and video," in *Computer Vision in Human-Computer Interaction*, vol. 3766. Springer Berlin Heidelberg, 2005, pp. 211–220.
- [35] S. Lee, K. N. Ha, and K. C. Lee, "A pyroelectric infrared sensor-based indoor location-aware system for the smart home," *IEEE Trans. Consum. Electron.*, vol. 52, no. 4, pp. 1311–1317, Nov. 2006.
- [36] M. A. Stelios, A. D. Nick, M. T. Effie, K. M. Dimitris, and S. C. A. Thomopoulos, "An indoor localization platform for ambient assisted living using UWB," in *Proc. 6th Int. Conf. Advances in Mobile Computing and Multimedia*, 2008, p. 178.
- [37] A. Rajgarhia, F. Stann, and J. Heidemann, "Privacy-sensitive monitoring with a mix of IR sensors and cameras," in *Proc. Second Int. Workshop on Sensor and Actor Network Protocols and Applications*, 2004, pp. 21–29.
- [38] S. Banerjee, F. Steenkeste, P. Couturier, M. Debray, and A. Franco, "Telesurveillance of elderly patients by use of passive infra-red sensors in a 'smart' room," *J. Telemed. Telecare*, vol. 9, no. 1, pp. 23–29, Feb. 2003.
- [39] T. L. T. Hayes, M. Pavel, N. Larimer, I. A. I. Tsay, J. Nutt, and A. G. Adami, "Simultaneous assessment of multiple individuals," *IEEE Pervasive Comput.*, vol. 6, no. 1, pp. 36–43, 2007.
- [40] A. Hein, M. Eichelberg, O. Nee, A. Schulz, A. Helmer, and M. Lipprandt, "A service oriented platform for health services and ambient assisted living," in *Proc. Int. Conf. Advanced Information Networking and Applications Workshops*, 2009, pp. 531–537.
- [41] V. Hers, D. Corbugy, I. Joslet, P. Hermant, J. Demarteau, B. Delhougne, G. Vandermoten, and J. P. Hermanne, "New concept using passive infrared (PIR) technology for a contactless detection of breathing movement: A pilot study involving a cohort of 169 adult patients," *J. Clin. Monit. Comput.*, vol. 27, no. 5, pp. 521–529, Apr. 2013.
- [42] A. Jin, B. Yin, G. Morren, H. Duric, and R. M. Aarts, "Performance evaluation of a tri-axial accelerometry-based respiration monitoring for ambient assisted living," in *Proc. Annu. Int. Conf. IEEE Engineering in Medicine and Biology Society*, 2009, pp. 5677–5680.
- [43] S. Pasler and W.-J. Fischer, "Acoustical method for objective food intake monitoring using a wearable sensor system," in *Proc. 5th Int. Conf. Pervasive Computing Technologies for Healthcare Workshops*, 2011, pp. 266–269.
- [44] J. Sachs, M. Helbig, R. Herrmann, M. Kmec, K. Schilling, and E. Zaikov, "Remote vital sign detection for rescue, security, and medical care by ultra-wide-band pseudo-noise radar," *Ad Hoc Netw.*, vol. 13, part A, pp. 42–53, 2014.
- [45] B. U. Töreyn, E. B. Soyer, I. Onaran, and E. E. Cetin, "Falling person detection using multisensor signal processing," *EURASIP J. Adv. Signal Process.*, vol. 2008, Jan. 2008.
- [46] E. Principi, P. Olivetti, S. Squartini, R. Bonfigli, and F. Piazza, "A floor acoustic sensor for fall classification," in *Proc. 138th Audio Engineering Soc. Convention*, 2015, pp. 949–958.
- [47] J. D. J. Dai, X. B. X. Bai, Z. Y. Z. Yang, Z. S. Z. Shen, and D. X. D. Xuan, "PerFallD: A pervasive fall detection system using mobile phones," in *Proc. 8th IEEE Int. Conf. Pervasive Computing and Communications Workshops (PERCOM Workshops)*, 2010, pp. 292–297.
- [48] Y. Cao, Y. Yang, and W. H. Liu, "E-FallD: A fall detection system using android-based smartphone," in *Proc. 9th Int. Conf. Fuzzy Systems and Knowledge Discovery*, 2012, pp. 1509–1513.
- [49] G. A. Koshmak, M. Linden, and A. Loutfi, "Evaluation of the android-based fall detection system with physiological data monitoring," in *Proc. Annu. Int. Conf. IEEE Engineering in Medicine and Biology Society*, 2013, pp. 1164–1168.
- [50] A. M. Khan, Y. K. Lee, S. Y. Lee, and T. S. Kim, "A triaxial accelerometer-based physical-activity recognition via augmented-signal features and a hierarchical recognizer," *IEEE Trans. Inf. Technol. Biomed.*, vol. 14, no. 5, pp. 1166–1172, 2010.
- [51] D. W. Kang, J. S. Choi, J. W. Lee, S. C. Chung, S. J. Park, and G. R. Tack, "Real-time elderly activity monitoring system based on a tri-axial accelerometer," *Disabil. Rehabil. Assist. Technol.*, vol. 5, no. 4, pp. 247–253, 2010.
- [52] D. M. Karantonis, M. R. Narayanan, M. Mathie, N. H. Lovell, and B. G. Celler, "Implementation of a real-time human movement classifier using a triaxial accelerometer for ambulatory monitoring," *IEEE Trans. Inf. Technol. Biomed.*, vol. 10, no. 1, pp. 156–167, 2006.
- [53] M. Yu, A. Rhuma, S. M. Naqvi, L. Wang, and J. Chambers, "A posture recognition-based fall detection system for monitoring an elderly person in a smart home environment," *IEEE Trans. Inf. Technol. Biomed.*, vol. 16, no. 6, pp. 1274–1286, 2012.
- [54] N. Noury, A. Galay, J. Pasquier, and M. Ballussaud, "Preliminary investigation into the use of autonomous fall detectors," in *Proc. Annu. Int. Conf. IEEE Engineering in Medicine and Biology Society*, 2008, pp. 2828–2831.
- [55] G. Wu, "Distinguishing fall activities from normal activities by velocity characteristics," *J. Biomech.*, vol. 33, no. 11, pp. 1497–1500, 2000.
- [56] C. Rougier, J. Meunier, A. St-Arnaud, and J. Rousseau, "Fall detection from human shape and motion history using video surveillance," in *Proc. 21st Int. Conf. Advanced Information Networking and Applications Workshops (AINAW)*, 2007, vol. 2, pp. 875–880.
- [57] A. N. Belbachir, A. Nowakowska, S. Schraml, G. Wiesmann, and R. Sablatnig, "Event-driven feature analysis in a 4-D spatiotemporal representation for ambient assisted living," in *Proc. IEEE Int. Conf. Computer Vision*, 2011, pp. 1570–1577.
- [58] H. Foroughi, A. Naseri, A. Saberi, and H. S. Yazdi, "An eigenspace-based approach for human fall detection using integrated time motion image and neural network," in *Proc. 9th Int. Conf. Signal Processing*, 2008, pp. 1499–1503.
- [59] S. G. Miaou, P. H. Sung, and C. Y. Huang, "A customized human fall detection system using omni-camera images and personal information," in *Proc. 1st Transdisciplinary Conf. Distributed Diagnosis and Home Healthcare*, 2006, vol. 2006, pp. 39–42.
- [60] B. Jansen and R. Deklerck, "Context aware inactivity recognition for visual fall detection," in *Proc. Pervasive Health Conf. and Workshops*, 2007, pp. 1–4.
- [61] A. N. Belbachir, M. Litzemberger, S. Schraml, M. Hofstatter, D. Bauer, P. Schon, M. Humenberger, C. Sulzbachner et al., "CARE: A dynamic stereo vision sensor system for fall detection," in *Proc. IEEE Int. Symp. Circuits and Systems*, 2012, pp. 731–734.
- [62] R. Hoyle, R. Templeman, S. Armes, D. Anthony, D. Crandall, and A. Kapadia, "Privacy behaviors of lifeloggers using wearable cameras," in *Proc. ACM Int. Joint Conf. Pervasive and Ubiquitous Computing*, 2014, pp. 571–582.
- [63] A. R. Doherty, S. E. Hodges, A. C. King, A. F. Smeaton, E. Berry, C. J. A. Moulin, S. E. Lindley, P. Kelly et al., "Wearable cameras in health: The state of the art and future possibilities," *Am. J. Prev. Med.*, vol. 44, no. 3, pp. 320–323, Mar. 2013.
- [64] P. Chen, P. Ahammad, C. Boyer, S. I. Huang, L. Lin, E. Lobaton, M. Meingast, S. Oh et al., "Citric: A low-bandwidth wireless camera network platform," in *Proc. 2nd ACM/IEEE Int. Conf. Distributed Smart Cameras*, 2008, pp. 110.
- [65] K. Zhan, F. Ramos, and S. Faux, "Activity recognition from a wearable camera," in *Proc. 12th Int. Conf. Control Automation Robotics Vision*, Dec. 2012, vol. 2012, pp. 365–370.
- [66] M. Moghimi, P. Azagra, L. Montesano, A. C. Murillo, S. Belongie, D. Ia, C. Tech, and N. York, "Experiments on an RGB-D Wearable Vision System for Egocentric Activity Recognition," in *Proc. IEEE Conf. Computer Vision and Pattern Recognition Workshops*, 2014, pp. 611–617.
- [67] S. Ishimaru, K. Kunze, and K. Kise, "In the Blink of an Eye – Combining Head Motion and Eye Blink Frequency for Activity Recognition with Google Glass," in *Proc. 5th Augmented Human Int. Conf.*, 2014, pp. 15:1–15:4