

UC San Diego

UC San Diego Previously Published Works

Title

The international anorectal physiology working group (IAPWG) recommendations: Standardized testing protocol and the London classification for disorders of anorectal function.

Permalink

<https://escholarship.org/uc/item/573142hx>

Journal

Neurogastroenterology and motility : the official journal of the European Gastrointestinal Motility Society, 32(1)

ISSN

1350-1925

Authors

Carrington, Emma V
Heinrich, Henriette
Knowles, Charles H
et al.

Publication Date

2020

DOI

10.1111/nmo.13679

Peer reviewed

The international anorectal physiology working group (IAPWG) recommendations: Standardized testing protocol and the London classification for disorders of anorectal function

Emma V. Carrington¹  | Henriette Heinrich²  | Charles H. Knowles¹ | Mark Fox²  | Satish Rao³  | Donato F. Altomare⁴  | Adil E. Bharucha⁵  | Rebecca Burgell⁶ | William D. Chey⁷ | Guiseppe Chiarioni⁸ | Philip Dinning⁹ | Anton Emmanuel¹⁰ | Ridzuan Farouk¹¹ | Richelle J. F. Felt-Bersma¹² | Kee Wook Jung¹³  | Anthony Lembo¹⁴  | Allison Malcolm¹⁵ | Ravinder K. Mittal¹⁶  | François Mion¹⁷ | Seung-Jae Myung¹³ | P. Ronan O'Connell¹⁸ | Christian Pehl¹⁹ | Jose María Remes-Troche²⁰ | R. Matthew Reveille²¹ | Carolynne J. Vaizey²² | Veronique Vitton²³  | William E. Whitehead²⁴  | Reuben K. Wong¹¹ | S. Mark Scott¹ | All members of the International Anorectal Physiology Working Group

¹Queen Mary, University of London, London, UK

²University of Zürich, Zürich, Switzerland

³Medical College of Georgia, Augusta, Georgia, USA

⁴University Aldo Moro of Bari, Bari, Italy

⁵Mayo Clinic, Rochester, Minnesota, USA

⁶Monash University and Alfred Health, Melbourne, Victoria, Australia

⁷Michigan Medicine, Ann Arbor, Michigan, USA

⁸AOUI Verona, Verona, Italy

⁹Flinders University, Adelaide, South Australia, Australia

¹⁰University College London, London, UK

¹¹National University Hospital Singapore, Singapore City, Singapore

¹²UMC Amsterdam, Amsterdam, The Netherlands

¹³Asan Medical Center, Seoul, Korea

¹⁴Harvard Medical School, St. Boston, Massachusetts, USA

¹⁵University of Sydney and Royal North Shore Hospital, Sydney, New South Wales, Australia

¹⁶University of California, Berkeley, California, USA

¹⁷Université de Lyon et Hospices Civils de Lyon, Lyon, France

¹⁸University College Dublin, Dublin, Ireland

¹⁹Krankenhaus Vilsbiburg and Technical University Munich, Munich, Germany

²⁰University of Veracruz, Veracruz, Mexico

²¹University of Colorado, Denver, Colorado, USA

Abbreviations: ARM, Anorectal manometry; BET, Balloon expulsion test; C1, Level 1 consensus; C2, Level 2 consensus; C3, Level 3 consensus; DDV, Defecatory desire volume; FCSV, First constant sensation volume; HR-ARM, High-resolution anorectal manometry; IAPWG, International Anorectal Physiology Working Group; LLN, Lower limit of normal; MTV, Maximum tolerated volume; RAIR, Rectoanal inhibitory reflex; RST, Rectal sensory test; ULN, Upper limit of normal.

This is an open access article under the terms of the Creative Commons Attribution License, which permits use, distribution and reproduction in any medium, provided the original work is properly cited.

© 2019 The Authors. *Neurogastroenterology & Motility* published by John Wiley & Sons, Ltd.

²²St Mark's Hospital and Imperial College
London, London, UK

²³AP-HM - Aix-Marseille University,
Marseille, France

²⁴University of North Carolina at Chapel
Hill, Chapel Hill, North Carolina, USA

Correspondence

Emma V Carrington, The Wingate Institute,
26 Ashfield Street, London, UK.
Email: e.v.carrington@qmul.ac.uk

Funding information

Financial support was provided by grants from the United European Gastroenterology (UEG) Education Committee to the International Working Group for Disorders of Gastrointestinal Motility and Function and the European Gastrointestinal Motility Hub plus sponsorship from manufacturers of physiological measurement equipment including Sandhill Scientific/Diversatek, Medtronic, and Medical Measurement Systems/Laborie. The following working group members would like to declare specific funding sources: Adil Bharucha: NIH, NIDDK grant RO1 DK78924; Anton Emmanuel: Biomedical Research Centre UCL; Jose María Remes-Troche: Newton Foundation-CONACYT; Satish Rao NIH grants U-01DK109191 and 5R21DK104127-02; and William Whitehead: NIH grant U01DK115575.

Abstract

Background: This manuscript summarizes consensus reached by the International Anorectal Physiology Working Group (IAPWG) for the performance, terminology used, and interpretation of anorectal function testing including anorectal manometry (focused on high-resolution manometry), the rectal sensory test, and the balloon expulsion test. Based on these measurements, a classification system for disorders of anorectal function is proposed.

Methods: Twenty-nine working group members (clinicians/academics in the field of gastroenterology, coloproctology, and gastrointestinal physiology) were invited to six face-to-face and three remote meetings to derive consensus between 2014 and 2018.

Key recommendations: The IAPWG protocol for the performance of anorectal function testing recommends a standardized sequence of maneuvers to test rectoanal reflexes, anal tone and contractility, rectoanal coordination, and rectal sensation. Major findings not seen in healthy controls defined by the classification are as follows: rectoanal areflexia, anal hypotension and hypocontractility, rectal hyposensitivity, and hypersensitivity. Minor and inconclusive findings that can be present in health and require additional information prior to diagnosis include anal hypertension and dyssynergia.

Conclusions and Inferences: This framework introduces the IAPWG protocol and the London classification for disorders of anorectal function based on objective physiological measurement. The use of a common language to describe results of diagnostic tests, standard operating procedures, and a consensus classification system is designed to bring much-needed standardization to these techniques.

KEYWORDS

anorectal function testing, anorectal manometry, balloon expulsion test, functional anorectal disorders, rectal sensory test

1 | INTRODUCTION

Symptoms of anorectal dysfunction, characterized by fecal incontinence and/or constipation/evacuation disorders, affect the quality of life of between 1% and 5% of the population.¹ Anorectal manometry (ARM), the rectal sensory test (RST), and the balloon expulsion test (BET) are the best established investigations for objective assessment of anorectal sensorimotor function, and comprehensive assessment involves a series of measurements that describe voluntary and involuntary control of the anal canal, voluntary and involuntary (reflex) rectoanal coordination, evacuatory function, and rectal sensation.²⁻⁴

Several studies have demonstrated that variations in hardware and protocol (particularly for ARM) influence results of these investigations,⁴⁻⁸ and could impact diagnosis and management. Previous position statements and working party reports have already provided guidance on technique for data acquisition, analysis, and reporting.^{4,9-11} Despite this, a recent study conducted by our group showed ongoing widespread discordance in practice between institutions.¹²

Key Points

- Anorectal function tests (comprising anorectal manometry, the rectal sensory test, and the balloon expulsion test) are commonly used to evaluate patients with symptoms of anorectal dysfunction; however, practice varies significantly.
- This document summarizes consensus reached by the International Anorectal Physiology Working Group (IAPWG) for the performance of anorectal function testing and introduces a consensus classification for disorders of anorectal function based on objective, physiological measurement.
- The four-part London classification addresses (a) disorder of the rectoanal inhibitory reflex; (b) disorders of anal tone and contractility; (c) disorders of rectoanal coordination; and (d) disorders of rectal sensation. Findings are defined as major, minor, or inconclusive.

The introduction of high-resolution ARM (HR-ARM) has increased the spatial resolution of data acquisition and provides a continuous visualization of pressure activity from the rectum and the anal canal.¹³ This technique is now used in greater than 50% of institutions performing anorectal physiological tests.¹² However, this advancement has added a further element of variability in practice, and unless efforts are made early to reach consensus on test performance, this technique may fall victim to the same lack of standardization that has bedeviled other investigations (eg, transit studies) in the field.

The International Anorectal Physiology Working Group (IAPWG) was convened to establish consensus and set minimum standards for the clinical measurement of anorectal function, with a particular focus on HR-ARM. The following IAPWG consensus guidelines provide a standardized protocol for the performance of anorectal function testing applicable to devices produced by any manufacturer. In addition, the group presents the London classification system for disorders of anorectal function based on objective physiological measurements.

2 | METHODS

2.1 | The International Anorectal Physiology Working Group (IAPWG)

The IAPWG is a collaborative of 29 gastroenterologists, coloproctologists, and physiologists from 12 countries (Australia, France, Germany, Ireland, Italy, Mexico, Netherlands, Singapore, South Korea, Switzerland, United Kingdom, and United States) each with an academic interest and clinical practice in anorectal function testing. Six face-to-face meetings were held between 2014 and 2018 with each meeting involving at least 12 faculty members and 3 further rounds of remote voting were held between 2016 and 2018, with each round involving all 29 faculty members.

2.2 | Consensus process

The main objectives of the consensus process were to reach agreement on (i) a minimum standard investigation protocol for HR-ARM, RST, and BET; (ii) to describe appropriate metrics for describing anorectal function; and (iii) to develop a classification for the interpretation of test results to facilitate more consistent description of pathophysiology.

A combined consensus approach was taken, comprising a Quaker-based model for face-to-face meetings (the principle of which is to reach consensus through discussion, measuring dissent, and achieving unity) and a Delphi method for remote voting (with questionnaires emailed to panel members). Using the latter, consensus for each protocol/terminology statement and each element of the London Classification (titles, decision points, diagnoses, clinical significance, and footnotes) was attained using two rounds of remote voting. Each working group member had

the opportunity to choose “agree” (if they agreed with the statement/element as written), “minor concern” (if they agreed with the statement/element in principle but had minor concerns about its description), or “disagree” (if they disagreed with the statement/element as written). To facilitate the binary nature of consensus voting, agree and minor concern votes were amalgamated for counting purposes. Individuals were encouraged to raise points for discussion in a free-text manner. The results of the Delphi consensus were collated by members of the steering committee (HH, EVC, and SMS) and used to modify statements/elements accordingly prior to rediscussion.

The documented consensus levels represent the final level achieved. The number of participants (>12) and four rounds of written revisions fulfilled the basic criteria required for a guideline decision group (National Institute for Health and Clinical Excellence, April 2007)¹⁴ and allowed sufficiently reliable estimates at an acceptable cost in terms of travel expenses, etc. The heterogeneity of the group (specialty, nationality, expertise, and equipment used) was deemed desirable to be representative of a range of stakeholders. Agreement was defined without ‘weighting’ of any participant’s views, although some participants contributed more than others to the process. All authors approved the final document.

2.3 | Levels of consensus

Levels of consensus were defined in advance of voting as follows:

- C1—Level 1 consensus (excellent) defined as > 90% unanimity;
- C2—Level 2 consensus (moderate) defined as 75%–90% unanimity; and
- C3—Level 3 consensus (none) defined as < 75% unanimity.

3 | RESULTS AND RECOMMENDATIONS

Recommendations were categorized into (a) study preparation (comprising study indications, patient preparation, digital rectal examination, test specifications); (b) study protocol (comprising study sequence, standard instructions, maneuver definitions, and descriptions); (c) measurements; (d) description of normality; and (e) the London classification. For the protocol and terminology recommendations, the level of consensus (C1, C2, or C3) for each statement discussed has been reported immediately following the respective statement in the text and is shown in Table S1. For the classification system, the level of consensus for each element is shown in Table S2.

3.1 | Study indications

Anorectal function testing should be performed after referral from a suitable specialist practitioner after organic pathology has been appropriately excluded (C1). Indications may include the following:

- assessment of symptoms of constipation/evacuation disorder (C1)—for identification/quantification of abnormalities of rectoanal coordination, parameters of evacuation and rectal sensitivity (particularly rectal hyposensitivity), and assessment of megarectum/megacolon to exclude hypo/aganglionosis;
- assessment of symptoms of fecal incontinence (C1)—for identification/quantification of impaired anal sphincter function and abnormal rectal sensitivity (both hyper- and hyposensitivity);
- assessment of symptoms of functional anorectal pain (C1)—for identification/quantification of anal sphincter hypertension and abnormalities of rectoanal coordination and parameters of evacuation;
- preoperative assessment of anorectal function (C1)—for description of anal sphincter function and parameters of evacuation, particularly if intervention is associated with risks to continence (eg, fistulotomy and lateral sphincterotomy) or ability to evacuate (eg, rectopexy); and
- assessment of anorectal function in patients after obstetric injury/traumatic birth (C1)—if the clinician and patient wish to quantify anal sphincter function prior to future deliveries.

The use of anorectal function testing as a tool for biofeedback was acknowledged by the group; however, guidance was felt beyond the scope of this working party process.

3.2 | Patient preparation

Prior to the procedure, continuation of all existing medications is acceptable (C1). Patients may eat and drink up until the time of the test (C1). A clinical interview should clarify information such as presenting symptoms, medications and allergies, and pertinent past medical, surgical, and obstetric events. The use of bowel preparation is optional, and patients should be allowed to open their bowels before the procedure should they desire (C1). Preprocedure use of a water or phosphate enema is not contraindicated; however, the use of an enema should be documented to highlight the potential effects on function (C1). Documentation of any medications, particularly those known to affect anorectal function (including analgesics), is recommended (C1).

Prior to commencement of testing, the procedure should be explained, questions answered, and verbal consent obtained. Advice regarding written consent is beyond the remit of these recommendations, and clinicians should follow local or national policy (C1).

3.3 | Digital rectal examination

Although not expected to be fully diagnostic, a digital rectal examination should be performed before intubation to (a) provide an initial clinical assessment of pelvic floor structure, function, and sensitivity; (b) exclude local pathology and fecal loading (if fecal loading is demonstrated the investigator may consider the use of a tap water or phosphate enema); and (c) check patient understanding of standard instructions such as “squeeze” and “push”.

3.4 | Test specifications

3.4.1 | HR-ARM

A number of HR-ARM systems are commercially available.^{15,16} There is little evidence to support one particular configuration over another. Ideally, manometric sensors should record circumferential *not* unidirectional pressure (C1). Recommendations are based on the use of solid-state systems (C3) but also have relevance to those using water-perfused HR systems (C2). A minimum longitudinal recording length of 6 cm is required (C1). Thin, flexible catheters are recommended. Rigid, 'high-definition' catheters may be used, however are not considered standard (C1).

Studies should be performed in the left lateral position (C1) with the hips and knees flexed. To assist probe placement, a non-anaesthetizing lubricant should be used (C1).

Care should be taken to ensure that the base of any rectal balloon attached to the ARM catheter is sited 3-5 cm above the upper border of the anal canal, to prevent the balloon impinging upon the anal canal during inflation (C1). The most distal recording sensor should be external to anal verge (C1). If any pain or discomfort is experienced, the probe should be immediately withdrawn. If, on second insertion, there is further discomfort, a medical assessment should be sought.

3.4.2 | RST

The test should also be performed in the left lateral position with hips and knees flexed (C1). Studies may be conducted with either an integrated balloon on the manometric probe or with a separate system (C2). Balloon capacity should be no less than 400 ml (as healthy volunteer studies indicate that the upper limit for maximum tolerated volume in health is no greater than 350 ml)^{17,18} (C2) and all components should be latex-free (C1). Either ramp (continuous) or phasic distension can be used¹⁹ (C1) though it should be noted that the results derived from each method are not interchangeable. Insufflation should always be performed with air (C1). For ramp distension, the rate should be between 1 and 5 mL/s, and for phasic distension, inflation rate should be set at 10 mL/s (C1).

3.4.3 | BET

The balloon expulsion test should ideally be performed using a flexible catheter, up to 16 Fr in diameter, with a non-latex, compliant balloon attached at the tip (C2). A fixed volume of 50 mL tepid water is recommended for balloon distension (C1), which should be introduced with the subject lying in the left lateral position. To perform the study, the subject should then be transferred to a sitting position, ideally on a toilet in privacy behind a curtain.²⁰⁻²² Alternative tests (eg, barium or MR defecography) may be employed to assess parameters of evacuation instead of BET (C1), although it should be noted that diagnostic agreement between these tests is fair at best.²³ The details of such methods were not discussed in this round of consensus.

4 | STUDY PROTOCOL

4.1 | Study sequence

The agreed standardized protocol for anorectal function testing is outlined in Figure 1, and this scheme as a whole achieved unanimity (C1). Particular attention should be paid to the recommended maneuver durations and to the recovery intervals between maneuvers. The levels of consensus reached for each element of the protocol are outlined in Supplementary Table 1 and are further described in "maneuver descriptions" below. The study time for the IAPWG protocol of HR-ARM, RST, and BET is expected to be between 15 and 20 minutes, though total time including a clinical assessment will vary between institutions.

4.2 | Maneuver descriptions

4.2.1 | HR-ARM

Stabilization period: Following catheter insertion and prior to test maneuvers, a 3-minute period of stabilization should be observed to allow anal tone to return to baseline after intubation (C1).

Rest: This is the maneuver that measures basal anal tone at rest. It is measured over 60-s (C2). During recording, the patient should be reminded to relax and remain quiet to avoid movement artifact (C1). During this maneuver, and during the familiarization period, ultraslow waves (occurring at a frequency of 0.5-2 cycles per minute) may be seen.

Squeeze: This is the maneuver that records the anal pressure during voluntary effort to contract the anus/pelvic floor (C1). Three squeezes are performed during the protocol, each of 5-second duration separated by a 30-s between-maneuver recovery interval. The best of three attempts is used for analysis (C1).

Long (endurance) squeeze: This is the maneuver that records the anal pressure during sustained voluntary effort over 30 seconds aiming principally to describe fatigue over time rather than purely contractile ability as measured during 'squeeze' (above). A single endurance squeeze is performed followed by a 60-s between-maneuver recovery interval (C1).

Cough: This is the maneuver that measures rectoanal pressure changes during cough, that is, assesses the reflex increase in anal sphincter pressure during an abrupt change in intra-abdominal/intrapelvic pressure. Two coughs are performed separated by a 30-s between-maneuver recovery interval. It is important that the practitioner ensures adequate effort during this maneuver and that each cough is a single (not double or multiple) cough. The best attempt (defined as the attempt associated with the greatest increase in rectal pressure) is used for analysis (C1).

Push: This is the maneuver that measures anal and rectal pressure changes during simulated defecation. Three pushes are performed during the protocol, each of 15-s duration (C3) separated by 30-s between-maneuver recovery intervals. Rectal balloon insufflation is not mandated during this maneuver (C1). Due to the high rate of false-positive results related to patient and technical factors,²

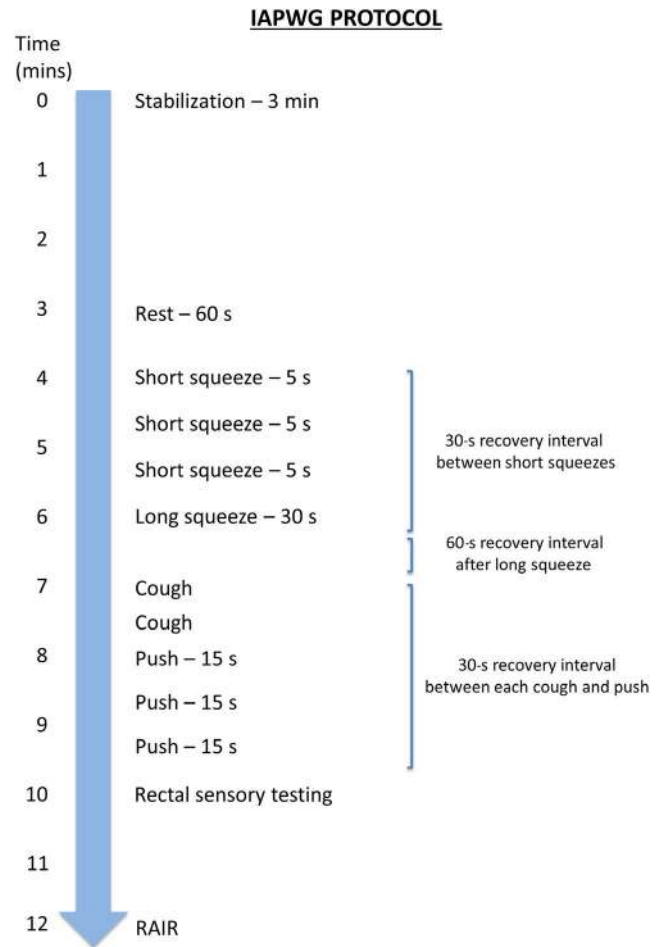


FIGURE 1 Schematic of the IAPWG standard protocol for high-resolution anorectal manometry and rectal sensory testing. The balloon expulsion test should be performed either immediately before or after this protocol of anorectal manometry and rectal sensory testing

the best (defined as the most qualitatively normal) of three attempts should be used for analysis (C1).

RAIR: This is the procedure which measures reflex anal response to rapid rectal distension. A normal response is characterized by an anal pressure decrease during rectal balloon distension. A single RAIR is performed with a starting volume of at least 30 mls, though it should be noted that failure to elicit the RAIR may be seen with low distending volumes in a large capacity rectum. Therefore, if megarectum is suspected, the test should be repeated with increasing balloon volumes (C1).

4.2.2 | RST

Rectal sensory test: This is the procedure that assesses rectal sensitivity to distension utilizing a rectal balloon placed at least 3-5 cm above the upper border of the anal canal (C1). The balloon volume is recorded for each of three patient-reported sensory thresholds: first constant sensation volume (FCSV), desire to defecate volume (DDV), and maximum tolerated volume (MTV) (C1). A fourth sensory threshold (sustained urgency volume) is optional (C1).

TABLE 1 Table describing recommended measurements for high-resolution anorectal manometry, the balloon expulsion test, and the rectal sensory test

Test	Maneuver	Measurement	Definition	Measurement type		
				Quantitative	Qualitative	Consensus
HR-ARM	Rest	Anal resting pressure	Mean maximum pressure measured from the whole anal canal over a 60-second recording period	x		C1
		Ultraslow waves	The presence of repeated pressure oscillations within the anal canal, occurring at 1-2 per min		x	C1
Squeeze		Anal squeeze pressure	Maximum incremental pressure observed during the 5-s short squeeze	x		C2
	Long squeeze	Endurance squeeze pressure	The duration of time the subject under study can voluntarily sustain an increase in anal pressure > 50% of maximum incremental squeeze pressure during the 30-second long squeeze	x		C1
Push		Rectal pressure change during push	Maximum pressure change recorded within the rectum during the push manoeuvre	x		C1
		Anal pressure change during push	Maximum pressure change recorded within the anal canal during the push manoeuvre	x		C1
Cough		Rectal pressure during cough	Maximum pressure recorded within the rectum during the cough manoeuvre	x		C1
		Anal pressure during cough	Maximum pressure recorded within the anal canal during the cough manoeuvre	x		C1
RAIR		Rectoanal inhibitory reflex	Reflex reduction in maximum anal pressure in response to rapid distension of the rectum		x	C1
		Balloon expulsion time	Time taken in seconds to expel a rectal balloon	x		C1
RST		First sensation volume	The minimum balloon insufflation volume required to elicit a sensory response	x		C1
	sensory thresholds ^c	Desire to defecate volume	The balloon insufflation volume required to elicit a sustained desire to defecate	x		C1
		Maximum tolerated volume	The balloon insufflation volume that causes an intolerable desire to defecate	x		C1

Abbreviations: HR-ARM: high-resolution anorectal manometry, RAIR: rectoanal inhibitory reflex, BET: balloon expulsion test, RST: rectal sensory test.

^aThe volume required to elicit the RAIR should also be documented.

^bThe presence or absence of the desire to defecate during the procedure should also be documented.

^cSustained urgency volume threshold is optional and defined as the balloon insufflation volume required to elicit a sense of fecal urgency.

4.2.3 | BET

Balloon expulsion: This is the procedure that measures ability, based on time taken, for a subject to expel a balloon from the rectum (C1).

4.3 | Standard instructions

Instruction and verbal feedback have been demonstrated to influence the results of anorectal function testing, particularly HR-ARM, and therefore, consistency of command is essential.⁸ The following statements have been provided as examples of how to simply describe test components, though it should be noted that significant cultural variation exists and that the exact language used for each instruction was not subject to consensus voting. Patient understanding of the commands should be assessed during clinical examination to prevent suboptimal results. During the study, instructions should be given shortly before each maneuver (C2).

4.3.1 | HR-ARM

Short squeeze: "Squeeze as hard as you can for 5-s as though you are stopping yourself passing wind or stopping yourself opening your bowels."

Long (endurance) squeeze: "Squeeze as hard as you can for as long as you can." The practitioner should give cues every 5-s saying "keep squeezing, keep squeezing."

Cough: "Please give a single cough." The practitioner should demonstrate a cough and emphasize that a single (not double) cough is required.

Push: "Push down as though you are sitting on the toilet opening your bowels/ passing a bowel movement/ trying to defaecate."

4.3.2 | RST

"I am going to put some air into the balloon. Tell me when you first feel a sensation inside your bottom that doesn't go away" (first constant sensation volume), "when you feel a constant urge to defaecate/ open your bowels" (desire to defecate volume), "and when it becomes too uncomfortable and you need me to stop" (maximum tolerated volume).

4.3.3 | BET

"Try to push the balloon out into the toilet like you're opening your bowels/ passing a bowel movement/ trying to defaecate."

4.4 | Measurements

A combination of qualitative and quantitative measurements for describing outcomes is recommended with definitions and units outlined in Table 1.

4.5 | Description of normality

In this first iteration of recommendations, due to the variability of existing equipment, protocol, and practice, it was felt beyond the remit of the group to recommend specific normal values. However, the description of normality was the subject of significant discussion. The following recommendations were agreed upon:

- if normal values are based on published data, equipment setup and procedure should be identical to that described in the referenced manuscript (C1); and
- if normal values are based on a local study of healthy volunteers, some consideration should be taken to appreciate variability seen in gender (C1), parity (C2), and age (C2).

4.6 | The London classification of anorectal physiological dysfunction

The following classification was developed to describe findings from the combined results of HR-ARM, BET, and RST.

Due to the multicomponent nature of anorectal function testing, it has been divided into four parts and a single study may have an outcome associated with more than one part of the classification:

- Part 1: disorder of the rectoanal inhibitory reflex (Figure 2);
- Part 2: disorders of anal tone and contractility (Figure 3);
- Part 3: disorders of anorectal coordination (Figure 4);
- Part 4: disorders of rectal sensation (Figure 5).

As per the Chicago Classification of esophageal motility disorders,²⁴ diagnoses are categorized accordingly:

- a *major finding* is a pattern not seen in control subjects and is likely to represent a physiological alteration associated with symptom generation;
- a *minor finding* is a pattern that is seen in patients with anorectal symptoms, however may also be seen in control subjects and may represent a physiological alteration associated with symptom generation; and
- an *inconclusive finding* is a pattern that is seen in patients with anorectal symptoms, but also seen in control subjects. Such findings may be associated with symptom generation, though the relevance is yet to be fully determined.

It should be noted that the results of two maneuvers (cough and long squeeze), though described in the protocol, do not form part of the diagnostic classification. The consensus group acknowledges the widespread use of these maneuvers but did not feel that inclusion in the classification could be justified at the present time.

For the purposes of uniformity, the diagnostic classification introduces some key terms to describe physiological features of

interest: (hypo/hyper)*tension* to describe anal resting tone, (hypo)-*contractility* to describe anal squeeze, *expulsion* to describe ability to expel a rectal balloon, *propulsion* to describe generation of an adequate increase in rectal pressure during push, *dyssynergia* to describe failure of coordinated anal relaxation during push, and (hypo/hyper)-*sensitivity* to describe rectal sensation.

Levels of agreement for each element of this classification are presented in Table S2.

5 | DISCUSSION

As patient-reported symptoms are known to be a poor indicator of underlying pathophysiology,^{18,25} anorectal function testing should be seen as a necessary component of clinical evaluation for patients in whom advanced management strategies are being considered.² The IAPWG recommendations for the performance and interpretation of anorectal manometry (ARM), the rectal sensitivity test (RST), and the balloon expulsion test (BET) mark a major step forward in the field of these investigations and, in particular, provide the first consensus-based approach to standardization of these investigations in the high-resolution (HR)-ARM era. Though little HR-ARM-specific guidance is presented, we see this as the necessary bridge to uptake of this technology as a whole. Additionally, the group presents “The

London Classification” for the diagnosis of disorders of anorectal function based on objective, physiological measurements. The clinical relevance of findings is indicated by the hierarchical division of findings into (a) major disorders that are not seen in health; (b) minor disorders that may be pathological in patients with symptoms, but that can also be seen in health; and (c) inconclusive findings that may be pathological but that require confirmation by additional testing. This approach follows the model of the Chicago Classification for disorders of esophageal motility and the Lyon Classification for gastroesophageal reflux disease.^{24,26} The IAPWG envisage that, similar to progress made in the upper gastrointestinal tract,²⁷ agreement on the performance and analysis of anorectal tests will improve the quality of investigations wherever applied, facilitate results interpretation, collaborative research, and technique development.

This new framework provides a common language with which to describe results of anorectal function testing and as such should be viewed as complimentary to existing disease classifications such as the Rome Classification.²⁸ The anorectal disorders section of Rome defines disease entities based on a combination of symptoms and physiological findings but provides limited advice on how to describe abnormal results. The IAPWG protocol and the London Classification provide a standard nomenclature for description of alterations in motor and sensory anorectal function. This working party propose that such a framework be embraced by a future iteration of Rome

LONDON CLASSIFICATION PART 1: DISORDER OF THE RECTOANAL INHIBITORY REFLEX

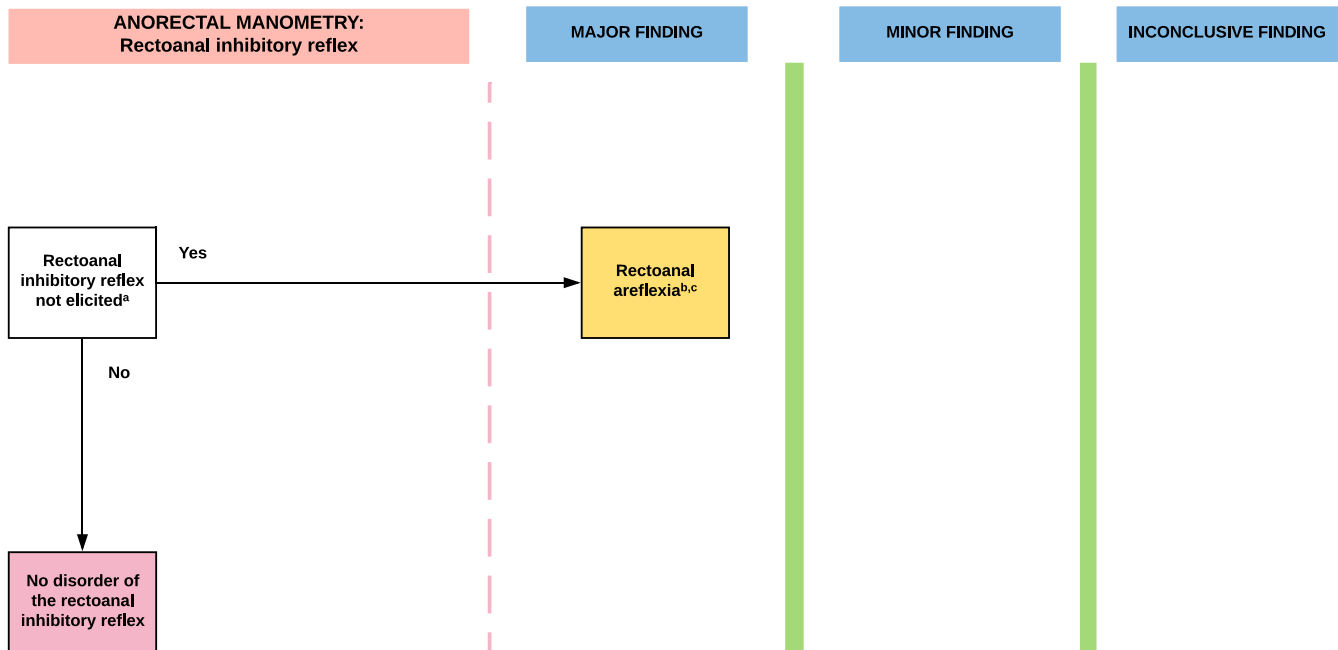


FIGURE 2 IAPWG classification part 1: Disorder of the rectoanal inhibitory reflex. For this and subsequent figures, the diagrams are color-coded for clarity: (i) white boxes represent manometric findings or decision points; (ii) yellow boxes represent the resultant diagnosis; and (iii) pink boxes represent a 'negative/normal' study. ^aMinimum volume required to elicit reflex not established in the literature: failure to elicit a RAIR may be seen with low distending volumes in a large capacity rectum. ^bRAIR not elicited is a pattern not seen in health but may be found in asymptomatic patients following rectal resection / ileal pouch anal anastomosis, anal hypotonia, faecal loading or megarectum. ^cMay indicate the need for further investigation to exclude aganglionosis especially in paediatric populations and adult patients with co-existent megarectum/megacolon. All results to be interpreted in the context of adjunctive testing

LONDON CLASSIFICATION PART II: DISORDERS OF ANAL TONE AND CONTRACTILITY

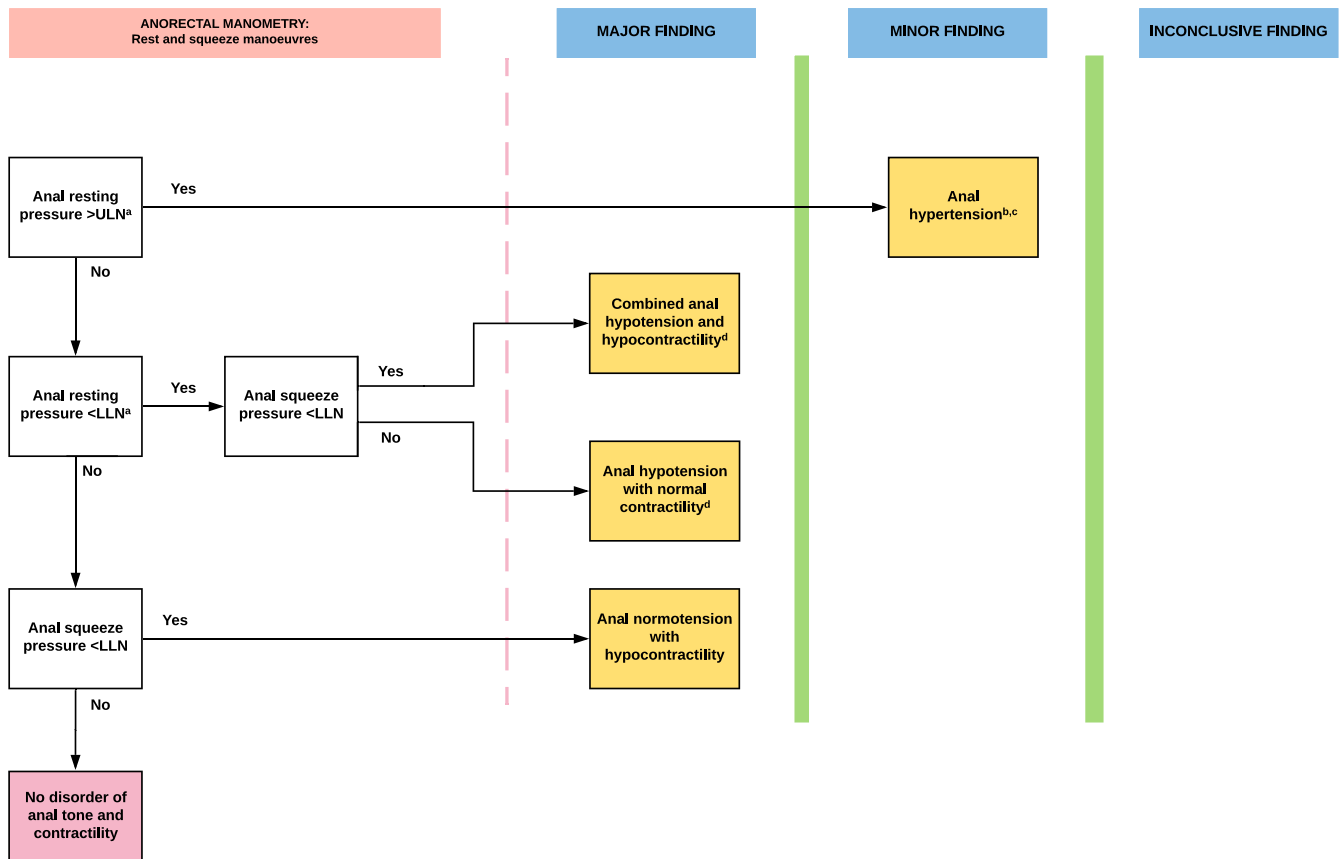


FIGURE 3 IAPWG classification part 2: Disorders of anal tone and contractility. ^aThe functional anal canal length may be measured, as a short anal canal can be associated with anal hypotonia, but its use as a diagnostic criterion in isolation is unproven. ^bmay be associated with slow and/or ultraslow waves, however the clinical significance of these has not been established. ^cthis finding may have greater clinical significance in certain patient groups (e.g. chronic anal fissure, levator ani syndrome or proctalgia fugax). ^daddition of an abnormal cough response may indicate a more severe phenotype (whereas preservation may suggest a target for biofeedback) but its use as a diagnostic criterion is unproven. All results to be interpreted in context of adjunctive testing LLN: Lower limit of normal ULN

where both incontinence and constipation/evacuation disorders could be subclassified according to physiological phenotypes. Given the results of recent studies that suggest treatment response differs according to the underlying causes of incontinence²⁹ and constipation,³⁰ a clear definition of disease phenotypes has the potential to aid treatment stratification and clinical outcomes.

5.1 | Limitations

The group acknowledge a number of limitations of this consensus document. Firstly, due to the nature of variability in current practice, paucity of data supporting protocol elements, and in particular the recent introduction of HR-ARM, the vast majority of recommendations reflect coalescence of expert opinion, rather than systematic review of clinical evidence. The reader should therefore bear in mind that what is not normal does not necessarily constitute disease and that outcome studies to assess the clinical utility of this classification for the direction of specific interventions are needed with refinement of the classification system as further data emerge.

Nevertheless, we believe that further improvement in practice can only begin from a common starting point, and the presented consensus reflects that sentiment.

Secondly, due to the nature of the task in hand, the consensus describes only 3 simple office-based tests of function. In particular, as multiple factors are involved in the control of continence and evacuation, the RST and the BET are generally considered as screening tests to be used prior to full assessment with other investigations. Should an abnormality be demonstrated, a comprehensive pelvic floor evaluation may involve more thorough assessment with complimentary investigations of structure or function such as endoanal ultrasound, barium/magnetic resonance defecography, and the rectal barostat which may confirm (or refute) physiological findings such as dyssynergia^{31,32} that are currently labeled as 'inconclusive' by the London Classification. It should be noted however (with particular regard to tests of evacuation) that there is considerable disagreement between the results of available investigations,²³ and though defecography has the advantage of better describing anatomical vs. functional causes of impaired evacuation, the BET in

LONDON CLASSIFICATION PART III: DISORDERS OF RECTOANAL COORDINATION

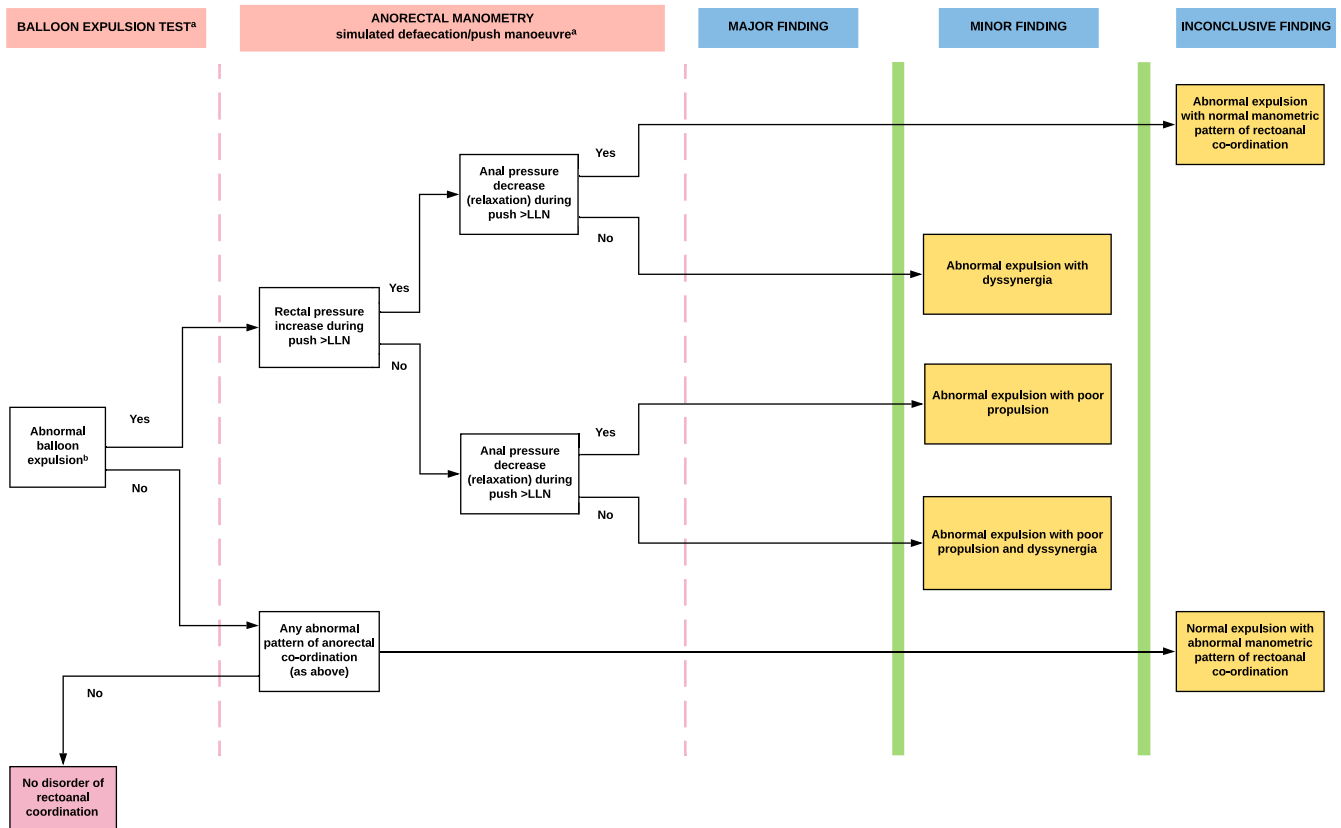


FIGURE 4 IAPWG classification part 3: Disorders of rectoanal coordination. ^arequires the use of both balloon expulsion test and anorectal manometry. ^bor impaired evacuation of contrast medium (prolonged evacuation end time and/or reduced percentage of contrast emptied) on alternative testing e.g. barium or MR defaecography. All results to be interpreted in context of adjunctive testing

particular is the only test which has been shown to predict the response to biofeedback.³⁰

Thirdly, due to the heterogeneity of current data and equipment available, we have not recommended specific, quantitative 'reference limits' for diagnosis of anorectal disorders but, instead, have elected to describe findings in accordance with the upper and lower limits of 'normal'. We acknowledge that female sex, advanced age, and parity are associated with a deleterious effect on sphincter and rectal sensory function and that normal ranges should reflect this. With time, based on the IAPWG protocol, normograms for the physiological variables will be generated as they have been for other biomarkers that vary with age in healthy women and men (eg, bone density³³).

Finally, although it was the aim of this group to facilitate standardization of *high-resolution* manometry, all current recommendations can be applied to conventional technology. This was principally because little published data existed to specifically support additional benefits of HR-ARM. These data are now emerging with recently published evidence, suggesting improved diagnostic accuracy of HR-ARM,^{34,35} and describing novel functional metrics which may prove worthy of inclusion in further iterations of this classification.³⁶ It is clear that publication of the Chicago Classification soon after high-resolution esophageal manometry 'moved from research into

clinical practice' was instrumental in driving its acceptance.³⁷ It is only at a later stage that esophageal HRM was shown to have higher interobserver agreement and to increase diagnostic yield and accuracy for motility disorders.^{27,38}

5.2 | Areas for future investigation

In general, an excellent level of agreement was achieved; however, several points failed to reach 90% consensus. This highlighted a number of areas with need for further investigation which include (a) the influence of HR-ARM software/hardware on results reporting (extrapolation from esophageal HRM suggests this may be important); (b) impact of HR-ARM with spatiotemporal presentation of pressure data on interobserver agreement; (c) the diagnostic and clinical utility (in terms of yield or disease stratification) of existing and novel HR-ARM metrics of anorectal function. For instance, the endurance squeeze and cough maneuvers have virtually no evidence to support their use as specific measures of anorectal function (despite, for instance, many working group members reporting the anecdotal utility of cough for describing a more severe phenotype of anal hypocontractility). In addition, previously reported manometric features of anal function (eg, transient anal sphincter relaxations) have been omitted due to time taken to observe these phenomena and the lack

LONDON CLASSIFICATION PART IV: DISORDERS OF RECTAL SENSATION

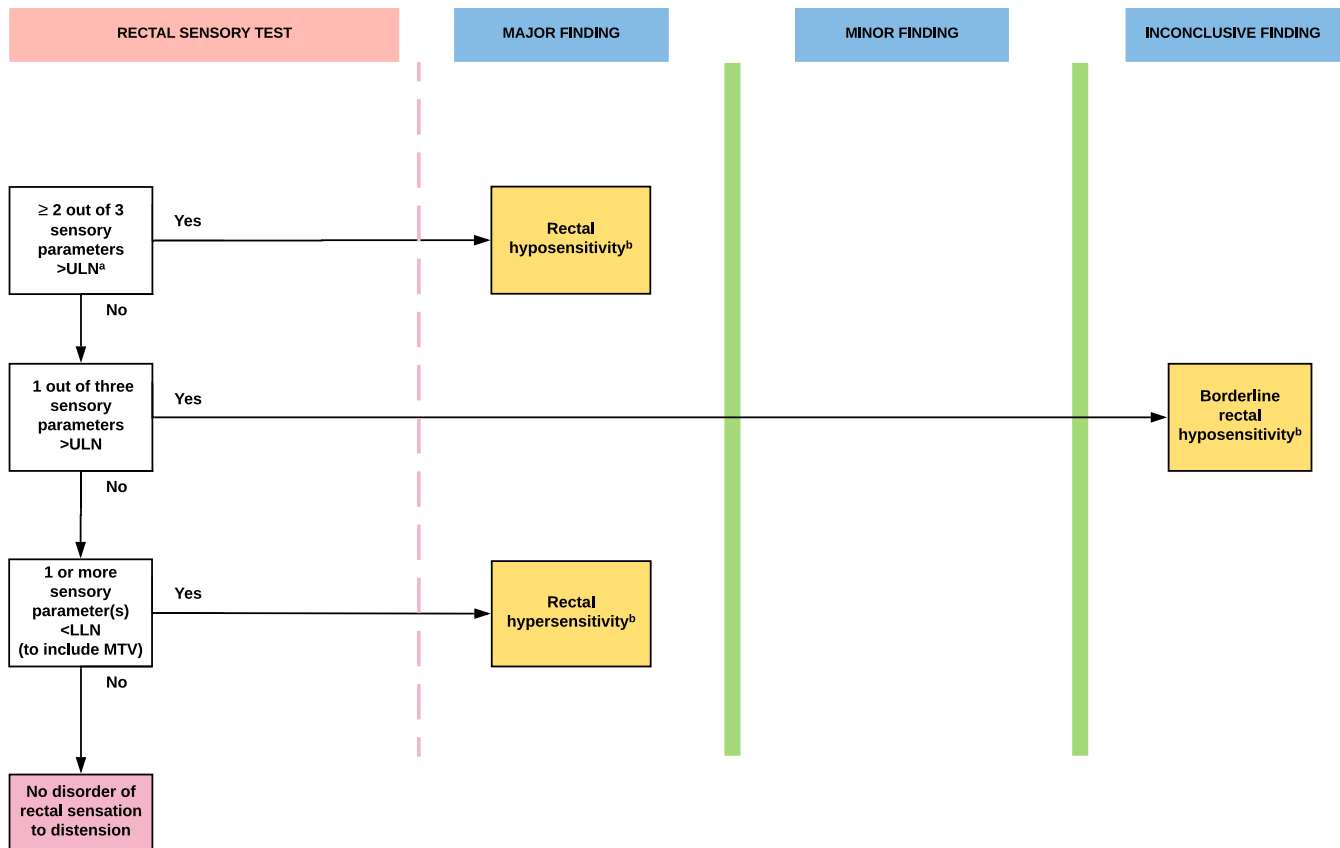


FIGURE 5 IAPWG classification part 4: Disorders of rectal sensation. ^asensory parameters are: first constant sensation volume (FCSV), desire to defecate volume (DDV) and maximum tolerated volume (MTV). ^babnormal results may be further described using additional methods (e.g. barostat to assess compliance). All results to be interpreted in context of adjunctive testing

of robust evidence of their clinical utility. High-quality diagnostic accuracy studies³⁹ are recommended, (d) re-evaluation of some currently used methods describing anorectal coordination. In particular, the qualitative description of dyssynergia by the Rao criteria is longstanding⁴⁰ and has been applied successfully also in HR-ARM studies^{31,41}; however, recent evidence has questioned the usefulness of quantitative metrics (eg, rectoanal pressure gradient) due to significant overlap between HR-ARM findings in patients with dyssynergia and those in apparently healthy volunteers.⁴² Definitions and clinical significance of HR-ARM in this area were both major areas of debate in group meetings and should be the focus of further study.

6 | CONCLUSIONS

The IAPWG protocol incorporating HR-ARM, RST, and BET together with the London Classification of anorectal disorders provides a much-needed framework for clinicians performing and interpreting tests of anorectal function. It is expected that these recommendations will evolve as experience with this technology increases and data from physiological and clinical studies emerge.

ACKNOWLEDGMENTS

The International Anorectal Physiology Working Group initiated the consensus meetings and provided material support for the consensus process. This process was endorsed by the European Society of Coloproctology (ESCP) and European Society of Neurogastroenterology and Motility (ESNM) with representation and support from members of the American Neurogastroenterology and Motility Society (ANMS), the South American and Latin Society (SLNG), the Asian Neurogastroenterology and Motility Association (ANMA), and the Australasian Neurogastroenterology and Motility Association (ANGMA).

CONFLICT OF INTEREST

Donato Altomare, William Chey, Phil Dinning, Anton Emmanuel, Ridzuan Farouk, Richelle Felt-Bersma, Kee Wook Jung, Anthony Lembo, Malcolm, Seung Jae Myung, and Christian Pehl: None; Adil Bharucha holds patents jointly with Medtronic Inc and Medspira Inc; Rebecca Burgell is a speaker for Bayer and advisory board member for Allergan and Anantara; Emma Carrington is a consultant provided lectures and training courses for Laborie; Guiseppe

Chiarioni is a member of the anorectal committee of the Rome Foundation; Mark Fox has received research funding from Covidien/Medtronic and speaker fees from Covidien/Medtronic, Sandhill, Medical Measurement Systems/Laborie, Reckitt Benckiser, and Mui Scientific; Henriette Heinrich is a member of Honorarium for teaching from Laborie; Charles Knowles is a consultant and invited speaker provided research grants for Medtronic; Allison; François Mion is a consultant for Laborie and lecturer for Medtronic; P. Ronan O'Connell is a consultant for Medtronic; Satish Rao is a advisory board member for and grant research support from Medtronic and Intone MV; Medtronics Incorporated and provided research grant support for advisory board; Jose María Remes-Troche is a member of Advisory Board for Takeda, Asofarma, and Astra Zeneca, received grants from Takeda, Sanfer, and Newton Foundation, is a speaker for Takeda, Asofarma, Sanfer, Sanofi Aventis, and Carnot; R. Matthew Reveille is a consultant for Diversatek Healthcare; S Mark Scott is a consultant and provided lectures and training courses for Laborie; Carolynne Vaizey provided research grants, and is a consultant, speaker, and educator for Medtronic Inc, and an educator for THD; Veronique Vitton is a consultant for Medtronic; William Whitehead provided research support from Medspira Instruments, Palette Life Sciences, and Allergan, and is a consultant for Ironwood, Takeda, and Valeant; Reuben Wong is a consultant for Laborie/MMS and Takeda.

AUTHOR CONTRIBUTIONS

EVC led the organization of the group and the consensus voting, drafted the manuscript, organized the revision of the manuscript, and approved the final version. HH co-organized group meetings and collated consensus voting, reviewed the manuscript, and approved the final version. CK, MF, and SMS acted as chairs of the group meetings reviewed the manuscript before circulation to the group as a whole, finalized the document with EVC, and approved the final version. SR acted as a chair of the group meetings and together with all other IAPWG members participated in the meetings, provided commentary on the manuscript, and approved the final version.

ORCID

Emma V. Carrington  <https://orcid.org/0000-0002-9467-9223>

Henriette Heinrich  <https://orcid.org/0000-0001-6355-0921>

Mark Fox  <https://orcid.org/0000-0003-4394-5584>

Satish Rao  <https://orcid.org/0000-0002-4446-8452>

Donato F. Altomare  <https://orcid.org/0000-0001-8980-2752>

Adil E. Bharucha  <https://orcid.org/0000-0002-7644-0390>

Kee Wook Jung  <https://orcid.org/0000-0002-3771-3691>

Anthony Lembo  <https://orcid.org/0000-0002-4479-1188>

Ravinder K. Mittal  <https://orcid.org/0000-0002-0181-9677>

Veronique Vitton  <https://orcid.org/0000-0002-1314-7111>

William E. Whitehead  <https://orcid.org/0000-0001-6587-7602>

REFERENCES

- Whitehead WE, Wald A, Diamant NE et al. Functional disorders of the anus and rectum. *Gut*. 1999;45(Suppl 2):li55-li59.
- Carrington EV, Scott SM, Bharucha A, et al. Expert consensus document: Advances in the evaluation of anorectal function. *Nat Rev Gastroenterol Hepatol*. 2018;15:309-323.
- Scott SM, Gladman MA. Manometric, sensorimotor, and neurophysiologic evaluation of anorectal function. *Gastroenterol Clin North Am*. 2008;37(511-38):vii.
- Rao SS, Azpiroz F, Diamant N, Enck P, Tougas G, Wald A. Minimum standards of anorectal manometry. *Neurogastroenterol Motil*. 2002;14:553-559.
- Schouten WR, van Vroonhoven TJ. A simple method of anorectal manometry. *Dis Colon Rectum*. 1983;26:721-724.
- Rao S, Hatfield R, Soffer E, Rao S, Beaty J, Conklin JL. Manometric tests of anorectal function in healthy adults. *Am J Gastroenterol*. 1999;94:773-783.
- Simpson RR, Kennedy ML, Nguyen MH, Dinning PG, Lubowski DZ. Anal manometry: a comparison of techniques. *Dis Colon Rectum*. 2006;49:1033-1038.
- Heinrich H, Fruehauf H, Sauter M, et al. The effect of standard compared to enhanced instruction and verbal feedback on anorectal manometry measurements. *Neurogastroenterol Motil*. 2013;25(230-7):e163.
- Barnett JL, Hasler WL, Camilleri M. American Gastroenterological Association medical position statement on anorectal testing techniques. *American Gastroenterological Association. Gastroenterology*. 1999;116:732-760.
- Azpiroz F, Enck P, Whitehead WE. Anorectal functional testing: review of collective experience. *Am J Gastroenterol*. 2002;97:232-240.
- Keighley M, Henry MM, Bartolo D, Mortensen N. Anorectal physiology measurement: report of a working party. *Br J Surg*. 1989;76:356-357.
- Carrington EV, Heinrich H, Knowles CH, Rao SS, Fox M, Scott SM. Methods of anorectal manometry vary widely in clinical practice: Results from an international survey. *Neurogastroenterol Motil*. 2017;n/a-n/a.
- Kahrilas P, Ghosh S, Pandolfino J. Esophageal motility disorders in terms of pressure topography: the Chicago Classification. *J Clin Gastroenterol*. 2008;42:627-635.
- <https://www.nice.org.uk/about/what-we-do/our-programmes/nice-guidance/nice-guidelines/shared-decision-making>. Accessed January 14, 2019
- Dinning PG, Carrington EV, Scott SM. The use of colonic and anorectal high-resolution manometry and its place in clinical work and in research. *Neurogastroenterol Motil*. 2015;27:1693-1708.
- Lee TH, Bharucha AE. How to perform and interpret a high-resolution anorectal manometry test. *J Neurogastroenterol Motil*. 2016;22:46-59.
- Jameson JS, Chia YW, Kamm MA, Speakman C, Chye YH, Henry MM. Effect of age, sex and parity on anorectal function. *Br J Surg*. 1994;81:1689-1692.
- Townsend DC, Carrington EV, Grossi U, et al. Pathophysiology of fecal incontinence differs between men and women: a case-matched study in 200 patients. *Neurogastroenterol Motil*. 2016;28:1580-1588.
- Sloots CE, Felt-Bersma RJ, Cuesta MA, et al. Rectal visceral sensitivity in healthy volunteers: influences of gender, age and methods. *Neurogastroenterol Motil*. 2000;12:361-368.

20. Chiarioni G, Kim SM, Vantini I, Whitehead WE. Validation of the balloon evacuation test: reproducibility and agreement with findings from anorectal manometry and electromyography. *Clin Gastroenterol Hepatol*. 2014;12:2049-2054.
21. Mazor Y, Prott G, Jones M, Kellow J, Ejova A, Malcolm A. Anorectal physiology in health: A randomized trial to determine the optimum catheter for the balloon expulsion test. *Neurogastroenterol Motil*. 2019;31:e13552.
22. Ratuapli S, Bharucha AE, Harvey D, Zinsmeister AR. Comparison of rectal balloon expulsion test in seated and left lateral positions. *Neurogastroenterol Motil*. 2013;25:e813-e820.
23. Palit S, Thin N, Knowles CH, Lunniss PJ, Bharucha AE, Scott SM. Diagnostic disagreement between tests of evacuatory function: a prospective study of 100 constipated patients. *Neurogastroenterology and motility : the official journal of the European Gastrointestinal Motility Society*. 2016;28:1589-1598.
24. Kahrilas PJ, Bredenoord AJ, Fox M, et al. The Chicago Classification of esophageal motility disorders, v3.0. *Neurogastroenterol Motil*. 2015;27:160-174.
25. Knowles CH, Scott SM, Legg PE, et al. Level of classification performance of KESS (symptom scoring system for constipation) validated in a prospective series of 105 patients. *Dis Colon Rectum*. 2002;45:842-843.
26. Gyawali CP, Kahrilas PJ, Savarino E, et al. Modern diagnosis of GERD: the Lyon Consensus. *Gut*. 2018;67:1351-1362.
27. Carlson DA, Ravi K, Kahrilas PJ, et al. Diagnosis of Esophageal Motility Disorders: Esophageal Pressure Topography vs. Conventional Line Tracing. *Am J Gastroenterol*. 2015;110:967-77; quiz 978.
28. Rao S, Bharucha AE, Chiarioni G, et al. Functional Anorectal Disorders. *Gastroenterology*. 2016.
29. Horrocks EJ, Chadi SA, Stevens NJ, Wexner SD, Knowles CH. Factors Associated With Efficacy of Percutaneous Tibial Nerve Stimulation for Fecal Incontinence, Based on Post-Hoc Analysis of Data From a Randomized Trial. *Clin Gastroenterol Hepatol*. 2017;15(1915-1921):e2.
30. Chiarioni G, Salandini L, Whitehead WE. Biofeedback benefits only patients with outlet dysfunction, not patients with isolated slow transit constipation. *Gastroenterology*. 2005;129:86-97.
31. Heinrich H, Sauter M, Fox M, et al. Assessment of Obstructive Defecation by High-Resolution Anorectal Manometry Compared With Magnetic Resonance Defecography. *Clin Gastroenterol Hepatol*. 2015;13(1310-1317):e1.
32. Prichard DO, Lee T, Parthasarathy G, Fletcher JG, Zinsmeister AR, Bharucha AE. High-resolution Anorectal Manometry for Identifying Defecatory Disorders and Rectal Structural Abnormalities in Women. *Clin Gastroenterol Hepatol*. 2017;15:412-420.
33. Kanis JA, Melton LJ, Christiansen C, Johnston CC, Khaltaev N. The diagnosis of osteoporosis. *J Bone Miner Res*. 1994;9:1137-1141.
34. Carrington EV, Knowles CH, Grossi U, et al. High-resolution Anorectal Manometry Measures Are More Accurate Than Conventional Measures in Detecting Anal Hypocontractility in Women With Fecal Incontinence. *Clin Gastroenterol Hepatol*. 2018.
35. Sauter M, Heinrich H, Fox M, et al. Toward more accurate measurements of anorectal motor and sensory function in routine clinical practice: validation of high-resolution anorectal manometry and Rapid Barostat Bag measurements of rectal function. *Neurogastroenterol Motil*. 2014;26:685-695.
36. Seo M, Joo S, Jung KW, Song EM, Rao S, Myung S-J. New Metrics in High-Resolution and High-Definition Anorectal Manometry. *Curr Gastroenterol Rep*. 2018;20:57.
37. Fox MR, Bredenoord AJ. Oesophageal high-resolution manometry: moving from research into clinical practice. *Gut*. 2008;57:405-423.
38. Roman S, Huot L, Zerbib F, et al. High-Resolution Manometry Improves the Diagnosis of Esophageal Motility Disorders in Patients With Dysphagia: A Randomized Multicenter Study. *Am J Gastroenterol*. 2016;111:372-380.
39. Bossuyt PM, Reitsma JB, Bruns DE, et al. The STARD statement for reporting studies of diagnostic accuracy: explanation and elaboration. *Ann Intern Med*. 2003;138:W1-12.
40. Rao SS. Dyssynergic defecation. *Gastroenterol Clin North Am*. 2001;30:97-114.
41. Ratuapli SK, Bharucha AE, Noelting J, Harvey DM, Zinsmeister AR. Phenotypic identification and classification of functional defecatory disorders using high-resolution anorectal manometry. *Gastroenterology*. 2013;144(314-322):e2.
42. Grossi U, Carrington EV, Bharucha AE, Horrocks EJ, Scott SM, Knowles CH. Diagnostic accuracy study of anorectal manometry for diagnosis of dyssynergic defecation. *Gut*. 2016;65:447-455.

SUPPORTING INFORMATION

Additional supporting information may be found online in the Supporting Information section at the end of the article.

How to cite this article: Carrington EV, Heinrich H, Knowles CH, et al. The international anorectal physiology working group (IAPWG) recommendations: Standardized testing protocol and the London classification for disorders of anorectal function. *Neurogastroenterol Motil*. 2020;32:e13679. <https://doi.org/10.1111/nmo.13679>