

 Open access • Proceedings Article • DOI:10.1109/ULTSYM.2018.8579808

Vortex Ring Phantom for Investigation of Ultrasound Vector Flow Imaging

— [Source link](#) 

[Emilia Badescu](#), [Simone Ambrogio](#), [John Fenner](#), [Herve Liebgott](#) ...+2 more authors

Institutions: [University of Lyon](#), [University of Sheffield](#)

Published on: 22 Oct 2018 - [International Ultrasonics Symposium](#)

Topics: [Imaging phantom](#), [Vortex ring](#), [Vortex](#), [Vector flow](#) and [Doppler effect](#)

Related papers:

- [An analytical phantom for the evaluation of medical flow imaging algorithms](#)
- [Vortex tracking in high density vector fields](#)
- [Optimization of 3-D Divergence-Free Flow Field Reconstruction Using 2-D Ultrasound Vector Flow Imaging.](#)
- [Flow quantification from time-resolved MRI vector fields](#)
- [Rapid mapping of flow velocity using a new PARSE method.](#)

Share this paper:    

View more about this paper here: <https://typeset.io/papers/vortex-ring-phantom-for-investigation-of-ultrasound-vector-1z0mok3dv4>



HAL
open science

Vortex ring phantom for investigation of ultrasound vector flow imaging

E. Badescu, S. Ambrogio, J. Fenner, H. Liebgott, D. Friboulet, David Garcia

► **To cite this version:**

E. Badescu, S. Ambrogio, J. Fenner, H. Liebgott, D. Friboulet, et al.. Vortex ring phantom for investigation of ultrasound vector flow imaging. IEEE International Ultrasonics Symposium, Oct 2018, Kobe, Japan. pp.1-4, 10.1109/ULTSYM.2018.8579808 . hal-01894169

HAL Id: hal-01894169

<https://hal.archives-ouvertes.fr/hal-01894169>

Submitted on 24 Mar 2019

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Vortex ring phantom for investigation of ultrasound Vector Flow Imaging

Emilia Badescu¹, Simone Ambrogio^{2,3,4}, John Fenner^{3,4}, Hervé Liebgott¹, Denis Friboulet¹, Damien Garcia¹

¹Université de Lyon, CREATIS ; CNRS UMR5220 ; Inserm U1206 ; INSA-Lyon ; Université Lyon 1, France, France,

²Leeds Test Objects Ltd., Boroughbridge, UK, United Kingdom,

³Mathematical Modelling in Medicine Group, Department of Infection, Immunity and Cardiovascular Disease, University of Sheffield, UK, United Kingdom,

⁴Insigneo Institute for In Silico Medicine, University of Sheffield, Sheffield, UK, United Kingdom

Email: emilia.badescu@creatis.insa-lyon.fr

Abstract— High frame rate ultrasound allows accurate quantification of the velocity flows, which could improve the current measurements that assist clinicians in diagnosis. The validation of novel approaches is essential before considering their translation to clinical ultrasound. To achieve this, we propose to use a vortex ring phantom, which presents two advantages. First, it offers complex three-dimensional flow patterns that closely reproduces intracardiac flow jets. Second, it is supposed to be controllable, reproducible and transportable, which is of key importance when validating new techniques. In this context, our objective was to evaluate if such a vortex phantom is a good candidate for validating and optimizing high-frame-rate velocity estimation methods. The 2D vortex kinematics was successfully recovered using speckle tracking and Doppler estimates. A good correlation ($r^2 = 0.95$) was found between the rotational and the translational velocity components for 315 estimations. Our preliminary 3-D results showed that Doppler velocities can be estimated in both sagittal and axial planes at thousands of volumes per second. In conclusion, the vortex phantom can be considered as a good candidate for testing novel high-frame-rate velocity estimation approaches.

Keywords—high-frame-rate imaging, vortex ring, vector flow, speckle tracking, Doppler

I. INTRODUCTION

The emergence of high-frame-rate ultrasound imaging has enabled significant progress in blood flow quantification, as it makes it possible to acquire wide field of views at fine temporal steps. Before considering bench-to-bedside translation, there is a need in evaluating the multi-component time-resolved velocity fields provided by the new imaging methods. *In vitro* test objects can be used to perform such an evaluation, since they provide realistic experimental conditions.

Several test devices have been proposed over time. A simple example is given by the flow tubular phantoms through which a blood mimicking fluid is usually pumped [1], [2]. Although the first attempts used c-flex rubber for constructing the walls of the vessels, this material caused a distortion of the ultrasound waves [3], which motivated the use of the vessel mimicking materials [4], [5]. Even if these phantoms provide a suitable experimental model, having acoustic properties similar to those of soft tissues, they do not take into account the major anatomical features, such as

arterial branching. In order to cope with this limitation, carotid bifurcation test objects have been proposed, which increases the complexity in terms of both anatomy and blood perfusion [6], [7]. Aneurysm aorta phantoms have also been proposed to reproduce realistic physiological conditions [8]. Other authors focused on developing rotating disk phantoms [9] enabling a wide range of velocity amplitudes and directions, as encountered in an *in vivo* flow. Additionally, assessing three-dimensional flows has become possible thanks to the *in vitro* spiral-flow model proposed by [10].

Although significant progress has been made for increasing the complexity of test objects and providing realistic physiological flows, the above mentioned phantoms are still insufficient to characterize a distinguishing feature of the intraventricular flow: the formation of vortices. The vortex dynamics has been shown to reveal physiological conditions that could allow early identification of cardiac abnormalities [11]. A realistic test object that simulates the left heart circulation and the vortex formation has been proposed in [12]. Although this phantom was successfully used to test vector flow mapping with conventional ultrasound [13], this *in vitro* model has the disadvantage of not being easily controllable and transportable. The vortex ring phantom proposed in [14] overcomes these limitations by offering a stable, reproducible and controllable model. Moreover, it makes it possible to generate vortices at different sizes and velocities. Thus, it provides a number of features that are of high relevance for the validation of high-frame-rate vector flow imaging by ultrasound [15].

In this context, the objective of this preliminary study was to evaluate if the vortex ring phantom is a good candidate for quantifying complex flows using high-frame-rate ultrasound methods. To achieve this purpose, we carried out 2-D and 3-D experiments.

II. METHODS

A. Vortex Ring

A vortex ring is a toroidal volume of fluid moving along the axis perpendicular to the torus plane (x -axis). The velocity along this axis (V_{trans}), represented in red in Fig. 1, is called “translational” in this manuscript. The toroidal vortex ring moves together with a flattened ellipsoidal volume which embraces it, called vortex atmosphere. Inside

the vortex atmosphere, the fluid circulates along the closed streamlines surrounding the toroidal core [16]. The toroidal core is constituted by concentric circles rotating at the angular velocity ω . The angular velocity together with the radius of the concentric circles give the rotational velocity, V_{rot} , as represented in green in Fig. 1.

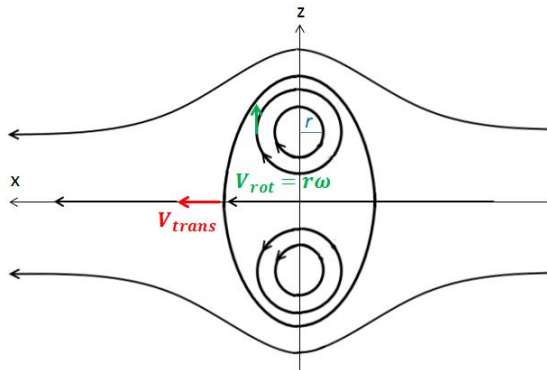


Fig. 1. Streamline pattern of the vortex ring

A vortex ring can be generated by using a cylinder-piston mechanism that ejects the fluid through a circular orifice. Such a system was proposed in [14]. The phantom used in this study was a recent prototype developed by the same authors.

B. 2D Acquisition set-up

Ultrasound 2-D images were acquired using a Vantage 256 research scanner (Verasonics Inc., Redmond, WA) controlling a 5-MHz linear transducer (ATL L7-4, 128 elements). We located the probe at approximately 10 cm downstream of the orifice, as shown in Fig. 2 A. Series of unsteered plane waves were transmitted through the seeded fluid and sets of vortex images were acquired through the plane illustrated in Fig. 2 B.

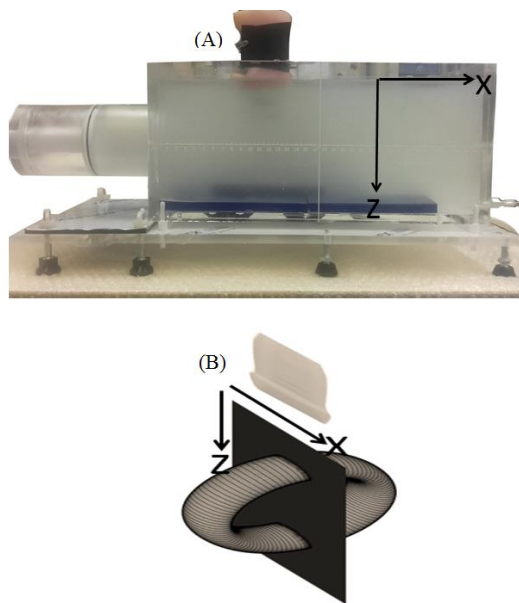


Fig. 2. The probe was located at approximately 10 cm downstream from the orifice (A), which allowed imaging vortex planes, as showed in (B)

C. 3D Acquisition set-up

Ultrasound volumes were acquired using four Vantage 256 scanners (Verasonics, Kirkland, WA, USA), synchronized to control a 3-MHz matrix-array transducer (Vermon, Tours, France). For more details about the 3D system, the reader can refer to [17].

D. Flow velocity estimation

Regarding 2D acquisitions, we estimated the vortex velocity fields using 1) echo-PIV by tracking the real-envelope speckle patterns using phase correlation [18]; and 2) a classical Doppler estimator based on a 2D autocorrelator applied on the I/Q data.

Since we did not have a reference at the time of the acquisitions, we acquired multiple sets of acquisitions to investigate the theoretical relationship between the vortical rotational and translational velocities. The maximum rotational component was retrieved from the Doppler velocity estimates. A series of successive Doppler maps were used to retrieve the translational component through a phase correlation method. Several diameters and velocities (2 and 2.5 cm, 1-7 cm/s) of the vortex phantom were used for this analysis. We acquired a total of 21 datasets consisting of 49 frames each. For each dataset, we estimated 15 pairs of rotational-translational velocity components.

Finally, regarding 3D acquisitions, we estimated Doppler velocity fields using a 2D autocorrelator, as for the 2D experiments.

III. RESULTS

A. 2D results

The velocity maps are shown in Fig. 3 for both Echo-PIV (A) and Doppler (B).

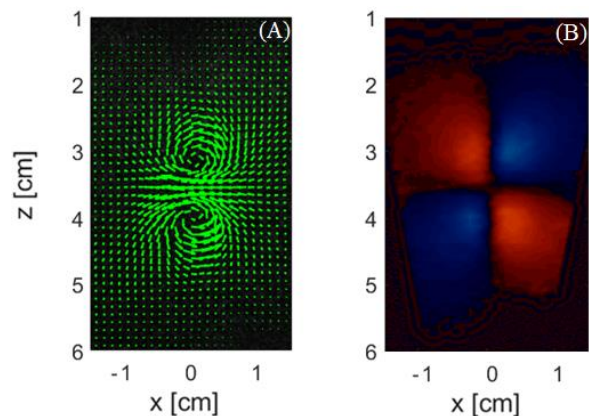


Fig. 3. Velocity estimation using Echo-PIV (A) and Doppler (B) for a translational velocity of 4 cm/s

The link between the rotational and translational velocity is shown in Fig. 4, where each set of points corresponds to a different set of acquisitions, acquired for a different translational velocity (between 1-7 cm/s) and for one of the two diameters: 2.5 cm (blue) and 2 cm (black). For each set of acquisitions, we show the median over 15 estimates and their deviation from the median (calculated as the absolute difference between median and the min/max estimated value

over the 15 pairs). The regression curve between the two velocity components is shown in red.

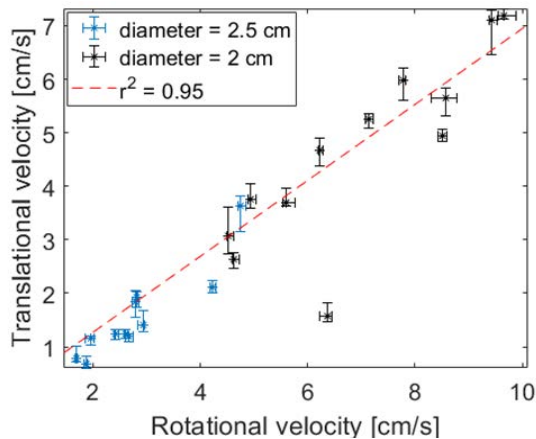


Fig. 4. Linear relationship between the rotational and the translational velocities for 2 orifice diameters (2.5 cm and 2 cm)

B. 3D preliminary results

Fig. 5 shows the Doppler maps obtained from a volumetric insonification of the vortex ring. Both x - z and y - z velocity maps are provided.

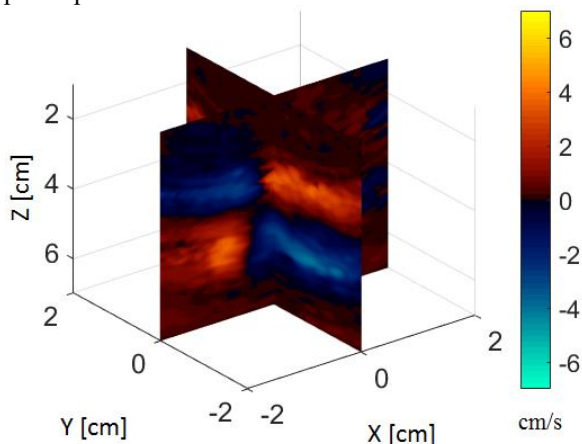


Fig. 5. 1D Doppler velocity components for the x - z and y - z planes

IV. DISCUSSION

Our preliminary results showed consistent observations with regards to the geometry and kinematics of the toroidal vortices, which tends to confirm that high-speed echo-PIV and Doppler by ultrafast ultrasound can be successfully used to evaluate the dynamics of cardiac-type vortices (Fig. 3). When the link between the rotational and translational speeds was investigated, the two velocity components were highly correlated ($r^2 = 0.95$, Fig. 4), in accordance with theory [19]. Although this shows a stable phantom behavior at a given position of the vortex propagation, a limitation of this study is that we did not compare our results with a reference. When developing new imaging-based diagnostic tools, the evaluation of their accuracy and reproducibility is of paramount importance. Indeed, this can have a significant impact on clinical decision. This is the reason why the knowledge of the ground-truth velocities is necessary; Therefore, an important perspective of this study will be the comparison of the ultrasound results against velocities yielded by an analytical model or computational fluid

dynamics. Ground-truth velocities can also be given directly by optical particle image velocimetry [20]. We also plan to design an MRI-compatible prototype to allow comparison against an alternative imaging modality, as done for vorticity in [21].

In spite of the current difficulty in providing a quantitative measure of accuracy, our promising 2D results in revealing the vortex kinematics, motivated us to extend our study to 3D. As observed in Fig. 5, in addition to the axial Doppler velocity components available when using a linear array (Fig. 3 B), the acquisitions with the 2D array allowed us to compute the sagittal Doppler components. Extending further the Doppler and the echo PIV approaches to 3D could offer a complete three-dimensional three-component vector field.

Although the 2D and 3D results presented in this study are preliminary, we illustrated the compatibility of the vortex ring generator with the ultrasound system.

V. CONCLUSION

High-frame-rate ultrasound can be used successfully to estimate complex vector flows such as the ones characterizing the ring vortices. 2D echo PIV and the Doppler estimator appear to be able to recover the vortex velocity maps. Preliminary 3D Doppler results showed that the Doppler velocities on both x - z and y - z planes can be recovered from series of volumetric insonifications.

Overall, this study showed that the vortex ring phantom is a good candidate for optimization and validation of ultrasound flow imaging methods in controllable, non-stationary, three-dimensional complex flows.

ACKNOWLEDGMENT

This project has received funding from the European Union's Horizon 2020 research and innovation programme under the Marie Skłodowska-Curie grant agreement No 642612, VPH-CaSE (www.vph-case.eu). This work was performed within the framework of the LABEX PRIMES (ANR-11-LABX-0063) of Université de Lyon, within the program "Investissements d'Avenir" (ANR-11-IDEX-0007) operated by the French National Research Agency (ANR). The Verasonics system was cofounded by the FEDER program, Saint-EtienneMetropole (SME) and Conseil General de la Loire (CG42) within the framework of the SonoCardioProtection Project led by Dr Pierre Croisille.

REFERENCES

- [1] Y. F. Law, R. S. Cobbold, K. W. Johnston, and P. A. Bascom, "Computer-controlled pulsatile pump system for physiological flow simulation.," *Med. Biol. Eng. Comput.*, vol. 25, no. 5, pp. 590–5, Sep. 1987.
- [2] P. R. Hoskins, T. Anderson, and W. N. McDicken, "A computer controlled flow phantom for generation of physiological Doppler waveforms.," *Phys. Med. Biol.*, vol. 34, no. 11, pp. 1709–17, Nov. 1989.
- [3] R. Steel and P. J. Fish, "Lumen pressure within obliquely insonated absorbent solid cylindrical shells with application to Doppler flow phantoms.," *IEEE Trans. Ultrason. Ferroelectr. Freq. Control*, vol. 49, no. 2, pp. 271–80, Feb. 2002.
- [4] D. M. King, C. M. Moran, J. D. McNamara, A. J. Fagan, and J. E. Browne, "Development of a Vessel-Mimicking Material for use in Anatomically Realistic Doppler Flow Phantoms," *Ultrasound Med. Biol.*, vol. 37, no. 5, pp. 813–826, May 2011.
- [5] X. Zhou, D. A. Kenwright, S. Wang, J. A. Hossack, and P. R. Hoskins, "Fabrication of Two Flow Phantoms for Doppler Ultrasound Imaging," *IEEE Trans. Ultrason. Ferroelectr. Freq. Control*, vol. 64, no. 1, pp. 53–65, Jan. 2017.
- [6] T. L. Poepping, H. N. Nikolov, R. N. Rankin, M. Lee, and D. W. Holdsworth, "An in vitro system for Doppler ultrasound flow studies in the stenosed carotid artery bifurcation.," *Ultrasound Med. Biol.*, vol. 28, no. 4, pp. 495–506, Apr. 2002.
- [7] S. Meagher, T. L. Poepping, K. V. Ramnarine, R. A. Black, and P. R. Hoskins, "Anatomical flow phantoms of the nonplanar carotid bifurcation, Part II: Experimental validation with Doppler ultrasound," *Ultrasound Med. Biol.*, vol. 33, no. 2, pp. 303–310, Feb. 2007.
- [8] V. Perrot, S. Meier, A. Bel-Brunon, H. Walter-Le Berre, B. Bou-Saïd, P. Chaudet, V. Detti, D. Vray, and H. Liebgott, "Biofidelic Abdominal Aorta Phantom: Cross-Over Preliminary Study Using UltraSound and Digital Image Stereo-Correlation," *IRBM*, vol. 38, no. 4, pp. 238–244, Aug. 2017.
- [9] O. D. Kripfgans, J. M. Rubin, A. L. Hall, and J. B. Fowlkes, "Vector Doppler imaging of a spinning disc ultrasound Doppler phantom," *Ultrasound Med. Biol.*, vol. 32, no. 7, pp. 1037–1046, Jul. 2006.
- [10] B. Y. S. Yiu and A. C. H. Yu, "Spiral Flow Phantom for Ultrasound Flow Imaging Experimentation," *IEEE Trans. Ultrason. Ferroelectr. Freq. Control*, vol. 64, no. 12, pp. 1840–1848, Dec. 2017.
- [11] G. Pedrizzetti, G. La Canna, O. Alfieri, and G. Tonti, "The vortex—an early predictor of cardiovascular outcome?," *Nat. Rev. Cardiol.*, vol. 11, no. 9, pp. 545–553, Sep. 2014.
- [12] D. Tanné, E. Bertrand, L. Kadem, P. Pibarot, and R. Rieu, "Assessment of left heart and pulmonary circulation flow dynamics by a new pulsed mock circulatory system," *Exp. Fluids*, vol. 48, no. 5, pp. 837–850, May 2010.
- [13] D. Garcia, J. C. del Álamo, D. Tanné, R. Yotti, C. Cortina, É. Bertrand, J. C. Antoranz, E. Pérez-David, R. Rieu, F. Fernández-Avilés, and J. Bermejo, "Two-Dimensional Intraventricular Flow Mapping by Digital Processing Conventional Color-Doppler Echocardiography Images," *IEEE Trans. Med. Imaging*, vol. 29, no. 10, pp. 1701–1713, Oct. 2010.
- [14] S. Ferrari, S. Ambrogio, A. Walker, A. J. Narracott, and J. W. Fenner, "The Ring Vortex: A Candidate for a Liquid-Based Complex Flow Phantom for Medical Imaging," Springer, Cham, 2018, pp. 893–902.
- [15] J. A. Jensen, S. I. Nikolov, A. C. H. Yu, and D. Garcia, "Ultrasound Vector Flow Imaging—Part II: Parallel Systems," *IEEE Trans. Ultrason. Ferroelectr. Freq. Control*, vol. 63, no. 11, pp. 1722–1732, Nov. 2016.
- [16] D. G. Akhmetov, "Theoretical Models of Vortex Rings," in *Vortex Rings*, Berlin, Heidelberg: Springer Berlin Heidelberg, 2009, pp. 5–32.
- [17] L. Petrusca, F. Varray, R. Souchon, A. Bernard, J.-Y. Chapelon, H. Liebgott, W. N'Djin, and M. Viallon, "Fast Volumetric Ultrasound B-Mode and Doppler Imaging with a New High-Channels Density Platform for Advanced 4D Cardiac Imaging/Therapy," *Appl. Sci.*, vol. 8, no. 2, p. 200, Jan. 2018.
- [18] P. Joos, J. Poree, H. Liebgott, D. Vray, M. Baudet, J. Faurie, F. Tournoux, G. Cloutier, B. Nicolas, and D. Garcia, "High-Frame-Rate Speckle-Tracking Echocardiography," *IEEE Trans. Ultrason. Ferroelectr. Freq. Control*, vol. 65, no. 5, pp. 720–728, May 2018.
- [19] A. Tinaikar, S. Advait, and S. Basu, "Understanding evolution of vortex rings in viscous fluids," *J. Fluid Mech.*, vol. 836, pp. 873–909, Feb. 2018.
- [20] A. Kheradvar, H. Houle, G. Pedrizzetti, G. Tonti, T. Belcik, M. Ashraf, J. R. Lindner, M. Gharib, and D. Sahn, "Echocardiographic Particle Image Velocimetry: A Novel Technique for Quantification of Left Ventricular Blood Vorticity Pattern," *J. Am. Soc. Echocardiogr.*, vol. 23, no. 1, pp. 86–94, Jan. 2010.
- [21] J. Faurie, M. Baudet, K. C. Assi, D. Auger, G. Gilbert, F. Tournoux, and D. Garcia, "Intracardiac Vortex Dynamics by High-Frame-Rate Doppler Vortography—In Vivo Comparison With Vector Flow Mapping and 4-D Flow MRI," *IEEE Trans. Ultrason. Ferroelectr. Freq. Control*, vol. 64, no. 2, pp. 424–432, Feb. 2017.